

LB131879


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

41243

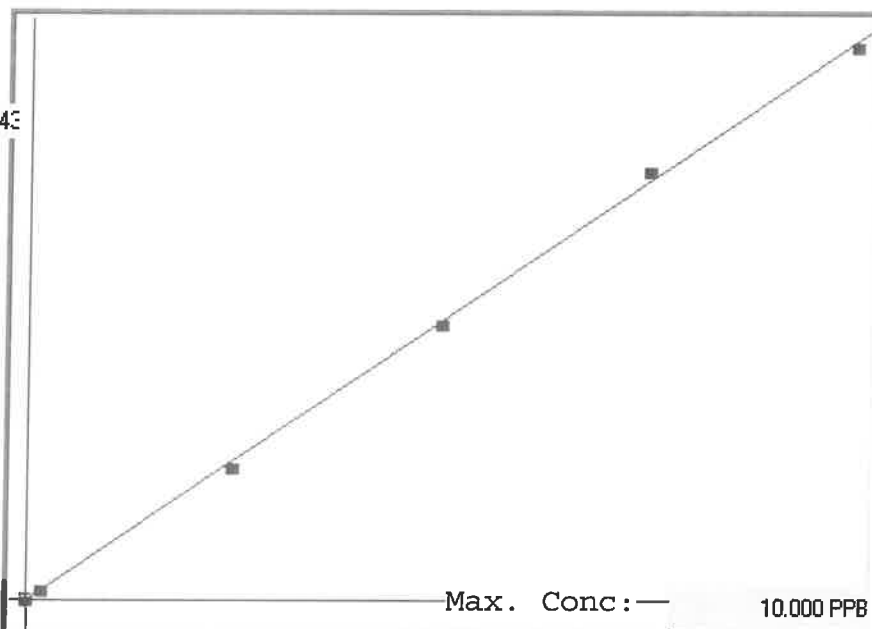

A= 0.0000e+000

B= 2.3954e-004

C= 2.2080e-002

Rho= 0.9996463

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	b/a)
0.0	0.000	0.037	0.037	63	0.000	63	0				1
0.2	0.200	0.221	0.021	832	0.0 %	832					1
2.5	2.500	2.394	-0.106	9902	0.0 %	9902					-4
5.0	5.000	4.963	-0.037	20625	0.0 %	20625					-1
7.5	7.500	7.683	0.183	31983	0.0 %	31983					2
10.0	10.000	9.901	-0.099	41243	0.0 %	41243					-1

LB131879 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 Aug 2024 13:34:50

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	5	63	-	0.0000	7470A	PPB	06 Aug 2024 13:43:45	S	Std
0.2 - 1	50.2	832	-	0.2000	7470A	PPB	06 Aug 2024 13:46:02	S	Std
2.5 - 1	52.5	9902	-	2.5000	7470A	PPB	06 Aug 2024 13:48:19	S	Std
5.0 - 1	57.5	20625	-	5.0000	7470A	PPB	06 Aug 2024 13:50:36	S	Std
7.5 - 1	57.5	31983	-	7.5000	7470A	PPB	06 Aug 2024 13:52:53	S	Std
10.0 - 1	510	41243	-	10.0000	7470A	PPB	06 Aug 2024 13:57:48	S	Std
ICV62 - 1	ICV62	17242	4.1523	-	7470A	PPB	06 Aug 2024 14:00:37	U	SMPL
ICB62 - 1	ICB62	-111	-0.0045	-	7470A	PPB	06 Aug 2024 14:02:52	U	SMPL
CCV01 - 1	CCV01	20672	4.9739	-	7470A	PPB	06 Aug 2024 14:05:09	U	SMPL
CCB01 - 1	CCB01	-137	-0.0107	-	7470A	PPB	06 Aug 2024 14:07:24	U	SMPL
CRA - 1	CRA	774	0.2075	-	7470A	PPB	06 Aug 2024 14:09:41	U	SMPL
HighStd - 1	HighStd	41240	9.9008	-	7470A	PPB	06 Aug 2024 14:11:56	U	SMPL
ChkStd - 1	ChkStd	29500	7.0885	-	7470A	PPB	06 Aug 2024 14:14:11	U	SMPL
PB162530BL - 1	PBW	-255	-0.0390	-	7470A	PPB	06 Aug 2024 14:16:29	U	SMPL
PB162530BS - 1	LCSW	16510	3.9769	-	7470A	PPB	06 Aug 2024 14:18:46	U	SMPL
P3448-02 - 1	TP1	-126	-0.0081	-	7470A	PPB	06 Aug 2024 14:21:02	U	SMPL
P3448-02DUP - 1	TP1DUP	37	0.0309	-	7470A	PPB	06 Aug 2024 14:23:20	U	SMPL
P3448-02MS - 1	TP1MS	17406	4.1915	-	7470A	PPB	06 Aug 2024 14:25:36	U	SMPL
P3448-02MSD - 1	TP1MSD	16849	4.0581	-	7470A	PPB	06 Aug 2024 14:27:53	U	SMPL
P3448-04 - 1	TP2	-115	-0.0055	-	7470A	PPB	06 Aug 2024 14:30:10	U	SMPL
CCV02 - 1	CCV02	20624	4.9624	-	7470A	PPB	06 Aug 2024 14:32:27	U	SMPL
CCB02 - 1	CCB02	-145	-0.0127	-	7470A	PPB	06 Aug 2024 14:34:42	U	SMPL
P3448-06 - 1	TP3	29	0.0290	-	7470A	PPB	06 Aug 2024 14:36:59	U	SMPL
P3448-08 - 1	TP4	36	0.0307	-	7470A	PPB	06 Aug 2024 14:39:14	U	SMPL
P3448-10 - 1	TP5	27	0.0285	-	7470A	PPB	06 Aug 2024 14:41:29	U	SMPL
P3448-12 - 1	TP6	41	0.0319	-	7470A	PPB	06 Aug 2024 14:43:45	U	SMPL
P3448-14 - 1	TP7	39	0.0314	-	7470A	PPB	06 Aug 2024 14:46:01	U	SMPL
PB162455TB - 1	PB162455TB	22	0.0274	-	7470A	PPB	06 Aug 2024 14:48:17	U	SMPL
P3448-02LX5 - 1		38	0.0312	-	7470A	PPB	06 Aug 2024 14:50:32	U	SMPL
P3448-02A - 1		16848	4.0579	-	7470A	PPB	06 Aug 2024 14:52:49	U	SMPL
CCV03 - 1	CCV03	20608	4.9585	-	7470A	PPB	06 Aug 2024 14:55:06	U	SMPL
CCB03 - 1	CCB03	-163	-0.0170	-	7470A	PPB	06 Aug 2024 14:57:23	U	SMPL