

LB131996


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

41578

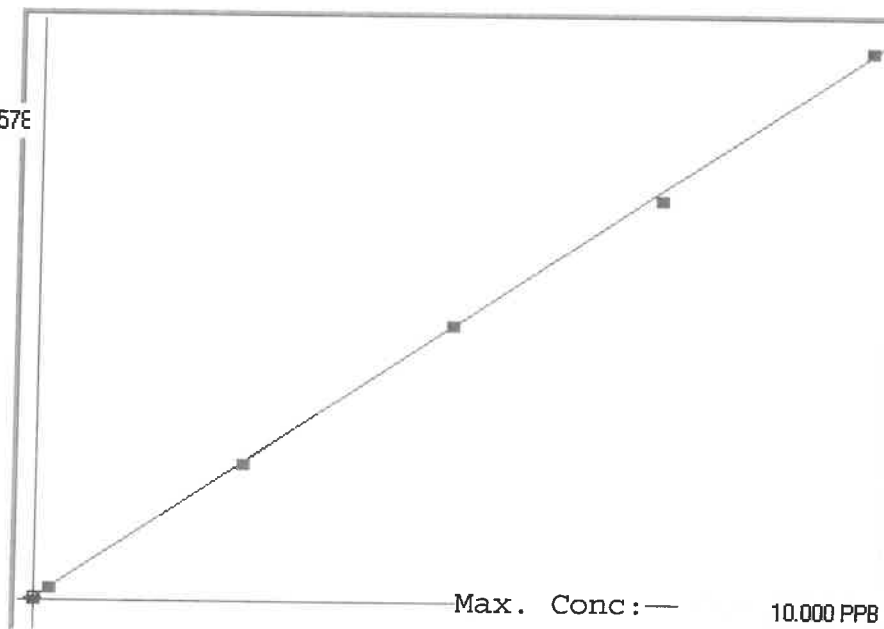

A= 0.0000e+000

B= 2.4343e-004

C= -4.3030e-002

Rho= 0.9998221

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.006	0.006	201	0.000	201	0				
0.2	0.200	0.204	0.004	1015	0.0 %	1015					
2.5	2.500	2.506	0.006	10470	0.0 %	10470					
5.0	5.000	5.049	0.049	20918	0.0 %	20918					
7.5	7.500	7.357	-0.143	30399	0.0 %	30399					
10.0	10.000	10.078	0.078	41578	0.0 %	41578					

120-121

LB131996 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 14 Aug 2024 07:29:12

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	201	-	0.0000	7470A	PPB	14 Aug 2024 07:37:56	S	Std
0.2 - 1	50.2	1015	-	0.2000	7470A	PPB	14 Aug 2024 07:40:13	S	Std
2.5 - 1	52.5	10470	-	2.5000	7470A	PPB	14 Aug 2024 07:42:30	S	Std
5.0 - 1	53	20918	-	5.0000	7470A	PPB	14 Aug 2024 07:44:46	S	Std
7.5 - 1	53.5	30399	-	7.5000	7470A	PPB	14 Aug 2024 07:47:03	S	Std
10.0 - 1	510	41578	-	10.0000	7470A	PPB	14 Aug 2024 07:54:38	S	Std
ICV74 - 1	ICV74	15863	3.8185	-	7470A	PPB	14 Aug 2024 07:57:23	U	SMPL
ICB74 - 1	ICB74	-69	-0.0598	-	7470A	PPB	14 Aug 2024 07:59:38	U	SMPL
CCV42 - 1	CCV42	20036	4.8343	-	7470A	PPB	14 Aug 2024 08:01:54	U	SMPL
CCB42 - 1	CCB42	-84	-0.0635	-	7470A	PPB	14 Aug 2024 08:06:44	U	SMPL
CRA - 1	CRA	1036	0.2092	-	7470A	PPB	14 Aug 2024 08:14:12	U	SMPL
HighStd - 1	HighStd	40943	9.9237	-	7470A	PPB	14 Aug 2024 08:16:26	U	SMPL
ChkStd - 1	ChkStd	28244	6.8324	-	7470A	PPB	14 Aug 2024 08:21:24	U	SMPL
PB162715BL - 1	PBW	0	-0.0430	-	7470A	PPB	14 Aug 2024 08:26:13	U	SMPL
PB162715BS - 1	LCSW	16160	3.8908	-	7470A	PPB	14 Aug 2024 08:31:10	U	SMPL
P3543-02 - 1	ARS20-0019	-5	-0.0442	-	7470A	PPB	14 Aug 2024 08:33:26	U	SMPL
P3548-02 - 1	72-12017-72-11934	77	-0.0243	-	7470A	PPB	14 Aug 2024 08:35:44	U	SMPL
P3548-05 - 1	RBR200036	94	-0.0201	-	7470A	PPB	14 Aug 2024 08:38:00	U	SMPL
P3548-08 - 1	343	30	-0.0357	-	7470A	PPB	14 Aug 2024 08:40:17	U	SMPL
P3548-11 - 1	289	-29	-0.0501	-	7470A	PPB	14 Aug 2024 08:42:32	U	SMPL
CCV43 - 1	CCV43	19858	4.7910	-	7470A	PPB	14 Aug 2024 08:44:47	U	SMPL
CCB43 - 1	CCB43	-196	-0.0907	-	7470A	PPB	14 Aug 2024 08:47:01	U	SMPL
P3548-14 - 1	IN-SITU-SOIL	-16	-0.0469	-	7470A	PPB	14 Aug 2024 08:49:18	U	SMPL
P3548-14DUP - 1	IN-SITU-SOILDUP	22	-0.0377	-	7470A	PPB	14 Aug 2024 08:51:33	U	SMPL
P3548-14MS - 1	IN-SITU-SOILMS	16437	3.9582	-	7470A	PPB	14 Aug 2024 08:56:30	U	SMPL
P3548-14MSD - 1	IN-SITU-SOILMSD	16060	3.8665	-	7470A	PPB	14 Aug 2024 08:58:45	U	SMPL
PB162621TB - 1	PB162621TB	-202	-0.0922	-	7470A	PPB	14 Aug 2024 09:01:03	U	SMPL
P3548-14LX5 - 1		-29	-0.0501	-	7470A	PPB	14 Aug 2024 09:03:20	U	SMPL
P3548-14A - 1		16379	3.9441	-	7470A	PPB	14 Aug 2024 09:05:36	U	SMPL
CCV44 - 1	CCV44	19900	4.8012	-	7470A	PPB	14 Aug 2024 09:07:53	U	SMPL
CCB44 - 1	CCB44	-192	-0.0898	-	7470A	PPB	14 Aug 2024 09:10:11	U	SMPL