


LB132023

7470A

INSTRUMENT ID: CV1

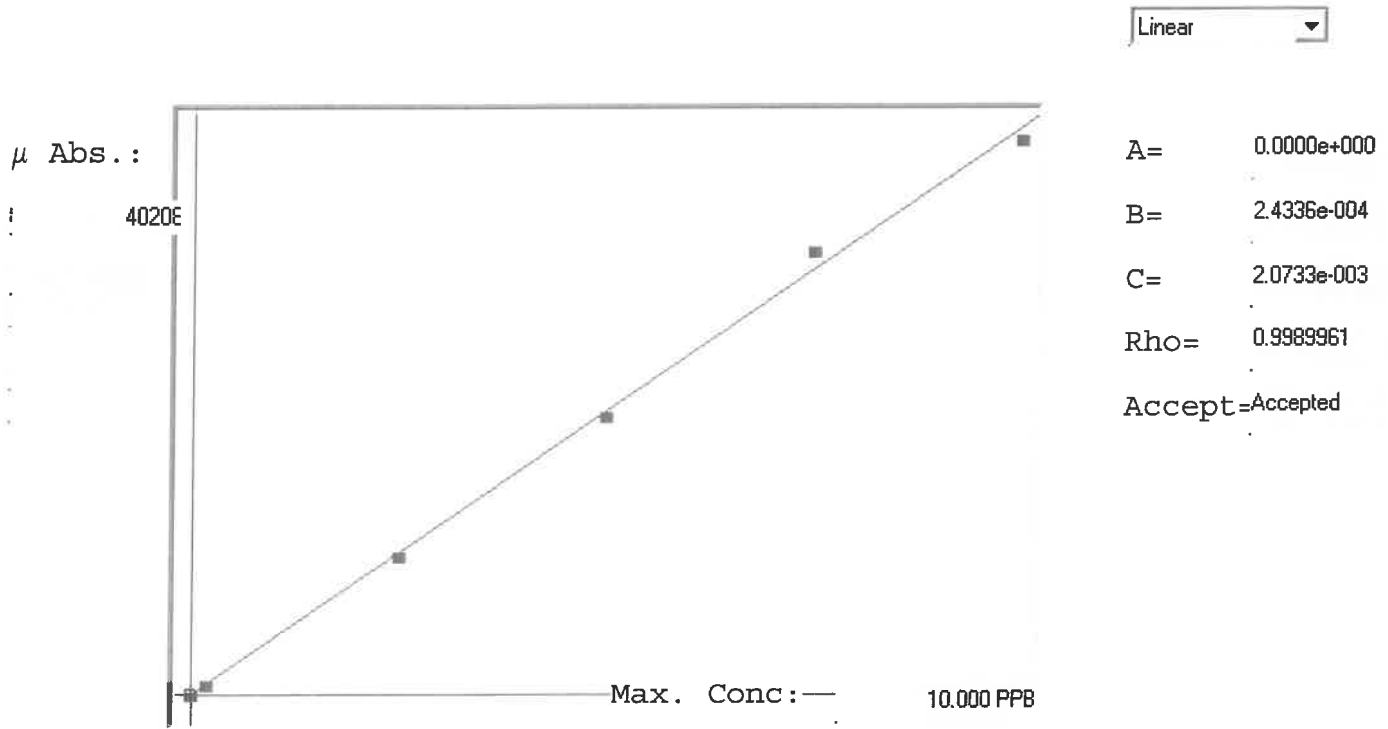

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/01)
0.0	0.000	0.022	0.022	82	0.000	82	0				-9
0.2	0.200	0.182	-0.018	741	0.0 %	741					-2
2.5	2.500	2.461	-0.039	10102	0.0 %	10102					-2
5.0	5.000	4.917	-0.083	20196	0.0 %	20196					4
7.5	7.500	7.831	0.331	32169	0.0 %	32169					-2
10.0	10.000	9.787	-0.213	40208	0.0 %	40208					

LB132023

Method: 7470A

Operator: Admin

Date of Analysis: 15 Aug 2024 10:16:07

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	82	-	0.0000	7470A	PPB	15 Aug 2024 10:16:25	S	Std
0.2 - 1	50.2	741	-	0.2000	7470A	PPB	15 Aug 2024 10:18:42	S	Std
2.5 - 1	52.5	10102	-	2.5000	7470A	PPB	15 Aug 2024 10:20:59	S	Std
5.0 - 1	55	20196	-	5.0000	7470A	PPB	15 Aug 2024 10:23:15	S	Std
7.5 - 1	57.5	32169	-	7.5000	7470A	PPB	15 Aug 2024 10:25:31	S	Std
10.0 - 1	510	40208	-	10.0000	7470A	PPB	15 Aug 2024 10:27:49	S	Std
ICV77 - 1	ICV77	16577	4.0363	-	7470A	PPB	15 Aug 2024 10:30:53	U	SMPL
ICB77 - 1	ICB77	-161	-0.0371	-	7470A	PPB	15 Aug 2024 10:33:08	U	SMPL
CCV50 - 1	CCV50	20400	4.9667	-	7470A	PPB	15 Aug 2024 10:35:24	U	SMPL
CCB50 - 1	CCB50	-140	-0.0320	-	7470A	PPB	15 Aug 2024 10:37:39	U	SMPL
CRA - 1	CRA	692	0.1705	-	7470A	PPB	15 Aug 2024 10:39:56	U	SMPL
HighStd - 1	HighStd	40870	9.9483	-	7470A	PPB	15 Aug 2024 10:42:11	U	SMPL
ChkStd - 1	ChkStd	30984	7.5424	-	7470A	PPB	15 Aug 2024 10:44:26	U	SMPL
PB162746BL - 1	PBW	-278	-0.0656	-	7470A	PPB	15 Aug 2024 10:46:44	U	SMPL
PB162746BS - 1	LCSW	16623	4.0475	-	7470A	PPB	15 Aug 2024 10:49:02	U	SMPL
P3577-01 - 1	OILY-DEBRIS	-136	-0.0310	-	7470A	PPB	15 Aug 2024 10:51:18	U	SMPL
P3597-02 - 1	SP-1-COMP	0	0.0021	-	7470A	PPB	15 Aug 2024 10:53:35	U	SMPL
P3597-02DUP - 1	SP-1-COMPDUP	31	0.0096	-	7470A	PPB	15 Aug 2024 10:55:52	U	SMPL
P3597-02MS - 1	SP-1-COMPMS	16551	4.0300	-	7470A	PPB	15 Aug 2024 10:58:09	U	SMPL
P3597-02MSD - 1	SP-1-COMPMSD	16335	3.9774	-	7470A	PPB	15 Aug 2024 11:00:24	U	SMPL
CCV51 - 1	CCV51	20248	4.9297	-	7470A	PPB	15 Aug 2024 11:02:41	U	SMPL
CCB51 - 1	CCB51	-126	-0.0286	-	7470A	PPB	15 Aug 2024 11:04:57	U	SMPL
PB162747BL - 1	PBW	19	0.0067	-	7470A	PPB	15 Aug 2024 11:07:14	U	SMPL
PB162747BS - 1	LCSW	17311	4.2149	-	7470A	PPB	15 Aug 2024 11:09:30	U	SMPL
P3574-02 - 1	WC-W-06-202408	-70	-0.0150	-	7470A	PPB	15 Aug 2024 11:11:45	U	SMPL
P3577-02 - 1	OILY-WATER	-1	0.0018	-	7470A	PPB	15 Aug 2024 11:14:02	U	SMPL
P3577-02DUP - 1	OILY-WATERDUP	6	0.0035	-	7470A	PPB	15 Aug 2024 11:16:18	U	SMPL
P3577-02MS - 1	OILY-WATERMS	13811	3.3632	-	7470A	PPB	15 Aug 2024 11:18:34	U	SMPL
P3577-02MSD - 1	OILY-WATERMSD	15589	3.7959	-	7470A	PPB	15 Aug 2024 11:20:50	U	SMPL
PB162762BL - 1	PBW	142	0.0366	-	7470A	PPB	15 Aug 2024 11:25:52	U	SMPL
PB162762BS - 1	LCSW	14199	3.4576	-	7470A	PPB	15 Aug 2024 11:28:09	U	SMPL
P3518-02 - 1	OU4-TS-01-080724	2249	0.5494	-	7470A	PPB	15 Aug 2024 11:30:25	U	SMPL
CCV52 - 1	CCV52	19645	4.7829	-	7470A	PPB	15 Aug 2024 11:32:41	U	SMPL
CCB52 - 1	CCB52	-186	-0.0432	-	7470A	PPB	15 Aug 2024 11:34:58	U	SMPL
P3518-04 - 1	OU4-TS-02-080724	730	0.1797	-	7470A	PPB	15 Aug 2024 11:37:16	U	SMPL
P3518-06 - 1	OU4-TS-03-080724	1450	0.3549	-	7470A	PPB	15 Aug 2024 11:39:31	U	SMPL
P3518-08 - 1	OU4-TS-04-080724	1301	0.3187	-	7470A	PPB	15 Aug 2024 11:41:46	U	SMPL
P3518-10 - 1	OU4-TS-05-080724	1301	0.3187	-	7470A	PPB	15 Aug 2024 11:44:02	U	SMPL
P3518-12 - 1	OU4-TS-06-080724	1360	0.3330	-	7470A	PPB	15 Aug 2024 11:46:17	U	SMPL
P3518-14 - 1	OU4-TS-07-080724	1166	0.2858	-	7470A	PPB	15 Aug 2024 11:48:33	U	SMPL
P3518-16 - 1	OU4-TS-08-080724	741	0.1824	-	7470A	PPB	15 Aug 2024 11:50:50	U	SMPL
P3518-18 - 1	OU4-TS-09-080724	323	0.0807	-	7470A	PPB	15 Aug 2024 11:53:07	U	SMPL
P3518-20 - 1	OU4-TS-10-080724	87	0.0232	-	7470A	PPB	15 Aug 2024 11:55:23	U	SMPL
P3518-22 - 1	OU4-TS-11-080724	1537	0.3761	-	7470A	PPB	15 Aug 2024 11:57:40	U	SMPL
CCV53 - 1	CCV53	19899	4.8447	-	7470A	PPB	15 Aug 2024 11:59:55	U	SMPL
CCB53 - 1	CCB53	-119	-0.0269	-	7470A	PPB	15 Aug 2024 12:02:11	U	SMPL
P3518-24 - 1	OU4-TS-12-080724	1341	0.3284	-	7470A	PPB	15 Aug 2024 12:04:27	U	SMPL
P3518-26 - 1	OU4-TS-13-080724	1164	0.2853	-	7470A	PPB	15 Aug 2024 12:06:42	U	SMPL
P3518-28 - 1	OU4-TS-14-080724	1238	0.3034	-	7470A	PPB	15 Aug 2024 12:08:58	U	SMPL
P3518-30 - 1	OU4-TS-15-080724	1486	0.3637	-	7470A	PPB	15 Aug 2024 12:11:13	U	SMPL
P3518-30DUP - 1	OU4-TS-15-080724DUP	1131	0.2773	-	7470A	PPB	15 Aug 2024 12:13:28	U	SMPL
P3518-30MS - 1	OU4-TS-15-080724MS	16940	4.1246	-	7470A	PPB	15 Aug 2024 12:18:42	U	SMPL
P3518-30MSD - 1	OU4-TS-15-080724MSD	17040	4.1490	-	7470A	PPB	15 Aug 2024 12:20:58	U	SMPL
PB162763BL - 1	PBW	-84	-0.0184	-	7470A	PPB	15 Aug 2024 12:23:17	U	SMPL
PB162763BS - 1	LCSW	16855	4.1040	-	7470A	PPB	15 Aug 2024 12:25:35	U	SMPL
P3519-02 - 1	OU4-TS-16-080724	295	0.0739	-	7470A	PPB	15 Aug 2024 12:27:50	U	SMPL
CCV54 - 1	CCV54	19655	4.7854	-	7470A	PPB	15 Aug 2024 12:30:07	U	SMPL
CCB54 - 1	CCB54	-148	-0.0339	-	7470A	PPB	15 Aug 2024 12:32:22	U	SMPL
P3519-04 - 1	OU4-TS-17-080724	258	0.0649	-	7470A	PPB	15 Aug 2024 12:34:39	U	SMPL
P3519-06 - 1	OU4-TS-18-080724	259	0.0651	-	7470A	PPB	15 Aug 2024 12:36:55	U	SMPL
P3519-08 - 1	OU4-TS-19-080724	63	0.0174	-	7470A	PPB	15 Aug 2024 12:39:10	U	SMPL
P3519-10 - 1	OU4-TS-20-080724	41	0.0121	-	7470A	PPB	15 Aug 2024 12:41:25	U	SMPL
P3519-12 - 1	OU4-TS-21-080724	52	0.0147	-	7470A	PPB	15 Aug 2024 12:43:41	U	SMPL
P3519-14 - 1	OU4-TS-22-080724	80	0.0215	-	7470A	PPB	15 Aug 2024 12:45:57	U	SMPL
P3519-16 - 1	OU4-TS-23-080724	58	0.0162	-	7470A	PPB	15 Aug 2024 12:48:13	U	SMPL
P3519-18 - 1	OU4-CF-01-080724	239	0.0602	-	7470A	PPB	15 Aug 2024 12:50:30	U	SMPL
P3519-20 - 1	OU4-CF-02-080724	86	0.0230	-	7470A	PPB	15 Aug 2024 12:52:46	U	SMPL
P3519-22 - 1	OU4-CF-03-080724	93	0.0247	-	7470A	PPB	15 Aug 2024 12:55:02	U	SMPL
CCV55 - 1	CCV55	19183	4.6705	-	7470A	PPB	15 Aug 2024 12:57:18	U	SMPL
CCB55 - 1	CCB55	-103	-0.0230	-	7470A	PPB	15 Aug 2024 12:59:34	U	SMPL
P3519-24 - 1	OU4-CF-04-080724	202	0.0512	-	7470A	PPB	15 Aug 2024 13:01:52	U	SMPL
P3519-26 - 1	OU4-CF-05-080724	101	0.0267	-	7470A	PPB	15 Aug 2024 13:04:08	U	SMPL
P3519-28 - 1	OU4-CF-06-080724	111	0.0291	-	7470A	PPB	15 Aug 2024 13:06:24	U	SMPL
P3519-30 - 1	OU4-CF-07-080724	51	0.0145	-	7470A	PPB	15 Aug 2024 13:08:39	U	SMPL
P3519-30DUP - 1	OU4-CF-07-080724DUP	34	0.0103	-	7470A	PPB	15 Aug 2024 13:10:56	U	SMPL
P3519-30MS - 1	OU4-CF-07-080724MS	17131	4.1711	-	7470A	PPB	15 Aug 2024 13:13:12	U	SMPL
P3519-30MSD - 1	OU4-CF-07-080724MSD	17246	4.1991	-	7470A	PPB	15 Aug 2024 13:15:28	U	SMPL
PB162764BL - 1	PBW	40	0.0118	-	7470A	PPB	15 Aug 2024 13:21:32	U	SMPL
PB162764BS - 1	LCSW	15563	3.7895	-	7470A	PPB	15 Aug 2024 13:23:49	U	SMPL
P3520-02 - 1	OU4-CF-08-080624	442	0.1096	-	7470A	PPB	15 Aug 2024 13:26:05	U	SMPL
CCV56 - 1	CCV56	20677	5.0341	-	7470A	PPB	15 Aug 2024 13:28:22	U	SMPL

LB132023

Method: 7470A

Operator: Admin

Date of Analysis: 15 Aug 2024 10:16:07

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
CCB56 - 1	CCB56	-129	-0.0293	-7470A	PPB		15 Aug 2024 13:30:38	U	SMPL
P3520-04 - 1	OU4-CF-09-080624	324	0.0809	-7470A	PPB		15 Aug 2024 13:32:56	U	SMPL
P3520-06 - 1	OU4-CF-10-080624	128	0.0332	-7470A	PPB		15 Aug 2024 13:35:12	U	SMPL
P3520-08 - 1	OU4-CF-11-080624	78	0.0211	-7470A	PPB		15 Aug 2024 13:37:28	U	SMPL
P3520-10 - 1	OU4-CF-12-080624	71	0.0194	-7470A	PPB		15 Aug 2024 13:39:44	U	SMPL
P3520-12 - 1	OU4-CF-13-080624	77	0.0208	-7470A	PPB		15 Aug 2024 13:42:00	U	SMPL
P3520-14 - 1	OU4-CF-14-080624	69	0.0189	-7470A	PPB		15 Aug 2024 13:44:16	U	SMPL
P3520-16 - 1	OU4-VSL-01-080624	92	0.0245	-7470A	PPB		15 Aug 2024 13:46:32	U	SMPL
P3520-18 - 1	OU4-57S-01-080624	40	0.0118	-7470A	PPB		15 Aug 2024 13:48:48	U	SMPL
P3520-18DUP - 1	OU4-57S-01-080624DUP	47	0.0135	-7470A	PPB		15 Aug 2024 13:51:05	U	SMPL
P3520-18MS - 1	OU4-57S-01-080624MS	15970	3.8886	-7470A	PPB		15 Aug 2024 13:53:22	U	SMPL
CCV57 - 1	CCV57	18712	4.5559	-7470A	PPB		15 Aug 2024 13:55:38	U	SMPL
CCB57 - 1	CCB57	-97	-0.0215	-7470A	PPB		15 Aug 2024 13:57:56	U	SMPL
P3520-18MSD - 1	OU4-57S-01-080624MSD	15359	3.7399	-7470A	PPB		15 Aug 2024 14:00:13	U	SMPL
PB162662TB - 1	PB162662TB	-55	-0.0113	-7470A	PPB		15 Aug 2024 14:02:30	U	SMPL
PB162613TB - 1	PB162613TB	148	0.0381	-7470A	PPB		15 Aug 2024 14:04:47	U	SMPL
PB162624TB - 1	PB162624TB	38	0.0113	-7470A	PPB		15 Aug 2024 14:10:02	U	SMPL
PB162682TB - 1	PB162682TB	39	0.0116	-7470A	PPB		15 Aug 2024 14:16:46	U	SMPL
PB162683TB - 1	PB162683TB	40	0.0118	-7470A	PPB		15 Aug 2024 14:19:02	U	SMPL
CCV58 - 1	CCV58	19330	4.7063	-7470A	PPB		15 Aug 2024 14:21:18	U	SMPL
CCB58 - 1	CCB58	-114	-0.0257	-7470A	PPB		15 Aug 2024 14:23:35	U	SMPL
P3597-02LX5 - 1		-12	-0.0008	-7470A	PPB		15 Aug 2024 14:25:53	U	SMPL
P3597-02A - 1		15444	3.7606	-7470A	PPB		15 Aug 2024 14:28:10	U	SMPL
P3577-02LX5 - 1		-119	-0.0269	-7470A	PPB		15 Aug 2024 14:30:25	U	SMPL
P3577-02A - 1		14065	3.4250	-7470A	PPB		15 Aug 2024 14:32:43	U	SMPL
P3518-30LX5 - 1		167	0.0427	-7470A	PPB		15 Aug 2024 14:34:59	U	SMPL
P3518-30A - 1		15425	3.7559	-7470A	PPB		15 Aug 2024 14:37:18	U	SMPL
P3519-30LX5 - 1		-147	-0.0337	-7470A	PPB		15 Aug 2024 14:39:34	U	SMPL
P3519-30A - 1		15775	3.8411	-7470A	PPB		15 Aug 2024 14:41:52	U	SMPL
P3520-18LX5 - 1		-142	-0.0325	-7470A	PPB		15 Aug 2024 14:44:09	U	SMPL
P3520-18A - 1		15274	3.7192	-7470A	PPB		15 Aug 2024 14:46:27	U	SMPL
CCV59 - 1	CCV59	20121	4.8988	-7470A	PPB		15 Aug 2024 14:48:43	U	SMPL
CCB59 - 1	CCB59	-158	-0.0364	-7470A	PPB		15 Aug 2024 14:51:02	U	SMPL