

66132029

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

8/15/2024 12:47

Reviewed by : RM

Instrument ID : Konelab

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.084	0.0	0.105	
ICB1	0.000	0.0	0.004	
CCV1	0.927	0.0	0.090	
CCB1	-0.002	0.0	0.004	
PB162737BL	0.002	0.0	0.004	
PB162737BS	1.085	0.0	0.105	
P3390-10	0.022	0.0	0.006	
P3390-11	0.047	0.0	0.008	
P3536-01	0.009	0.0	0.005	
P3536-01DUP	0.007	0.0	0.005	
P3536-01MS	1.151	0.0	0.111	
P3536-01MSD	1.154	0.0	0.111	
CCV2	0.918	0.0	0.089	
CCB2	-0.003	0.0	0.004	

N 14
Mean 0.457
SD 0.5398
CV% 118.09

Aquakem v. 7.2AQ1

Results from time period:

Thu Aug 15 11:54:56 2024

Thu Aug 15 12:46:46 2024

Sample Id	Sam/Ctr/c/	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0025	mg/l	8/15/2024 11:54:56	
0.05PPM	A	Phenolics-	P	0.059	mg/l	8/15/2024 11:54:57	
0.1PPM	A	Phenolics-	P	0.1034	mg/l	8/15/2024 11:54:58	
0.25PPM	A	Phenolics-	P	0.2485	mg/l	8/15/2024 11:54:59	
0.50PPM	A	Phenolics-	P	0.4909	mg/l	8/15/2024 11:55:00	
1.0PPM	A	Phenolics-	P	0.9875	mg/l	8/15/2024 11:55:01	
2.0PPM	A	Phenolics-	P	2.0083	mg/l	8/15/2024 11:55:02	
ICV1	S	Phenolics-	P	1.084	mg/l	8/15/2024 12:32:45	
ICB1	S	Phenolics-	P	0.0003	mg/l	8/15/2024 12:32:48	
CCV1	S	Phenolics-	P	0.9268	mg/l	8/15/2024 12:32:49	
CCB1	S	Phenolics-	P	-0.0025	mg/l	8/15/2024 12:32:51	
PB162737BL	S	Phenolics-	P	0.0016	mg/l	8/15/2024 12:32:53	
PB162737BS	S	Phenolics-	P	1.0852	mg/l	8/15/2024 12:32:56	
P3390-10	S	Phenolics-	P	0.0218	mg/l	8/15/2024 12:42:48	
P3390-11	S	Phenolics-	P	0.047	mg/l	8/15/2024 12:42:50	
P3536-01	S	Phenolics-	P	0.0088	mg/l	8/15/2024 12:42:52	
P3536-01DUP	S	Phenolics-	P	0.0073	mg/l	8/15/2024 12:42:53	
P3536-01MS	S	Phenolics-	P	1.1511	mg/l	8/15/2024 12:42:55	
P3536-01MSD	S	Phenolics-	P	1.1541	mg/l	8/15/2024 12:42:56	
CCV2	S	Phenolics-	P	0.9175	mg/l	8/15/2024 12:42:57	
CCB2	S	Phenolics-	P	-0.0033	mg/l	8/15/2024 12:46:46	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

8/15/2024 11:59 Reviewed by : RM Instrument ID : Konelab


Test Phenolics-

Accepted 8/15/2024 11:59

Factor 10.79
Bias 0.004

Coeff. of det. 0.999870

Errors

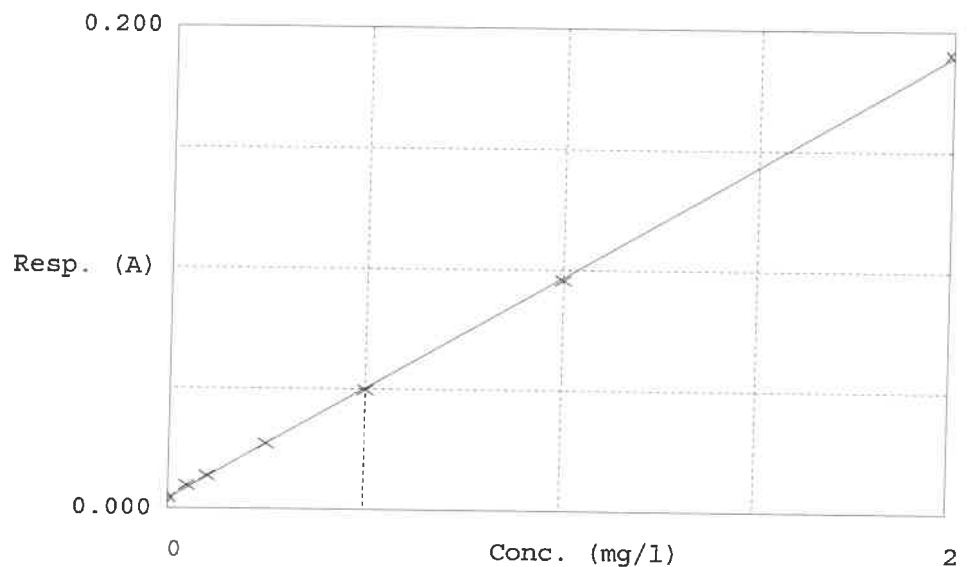

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.004	0.0025	0.0000	-
2	Phenol-2	0.010	0.0590	0.0500	18.0
3	Phenol-2	0.014	0.1034	0.1000	3.4
4	Phenol-2	0.027	0.2485	0.2500	-0.6
5	Phenol-2	0.050	0.4909	0.5000	-1.8
6	Phenol-2	0.096	0.9875	1.0000	-1.3
7	Phenol-2	0.190	2.0083	2.0000	0.4

08/15/2024
RM