

66132032

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

8/15/2024 13:49

Reviewed by : RM Instrument ID : Konelab

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.086	0.0	0.105	
ICB1	0.001	0.0	0.004	
CCV1	0.924	0.0	0.090	
CCB1	0.002	0.0	0.004	
PB162736BL	-0.003	0.0	0.004	
PB162736BS	1.080	0.0	0.104	
P3390-01	0.024	0.0	0.006	
P3390-02	0.048	0.0	0.009	
PB162738BL	-0.001	0.0	0.004	
PB162738BS	1.079	0.0	0.104	
P3390-07	0.023	0.0	0.006	
P3390-08	0.047	0.0	0.008	
CCV2	0.935	0.0	0.091	
CCB2	0.002	0.0	0.004	

N	14
Mean	0.375
SD	0.5021
CV%	133.95

Aquakem v. 7.2AQ1

Results from time period:

Thu Aug 15 13:25:08 2024

Thu Aug 15 13:40:07 2024

Sample Id	Sam/Ctr/cf	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0025	mg/l	8/15/2024 11:54:56	
0.05PPM	A	Phenolics-	P	0.059	mg/l	8/15/2024 11:54:57	
0.1PPM	A	Phenolics-	P	0.1034	mg/l	8/15/2024 11:54:58	
0.25PPM	A	Phenolics-	P	0.2485	mg/l	8/15/2024 11:54:59	
0.50PPM	A	Phenolics-	P	0.4909	mg/l	8/15/2024 11:55:00	
1.0PPM	A	Phenolics-	P	0.9875	mg/l	8/15/2024 11:55:01	
2.0PPM	A	Phenolics-	P	2.0083	mg/l	8/15/2024 11:55:02	
ICV1	S	Phenolics-	P	1.0863	mg/l	8/15/2024 13:25:08	
ICB1	S	Phenolics-	P	0.0009	mg/l	8/15/2024 13:25:11	
CCV1	S	Phenolics-	P	0.9237	mg/l	8/15/2024 13:25:13	
CCB1	S	Phenolics-	P	0.0016	mg/l	8/15/2024 13:25:14	
PB162736BL	S	Phenolics-	P	-0.0028	mg/l	8/15/2024 13:25:16	
PB162736BS	S	Phenolics-	P	1.0796	mg/l	8/15/2024 13:25:19	
P3390-01	S	Phenolics-	P	0.0242	mg/l	8/15/2024 13:35:10	
P3390-02	S	Phenolics-	P	0.0485	mg/l	8/15/2024 13:35:13	
PB162738BL	S	Phenolics-	P	-0.0006	mg/l	8/15/2024 13:35:15	
PB162738BS	S	Phenolics-	P	1.0791	mg/l	8/15/2024 13:35:17	
P3390-07	S	Phenolics-	P	0.023	mg/l	8/15/2024 13:35:19	
P3390-08	S	Phenolics-	P	0.0468	mg/l	8/15/2024 13:35:21	
CCV2	S	Phenolics-	P	0.9353	mg/l	8/15/2024 13:40:04	
CCB2	S	Phenolics-	P	0.0017	mg/l	8/15/2024 13:40:07	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

8/15/2024 11:59

Reviewed by : RM

Instrument ID : Konelab


Test Phenolics-

Accepted 8/15/2024 11:59

Factor 10.79
Bias 0.004

Coeff. of det. 0.999870

Errors

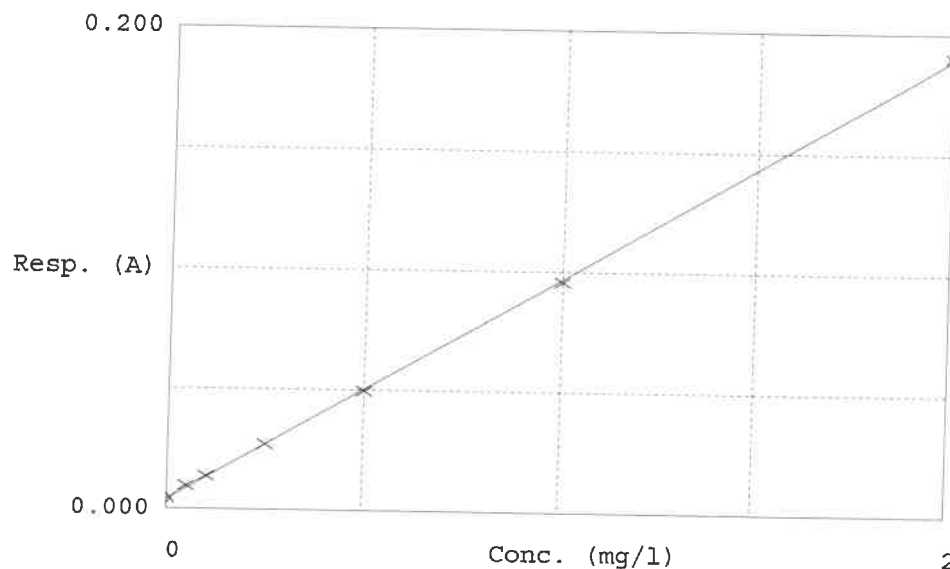

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.004	0.0025	0.0000	-
2	Phenol-2	0.010	0.0590	0.0500	18.0
3	Phenol-2	0.014	0.1034	0.1000	3.4
4	Phenol-2	0.027	0.2485	0.2500	-0.6
5	Phenol-2	0.050	0.4909	0.5000	-1.8
6	Phenol-2	0.096	0.9875	1.0000	-1.3
7	Phenol-2	0.190	2.0083	2.0000	0.4

08/15/2024
RM