


LB132045

7471B

INSTRUMENT ID: CV1

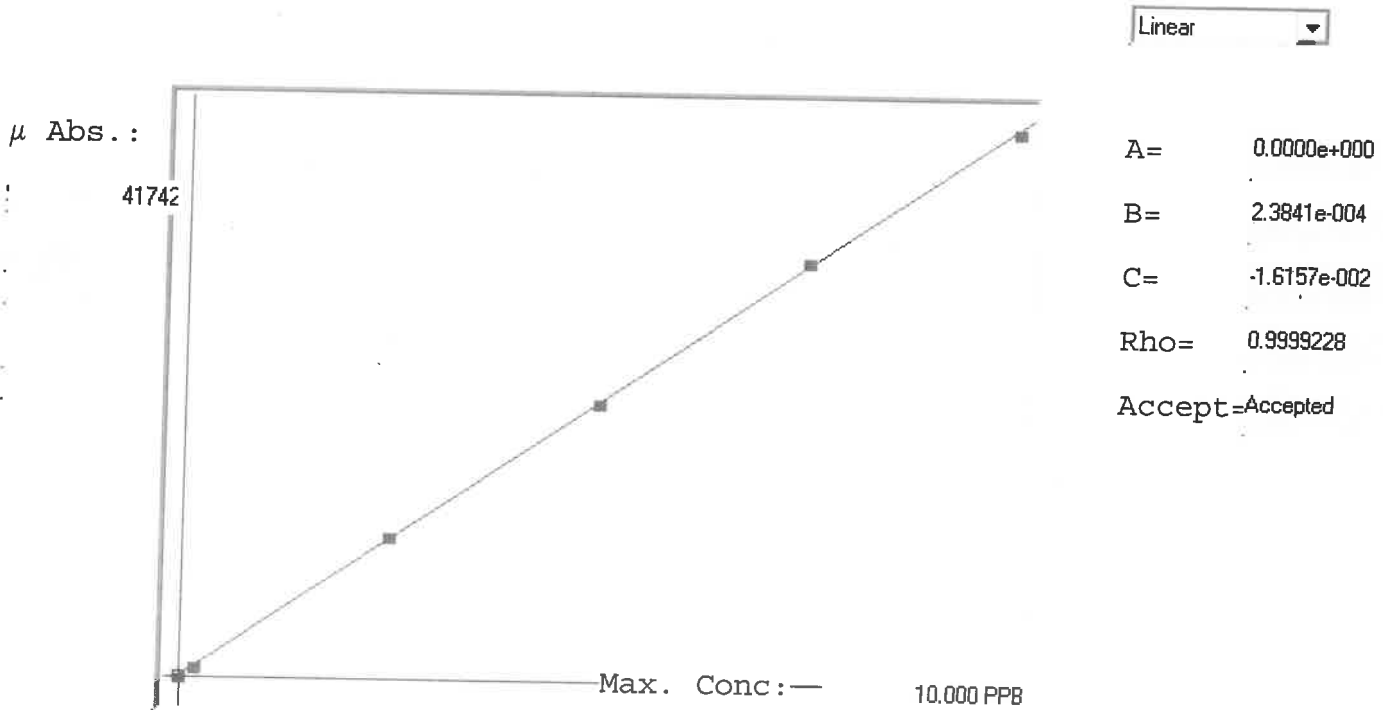

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	-0.016	-0.016	2	0.000	2					9/0/0
0.2	0.200	0.176	-0.024	806	0.0 %	806					-12
2.5	2.500	2.533	0.033	10694	0.0 %	10694					1
5.0	5.000	4.991	-0.009	21002	0.0 %	21002					0
7.5	7.500	7.580	0.080	31863	0.0 %	31863					1
10.0	10.000	9.935	-0.065	41742	0.0 %	41742					-1

LB132045 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 16 Aug 2024 10:14:42

Sample ID	Extended ID	μ Abs.	Conc.	Stnd Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	2	-	0.0000	7471B	PPB	16 Aug 2024 10:26:17	S	Std
0.2 - 1	10.2	806	-	0.2000	7471B	PPB	16 Aug 2024 10:28:34	S	Std
2.5 - 1	52.5	10694	-	2.5000	7471B	PPB	16 Aug 2024 10:30:51	S	Std
5.0 - 1	35	21002	-	5.0000	7471B	PPB	16 Aug 2024 10:33:08	S	Std
7.5 - 1	57.5	31863	-	7.5000	7471B	PPB	16 Aug 2024 10:35:26	S	Std
10.0 - 1	50	41742	-	10.0000	7471B	PPB	16 Aug 2024 10:37:45	S	Std
ICV78 - 1	ICV78	17190	4.0820	-	7471B	PPB	16 Aug 2024 10:40:43	U	SMPL
ICB78 - 1	ICB78	-236	-0.0724	-	7471B	PPB	16 Aug 2024 10:42:58	U	SMPL
CCV59 - 1	CCV59	21432	5.0933	-	7471B	PPB	16 Aug 2024 10:45:16	U	SMPL
CCB59 - 1	CCB59	-243	-0.0741	-	7471B	PPB	16 Aug 2024 10:47:31	U	SMPL
CRA - 1	CRA	779	0.1696	-	7471B	PPB	16 Aug 2024 10:49:51	U	SMPL
HighStd - 1	HighStd	41916	9.9768	-	7471B	PPB	16 Aug 2024 10:52:07	U	SMPL
ChkStd - 1	ChkStd	30800	7.3267	-	7471B	PPB	16 Aug 2024 10:54:22	U	SMPL
PB162776BL - 1	PB162776BL	-333	-0.0955	-	7471B	PPB	16 Aug 2024 10:56:45	U	SMPL
PB162776BS - 1	PB162776BS	16882	4.0086	-	7471B	PPB	16 Aug 2024 10:59:07	U	SMPL
P3579-02 - 1	VCPS-B1-081224-0-16	12844	3.0459	-	7471B	PPB	16 Aug 2024 11:01:23	U	SMPL
P3580-01 - 1	926-KI-SD-0-0.5-081224	12660	3.0021	-	7471B	PPB	16 Aug 2024 11:03:42	U	SMPL
P3580-02 - 1	926-KI-SD-0.5-1-081224	758	0.1646	-	7471B	PPB	16 Aug 2024 11:06:02	U	SMPL
P3580-03 - 1	925-KI-SD-0-0.5-081224	1382	0.3133	-	7471B	PPB	16 Aug 2024 11:08:21	U	SMPL
P3580-04 - 1	925-KI-SD-0.5-1-081224	1030	0.2294	-	7471B	PPB	16 Aug 2024 11:10:37	U	SMPL
CCV60 - 1	CCV60	20996	4.9894	-	7471B	PPB	16 Aug 2024 11:12:52	U	SMPL
CCB60 - 1	CCB60	-175	-0.0579	-	7471B	PPB	16 Aug 2024 11:15:08	U	SMPL
P3580-05 - 1	923-KI-SD-0-0.5-081224	10593	2.5093	-	7471B	PPB	16 Aug 2024 11:17:26	U	SMPL
P3580-06 - 1	923-KI-SD-0.5-1-081224	956	0.2118	-	7471B	PPB	16 Aug 2024 11:19:41	U	SMPL
P3580-07 - 1	922-KI-SD-0-0.5-081224	63964	15.2332	-	7471B	PPB	16 Aug 2024 11:21:59	U	SMPL
P3580-08 - 1	922-KI-SD-0.5-1-081224	2962	0.6900	-	7471B	PPB	16 Aug 2024 11:24:15	U	SMPL
P3597-01 - 1	SP-1-COMP	1039	0.2315	-	7471B	PPB	16 Aug 2024 11:26:41	U	SMPL
P3598-01 - 1	JC-03-081324-A	2818	0.6557	-	7471B	PPB	16 Aug 2024 11:28:58	U	SMPL
P3598-03 - 1	JC-03-081324-B	959	0.2125	-	7471B	PPB	16 Aug 2024 11:31:15	U	SMPL
P3600-02 - 1	VCPS-B2-081324-0-12	4863	1.1432	-	7471B	PPB	16 Aug 2024 11:33:32	U	SMPL
P3600-04 - 1	VCPS-B3-081324-0-10	10942	2.5925	-	7471B	PPB	16 Aug 2024 11:35:50	U	SMPL
P3600-06 - 1	VCPS-B3-081324-10-18	3844	0.9003	-	7471B	PPB	16 Aug 2024 11:38:07	U	SMPL
CCV61 - 1	CCV61	21334	5.0700	-	7471B	PPB	16 Aug 2024 11:40:25	U	SMPL
CCB61 - 1	CCB61	-174	-0.0576	-	7471B	PPB	16 Aug 2024 11:42:42	U	SMPL
P3607-01 - 1	NB-08-08142024	925	0.2044	-	7471B	PPB	16 Aug 2024 11:45:00	U	SMPL
P3607-01DUP - 1	NB-08-08142024DUP	742	0.1607	-	7471B	PPB	16 Aug 2024 11:47:16	U	SMPL
P3607-01MS - 1	NB-08-08142024MS	18054	4.2880	-	7471B	PPB	16 Aug 2024 11:49:31	U	SMPL
P3607-01MSD - 1	NB-08-08142024MSD	17562	4.1707	-	7471B	PPB	16 Aug 2024 11:51:47	U	SMPL
PB162777BL - 1	PB162777BL	-144	-0.0505	-	7471B	PPB	16 Aug 2024 11:54:06	U	SMPL
PB162777BS - 1	PB162777BS	16597	3.9407	-	7471B	PPB	16 Aug 2024 11:56:25	U	SMPL
P3614-01 - 1	OK-01-081424	1388	0.3147	-	7471B	PPB	16 Aug 2024 11:58:41	U	SMPL
P3614-01DUP - 1	OK-01-081424DUP	1501	0.3417	-	7471B	PPB	16 Aug 2024 12:01:00	U	SMPL
P3614-01MS - 1	OK-01-081424MS	19035	4.5219	-	7471B	PPB	16 Aug 2024 12:03:17	U	SMPL
P3614-01MSD - 1	OK-01-081424MSD	17651	4.1919	-	7471B	PPB	16 Aug 2024 12:05:32	U	SMPL
CCV62 - 1	CCV62	21394	5.0843	-	7471B	PPB	16 Aug 2024 12:07:51	U	SMPL
CCB62 - 1	CCB62	-174	-0.0576	-	7471B	PPB	16 Aug 2024 12:10:09	U	SMPL
P3615-01 - 1	HR-01-081424	5669	1.3354	-	7471B	PPB	16 Aug 2024 12:12:28	U	SMPL
P3615-03 - 1	HR-02-081424	1184	0.2661	-	7471B	PPB	16 Aug 2024 12:14:43	U	SMPL
P3615-05 - 1	HR-03-081424	3440	0.8040	-	7471B	PPB	16 Aug 2024 12:17:01	U	SMPL
P3615-07 - 1	HR-04-081424	920	0.2032	-	7471B	PPB	16 Aug 2024 12:19:17	U	SMPL
P3617-07 - 1	VCPS-B4-081424-0-10	10812	2.5615	-	7471B	PPB	16 Aug 2024 12:21:34	U	SMPL
P3617-08 - 1	VCPS-B4-081424-10-16	18869	4.4823	-	7471B	PPB	16 Aug 2024 12:23:50	U	SMPL
P3617-12 - 1	VCPS-B5-081424-0-10	22854	5.4324	-	7471B	PPB	16 Aug 2024 12:26:08	U	SMPL
P3617-13 - 1	VCPS-B5-081424-10-14	112910	26.9022	-	7471B	PPB	16 Aug 2024 12:28:28	U	SMPL
P3634-01 - 1	TR-06-08152024	1007	0.2239	-	7471B	PPB	16 Aug 2024 12:30:49	U	SMPL
P3640-01 - 1	SP-1-COMP	2229	0.5152	-	7471B	PPB	16 Aug 2024 12:33:22	U	SMPL
CCV63 - 1	CCV63	21457	5.0993	-	7471B	PPB	16 Aug 2024 12:35:37	U	SMPL
CCB63 - 1	CCB63	-181	-0.0593	-	7471B	PPB	16 Aug 2024 12:37:53	U	SMPL
P3607-01LX5 - 1		109	0.0098	-	7471B	PPB	16 Aug 2024 12:40:11	U	SMPL
P3607-01A - 1		18073	4.2925	-	7471B	PPB	16 Aug 2024 12:42:27	U	SMPL
P3614-01LX5 - 1		25	-0.0102	-	7471B	PPB	16 Aug 2024 12:44:43	U	SMPL
P3614-01A - 1		18677	4.4365	-	7471B	PPB	16 Aug 2024 12:47:00	U	SMPL
P3580-07DLX5 - 1		13549	3.2140	-	7471B	PPB	16 Aug 2024 12:50:46	U	SMPL
P3617-13DLX5 - 1		21657	5.1470	-	7471B	PPB	16 Aug 2024 12:53:01	U	SMPL
CCV64 - 1	CCV64	21222	5.0433	-	7471B	PPB	16 Aug 2024 12:55:19	U	SMPL
CCB64 - 1	CCB64	-160	-0.0543	-	7471B	PPB	16 Aug 2024 12:57:39	U	SMPL