


LB132052

SFAM01.1

INSTRUMENT ID: CV1

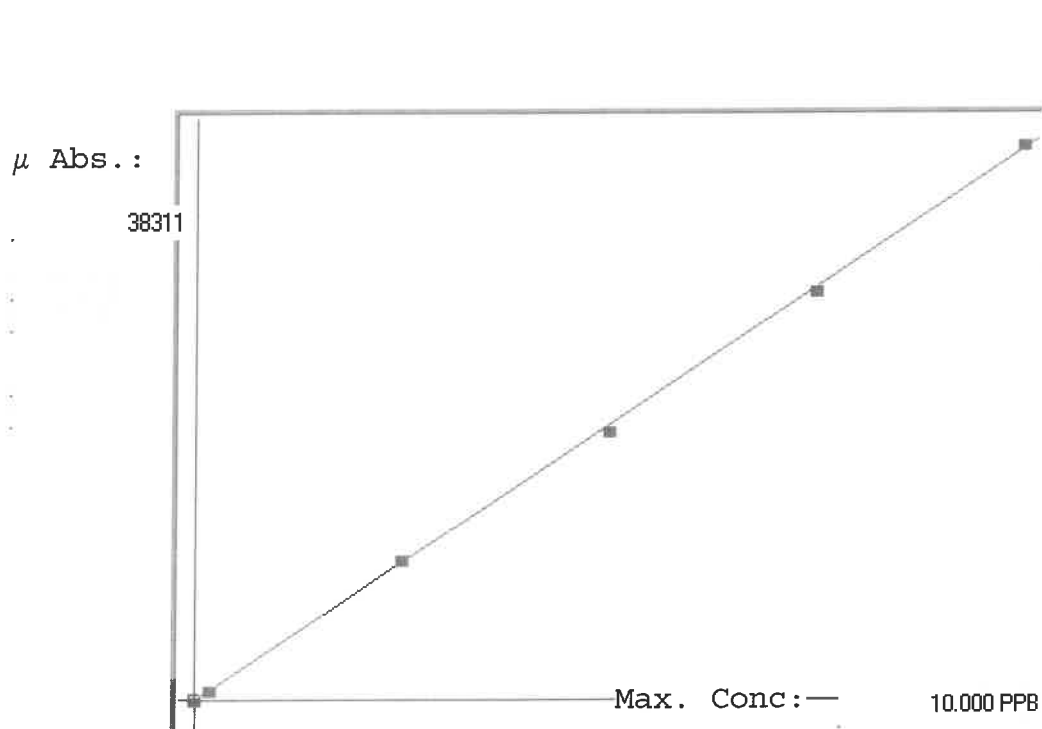

Linear

A= 0.0000e+000

B= 2.6273e-004 slope

C= 1.3637e-002 $\pm 101\% \text{ error}$

Rho= 0.9998496

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	g/d
0.00	0.000	0.023	0.023	34	0.000	34					=
0.05	0.050					442	0				0
0.20	0.200	0.200	0.000	711	0.0 %	711					2
2.50	2.500	2.561	0.061	9695	0.0 %	9695					2
5.00	5.000	4.898	-0.102	18592	0.0 %	18592					-2
7.50	7.500	7.439	-0.061	28261	0.0 %	28261					1
10.0	10.000	10.079	0.079	38311	0.0 %	38311					1

LB132052

INSTRUMENT ID : V1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	34	-		0 SFAM01.1	PPB	8/16/2024 14:26	Std
	0.2 S01	711	-		0.2 SFAM01.1	PPB	8/16/2024 14:28	Std
	2.5 S02	9695	-		2.5 SFAM01.1	PPB	8/16/2024 14:31	Std
	5 S03	18592	-		5 SFAM01.1	PPB	8/16/2024 14:33	Std
	7.5 S04	28261	-		7.5 SFAM01.1	PPB	8/16/2024 14:35	Std
	10 S05	38311	-		10 SFAM01.1	PPB	8/16/2024 14:37	Std
ICV079	ICV079	15333	4.0421 -		SFAM01.1	PPB	8/16/2024 14:40	SMPL
ICB079	ICB079	-150	-0.0258 -		SFAM01.1	PPB	8/16/2024 14:42	SMPL
CCV065	CCV065	18497	4.8734 -		SFAM01.1	PPB	8/16/2024 14:45	SMPL
CCB065	CCB065	-154	-0.0268 -		SFAM01.1	PPB	8/16/2024 14:47	SMPL
PB162804BL	PBW804	12	0.0168 -		SFAM01.1	PPB	8/16/2024 14:49	SMPL
P3605-01	E0CL4	12	0.0168 -		SFAM01.1	PPB	8/16/2024 14:51	SMPL
P3605-02	E0CL4D	57	0.0286 -		SFAM01.1	PPB	8/16/2024 14:54	SMPL
P3605-03	E0CL4S	4001	1.0648 -		SFAM01.1	PPB	8/16/2024 15:02	SMPL
CCV066	CCV066	18534	4.8831 -		SFAM01.1	PPB	8/16/2024 15:04	SMPL
CCB066	CCB066	-161	-0.0287 -		SFAM01.1	PPB	8/16/2024 15:07	SMPL