


LB132070

7470A

INSTRUMENT ID: CV1

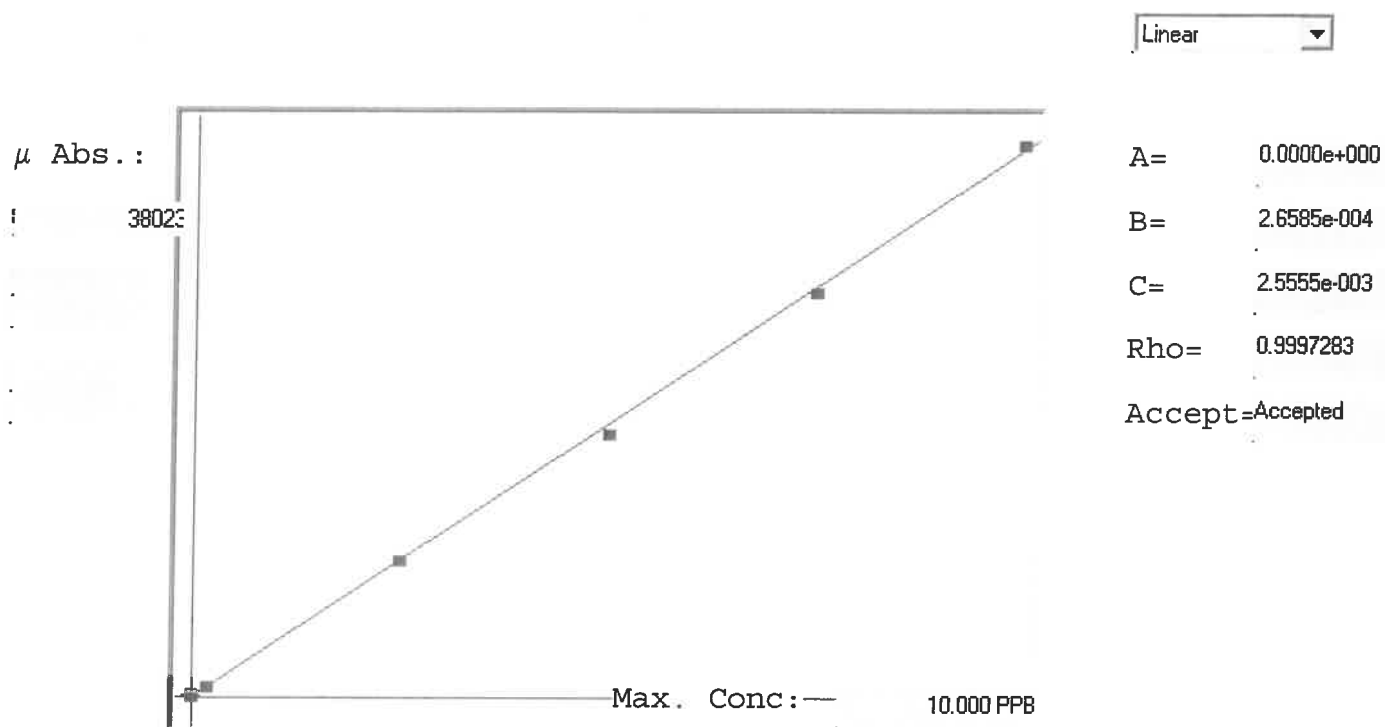

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	b/h
0.0	0.000	0.052	0.052	186	0.000	186	0				12
0.2	0.200	0.224	0.024	833	0.0 %	833					1
2.5	2.500	2.529	0.029	9504	0.0 %	9504					3
5.0	5.000	4.844	-0.156	18212	0.0 %	18212					1
7.5	7.500	7.439	-0.061	27974	0.0 %	27974					1
10.0	10.000	10.111	0.111	38023	0.0 %	38023					1

LB132070 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 19 Aug 2024 10:31:44

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	186	-	0.0000	7470A	PPB	19 Aug 2024 10:35:36	S	Std
0.2 - 1	50.2	833	-	0.2000	7470A	PPB	19 Aug 2024 10:37:53	S	Std
2.5 - 1	52.5	9504	-	2.5000	7470A	PPB	19 Aug 2024 10:40:10	S	Std
5.0 - 1	55	18212	-	5.0000	7470A	PPB	19 Aug 2024 10:42:27	S	Std
7.5 - 1	57.15	27974	-	7.5000	7470A	PPB	19 Aug 2024 10:44:43	S	Std
10.0 - 1	510	38023	-	10.0000	7470A	PPB	19 Aug 2024 10:52:11	S	Std
ICV83 - 1	ICV83	14545	3.8694	-	7470A	PPB	19 Aug 2024 10:55:00	U	SMPL
ICB83 - 1	ICB83	-38	-0.0075	-	7470A	PPB	19 Aug 2024 10:57:15	U	SMPL
CCV77 - 1	CCV77	17666	4.6991	-	7470A	PPB	19 Aug 2024 11:02:03	U	SMPL
CCB77 - 1	CCB77	-37	-0.0073	-	7470A	PPB	19 Aug 2024 11:04:18	U	SMPL
CRA - 1	CRA	743	0.2001	-	7470A	PPB	19 Aug 2024 11:06:35	U	SMPL
HighStd - 1	HighStd	37380	9.9401	-	7470A	PPB	19 Aug 2024 11:08:51	U	SMPL
ChkStd - 1	ChkStd	25906	6.8897	-	7470A	PPB	19 Aug 2024 11:11:06	U	SMPL
PB162820BL - 1	PBW	-181	-0.0456	-	7470A	PPB	19 Aug 2024 11:13:24	U	SMPL
PB162820BS - 1	LCSW	15147	4.0294	-	7470A	PPB	19 Aug 2024 11:15:42	U	SMPL
P3596-01 - 1	918-J-WS-081324	32	0.0111	-	7470A	PPB	19 Aug 2024 11:18:00	U	SMPL
P3596-02 - 1	918-J-WS-081324-FD	136	0.0387	-	7470A	PPB	19 Aug 2024 11:20:18	U	SMPL
P3610-01 - 1	A6934	68	0.0206	-	7470A	PPB	19 Aug 2024 11:22:35	U	SMPL
P3610-02 - 1	M21005	94	0.0275	-	7470A	PPB	19 Aug 2024 11:24:52	U	SMPL
P3617-02 - 1	Field Blank	93	0.0273	-	7470A	PPB	19 Aug 2024 11:27:07	U	SMPL
CCV78 - 1	CCV78	18665	4.9647	-	7470A	PPB	19 Aug 2024 11:33:52	U	SMPL
CCB78 - 1	CCB78	-89	-0.0211	-	7470A	PPB	19 Aug 2024 11:36:07	U	SMPL
P3617-03 - 1	VCPS-B2-081424-6W	4788	1.2755	-	7470A	PPB	19 Aug 2024 11:49:38	U	SMPL
P3617-03DUP - 1	VCPS-B2-081424-6WDUP	4226	1.1260	-	7470A	PPB	19 Aug 2024 11:51:53	U	SMPL
P3617-03MS - 1	VCPS-B2-081424-6WMS	17569	4.6733	-	7470A	PPB	19 Aug 2024 11:54:09	U	SMPL
P3617-03MSD - 1	VCPS-B2-081424-6WMSD	19386	5.1564	-	7470A	PPB	19 Aug 2024 12:01:40	U	SMPL
P3617-14 - 1	VCPS-B2-081424-6W	-25	-0.0041	-	7470A	PPB	19 Aug 2024 12:06:13	U	SMPL
P3617-15 - 1	VCPS-B2-081424-6W-DUP	227	0.0629	-	7470A	PPB	19 Aug 2024 12:08:32	U	SMPL
P3628-01 - 1	371	227	0.0629	-	7470A	PPB	19 Aug 2024 12:10:51	U	SMPL
P3645-01 - 1	914-J-WS-081524	289	0.0794	-	7470A	PPB	19 Aug 2024 12:13:08	U	SMPL
P3645-02 - 1	916-J-WS-081524	93	0.0273	-	7470A	PPB	19 Aug 2024 12:15:24	U	SMPL
CCV79 - 1	CCV79	18276	4.8613	-	7470A	PPB	19 Aug 2024 12:17:39	U	SMPL
CCB79 - 1	CCB79	-67	-0.0153	-	7470A	PPB	19 Aug 2024 12:19:54	U	SMPL
P3650-01 - 1	RW7-SP100-20240814	91	0.0267	-	7470A	PPB	19 Aug 2024 12:22:11	U	SMPL
P3650-04 - 1	RW7-SP303-20240814	86	0.0254	-	7470A	PPB	19 Aug 2024 12:24:26	U	SMPL
P3617-04 - 1	VCPS-B2-081424-6W-DUP	5012	1.3350	-	7470A	PPB	19 Aug 2024 12:27:08	U	SMPL
P3617-03LX5 - 1	733	733	0.1974	-	7470A	PPB	19 Aug 2024 12:29:44	U	SMPL
P3617-03A - 1	18290	18290	4.8650	-	7470A	PPB	19 Aug 2024 12:32:00	U	SMPL
CCV80 - 1	CCV80	18243	4.8525	-	7470A	PPB	19 Aug 2024 12:34:15	U	SMPL
CCB80 - 1	CCB80	-48	-0.0102	-	7470A	PPB	19 Aug 2024 12:36:33	U	SMPL