


LB132119

245.1

INSTRUMENT 1A: CVI

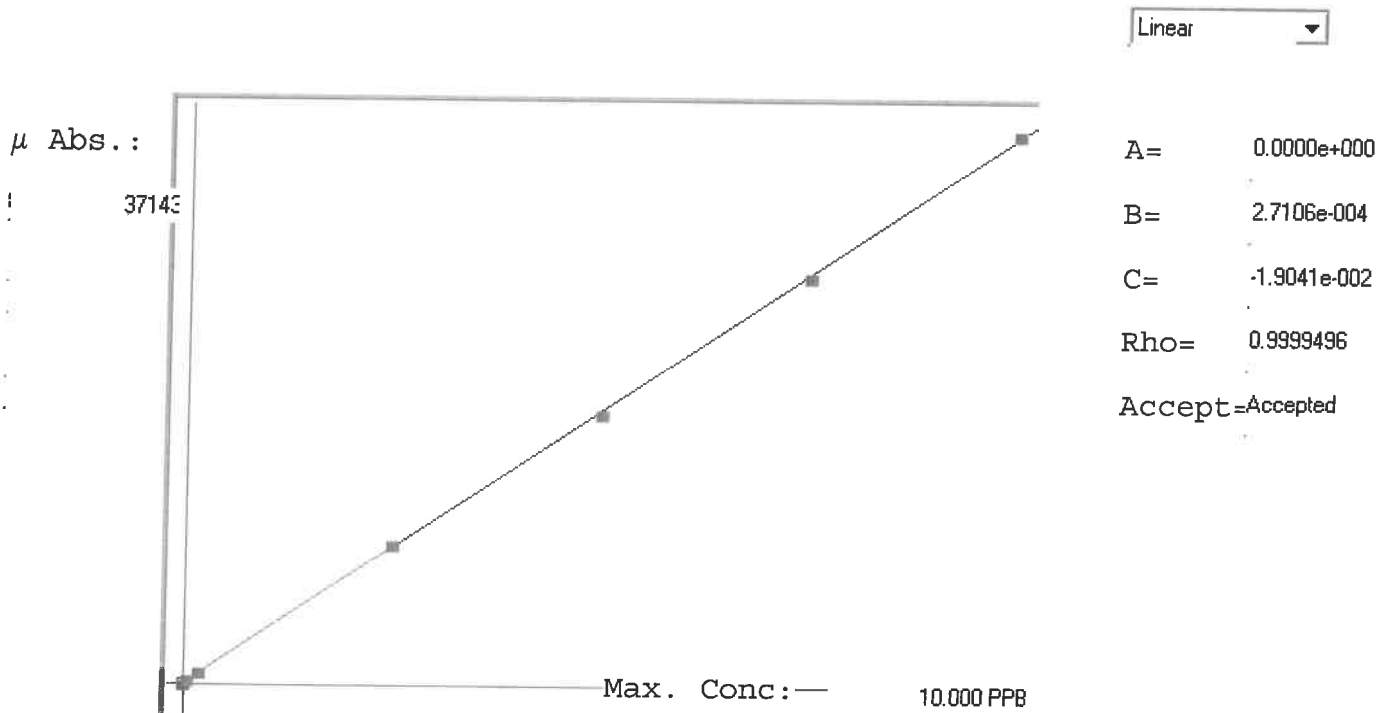

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.002	0.002	76	0.000	76					9.00
0.05	0.050	0.062	0.012	298	0.0 %	298	0				24
0.2	0.200	0.204	0.004	822	0.0 %	822					2
2.5	2.500	2.536	0.036	9426	0.0 %	9426					1
5.0	5.000	4.930	-0.070	18259	0.0 %	18259					1
7.5	7.500	7.468	-0.032	27622	0.0 %	27622					0
10.0	10.000	10.049	0.049	37143	0.0 %	37143					0

LB132119 INSTRME 1

Method: 245.1

Operator: Admin

Date of Analysis: 22 Aug 2024 10:33:20

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	76	-	0.0000	245.1	PPB	22 Aug 2024 10:44:52	S	Std
0.05 - 1	50.15	298	-	0.0500	245.1	PPB	22 Aug 2024 10:47:09	S	Std
0.2 - 1	50.2	822	-	0.2000	245.1	PPB	22 Aug 2024 10:49:26	S	Std
2.5 - 1	52.5	9426	-	2.5000	245.1	PPB	22 Aug 2024 10:51:42	S	Std
5.0 - 1	55	18259	-	5.0000	245.1	PPB	22 Aug 2024 10:53:59	S	Std
7.5 - 1	57.5	27622	-	7.5000	245.1	PPB	22 Aug 2024 10:56:15	S	Std
10.0 - 1	510	37143	-	10.0000	245.1	PPB	22 Aug 2024 11:14:08	S	Std
ICV89 - 1	ICV89	14315	3.8611	-245.1		PPB	22 Aug 2024 11:16:59	U	SMPL
ICB89 - 1	ICB89	-201	-0.0735	-245.1		PPB	22 Aug 2024 11:19:14	U	SMPL
CCV01 - 1	CCV01	18868	5.0952	-245.1		PPB	22 Aug 2024 11:21:31	U	SMPL
CCB01 - 1	CCB01	-201	-0.0735	-245.1		PPB	22 Aug 2024 11:23:46	U	SMPL
CRA - 1	CRA	231	0.0436	-245.1		PPB	22 Aug 2024 11:28:46	U	SMPL
HighStd - 1	HighStd	37017	10.0146	-245.1		PPB	22 Aug 2024 11:31:01	U	SMPL
ChkStd - 1	ChkStd	27146	7.3390	-245.1		PPB	22 Aug 2024 11:33:16	U	SMPL
PB162908BL - 1	PBW	17	-0.0144	-245.1		PPB	22 Aug 2024 11:38:56	U	SMPL
PB162908BS - 1	LCSW	13849	3.7348	-245.1		PPB	22 Aug 2024 11:41:12	U	SMPL
P3536-01 - 1	MANHOLE	-152	-0.0602	-245.1		PPB	22 Aug 2024 11:43:28	U	SMPL
P3536-01DUP - 1	MANHOLEDUP	-15	-0.0231	-245.1		PPB	22 Aug 2024 11:45:46	U	SMPL
P3536-01MS - 1	MANHOLEMS	13784	3.7172	-245.1		PPB	22 Aug 2024 11:48:03	U	SMPL
P3536-01MSD - 1	MANHOLEMSD	12120	3.2662	-245.1		PPB	22 Aug 2024 11:50:20	U	SMPL
P3657-01 - 1	917-J-WS-081624	-18	-0.0239	-245.1		PPB	22 Aug 2024 11:52:36	U	SMPL
CCV02 - 1	CCV02	18997	5.1302	-245.1		PPB	22 Aug 2024 11:54:52	U	SMPL
CCB02 - 1	CCB02	-209	-0.0757	-245.1		PPB	22 Aug 2024 11:57:07	U	SMPL
P3536-01LX5 - 1		-72	-0.0386	-245.1		PPB	22 Aug 2024 11:59:24	U	SMPL
P3536-01A - 1		14467	3.9023	-245.1		PPB	22 Aug 2024 12:01:39	U	SMPL
CCV03 - 1	CCV03	18955	5.1188	-245.1		PPB	22 Aug 2024 12:03:55	U	SMPL
CCB03 - 1	CCB03	-203	-0.0741	-245.1		PPB	22 Aug 2024 12:06:12	U	SMPL