

(b132223)

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

8/30/2024 13:17

Reviewed by : RM

Instrument ID : Konelab

Test: CNEPA-NEW

Sample Id	Result	Dil. 1 +	Response	Errors
ICV001 ICV001	95.964	0.0	0.090	
ICB001 ICB001	0.866	0.0	0.001	
CCV001 CCV001	241.522	0.0	0.225	
CCB001 CCB001	0.307	0.0	0.001	
08/30/24 RM PB163005BL PBS005	0.396	0.0	0.001	
P3677-01 MX120	1901.109	0.0	1.769	Test limit high
08/30/24 RM PB3677-01DLX5 MX120	379.400	0.0	0.354	
PB163006BL PBW006	0.372	0.0	0.001	
P3677-03 MX123	142.942	0.0	0.134	
CCV002 CCV002	249.576	0.0	0.233	
CCB002 CCB002	0.398	0.0	0.001	

N	11
Mean	273.896
SD	555.2672
CV%	202.73

Aquakem v. 7.2AQ1

Results from time period:

Fri Aug 30 12:32:33 2024

Fri Aug 30 13:16:42 2024

Sample Id	Sam/Ctr/c#	Test short r	Test type	Result	Result unit	Result date and time
S0.0	A	CNEPA-NE\ P		-0.0505	µg/l	8/30/2024 12:32:33
S5.0	A	CNEPA-NE\ P		5.1301	µg/l	8/30/2024 12:32:34
S10.0	A	CNEPA-NE\ P		9.489	µg/l	8/30/2024 12:32:35
S100.0	A	CNEPA-NE\ P		100.0545	µg/l	8/30/2024 12:32:36
S250.0	A	CNEPA-NE\ P		250.7578	µg/l	8/30/2024 12:32:37
S500.0	A	CNEPA-NE\ P		499.6191	µg/l	8/30/2024 12:32:38
ICV001 ICV001	S	CNEPA-NE\ P		95.9637	µg/l	8/30/2024 13:04:49
ICB001 ICB001	S	CNEPA-NE\ P		0.8659	µg/l	8/30/2024 13:04:50
CCV001 CCV001	S	CNEPA-NE\ P		241.5218	µg/l	8/30/2024 13:04:53
CCB001 CCB001	S	CNEPA-NE\ P		0.3067	µg/l	8/30/2024 13:04:55
PB163005BL PBS005	S	CNEPA-NE\ P		0.3961	µg/l	8/30/2024 13:04:56
P3677-01 MX120	S	CNEPA-NE\ P		1901.109	µg/l	8/30/2024 13:04:58
P3677-01DLX5 MX120	S	CNEPA-NE\ P		379.4002	µg/l	8/30/2024 13:12:23
PB163006BL PBW006	S	CNEPA-NE\ P		0.3715	µg/l	8/30/2024 13:12:26
P3677-03 MX123	S	CNEPA-NE\ P		142.9419	µg/l	8/30/2024 13:12:29
CCV002 CCV002	S	CNEPA-NE\ P		249.5763	µg/l	8/30/2024 13:16:39
CCB002 CCB002	S	CNEPA-NE\ P		0.3982	µg/l	8/30/2024 13:16:42

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

8/30/2024 12:32

Test CNEPA-NEW

Accepted

8/30/2024 12:32

~~Factor~~ Slope

1075 0.000930

~~Bias y~~ Intercept


0.001

09/03/2024
RM

Coeff. of det.

0.999995

Errors

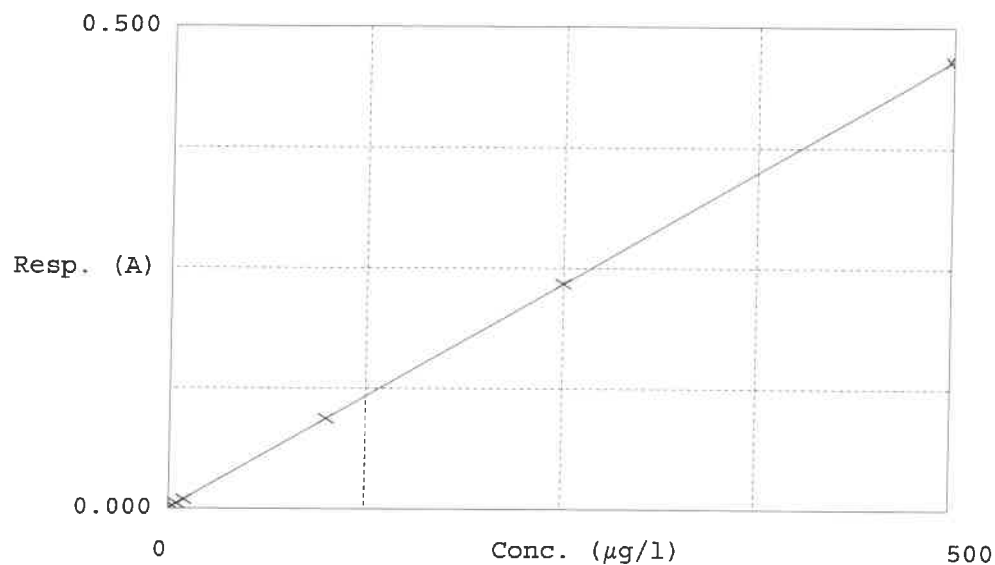

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN\$6.6	0.001	-0.0505	0.0000	-
2	5.0PPBCN\$5.6	0.005	5.1301	5.0000	2.6
3	10PPBCN\$10.6	0.010	9.4890	10.0000	-5.1
4	100PPBCN\$100.0	0.094	100.0545	100.0000	0.1
5	250PPBCN\$250.0	0.234	250.7578	250.0000	0.3
6	500PPBCN\$500.0	0.465	499.6191	500.0000	-0.1

08/30/2024
RM