


LB132237

7470A

INSTRUMENT ID: CV1

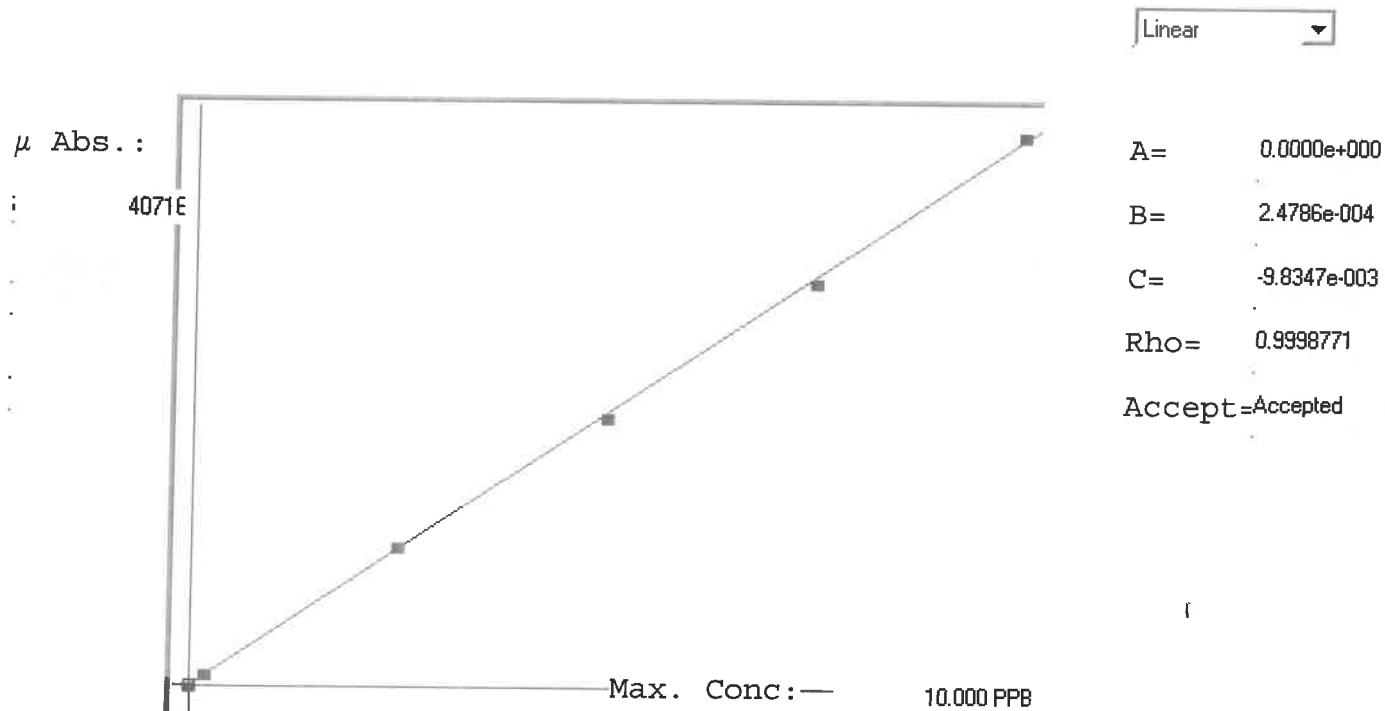

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o/v
0.0	0.000	0.017	0.017	109	0.000	109	0				0/0
0.2	0.200	0.204	0.004	864	0.0 %	864					1
2.5	2.500	2.544	0.044	10304	0.0 %	10304					2
5.0	5.000	4.938	-0.062	19961	0.0 %	19961					1
7.5	7.500	7.415	-0.085	29956	0.0 %	29956					1
10.0	10.000	10.082	0.082	40716	0.0 %	40716					1

LB132237 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 03 Sep 2024 10:35:24

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SO	109	-	0.0000	7470A	PPB	03 Sep 2024 10:59:57	S	Std
0.2 - 1	SO-2	864	-	0.2000	7470A	PPB	03 Sep 2024 11:02:15	S	Std
2.5 - 1	SO-5	10304	-	2.5000	7470A	PPB	03 Sep 2024 11:04:31	S	Std
5.0 - 1	SO-5	19961	-	5.0000	7470A	PPB	03 Sep 2024 11:06:48	S	Std
7.5 - 1	SO-5	29956	-	7.5000	7470A	PPB	03 Sep 2024 11:11:20	S	Std
10.0 - 1	SO-10	40716	-	10.0000	7470A	PPB	03 Sep 2024 11:13:35	S	Std
ICV04 - 1	ICV04	16132	3.9886	-	7470A	PPB	03 Sep 2024 11:16:33	U	SMPL
ICB04 - 1	ICB04	-83	-0.0304	-	7470A	PPB	03 Sep 2024 11:18:47	U	SMPL
CCV17 - 1	CCV17	20113	4.9753	-	7470A	PPB	03 Sep 2024 11:21:03	U	SMPL
CCB17 - 1	CCB17	-130	-0.0421	-	7470A	PPB	03 Sep 2024 11:23:18	U	SMPL
CRA - 1	CRA	788	0.1855	-	7470A	PPB	03 Sep 2024 11:25:35	U	SMPL
HighStd - 1	HighStd	41228	10.2088	-	7470A	PPB	03 Sep 2024 11:27:50	U	SMPL
ChkStd - 1	ChkStd	27145	6.7182	-	7470A	PPB	03 Sep 2024 11:30:05	U	SMPL
PB163101BL - 1	PBW	-250	-0.0718	-	7470A	PPB	03 Sep 2024 11:32:23	U	SMPL
PB163101BS - 1	LCSW	14501	3.5843	-	7470A	PPB	03 Sep 2024 11:34:42	U	SMPL
P3787-02 - 1	SB-1	2109	0.5129	-	7470A	PPB	03 Sep 2024 11:36:58	U	SMPL
P3787-02DUP - 1	SB-1DUP	2135	0.5193	-	7470A	PPB	03 Sep 2024 11:39:16	U	SMPL
P3787-02MS - 1	SB-1MS	18201	4.5014	-	7470A	PPB	03 Sep 2024 11:41:33	U	SMPL
P3787-02MSD - 1	SB-1MSD	17479	4.3224	-	7470A	PPB	03 Sep 2024 11:43:50	U	SMPL
P3787-04 - 1	SB-2	1196	0.2866	-	7470A	PPB	03 Sep 2024 11:46:08	U	SMPL
CCV18 - 1	CCV18	19585	4.8444	-	7470A	PPB	03 Sep 2024 11:48:24	U	SMPL
CCB18 - 1	CCB18	-235	-0.0681	-	7470A	PPB	03 Sep 2024 11:50:41	U	SMPL
P3787-06 - 1	SB-3	966	0.2296	-	7470A	PPB	03 Sep 2024 11:52:58	U	SMPL
PB163102BL - 1	PBW	-36	-0.0188	-	7470A	PPB	03 Sep 2024 11:55:13	U	SMPL
PB163102BS - 1	LCSW	14845	3.6696	-	7470A	PPB	03 Sep 2024 12:00:29	U	SMPL
P3772-01 - 1	BUR-1649	230	0.0472	-	7470A	PPB	03 Sep 2024 12:09:30	U	SMPL
P3772-01DUP - 1	BUR-1649DUP	146	0.0264	-	7470A	PPB	03 Sep 2024 12:11:46	U	SMPL
P3772-01MS - 1	BUR-1649MS	15447	3.8188	-	7470A	PPB	03 Sep 2024 12:14:02	U	SMPL
P3772-01MSD - 1	BUR-1649MSD	15669	3.8738	-	7470A	PPB	03 Sep 2024 12:16:18	U	SMPL
P3795-01 - 1	2885	285	0.0608	-	7470A	PPB	03 Sep 2024 12:18:37	U	SMPL
P3799-07 - 1	WELL-1	4959	1.2193	-	7470A	PPB	03 Sep 2024 12:20:55	U	SMPL
P3799-08 - 1	WELL-2	1061	0.2531	-	7470A	PPB	03 Sep 2024 12:23:16	U	SMPL
CCV19 - 1	CCV19	18488	4.5725	-	7470A	PPB	03 Sep 2024 12:25:33	U	SMPL
CCB19 - 1	CCB19	-248	-0.0713	-	7470A	PPB	03 Sep 2024 12:27:49	U	SMPL
P3799-09 - 1	WELL-4	22598	5.5912	-	7470A	PPB	03 Sep 2024 12:30:07	U	SMPL
P-B163071TB - 1		433	0.0975	-	7470A	PPB	03 Sep 2024 12:32:23	U	SMPL
P3787-02LX5 - 1		153	0.0281	-	7470A	PPB	03 Sep 2024 12:34:41	U	SMPL
P3787-02A - 1		17699	4.3770	-	7470A	PPB	03 Sep 2024 12:36:56	U	SMPL
P3772-01LX5 - 1		-153	-0.0478	-	7470A	PPB	03 Sep 2024 12:39:12	U	SMPL
P3772-01A - 1		16129	3.9878	-	7470A	PPB	03 Sep 2024 12:41:30	U	SMPL
CCV20 - 1	CCV20	21202	5.2452	-	7470A	PPB	03 Sep 2024 12:50:07	U	SMPL
CCB20 - 1	CCB20	-188	-0.0564	-	7470A	PPB	03 Sep 2024 12:52:24	U	SMPL