

C6132257

=====

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

9/3/2024 16:01

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.980	0.0	0.111	
ICB1	0.002	0.0	0.008	
CCV1	0.972	0.0	0.110	
CCB1	-0.001	0.0	0.008	
PB162893BL	0.002	0.0	0.008	
PB162893BS	0.968	0.0	0.110	
P3390-03	0.025	0.0	0.011	
PB162895BL	0.002	0.0	0.008	
PB162895BS	0.974	0.0	0.110	
P3390-09	0.024	0.0	0.011	
CCV2	0.970	0.0	0.110	
CCB2	0.001	0.0	0.008	

N	12
Mean	0.410
SD	0.4970
CV%	121.25

Aquakem v. 7.2AQ1

Results from time period:

Tue Sep 03 15:44:49 2024

Tue Sep 03 15:58:50 2024

Sample Id	Sam/Ctr/c/	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.0025	mg/l	9/3/2024 14:27:55	
0.05PPM	A	Phenolics-	P	0.0509	mg/l	9/3/2024 14:27:56	
0.1PPM	A	Phenolics-	P	0.1038	mg/l	9/3/2024 14:27:57	
0.25PPM	A	Phenolics-	P	0.2504	mg/l	9/3/2024 14:27:58	
0.50PPM	A	Phenolics-	P	0.5002	mg/l	9/3/2024 14:27:59	
1.0PPM	A	Phenolics-	P	0.9948	mg/l	9/3/2024 14:28:00	
2.0PPM	A	Phenolics-	P	2.0023	mg/l	9/3/2024 14:28:01	
ICV1	S	Phenolics-	P	0.9801	mg/l	9/3/2024 15:44:49	
ICB1	S	Phenolics-	P	0.0023	mg/l	9/3/2024 15:44:51	
CCV1	S	Phenolics-	P	0.972	mg/l	9/3/2024 15:44:53	
CCB1	S	Phenolics-	P	-0.0011	mg/l	9/3/2024 15:44:55	
PB162893BL	S	Phenolics-	P	0.0016	mg/l	9/3/2024 15:44:58	
PB162893BS	S	Phenolics-	P	0.9679	mg/l	9/3/2024 15:44:59	
P3390-03	S	Phenolics-	P	0.0247	mg/l	9/3/2024 15:54:51	
PB162895BL	S	Phenolics-	P	0.0019	mg/l	9/3/2024 15:54:54	
PB162895BS	S	Phenolics-	P	0.9741	mg/l	9/3/2024 15:54:56	
P3390-09	S	Phenolics-	P	0.024	mg/l	9/3/2024 15:55:00	
CCV2	S	Phenolics-	P	0.9703	mg/l	9/3/2024 15:55:02	
CCB2	S	Phenolics-	P	0.0012	mg/l	9/3/2024 15:58:49	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM Instrument ID : Konelab

9/3/2024 14:33


Test Phenolics-

Accepted 9/3/2024 14:33

Factor 9.511
Bias 0.008

Coeff. of det. 0.999983

Errors

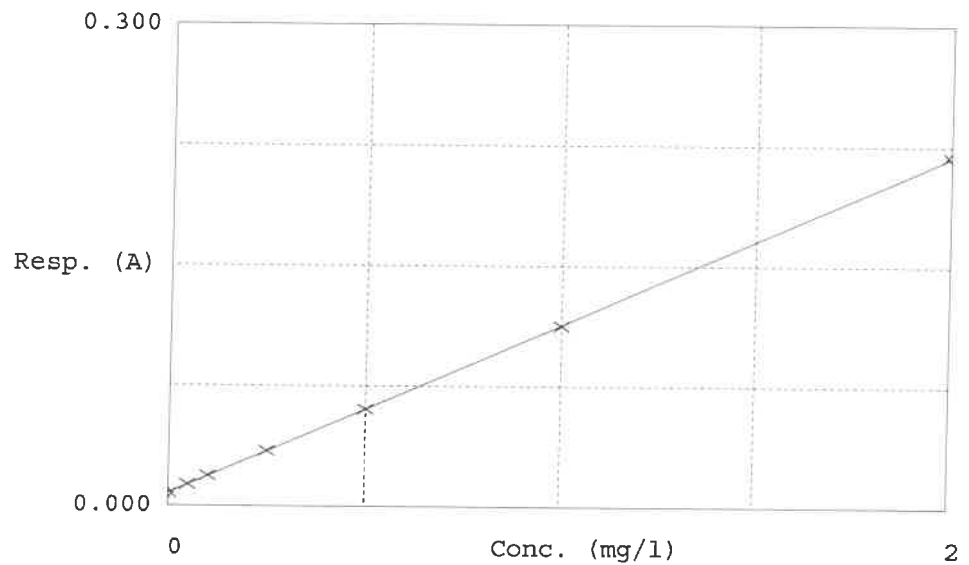

	Calibrator	Response	Calc. con.	Conc.	^{RM} Errors
1	0.00PPM	0.008	-0.0025	0.0000	-
2	Phenol-2	0.013	0.0509	0.0500	1.8
3	Phenol-2	0.019	0.1038	0.1000	3.8
4	Phenol-2	0.034	0.2504	0.2500	0.2
5	Phenol-2	0.061	0.5002	0.5000	0.0
6	Phenol-2	0.113	0.9948	1.0000	-0.5
7	Phenol-2	0.219	2.0023	2.0000	0.1

09/03/2024
RM