


LB132330

SFAM01.1

INSTRUMENT ID: CV1

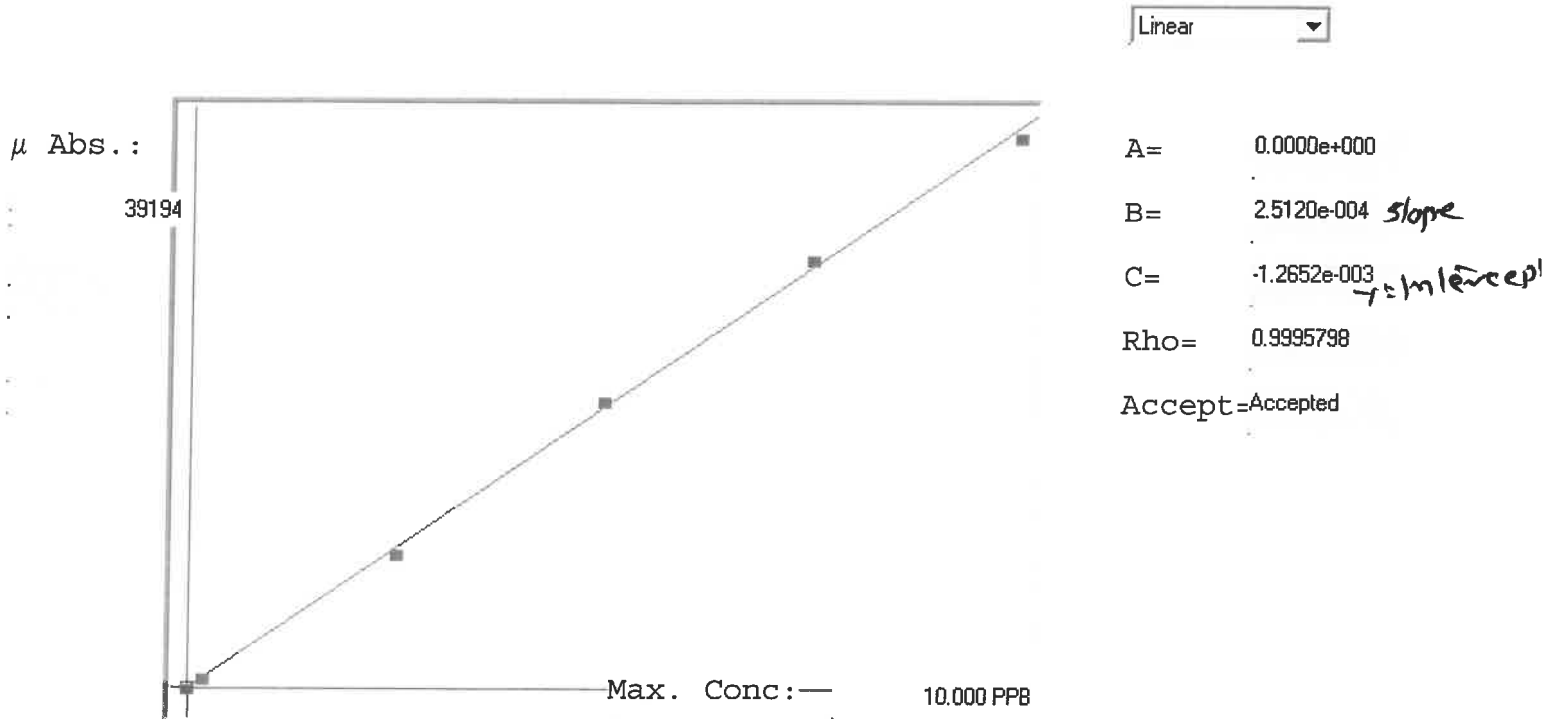

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% h
0.00	0.000	-0.007	-0.007	-23	0.000	-23					7
0.05	0.050					442	0				-8
0.20	0.200	0.184	-0.016	737	0.0 %	737					-4
2.50	2.500	2.412	-0.088	9606	0.0 %	9606					2
5.00	5.000	5.116	0.116	20373	0.0 %	20373					2
7.50	7.500	7.651	0.151	30462	0.0 %	30462					2
10.0	10.000	9.844	-0.156	39194	0.0 %	39194					-2

LB132330

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	-23	-		0 SFAM01.1	PPB	9/9/2024 13:55	Std
	0.2 S01	737	-		0.2 SFAM01.1	PPB	9/9/2024 13:57	Std
	2.5 S02	9606	-		2.5 SFAM01.1	PPB	9/9/2024 14:00	Std
	5 S03	20373	-		5 SFAM01.1	PPB	9/9/2024 14:02	Std
	7.5 S04	30462	-		7.5 SFAM01.1	PPB	9/9/2024 14:04	Std
	10 S05	39194	-		10 SFAM01.1	PPB	9/9/2024 14:07	Std
ICV014	ICV014	16074	4.0365 -		SFAM01.1	PPB	9/9/2024 14:09	SMPL
ICB014	ICB014	-277	-0.0708 -		SFAM01.1	PPB	9/9/2024 14:12	SMPL
CCV048	CCV048	20290	5.0956 -		SFAM01.1	PPB	9/9/2024 14:14	SMPL
CCB048	CCB048	-285	-0.0729 -		SFAM01.1	PPB	9/9/2024 14:16	SMPL
PB163235BL	PBS235	271	0.0668 -		SFAM01.1	PPB	9/9/2024 14:18	SMPL
P3908-01	E1KJ6	3740	0.9382 -		SFAM01.1	PPB	9/9/2024 14:21	SMPL
P3908-02	E1KJ8	133	0.0321 -		SFAM01.1	PPB	9/9/2024 14:23	SMPL
P3908-03	E1KK1	325	0.0804 -		SFAM01.1	PPB	9/9/2024 14:25	SMPL
P3908-04	E1KK2	868	0.2168 -		SFAM01.1	PPB	9/9/2024 14:32	SMPL
P3908-05	E1KK2D	770	0.1922 -		SFAM01.1	PPB	9/9/2024 14:35	SMPL
P3908-06	E1KK2S	12072	3.0312 -		SFAM01.1	PPB	9/9/2024 14:37	SMPL
P3908-07	E1KK7	970	0.2424 -		SFAM01.1	PPB	9/9/2024 14:39	SMPL
P3908-08	E1KK9	731	0.1824 -		SFAM01.1	PPB	9/9/2024 14:41	SMPL
CCV049	CCV049	19197	4.821 -		SFAM01.1	PPB	9/9/2024 14:44	SMPL
CCB049	CCB049	-211	-0.0543 -		SFAM01.1	PPB	9/9/2024 14:46	SMPL