


LB132344

7470A

INSTRUMENT ID: CV1

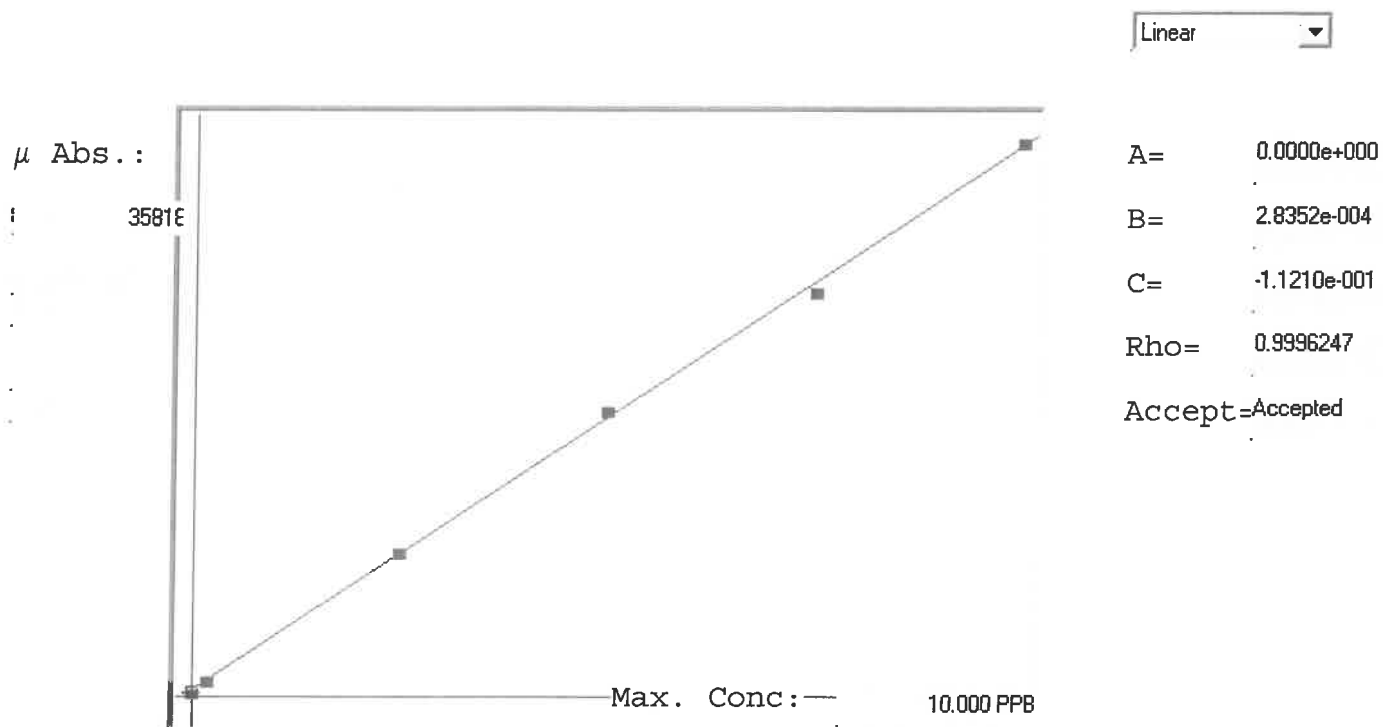

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/0D
0.0	0.000	-0.035	-0.035	273	0.000	273	0				
0.2	0.200	0.176	-0.024	1016	0.0 %	1016					-12
2.5	2.500	2.545	0.045	9373	0.0 %	9373					2
5.0	5.000	5.151	0.151	18564	0.0 %	18564					3
7.5	7.500	7.319	-0.181	26210	0.0 %	26210					-2
10.0	10.000	10.043	0.043	35818	0.0 %	35818					0

LB132344 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 10 Sep 2024 11:27:15

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	273	-	0.0000	7470A	PPB	10 Sep 2024 11:37:03	S	Std
0.2 - 1	50.2	1016	-	0.2000	7470A	PPB	10 Sep 2024 11:45:21	S	Std
2.5 - 1	52.5	9373	-	2.5000	7470A	PPB	10 Sep 2024 11:47:38	S	Std
5.0 - 1	55	18564	-	5.0000	7470A	PPB	10 Sep 2024 11:49:54	S	Std
7.5 - 1	57.5	26210	-	7.5000	7470A	PPB	10 Sep 2024 11:52:11	S	Std
10.0 - 1	510	35818	-	10.0000	7470A	PPB	10 Sep 2024 11:54:28	S	Std
ICV14 - 1	ICV14	14017	3.8620	-	7470A	PPB	10 Sep 2024 11:57:51	U	SMPL
ICB14 - 1	ICB14	140	-0.0724	-	7470A	PPB	10 Sep 2024 12:00:06	U	SMPL
CCV48 - 1	CCV48	17824	4.9414	-	7470A	PPB	10 Sep 2024 12:02:22	U	SMPL
CCB48 - 1	CCB48	220	-0.0497	-	7470A	PPB	10 Sep 2024 12:04:38	U	SMPL
CRA - 1	CRA	1062	0.1890	-	7470A	PPB	10 Sep 2024 12:06:58	U	SMPL
HighStd - 1	HighStd	35892	10.0641	-	7470A	PPB	10 Sep 2024 12:09:13	U	SMPL
ChkStd - 1	ChkStd	25159	7.0211	-	7470A	PPB	10 Sep 2024 12:11:28	U	SMPL
PB163223BL - 1	PBW	296	-0.0282	-	7470A	PPB	10 Sep 2024 12:15:50	U	SMPL
PB163223BS - 1	LCSW	15158	4.1855	-	7470A	PPB	10 Sep 2024 12:18:06	U	SMPL
P3852-01 - 1	D3656	585	0.0538	-	7470A	PPB	10 Sep 2024 12:20:22	U	SMPL
P3857-02 - 1	WC-C1-COMP	143	-0.0716	-	7470A	PPB	10 Sep 2024 12:22:41	U	SMPL
P3857-05 - 1	WC-C2-COMP	197	-0.0562	-	7470A	PPB	10 Sep 2024 12:24:57	U	SMPL
P3857-08 - 1	WC-D1-COMP	218	-0.0503	-	7470A	PPB	10 Sep 2024 12:27:14	U	SMPL
P3857-11 - 1	WC-D2-COMP	190	-0.0582	-	7470A	PPB	10 Sep 2024 12:29:30	U	SMPL
CCV49 - 1	CCV49	17563	4.8674	-	7470A	PPB	10 Sep 2024 12:31:45	U	SMPL
CCB49 - 1	CCB49	178	-0.0616	-	7470A	PPB	10 Sep 2024 12:34:00	U	SMPL
P3857-11DUP - 1	WC-D2-COMPDUP	180	-0.0611	-	7470A	PPB	10 Sep 2024 12:36:17	U	SMPL
P3857-11MS - 1	WC-D2-COMPMS	14281	3.9369	-	7470A	PPB	10 Sep 2024 12:38:32	U	SMPL
P3857-11MSD - 1	WC-D2-COMPMSD	15430	4.2627	-	7470A	PPB	10 Sep 2024 12:40:47	U	SMPL
PB163224BL - 1	PBW	435	0.0112	-	7470A	PPB	10 Sep 2024 12:46:00	U	SMPL
PB163224BS - 1	LCSW	15478	4.2763	-	7470A	PPB	10 Sep 2024 12:48:16	U	SMPL
P3852-06 - 1	D3659	696	0.0852	-	7470A	PPB	10 Sep 2024 12:56:03	U	SMPL
P3852-06DUP - 1	D3659DUP	644	0.0705	-	7470A	PPB	10 Sep 2024 12:58:20	U	SMPL
P3852-06MS - 1	D3659MS	11256	3.0792	-	7470A	PPB	10 Sep 2024 13:02:29	U	SMPL
P3852-06MSD - 1	D3659MSD	10985	3.0024	-	7470A	PPB	10 Sep 2024 13:04:46	U	SMPL
CCV50 - 1	CCV50	15449	4.2680	-	7470A	PPB	10 Sep 2024 13:07:03	U	SMPL
CCB50 - 1	CCB50	183	-0.0602	-	7470A	PPB	10 Sep 2024 13:09:20	U	SMPL
PB163170TB - 1	PB163170TB	44	-0.0996	-	7470A	PPB	10 Sep 2024 13:11:38	U	SMPL
PB163171TB - 1	PB163171TB	76	-0.0906	-	7470A	PPB	10 Sep 2024 13:13:54	U	SMPL
P3857-11LX5 - 1		146	-0.0707	-	7470A	PPB	10 Sep 2024 13:16:09	U	SMPL
P3857-11A - 1		14495	3.9976	-	7470A	PPB	10 Sep 2024 13:18:24	U	SMPL
P3852-06LX5 - 1		132	-0.0747	-	7470A	PPB	10 Sep 2024 13:20:40	U	SMPL
P3852-06A - 1		14077	3.8791	-	7470A	PPB	10 Sep 2024 13:22:57	U	SMPL
CCV51 - 1	CCV51	18955	5.2621	-	7470A	PPB	10 Sep 2024 13:25:13	U	SMPL
CCB51 - 1	CCB51	189	-0.0585	-	7470A	PPB	10 Sep 2024 13:32:57	U	SMPL