


LB132372

7471B

INSTRUMENT ID: CYL

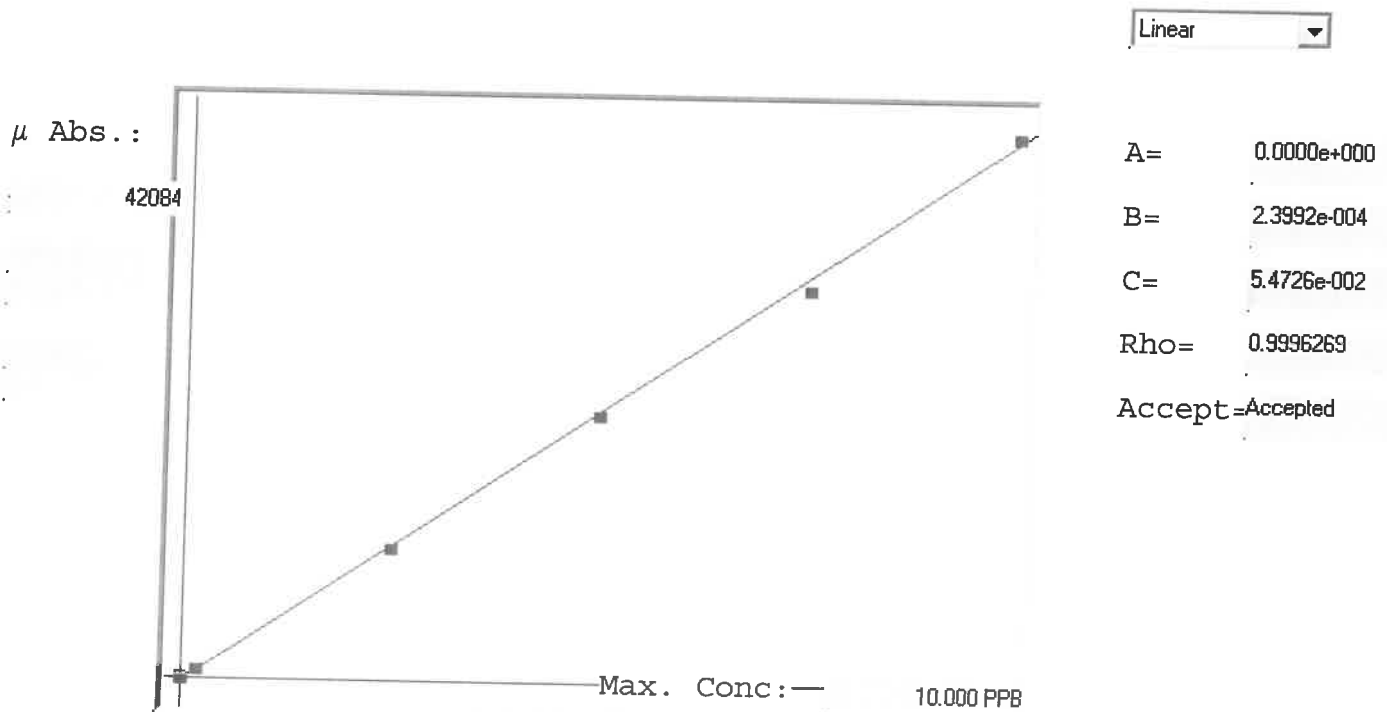

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	U/L
0.0	0.000	0.053	0.053	-9	0.000	-9					
0.2	0.200	0.231	0.031	735	0.0 %	735					16
2.5	2.500	2.482	-0.018	10118	0.0 %	10118					1
5.0	5.000	4.963	-0.037	20458	0.0 %	20458					1
7.5	7.500	7.320	-0.180	30280	0.0 %	30280					2
10.0	10.000	10.152	0.152	42084	0.0 %	42084					2

LB132372 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 11 Sep 2024 11:54:49

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-9	-	0.0000	7471B	PPB	11 Sep 2024 11:57:55	S	Std
0.2 - 1	50.2	735	-	0.2000	7471B	PPB	11 Sep 2024 12:00:12	S	Std
2.5 - 1	51.5	10118	-	2.5000	7471B	PPB	11 Sep 2024 12:02:28	S	Std
5.0 - 1	55	20458	-	5.0000	7471B	PPB	11 Sep 2024 12:04:45	S	Std
7.5 - 1	57.5	30280	-	7.5000	7471B	PPB	11 Sep 2024 12:07:03	S	Std
10.0 - 1	60	42084	-	10.0000	7471B	PPB	11 Sep 2024 12:09:21	S	Std
ICV18 - 1	ICV18	15652	3.8100	-7471B	PPB	11 Sep 2024 12:12:15	U	SMPL	
ICB18 - 1	ICB18	-288	-0.0144	-7471B	PPB	11 Sep 2024 12:14:31	U	SMPL	
CCV61 - 1	CCV61	20208	4.9030	-7471B	PPB	11 Sep 2024 12:16:48	U	SMPL	
CCB61 - 1	CCB61	-275	-0.0113	-7471B	PPB	11 Sep 2024 12:19:03	U	SMPL	
CRA - 1	CRA	744	0.2332	-7471B	PPB	11 Sep 2024 12:21:21	U	SMPL	
HighStd - 1	HighStd	41669	10.0520	-7471B	PPB	11 Sep 2024 12:23:35	U	SMPL	
ChkStd - 1	ChkStd	28867	6.9805	-7471B	PPB	11 Sep 2024 12:25:51	U	SMPL	
PB163303BL - 1	PBS	-359	-0.0314	-7471B	PPB	11 Sep 2024 12:28:12	U	SMPL	
PB163303BS - 1	LCSS	14356	3.4990	-7471B	PPB	11 Sep 2024 12:30:33	U	SMPL	
P3857-01 - 1	WC-C1-COMP	9798	2.4055	-7471B	PPB	11 Sep 2024 12:32:49	U	SMPL	
P3857-04 - 1	WC-C2-COMP	3199	0.8222	-7471B	PPB	11 Sep 2024 12:35:08	U	SMPL	
P3857-07 - 1	WC-D1-COMP	2208	0.5845	-7471B	PPB	11 Sep 2024 12:37:28	U	SMPL	
P3857-10 - 1	WC-D2-COMP	2140	0.5682	-7471B	PPB	11 Sep 2024 12:39:47	U	SMPL	
P3861-01 - 1	DN-B-37	5360	1.3407	-7471B	PPB	11 Sep 2024 12:42:03	U	SMPL	
CCV62 - 1	CCV62	19944	4.8397	-7471B	PPB	11 Sep 2024 12:44:18	U	SMPL	
CCB62 - 1	CCB62	-218	0.0024	-7471B	PPB	11 Sep 2024 12:46:36	U	SMPL	
P3888-01 - 1	DN-B-36	840	0.2563	-7471B	PPB	11 Sep 2024 12:53:27	U	SMPL	
P3888-02 - 1	DN-W-02	4213	1.0655	-7471B	PPB	11 Sep 2024 12:55:43	U	SMPL	
P3891-01 - 1	AUD-SBG	2253	0.5953	-7471B	PPB	11 Sep 2024 12:57:59	U	SMPL	
P3892-01 - 1	ARS20-005	2093	0.5569	-7471B	PPB	11 Sep 2024 13:00:17	U	SMPL	
P3905-01 - 1	TP-3A	1231	0.3501	-7471B	PPB	11 Sep 2024 13:08:49	U	SMPL	
P3905-01DUP - 1	TP-3ADUP	1178	0.3374	-7471B	PPB	11 Sep 2024 13:11:05	U	SMPL	
P3905-01MS - 1	TP-3AMS	19806	4.8066	-7471B	PPB	11 Sep 2024 13:13:22	U	SMPL	
P3905-01MSD - 1	TP-3AMSD	17713	4.3044	-7471B	PPB	11 Sep 2024 13:15:38	U	SMPL	
CCV63 - 1	CCV63	20709	5.0232	-7471B	PPB	11 Sep 2024 13:17:56	U	SMPL	
CCB63 - 1	CCB63	-163	0.0156	-7471B	PPB	11 Sep 2024 13:20:15	U	SMPL	
P3905-03 - 1	TP-3B	2947	0.7618	-7471B	PPB	11 Sep 2024 13:22:34	U	SMPL	
P3905-05 - 1	COMP-1	1207	0.3443	-7471B	PPB	11 Sep 2024 13:24:50	U	SMPL	
PB163304BL - 1	PBS	-13	0.0516	-7471B	PPB	11 Sep 2024 13:27:07	U	SMPL	
PB163304BS - 1	LCSS	15201	3.7018	-7471B	PPB	11 Sep 2024 13:29:23	U	SMPL	
P3906-01 - 1	SU-701-COMP-01	2565	0.6701	-7471B	PPB	11 Sep 2024 13:31:38	U	SMPL	
P3906-07 - 1	SU-701-COMP-02	3628	0.9252	-7471B	PPB	11 Sep 2024 13:33:57	U	SMPL	
P3906-13 - 1	SU-701-COMP-03	35313	8.5271	-7471B	PPB	11 Sep 2024 13:36:14	U	SMPL	
P3907-01 - 1	PL-701-COMP-54	1532	0.4223	-7471B	PPB	11 Sep 2024 13:38:32	U	SMPL	
P3907-07 - 1	PL-701-COMP-55	10223	2.5074	-7471B	PPB	11 Sep 2024 13:40:56	U	SMPL	
P3911-01 - 1	SP-1	4528	1.1411	-7471B	PPB	11 Sep 2024 13:43:12	U	SMPL	
CCV64 - 1	CCV64	20863	5.0602	-7471B	PPB	11 Sep 2024 13:45:29	U	SMPL	
CCB64 - 1	CCB64	-194	0.0082	-7471B	PPB	11 Sep 2024 13:47:46	U	SMPL	
P3911-03 - 1	SP-2	7825	1.9321	-7471B	PPB	11 Sep 2024 13:50:05	U	SMPL	
P3911-05 - 1	SP-3	6855	1.6994	-7471B	PPB	11 Sep 2024 13:52:20	U	SMPL	
P3914-01 - 1	904	345	0.1375	-7471B	PPB	11 Sep 2024 13:54:37	U	SMPL	
P3916-01 - 1	SU-04-090924	924	0.2764	-7471B	PPB	11 Sep 2024 13:56:55	U	SMPL	
P3917-01 - 1	DN-B-35	17539	4.2627	-7471B	PPB	11 Sep 2024 13:59:10	U	SMPL	
P3917-01DUP - 1	DN-B-35DUP	17235	4.1898	-7471B	PPB	11 Sep 2024 14:01:27	U	SMPL	
P3917-01MS - 1	DN-B-35MS	34393	8.3063	-7471B	PPB	11 Sep 2024 14:03:48	U	SMPL	
P3917-01MSD - 1	DN-B-35MSD	34336	8.2927	-7471B	PPB	11 Sep 2024 14:12:36	U	SMPL	
P3880-01 - 1	SHEEPSHEAD-SOIL-PILE	8209	2.0242	-7471B	PPB	11 Sep 2024 14:14:53	U	SMPL	
P3881-01 - 1	VNJ-217	706	0.2241	-7471B	PPB	11 Sep 2024 14:17:13	U	SMPL	
CCV65 - 1	CCV65	21677	5.2555	-7471B	PPB	11 Sep 2024 14:19:31	U	SMPL	
CCB65 - 1	CCB65	-169	0.0142	-7471B	PPB	11 Sep 2024 14:21:46	U	SMPL	
P3905-01LX5 - 1		145	0.0895	-7471B	PPB	11 Sep 2024 16:49:46	U	SMPL	
P3905-01A - 1		18294	4.4438	-7471B	PPB	11 Sep 2024 16:52:00	U	SMPL	
P3917-01LX5 - 1		2773	0.7200	-7471B	PPB	11 Sep 2024 16:54:16	U	SMPL	
P3917-01A - 1		33358	8.0580	-7471B	PPB	11 Sep 2024 16:56:34	U	SMPL	
CCV66 - 1	CCV66	21445	5.1998	-7471B	PPB	11 Sep 2024 16:58:49	U	SMPL	
CCB66 - 1	CCB66	-288	-0.0144	-7471B	PPB	11 Sep 2024 17:01:08	U	SMPL	