


LB132451, ANALYSIS DATE:092124, INSTRUMENT ID:CV1

SFAM01.1

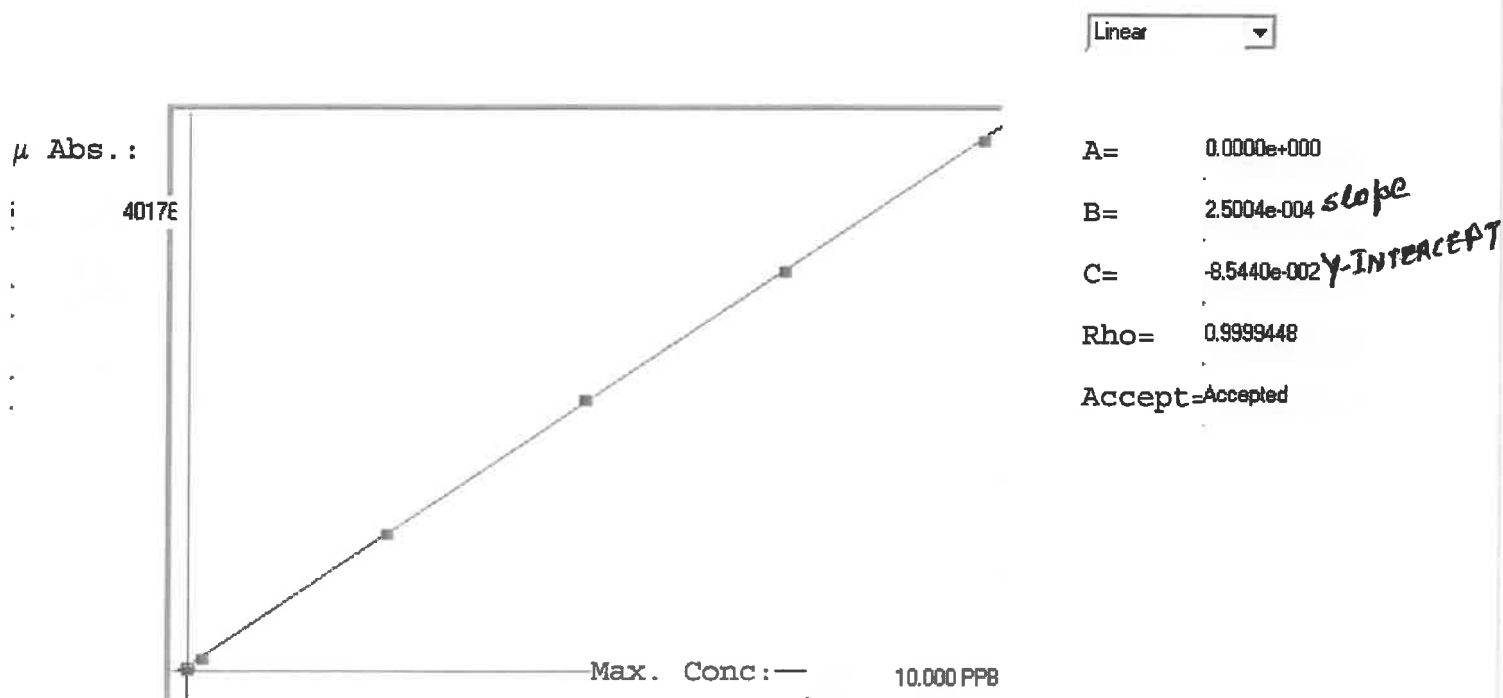

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.00	0.000	-0.033	-0.033	210	0.000	210				
0.05	0.050					442	0			
0.20	0.200	0.176	-0.024	1044	0.0 %	1044				
2.50	2.500	2.533	0.033	10471	0.0 %	10471				
5.00	5.000	5.068	0.068	20612	0.0 %	20612				
7.50	7.500	7.496	-0.004	30323	0.0 %	30323				
10.0	10.000	9.960	-0.040	40176	0.0 %	40176				

Handwritten notes on the right side of the table:

7.12

-12

1

000

LB132451, ANALYSIS DATE:092124, INSTRUMENT ID:CV1

Sample ID	Extended II μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
0 S0	210	-		0 SFAM01.1	PPB	9/21/2024 18:52	Std
0.2 S01	1044	-		0.2 SFAM01.1	PPB	9/21/2024 18:56	Std
2.5 S02	10471	-		2.5 SFAM01.1	PPB	9/21/2024 18:58	Std
5 S03	20612	-		5 SFAM01.1	PPB	9/21/2024 19:01	Std
7.5 S04	30323	-		7.5 SFAM01.1	PPB	9/21/2024 19:03	Std
10 S05	40176	-		10 SFAM01.1	PPB	9/21/2024 19:05	Std
ICV001	ICV001	15752	3.8531 -	SFAM01.1	PPB	9/21/2024 19:08	SMPL
ICB001	ICB001	10	-0.0829 -	SFAM01.1	PPB	9/21/2024 19:11	SMPL
CCV001	CCV001	20985	5.1616 -	SFAM01.1	PPB	9/21/2024 19:13	SMPL
CCB001	CCB001	6	-0.0839 -	SFAM01.1	PPB	9/21/2024 19:15	SMPL
PB163581F	PBW581	194	-0.0369 -	SFAM01.1	PPB	9/21/2024 19:18	SMPL
P3951-01	MC0B25	126	-0.0539 -	SFAM01.1	PPB	9/21/2024 19:20	SMPL
P3951-02	MC0B26	219	-0.0307 -	SFAM01.1	PPB	9/21/2024 19:22	SMPL
P3951-03	MC0B35	159	-0.0457 -	SFAM01.1	PPB	9/21/2024 19:24	SMPL
P3951-04	MC0B48	190	-0.0379 -	SFAM01.1	PPB	9/21/2024 19:27	SMPL
P3951-05	MC0B52	185	-0.0392 -	SFAM01.1	PPB	9/21/2024 19:29	SMPL
P3951-06	MC0B65	215	-0.0317 -	SFAM01.1	PPB	9/21/2024 19:31	SMPL
P3951-07	MC0B38	213	-0.0322 -	SFAM01.1	PPB	9/21/2024 19:33	SMPL
P3951-08	MC0B40	207	-0.0337 -	SFAM01.1	PPB	9/21/2024 19:36	SMPL
P3951-09	MC0B49	198	-0.0359 -	SFAM01.1	PPB	9/21/2024 19:38	SMPL
P3951-10	MC0B51	1438	0.2741 -	SFAM01.1	PPB	9/21/2024 19:40	SMPL
P3951-11	MC0B51D	1502	0.2901 -	SFAM01.1	PPB	9/21/2024 19:42	SMPL
P3951-12	MC0B51S	6481	1.535 -	SFAM01.1	PPB	9/21/2024 19:45	SMPL
P3951-13	MC0B57	163	-0.0447 -	SFAM01.1	PPB	9/21/2024 19:47	SMPL
P3951-14	MC0B63	1117	0.1938 -	SFAM01.1	PPB	9/21/2024 19:49	SMPL
P3951-15	MC0B20	48	-0.0734 -	SFAM01.1	PPB	9/21/2024 19:51	SMPL
P3951-16	MC0B24	147	-0.0487 -	SFAM01.1	PPB	9/21/2024 19:54	SMPL
P3951-17	MC0B29	174	-0.0419 -	SFAM01.1	PPB	9/21/2024 19:56	SMPL
P3951-18	MC0B31	289	-0.0132 -	SFAM01.1	PPB	9/21/2024 19:58	SMPL
P3951-19	MC0B46	170	-0.0429 -	SFAM01.1	PPB	9/21/2024 20:01	SMPL
P3951-20	MC0B67	198	-0.0359 -	SFAM01.1	PPB	9/21/2024 20:03	SMPL
P3951-21	MC0B70	159	-0.0457 -	SFAM01.1	PPB	9/21/2024 20:05	SMPL
CCV002	CCV002	19665	4.8315 -	SFAM01.1	PPB	9/21/2024 20:07	SMPL
CCB002	CCB002	51	-0.0727 -	SFAM01.1	PPB	9/21/2024 20:10	SMPL