


LB132659

7470A

INSTRUMENT ID: CV1

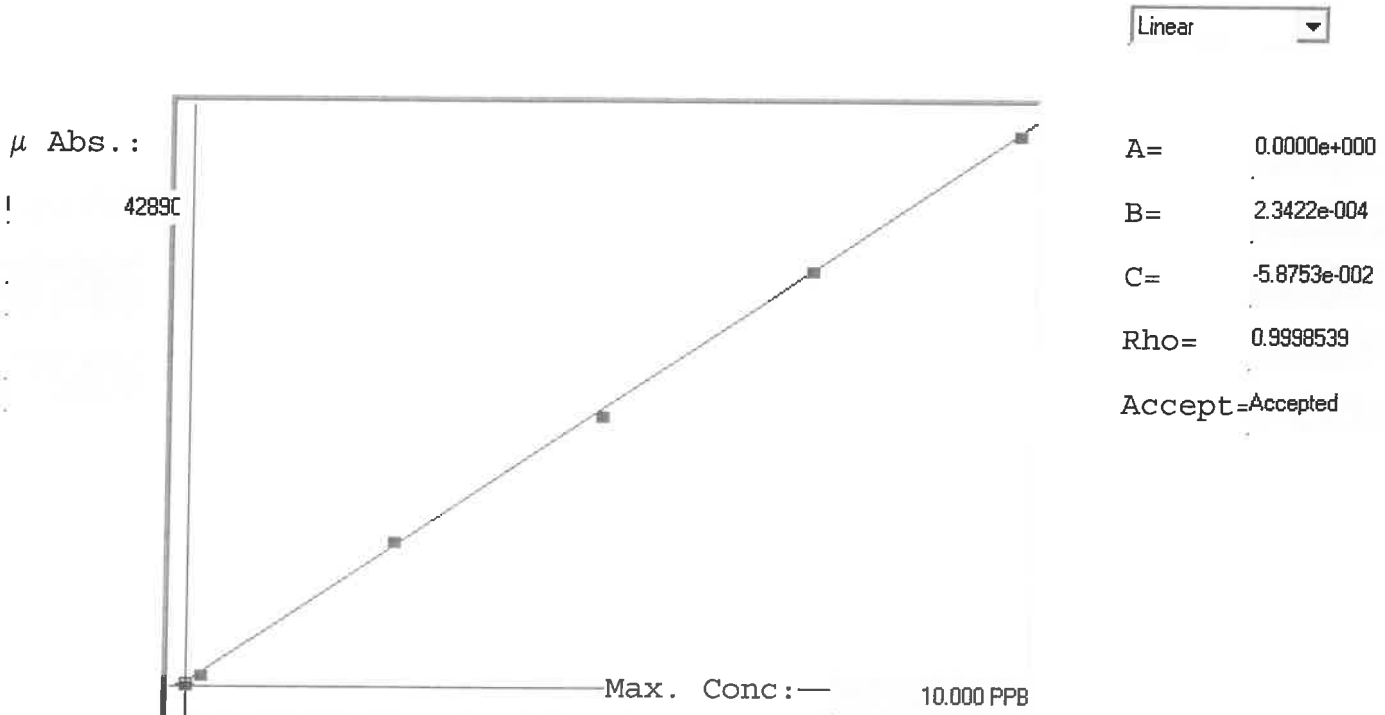

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/00
0.0	0.000	-0.011	-0.011	203	0.000	203	0				
0.2	0.200	0.176	-0.024	1001	0.0 %	1001					
2.5	2.500	2.601	0.101	11357	0.0 %	11357					
5.0	5.000	4.898	-0.102	21165	0.0 %	21165					
7.5	7.500	7.549	0.049	32482	0.0 %	32482					
10.0	10.000	9.987	-0.013	42890	0.0 %	42890					

LB132659 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 30 Sep 2024 08:45:56

Sample ID	Extended ID	μ Abs	Conc	Strnd Conc	Method	Units	Date	Type	Type
0.0 - 1	50	203	-	0.0000	7470A	PPB	30 Sep 2024 09:53:25	S	Std
0.2 - 1	50.2	1001	-	0.2000	7470A	PPB	30 Sep 2024 09:58:14	S	Std
2.5 - 1	52.8	11357	-	2.5000	7470A	PPB	30 Sep 2024 10:00:31	S	Std
5.0 - 1	55	21165	-	5.0000	7470A	PPB	30 Sep 2024 10:02:48	S	Std
7.5 - 1	57.5	32482	-	7.5000	7470A	PPB	30 Sep 2024 10:05:05	S	Std
10.0 - 1	59.5	42890	-	10.0000	7470A	PPB	30 Sep 2024 10:07:22	S	Std
ICV14 - 1	ICV14	16050	3.7004	-	7470A	PPB	30 Sep 2024 10:10:09	U	SMPL
ICB14 - 1	ICB14	0	-0.0588	-	7470A	PPB	30 Sep 2024 10:12:23	U	SMPL
CCV41 - 1	CCV41	21811	5.0497	-	7470A	PPB	30 Sep 2024 10:14:40	U	SMPL
CCB41 - 1	CCB41	-36	-0.0672	-	7470A	PPB	30 Sep 2024 10:16:55	U	SMPL
CRA - 1	CRA	1166	0.2143	-	7470A	PPB	30 Sep 2024 10:19:11	U	SMPL
HighStd - 1	HighStd	42740	9.9516	-	7470A	PPB	30 Sep 2024 10:21:26	U	SMPL
ChkStd - 1	ChkStd	29902	6.9448	-	7470A	PPB	30 Sep 2024 10:23:41	U	SMPL
PB163750BL - 1	PBW	250	-0.0002	-	7470A	PPB	30 Sep 2024 10:28:35	U	SMPL
PB163750BS - 1	LCSW	17195	3.9686	-	7470A	PPB	30 Sep 2024 10:30:51	U	SMPL
P4190-04 - 1	TP-T	-20	-0.0634	-	7470A	PPB	30 Sep 2024 10:33:07	U	SMPL
P4192-02 - 1	VNU-222	119	-0.0309	-	7470A	PPB	30 Sep 2024 10:35:24	U	SMPL
P4192-04 - 1	ETGI-355	132	-0.0278	-	7470A	PPB	30 Sep 2024 10:37:40	U	SMPL
P4192-04DUP - 1	ETGI-355DUP	4	-0.0578	-	7470A	PPB	30 Sep 2024 10:39:57	U	SMPL
P4192-04MS - 1	ETGI-355MS	16671	3.8459	-	7470A	PPB	30 Sep 2024 10:44:47	U	SMPL
CCV42 - 1	CCV42	21490	4.9746	-	7470A	PPB	30 Sep 2024 10:47:03	U	SMPL
CCB42 - 1	CCB42	-83	-0.0782	-	7470A	PPB	30 Sep 2024 10:49:20	U	SMPL
P4192-04MSD - 1	ETGI-355MSD	17418	4.0208	-	7470A	PPB	30 Sep 2024 10:51:37	U	SMPL
PB163751BL - 1	PBW	-6	-0.0602	-	7470A	PPB	30 Sep 2024 10:53:52	U	SMPL
PB163751BS - 1	LCSW	17318	3.9974	-	7470A	PPB	30 Sep 2024 10:56:08	U	SMPL
P4194-02 - 1	MANHOLE-119-KEARNY	78	-0.0405	-	7470A	PPB	30 Sep 2024 10:58:24	U	SMPL
P4194-02DUP - 1	MANHOLE-119-KEARNYDUP	-22	-0.0639	-	7470A	PPB	30 Sep 2024 11:00:40	U	SMPL
P4194-02MS - 1	MANHOLE-119-KEARNYMS	17250	3.9815	-	7470A	PPB	30 Sep 2024 11:02:57	U	SMPL
P4194-02MSD - 1	MANHOLE-119-KEARNYMSD	20370	4.7122	-	7470A	PPB	30 Sep 2024 11:05:13	U	SMPL
PB163752BL - 1	PBW	-124	-0.0878	-	7470A	PPB	30 Sep 2024 11:07:31	U	SMPL
PB163752BS - 1	LCSW	17728	4.0934	-	7470A	PPB	30 Sep 2024 11:12:29	U	SMPL
P4172-01 - 1	FMI120	-81	-0.0777	-	7470A	PPB	30 Sep 2024 11:14:44	U	SMPL
CCV43 - 1	CCV43	21652	5.0125	-	7470A	PPB	30 Sep 2024 11:17:00	U	SMPL
CCB43 - 1	CCB43	-81	-0.0777	-	7470A	PPB	30 Sep 2024 11:19:15	U	SMPL
P4194-01 - 1	MANHOLE-119-KEARNY	-55	-0.0716	-	7470A	PPB	30 Sep 2024 11:21:32	U	SMPL
P4204-02 - 1	BP-RW5FRACTANKSED-20240925	232	-0.0044	-	7470A	PPB	30 Sep 2024 11:23:48	U	SMPL
P4209-01 - 1	DRUM-1	9014	2.0525	-	7470A	PPB	30 Sep 2024 11:26:03	U	SMPL
P4209-02 - 1	DRUM-2	-154	-0.0948	-	7470A	PPB	30 Sep 2024 11:28:19	U	SMPL
P4209-02DUP - 1	DRUM-2DUP	254	0.0007	-	7470A	PPB	30 Sep 2024 11:30:38	U	SMPL
P4209-02MS - 1	DRUM-2MS	20330	4.7029	-	7470A	PPB	30 Sep 2024 11:32:54	U	SMPL
P4209-02MSD - 1	DRUM-2MSD	18090	4.1782	-	7470A	PPB	30 Sep 2024 11:35:11	U	SMPL
PB168688TB - 1	PB168688TB	60	-0.0447	-	7470A	PPB	30 Sep 2024 11:37:29	U	SMPL
PB163710TB - 1	PB163710TB	-32	-0.0662	-	7470A	PPB	30 Sep 2024 11:39:47	U	SMPL
CCV44 - 1	CCV44	22070	5.1104	-	7470A	PPB	30 Sep 2024 11:47:05	U	SMPL
CCB44 - 1	CCB44	20	-0.0541	-	7470A	PPB	30 Sep 2024 11:49:20	U	SMPL
P4192-04LX5 - 1		51	-0.0468	-	7470A	PPB	30 Sep 2024 11:51:37	U	SMPL
P4192-04A - 1		16635	3.8374	-	7470A	PPB	30 Sep 2024 11:53:52	U	SMPL
P4194-02LX5 - 1		76	-0.0410	-	7470A	PPB	30 Sep 2024 11:56:07	U	SMPL
P4194-02A - 1		16687	3.8498	-	7470A	PPB	30 Sep 2024 11:58:23	U	SMPL
P4209-02LX5 - 1		233	-0.0042	-	7470A	PPB	30 Sep 2024 12:00:38	U	SMPL
P4209-02A - 1		17341	4.0028	-	7470A	PPB	30 Sep 2024 12:02:55	U	SMPL
CCV45 - 1	CCV45	21971	5.0872	-	7470A	PPB	30 Sep 2024 12:05:11	U	SMPL
CCB45 - 1	CCB45	-3	-0.0595	-	7470A	PPB	30 Sep 2024 12:07:28	U	SMPL