


LB182696

7470A

INSTRUMENT ID: CV1

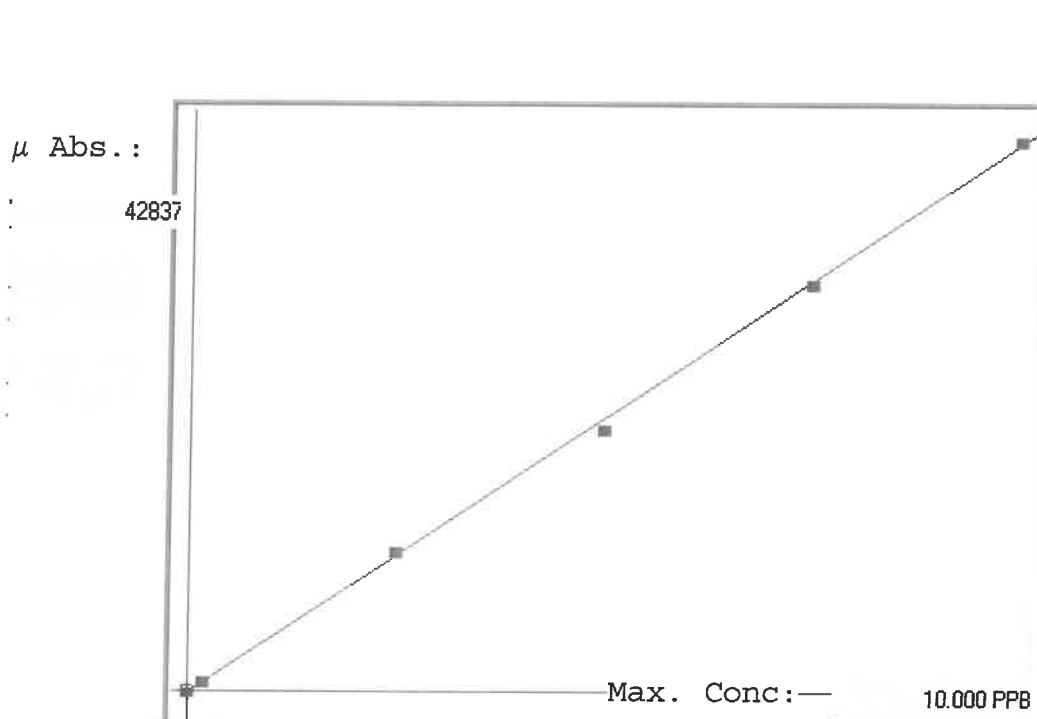

Linear

A= 0.0000e+000

B= 2.3429e-004

C= 4.3856e-002

Rho= 0.9996962

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%ad
0.0	0.000	0.017	0.017	-114	0.000	-114	0				10
0.2	0.200	0.220	0.020	752	0.0 %	752					4
2.5	2.500	2.588	0.088	10858	0.0 %	10858					4
5.0	5.000	4.814	-0.186	20362	0.0 %	20362					4
7.5	7.500	7.480	-0.020	31741	0.0 %	31741					0
10.0	10.000	10.080	0.080	42837	0.0 %	42837					1

LB132696 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 02 Oct 2024 09:07:07

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-114	-	0.0000	7470A	PPB	02 Oct 2024 09:19:02	S	Std
0.2 - 1	51.2	752	-	0.2000	7470A	PPB	02 Oct 2024 09:21:19	S	Std
2.5 - 1	52.5	10858	-	2.5000	7470A	PPB	02 Oct 2024 09:23:36	S	Std
5.0 - 1	55	20362	-	5.0000	7470A	PPB	02 Oct 2024 09:25:52	S	Std
7.5 - 1	57.5	31741	-	7.5000	7470A	PPB	02 Oct 2024 09:28:10	S	Std
10.0 - 1	510	42837	-	10.0000	7470A	PPB	02 Oct 2024 09:33:02	S	Std
ICV19 - 1	ICV19	16760	3.9706	-	7470A	PPB	02 Oct 2024 09:35:47	U	SMPL
ICB19 - 1	ICB19	-289	-0.0239	-	7470A	PPB	02 Oct 2024 09:38:03	U	SMPL
CCV58 - 1	CCV58	20189	4.7739	-	7470A	PPB	02 Oct 2024 09:40:20	U	SMPL
CCB58 - 1	CCB58	-170	0.0040	-	7470A	PPB	02 Oct 2024 09:42:35	U	SMPL
CRA - 1	CRA	637	0.1931	-	7470A	PPB	02 Oct 2024 09:44:52	U	SMPL
HighStd - 1	HighStd	41578	9.7852	-	7470A	PPB	02 Oct 2024 09:47:06	U	SMPL
ChkStd - 1	ChkStd	29215	6.8886	-	7470A	PPB	02 Oct 2024 09:49:22	U	SMPL
PB163827BL - 1	PBW	-36	0.0354	-	7470A	PPB	02 Oct 2024 09:54:27	U	SMPL
PB163827BS - 1	LCSW	17700	4.1908	-	7470A	PPB	02 Oct 2024 09:56:42	U	SMPL
P4214-02 - 1	CONCRETE-WC-1	-54	0.0312	-	7470A	PPB	02 Oct 2024 09:58:59	U	SMPL
P4222-04 - 1	TP-5	184	0.0870	-	7470A	PPB	02 Oct 2024 10:01:18	U	SMPL
P4232-04 - 1	TP-R	-101	0.0202	-	7470A	PPB	02 Oct 2024 10:03:36	U	SMPL
P4236-04 - 1	TP4	39	0.0530	-	7470A	PPB	02 Oct 2024 10:05:52	U	SMPL
P4236-08 - 1	TP3	382	0.1334	-	7470A	PPB	02 Oct 2024 10:08:07	U	SMPL
CCV59 - 1	CCV59	21521	5.0860	-	7470A	PPB	02 Oct 2024 10:10:23	U	SMPL
CCB59 - 1	CCB59	73	0.0610	-	7470A	PPB	02 Oct 2024 10:22:28	U	SMPL
P4236-12 - 1	TP1	1632	0.4262	-	7470A	PPB	02 Oct 2024 10:24:43	U	SMPL
P4236-16 - 1	TP2	1974	0.5063	-	7470A	PPB	02 Oct 2024 10:26:58	U	SMPL
P4236-16DUP - 1	TP2DUP	2275	0.5769	-	7470A	PPB	02 Oct 2024 10:29:13	U	SMPL
P4236-16MS - 1	TP2MS	18894	4.4705	-	7470A	PPB	02 Oct 2024 10:31:28	U	SMPL
P4236-16MSD - 1	TP2MSD	16386	3.8829	-	7470A	PPB	02 Oct 2024 10:33:44	U	SMPL
PB163746TB - 1	PB163746TB	-155	0.0075	-	7470A	PPB	02 Oct 2024 10:36:02	U	SMPL
PB163805TB - 1	PB163805TB	-89	0.0230	-	7470A	PPB	02 Oct 2024 10:38:19	U	SMPL
P4236-16LX5 - 1		541	0.1706	-	7470A	PPB	02 Oct 2024 10:40:36	U	SMPL
P4236-16A - 1		17021	4.0317	-	7470A	PPB	02 Oct 2024 10:42:52	U	SMPL
CCV60 - 1	CCV60	21833	5.1591	-	7470A	PPB	02 Oct 2024 10:45:08	U	SMPL
CCB60 - 1	CCB60	4993	1.2137	-	7470A	PPB	02 Oct 2024 10:47:25	U	SMPL
CCB60 - 1	CCB60	232	0.0982	-	7470A	PPB	02 Oct 2024 10:50:01	U	SMPL