


LB132700

7471B

INSTRUMENT ID: CV2

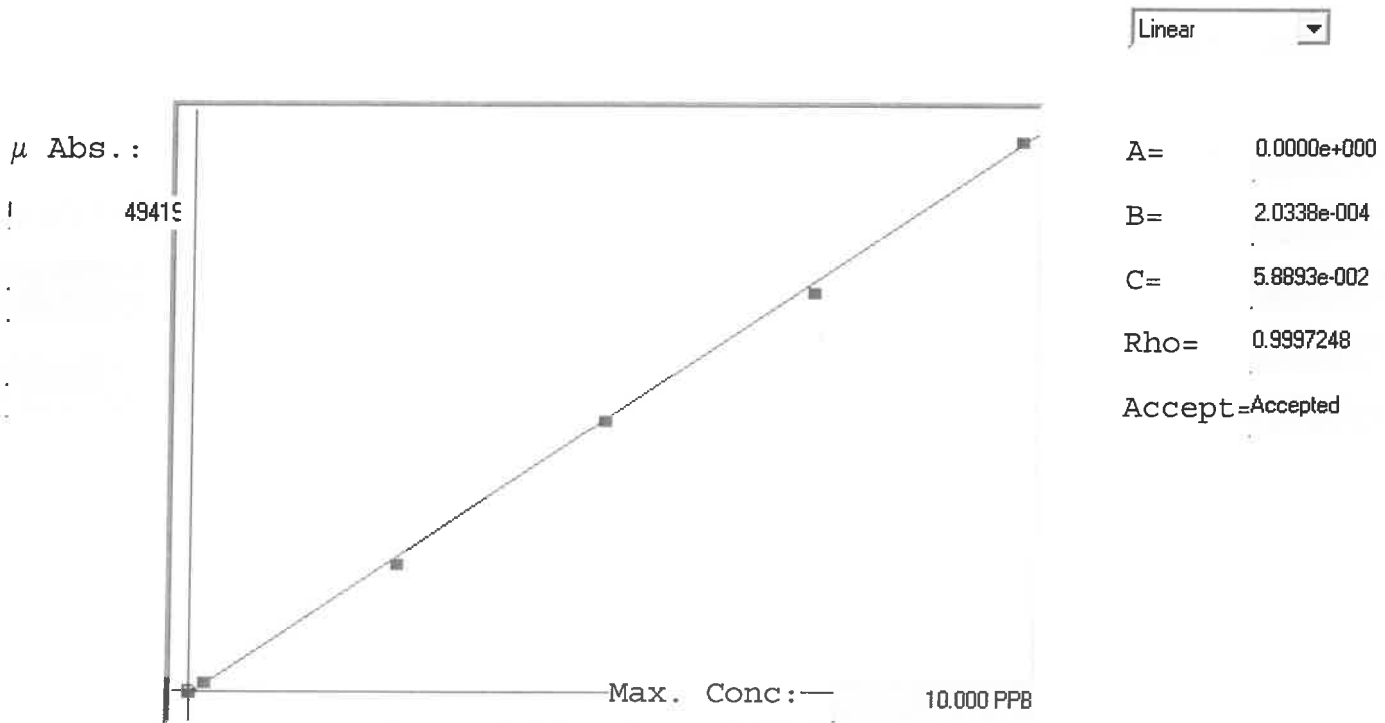

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/00
0.0	0.000	0.053	0.053	-30	0.000	-30					19
0.2	0.200	0.238	0.038	881	0.0 %	881					-3
2.5	2.500	2.415	-0.085	11584	0.0 %	11584					1
5.0	5.000	5.028	0.028	24435	0.0 %	24435					-2
7.5	7.500	7.356	-0.144	35881	0.0 %	35881					1
10.0	10.000	10.110	0.110	49419	0.0 %	49419					

LB132700 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 02 Oct 2024 11:20:03

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-30	-	0.0000	7471B	PPB	02 Oct 2024 11:20:13	S	Std
0.2 - 1	50.2	881	-	0.2000	7471B	PPB	02 Oct 2024 11:22:30	S	Std
2.5 - 1	52.5	11584	-	2.5000	7471B	PPB	02 Oct 2024 11:24:48	S	Std
5.0 - 1	55	24435	-	5.0000	7471B	PPB	02 Oct 2024 11:27:04	S	Std
7.5 - 1	57.5	35881	-	7.5000	7471B	PPB	02 Oct 2024 11:29:23	S	Std
10.0 - 1	510	49419	-	10.0000	7471B	PPB	02 Oct 2024 11:31:43	S	Std
ICV20 - 1	ICV20	17848	3.6888	-	7471B	PPB	02 Oct 2024 11:34:42	U	SMPL
ICB20 - 1	ICB20	-331	-0.0084	-	7471B	PPB	02 Oct 2024 11:36:58	U	SMPL
CCV61 - 1	CCV61	24441	5.0296	-	7471B	PPB	02 Oct 2024 11:39:16	U	SMPL
CCB61 - 1	CCB61	-271	0.0038	-	7471B	PPB	02 Oct 2024 11:41:31	U	SMPL
CRA - 1	CRA	725	0.2063	-	7471B	PPB	02 Oct 2024 11:47:11	U	SMPL
HighStd - 1	HighStd	49057	10.0360	-	7471B	PPB	02 Oct 2024 11:49:25	U	SMPL
ChkStd - 1	ChkStd	33406	6.8529	-	7471B	PPB	02 Oct 2024 11:51:41	U	SMPL
PB163856BL - 1	PBS	150	0.0894	-	7471B	PPB	02 Oct 2024 11:56:26	U	SMPL
PB163856BS - 1	LCSS	19950	4.1163	-	7471B	PPB	02 Oct 2024 12:02:17	U	SMPL
P4232-01 - 1	TP-R	5229	1.1224	-	7471B	PPB	02 Oct 2024 12:04:33	U	SMPL
P4234-01 - 1	EO-02-093024	11128	2.3221	-	7471B	PPB	02 Oct 2024 12:06:52	U	SMPL
P4236-01 - 1	TP4	970	0.2562	-	7471B	PPB	02 Oct 2024 12:09:11	U	SMPL
P4236-05 - 1	TP3	2451	0.5574	-	7471B	PPB	02 Oct 2024 12:11:31	U	SMPL
P4236-09 - 1	TP1	19356	3.9955	-	7471B	PPB	02 Oct 2024 12:13:47	U	SMPL
CCV62 - 1	CCV62	24833	5.1094	-	7471B	PPB	02 Oct 2024 12:16:03	U	SMPL
CCB62 - 1	CCB62	-185	0.0213	-	7471B	PPB	02 Oct 2024 12:18:22	U	SMPL
P4236-13 - 1	TP2	11314	2.3599	-	7471B	PPB	02 Oct 2024 12:20:40	U	SMPL
P4242-01 - 1	TP-Q	9193	1.9285	-	7471B	PPB	02 Oct 2024 12:22:55	U	SMPL
P4254-01 - 1	MH-147-SLUDGE	10875	2.2706	-	7471B	PPB	02 Oct 2024 12:25:13	U	SMPL
P4255-01 - 1	OR-03-100124	4727	1.0203	-	7471B	PPB	02 Oct 2024 12:27:30	U	SMPL
P4257-01 - 1	VNJ-240	6287	1.3375	-	7471B	PPB	02 Oct 2024 12:29:49	U	SMPL
P4257-01DUP - 1	VNJ-240DUP	6292	1.3385	-	7471B	PPB	02 Oct 2024 12:32:06	U	SMPL
P4257-01MS - 1	VNJ-240MS	26425	5.4331	-	7471B	PPB	02 Oct 2024 12:34:25	U	SMPL
P4257-01MSD - 1	VNJ-240MSD	27461	5.6438	-	7471B	PPB	02 Oct 2024 12:36:43	U	SMPL
P4257-01LX5 - 1		1090	0.2806	-	7471B	PPB	02 Oct 2024 12:39:06	U	SMPL
P4257-01A - 1		27146	5.5798	-	7471B	PPB	02 Oct 2024 12:41:26	U	SMPL
CCV63 - 1	CCV63	25227	5.1895	-	7471B	PPB	02 Oct 2024 12:43:44	U	SMPL
CCB63 - 1	CCB63	-270	0.0040	-	7471B	PPB	02 Oct 2024 12:46:04	U	SMPL