


Instrument IC-1				Analyst: NF		Method: 300.0 / 9056A						
Ident	Con F-	Con CL-		Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	Initial wt	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-091624	9/16/2024 11:39	10	NF/IZ
STD2	0.4240	0.6370	0.6450	2.1330	0.5360	1.0710	3.3060	IC1-091624	9/16/2024 12:00	10	NF/IZ	
STD3	0.8020	1.2020	1.2050	4.0080	1.0020	2.0240	6.0410	IC1-091624	9/16/2024 12:22	10	NF/IZ	
STD4	1.0070	1.5230	1.5170	5.0640	1.2670	2.5210	7.5910	IC1-091624	9/16/2024 12:43	10	NF/IZ	
STD5	1.9640	2.9360	2.9280	9.7810	2.4450	4.8600	14.5520	IC1-091624	9/16/2024 13:05	10	NF/IZ	
STD6	3.9620	5.9210	5.9210	19.7550	4.9240	9.9100	29.3540	IC1-091624	9/16/2024 13:26	10	NF/IZ	
STD7	5.0410	7.5810	7.5840	25.2590	6.3260	12.6140	37.6550	IC1-091624	9/16/2024 13:47	10	NF/IZ	
ICV	1.9500	2.9330	2.9300	9.7980	2.4400	4.9380	14.4910	IC1-091624	9/16/2024 15:00	10	NF/IZ	
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-091624	9/16/2024 15:21	10	NF/IZ	
CCV	1.9890	2.9500	2.9420	9.8510	2.4320	4.9270	14.6400	IC1-091624	10/14/2024 17:12	10	NF/IZ	
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-091624	10/14/2024 17:33	10	NF/IZ	
LB132938BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-091624	10/14/2024 17:55	10	NF/IZ	
LB132938BSW	1.9870	2.9480	2.9420	9.8350	2.4390	4.9180	14.5870	IC1-091624	10/14/2024 18:16	10	NF/IZ	
P4368-09	0.2350	0.3410	0.3590	1.1660	0.2870	0.6120	1.8840	IC1-091624	10/14/2024 18:38	10	NF/IZ	
P4368-09RE	0.1350	0.1980	0.2190	0.6810	0.1710	0.3560	1.1420	IC1-091624	10/14/2024 19:00	10	NF/IZ	
CCV	1.9920	2.9560	2.9480	9.8550	2.4470	4.9400	14.6750	IC1-091624	10/14/2024 19:21	10	NF/IZ	
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-091624	10/14/2024 19:43	10	NF/IZ	

Clear table

Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A										
ident	concentratio tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio n HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-091624	2024-09-16 11:39:1	10 NF/IZ
STD2	0.424	0.637	0.645	2.133	0.536	1.071	3.306	IC1-091624	2024-09-16 12:00:1	10 NF/IZ
STD3	0.802	1.202	1.205	4.008	1.002	2.024	6.041	IC1-091624	2024-09-16 12:22:1	10 NF/IZ
STD4	1.007	1.523	1.517	5.064	1.267	2.521	7.591	IC1-091624	2024-09-16 12:43:1	10 NF/IZ
STD5	1.964	2.936	2.928	9.781	2.445	4.86	14.552	IC1-091624	2024-09-16 13:05:1	10 NF/IZ
STD6	3.962	5.921	5.921	19.755	4.924	9.91	29.354	IC1-091624	2024-09-16 13:26:1	10 NF/IZ
STD7	5.041	7.581	7.584	25.259	6.326	12.614	37.655	IC1-091624	2024-09-16 13:47:1	10 NF/IZ
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4			
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000			
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000			
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000			
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000			
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000			
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000			
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000			
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4			
STD1										
STD2	6.0000	6.1667	7.5000	6.6500	7.2000	7.1000	10.2000			
STD3	0.2500	0.1667	0.4167	0.2000	0.2000	1.2000	0.6833			
STD4	0.7000	1.5333	1.1333	1.2800	1.3600	0.8400	1.2133			
STD5	-1.8000	-2.1333	-2.4000	-2.1900	-2.2000	-2.8000	-2.9867			
STD6	-0.9500	-1.3167	-1.3167	-1.2250	-1.5200	-0.9000	-2.1533			
STD7	0.8200	1.0800	1.1200	1.0360	1.2160	0.9120	1.7703			

Fluoride (Anions)

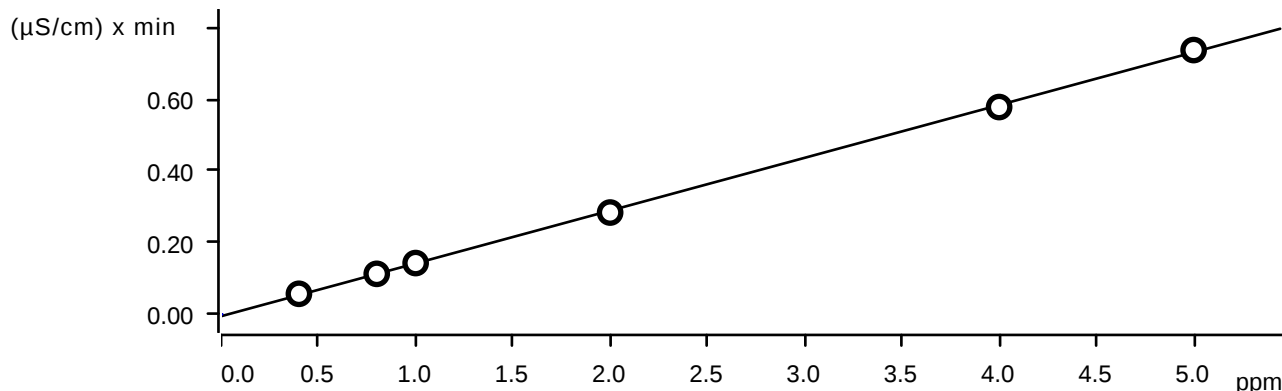


Function: $A = -5.20226E-3 + 0.0147183 \times Q$

Relative standard deviation 1.655264 %

Correlation coefficient 0.999855

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-09-16 11:39:22 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.057	STD2	2024-09-16 12:00:45 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.113	STD3	2024-09-16 12:22:09 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.143	STD4	2024-09-16 12:43:34 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.284	STD5	2024-09-16 13:05:00 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.578	STD6	2024-09-16 13:26:26 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.737	STD7	2024-09-16 13:47:53 UTC-4	used


Chloride (Anions)

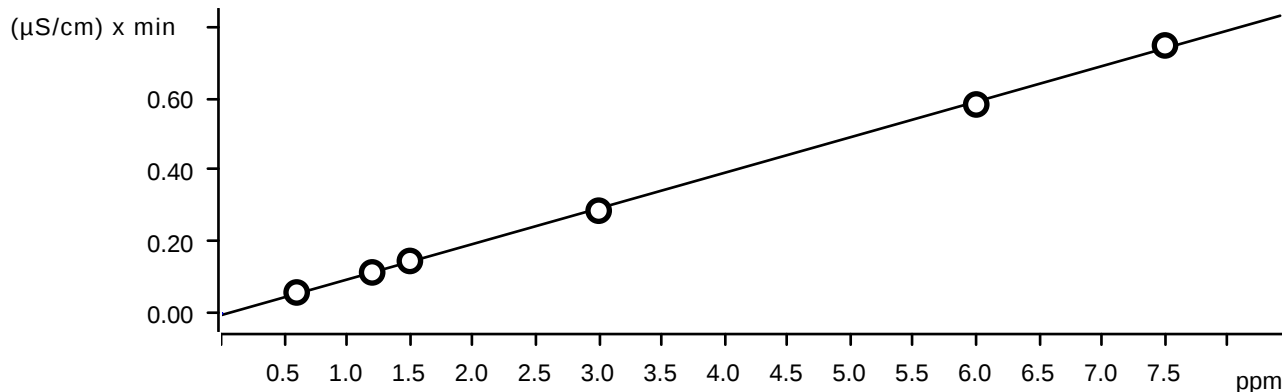

Function: $A = -4.73518E-3 + 9.92061E-3 \times Q$

Relative standard deviation 2.104599 %
Correlation coefficient 0.999766


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-09-16 11:39:22 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.058	STD2	2024-09-16 12:00:45 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.114	STD3	2024-09-16 12:22:09 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2024-09-16 12:43:34 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.287	STD5	2024-09-16 13:05:00 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.583	STD6	2024-09-16 13:26:26 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.747	STD7	2024-09-16 13:47:53 UTC-4	used

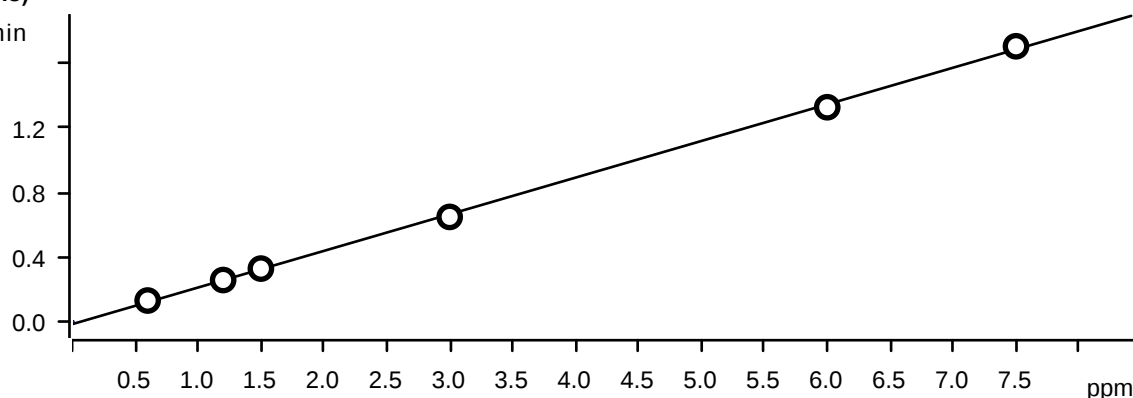Nitrite (Anions) $(\mu\text{S/cm}) \times \text{min}$ 

Function: $A = -0.0172576 + 0.0227000 \times Q$
Relative standard deviation 2.245267 %
Correlation coefficient 0.999738

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-09-16 11:39:22 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.129	STD2	2024-09-16 12:00:45 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.256	STD3	2024-09-16 12:22:09 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.327	STD4	2024-09-16 12:43:34 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.647	STD5	2024-09-16 13:05:00 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.327	STD6	2024-09-16 13:26:26 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.704	STD7	2024-09-16 13:47:53 UTC-4	used

Bromide (Anions)

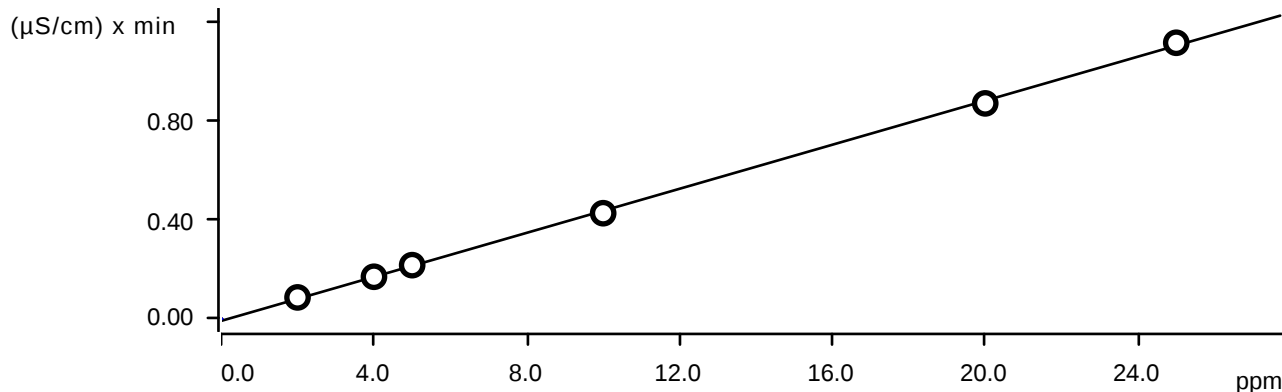


Function: $A = -8.29886E-3 + 4.43473E-3 \times Q$

Relative standard deviation: 2.051807 %

Correlation coefficient: 0.999778

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-09-16 11:39:22 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.086	STD2	2024-09-16 12:00:45 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.169	STD3	2024-09-16 12:22:09 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.216	STD4	2024-09-16 12:43:34 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.425	STD5	2024-09-16 13:05:00 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.868	STD6	2024-09-16 13:26:26 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.112	STD7	2024-09-16 13:47:53 UTC-4	used

Nitrate (Anions)

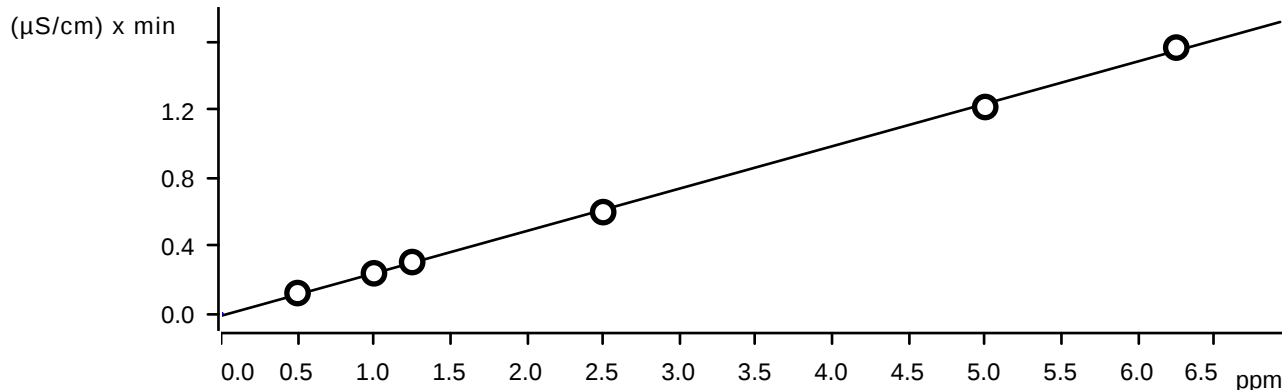

Function: $A = -0.0140308 + 0.0249539 \times Q$


Relative standard deviation: 2.352995 %

Correlation coefficient 0.999711

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-09-16 11:39:22 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.120	STD2	2024-09-16 12:00:45 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.236	STD3	2024-09-16 12:22:09 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.302	STD4	2024-09-16 12:43:34 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.596	STD5	2024-09-16 13:05:00 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.215	STD6	2024-09-16 13:26:26 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.565	STD7	2024-09-16 13:47:53 UTC-4	used

Phosphate (Anions)

(μS/cm) x min

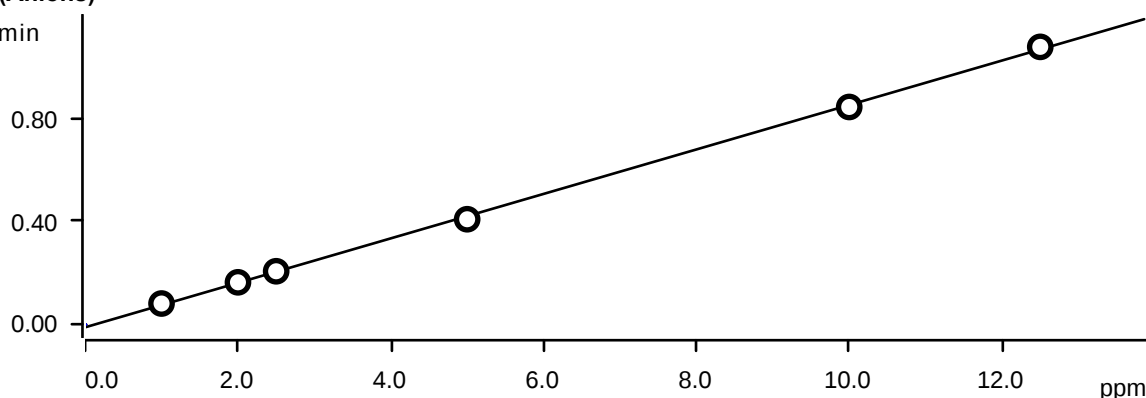
Function: $A = -0.0104137 + 8.60889E-3 \times Q$

Relative standard deviation 2.003622 %

Correlation coefficient 0.999791

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-09-16 11:39:22 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.082	STD2	2024-09-16 12:00:45 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.164	STD3	2024-09-16 12:22:09 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.207	STD4	2024-09-16 12:43:34 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.408	STD5	2024-09-16 13:05:00 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.843	STD6	2024-09-16 13:26:26 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.075	STD7	2024-09-16 13:47:53 UTC-4	used

Sulfate (Anions)

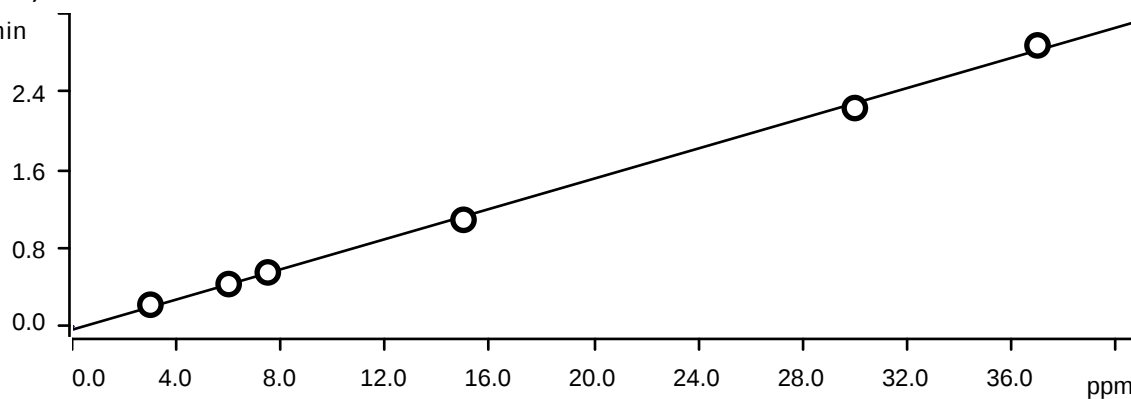 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0328706 + 7.71866E-3 \times Q$

Relative standard deviation 3.353471 %

Correlation coefficient 0.999413

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-09-16 11:39:22 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.222	STD2	2024-09-16 12:00:45 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.433	STD3	2024-09-16 12:22:09 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.553	STD4	2024-09-16 12:43:34 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.090	STD5	2024-09-16 13:05:00 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.233	STD6	2024-09-16 13:26:26 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.874	STD7	2024-09-16 13:47:53 UTC-4	used


Sample data

Ident STD1
Sample type Standard 1
Determination start 2024-09-16 11:39:22 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

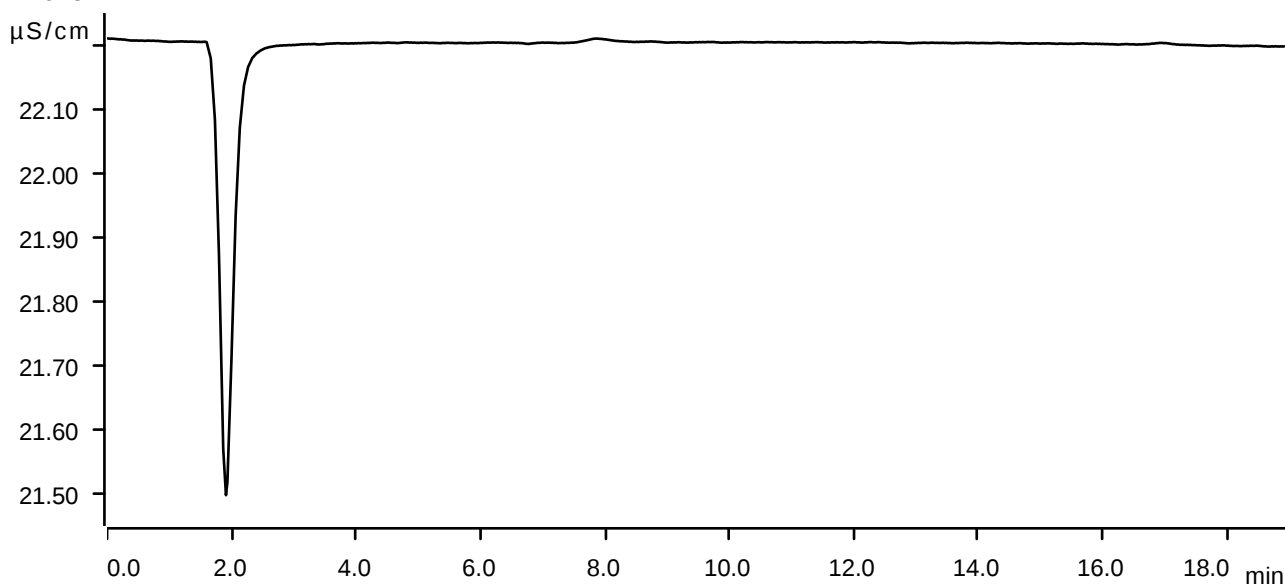


Sample data

Ident STD2
Sample type Standard 2
Determination start 2024-09-16 12:00:45 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.33 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

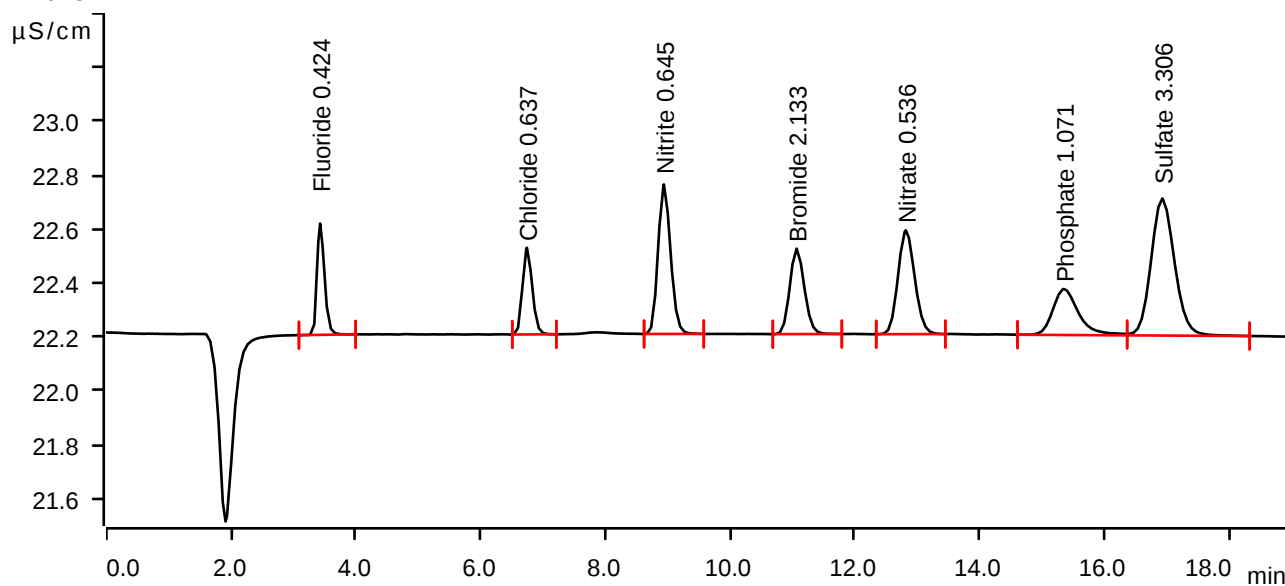

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.428	0.0572	0.413	0.424	Fluoride
2	6.743	0.0585	0.322	0.637	Chloride
3	8.940	0.1292	0.555	0.645	Nitrite
4	11.067	0.0863	0.317	2.133	Bromide
5	12.818	0.1197	0.385	0.536	Nitrate
6	15.352	0.0818	0.171	1.071	Phosphate
7	16.930	0.2223	0.508	3.306	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2024-09-16 12:22:09 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

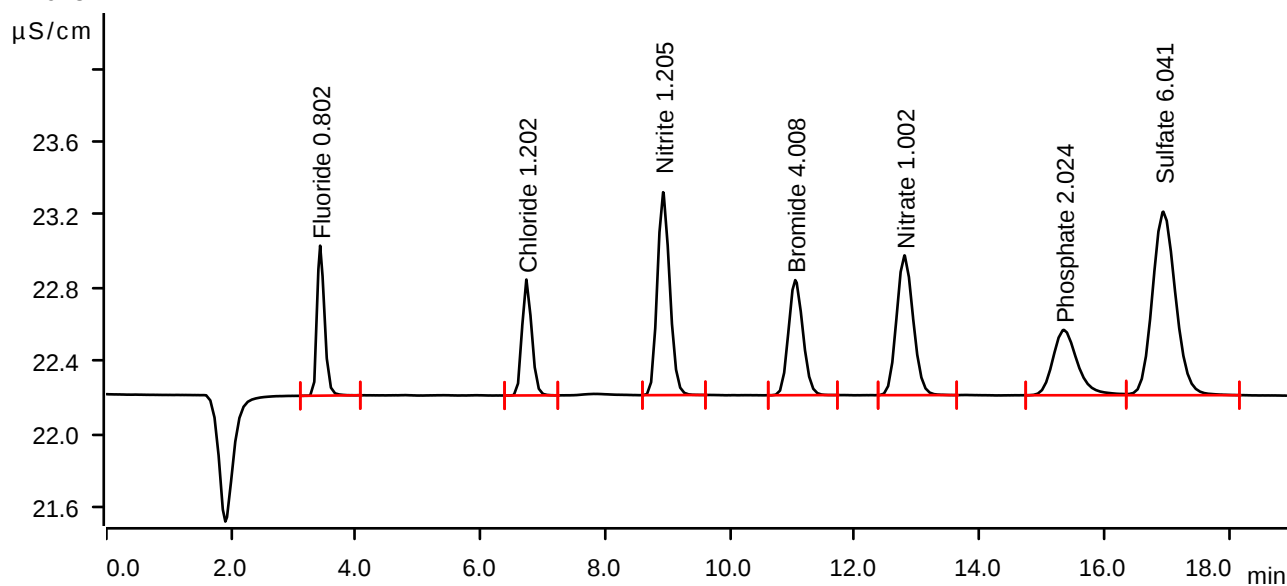

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.428	0.1129	0.820	0.802	Fluoride
2	6.735	0.1145	0.634	1.202	Chloride
3	8.927	0.2562	1.109	1.205	Nitrite
4	11.045	0.1695	0.629	4.008	Bromide
5	12.795	0.2360	0.764	1.002	Nitrate
6	15.353	0.1638	0.357	2.024	Phosphate
7	16.947	0.4334	1.003	6.041	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2024-09-16 12:43:34 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

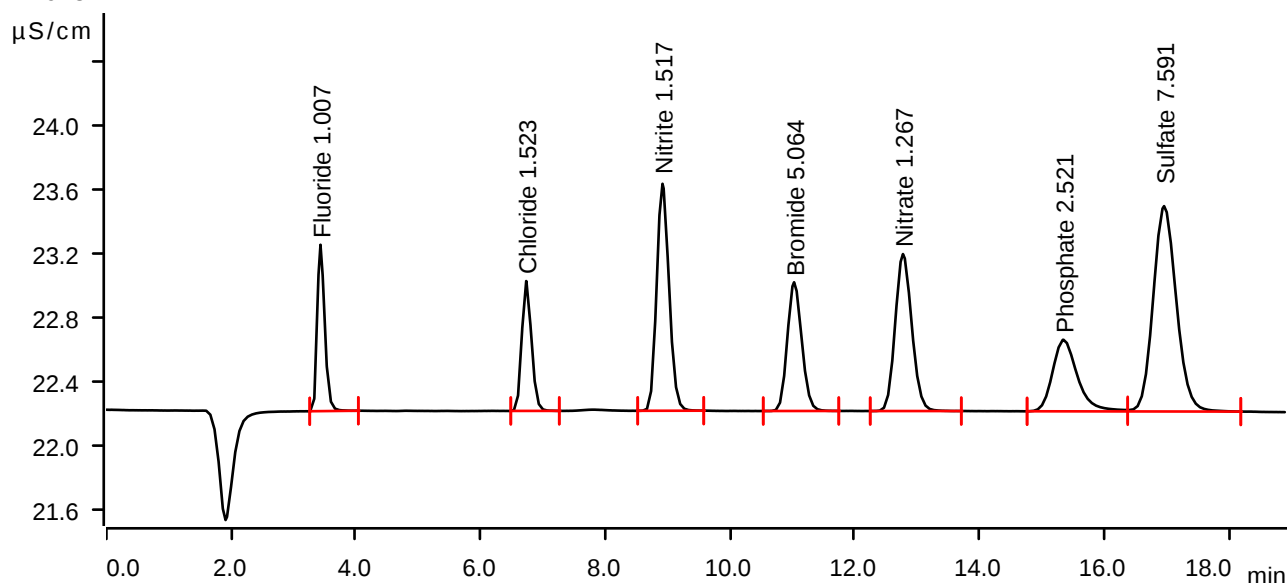

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.433	0.1429	1.040	1.007	Fluoride
2	6.732	0.1464	0.811	1.523	Chloride
3	8.917	0.3271	1.418	1.517	Nitrite
4	11.027	0.2163	0.804	5.064	Bromide
5	12.772	0.3021	0.981	1.267	Nitrate
6	15.345	0.2066	0.448	2.521	Phosphate
7	16.958	0.5530	1.283	7.591	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2024-09-16 13:05:00 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

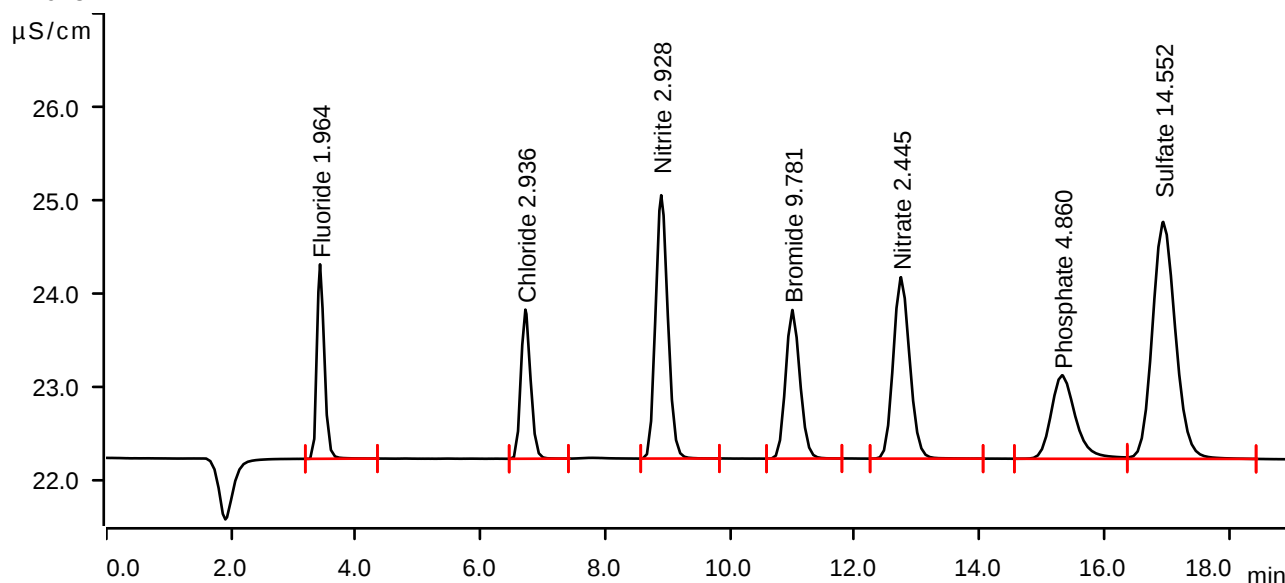

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.427	0.2838	2.088	1.964	Fluoride
2	6.718	0.2865	1.601	2.936	Chloride
3	8.897	0.6473	2.828	2.928	Nitrite
4	10.998	0.4255	1.596	9.781	Bromide
5	12.740	0.5961	1.949	2.445	Nitrate
6	15.323	0.4080	0.897	4.860	Phosphate
7	16.945	1.0904	2.544	14.552	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2024-09-16 13:26:26 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

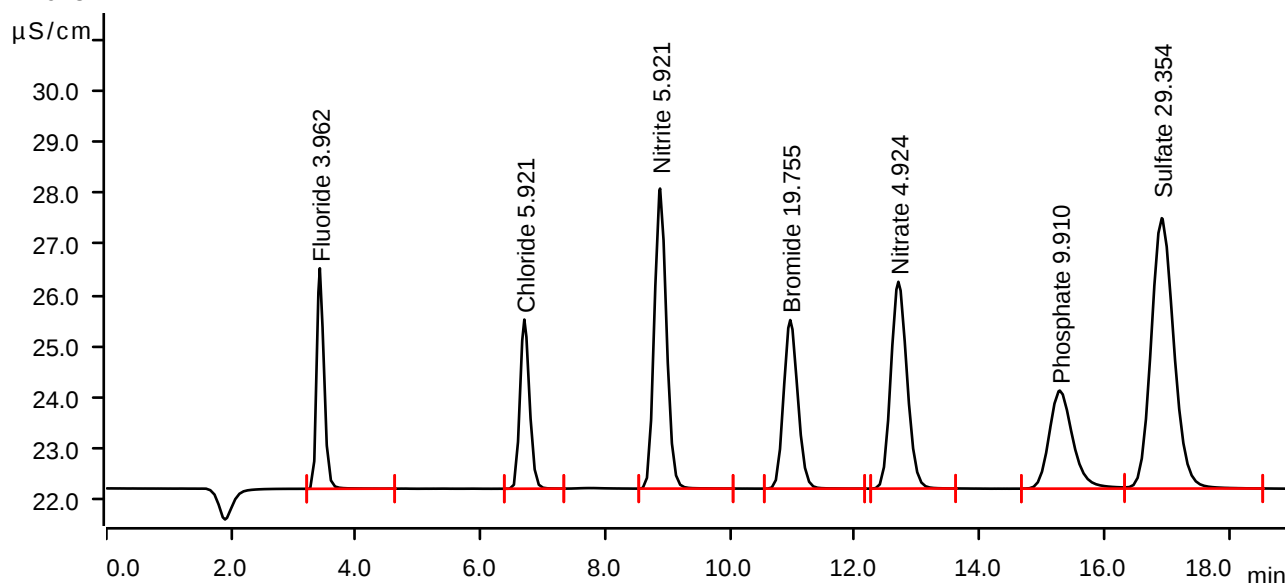

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.423	0.5779	4.306	3.962	Fluoride
2	6.702	0.5827	3.302	5.921	Chloride
3	8.878	1.3268	5.858	5.921	Nitrite
4	10.965	0.8678	3.292	19.755	Bromide
5	12.698	1.2148	4.037	4.924	Nitrate
6	15.287	0.8428	1.914	9.910	Phosphate
7	16.922	2.2329	5.279	29.354	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2024-09-16 13:47:53 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

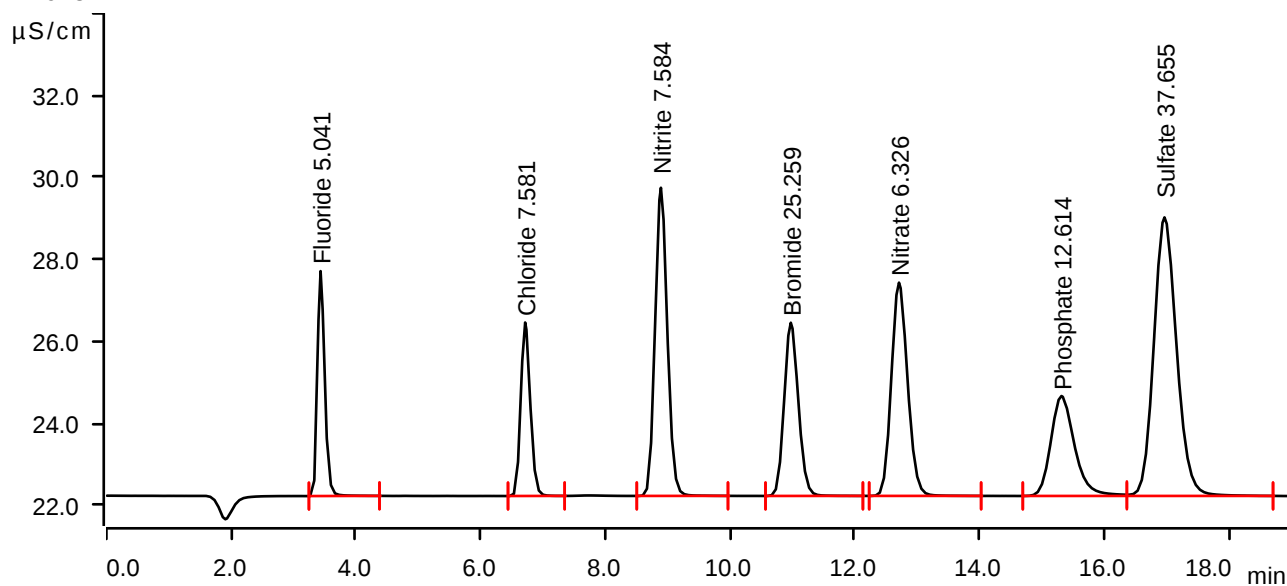

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.435	0.7368	5.489	5.041	Fluoride
2	6.715	0.7473	4.234	7.581	Chloride
3	8.892	1.7044	7.521	7.584	Nitrite
4	10.973	1.1119	4.227	25.259	Bromide
5	12.708	1.5645	5.205	6.326	Nitrate
6	15.313	1.0755	2.439	12.614	Phosphate
7	16.965	2.8736	6.798	37.655	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2024-09-16 15:00:21 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

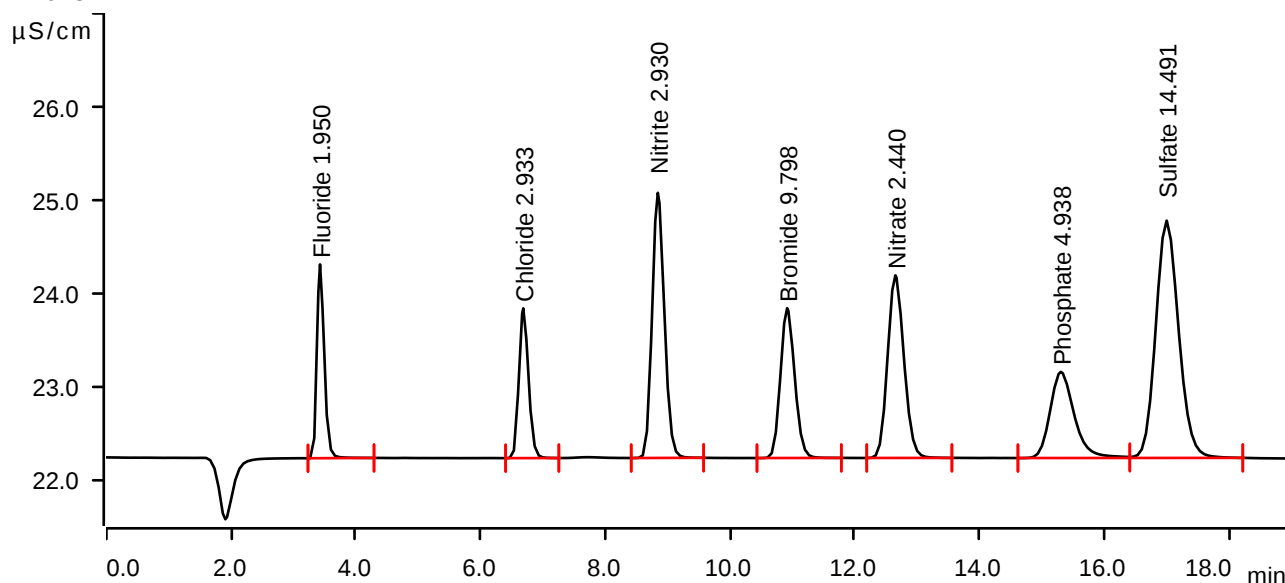

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.427	0.2818	2.081	1.950	Fluoride
2	6.685	0.2862	1.608	2.933	Chloride
3	8.842	0.6478	2.847	2.930	Nitrite
4	10.915	0.4262	1.608	9.798	Bromide
5	12.650	0.5947	1.960	2.440	Nitrate
6	15.303	0.4147	0.925	4.938	Phosphate
7	16.998	1.0857	2.548	14.491	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2024-09-16 15:21:50 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

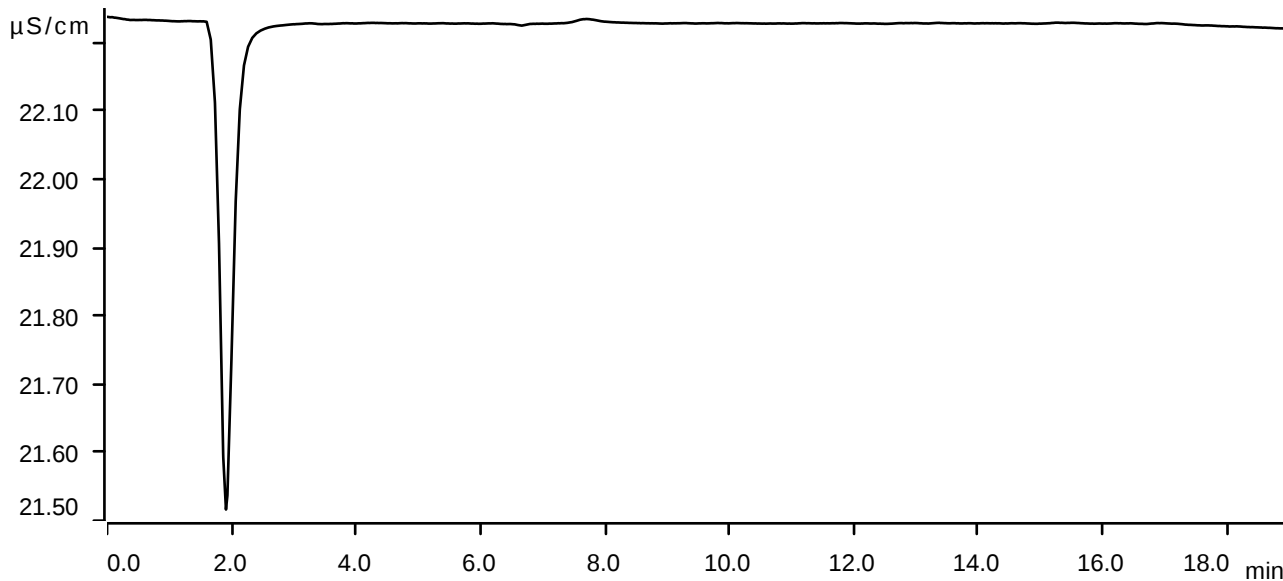


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-10-14 17:12:24 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

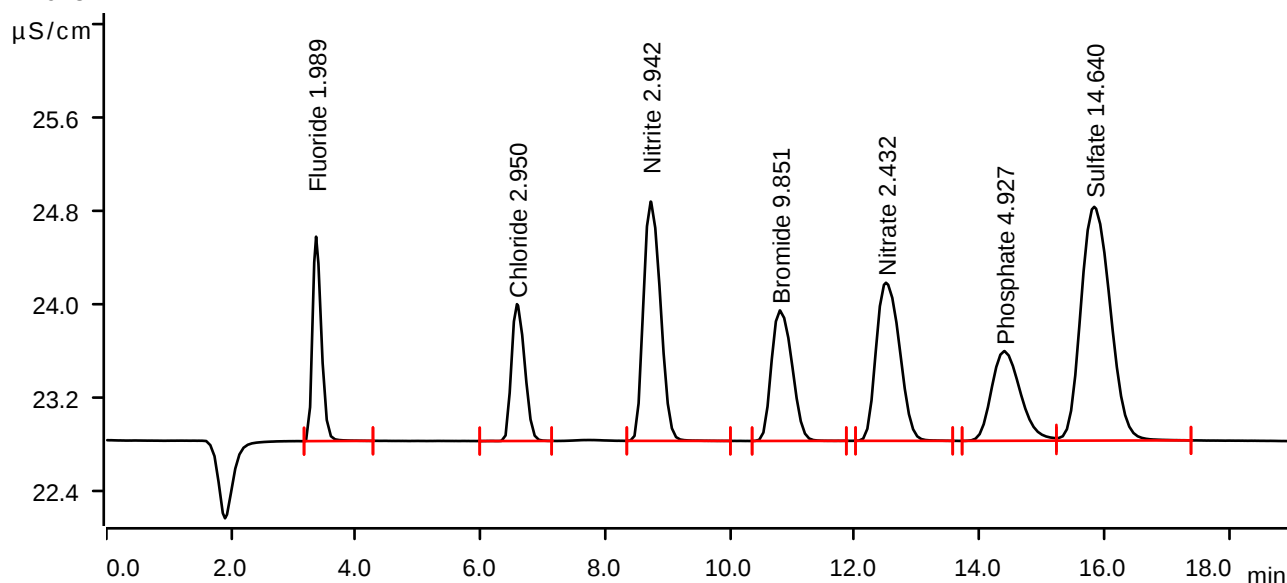


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.363	0.2875	1.756	1.989	Fluoride
2	6.583	0.2880	1.176	2.950	Chloride
3	8.727	0.6506	2.056	2.942	Nitrite
4	10.798	0.4286	1.121	9.851	Bromide
5	12.500	0.5928	1.358	2.432	Nitrate
6	14.395	0.4138	0.771	4.927	Phosphate
7	15.838	1.0972	2.008	14.640	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2024-10-14 17:33:54 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

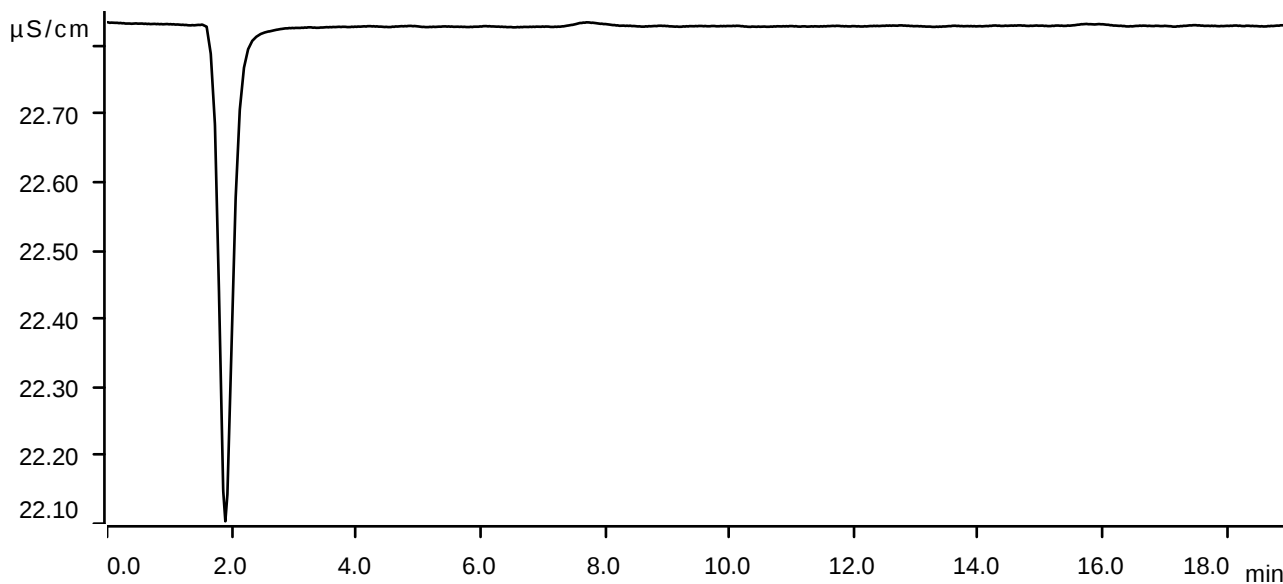Anions


Sample data

Ident LB132938BLW
Sample type Sample
Determination start 2024-10-14 17:55:24 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

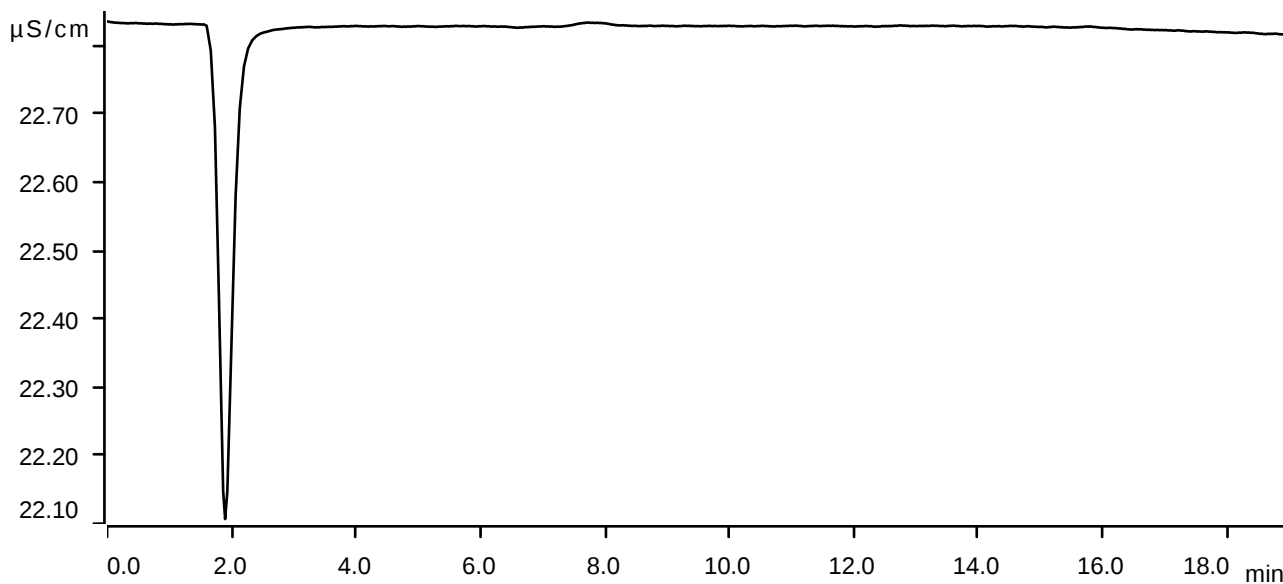


Sample data

Ident LB132938BSW
Sample type Check standard 1
Determination start 2024-10-14 18:16:55 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

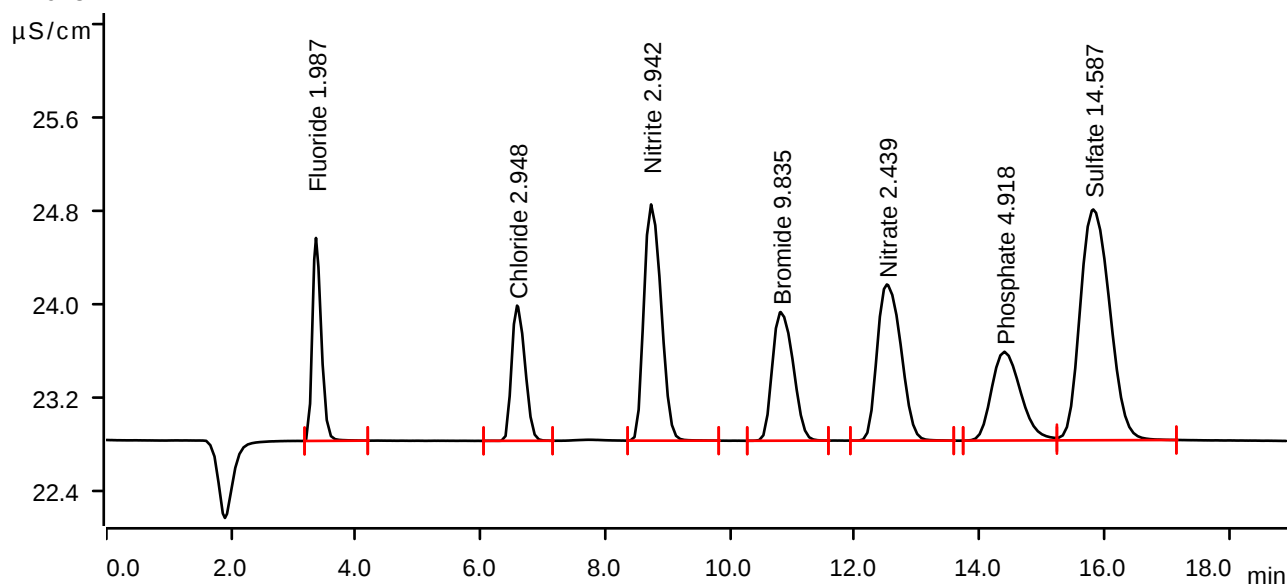

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.362	0.2873	1.743	1.987	Fluoride
2	6.585	0.2878	1.161	2.948	Chloride
3	8.733	0.6505	2.029	2.942	Nitrite
4	10.812	0.4279	1.105	9.835	Bromide
5	12.513	0.5945	1.341	2.439	Nitrate
6	14.398	0.4130	0.762	4.918	Phosphate
7	15.823	1.0930	1.982	14.587	Sulfate


Sample data

Ident P4368-09
Sample type Sample
Determination start 2024-10-14 18:38:28 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

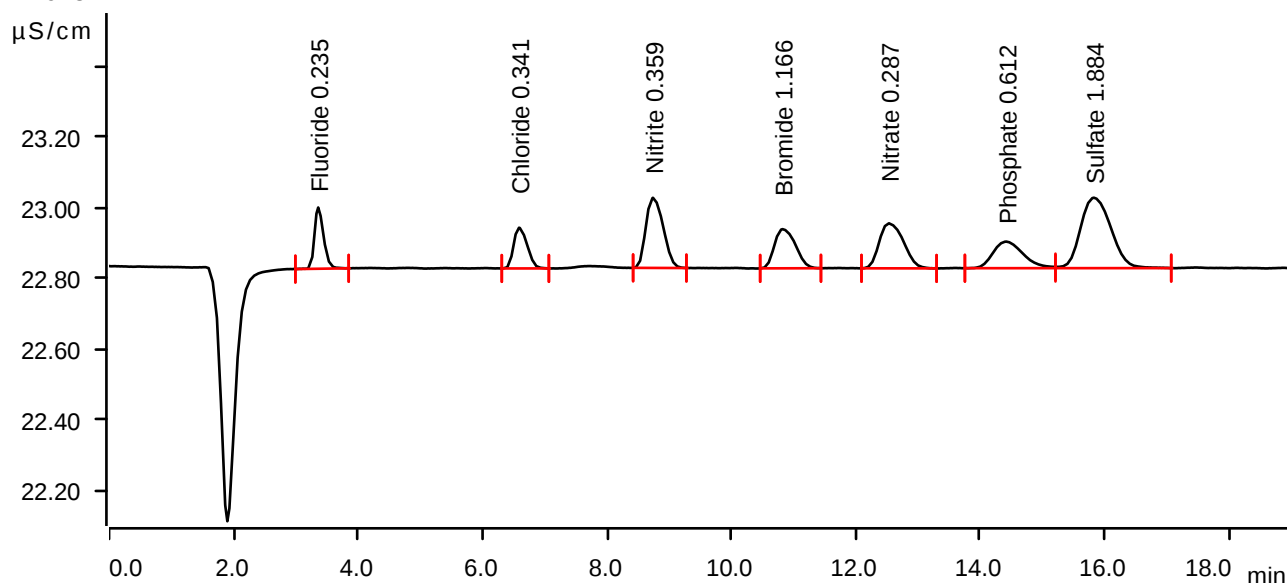

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.362	0.0294	0.173	0.235	Fluoride
2	6.588	0.0291	0.115	0.341	Chloride
3	8.742	0.0643	0.198	0.359	Nitrite
4	10.823	0.0434	0.111	1.166	Bromide
5	12.532	0.0576	0.127	0.287	Nitrate
6	14.420	0.0422	0.075	0.612	Phosphate
7	15.827	0.1125	0.199	1.884	Sulfate


Sample data

Ident P4368-09RE
Sample type Sample
Determination start 2024-10-14 19:00:00 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

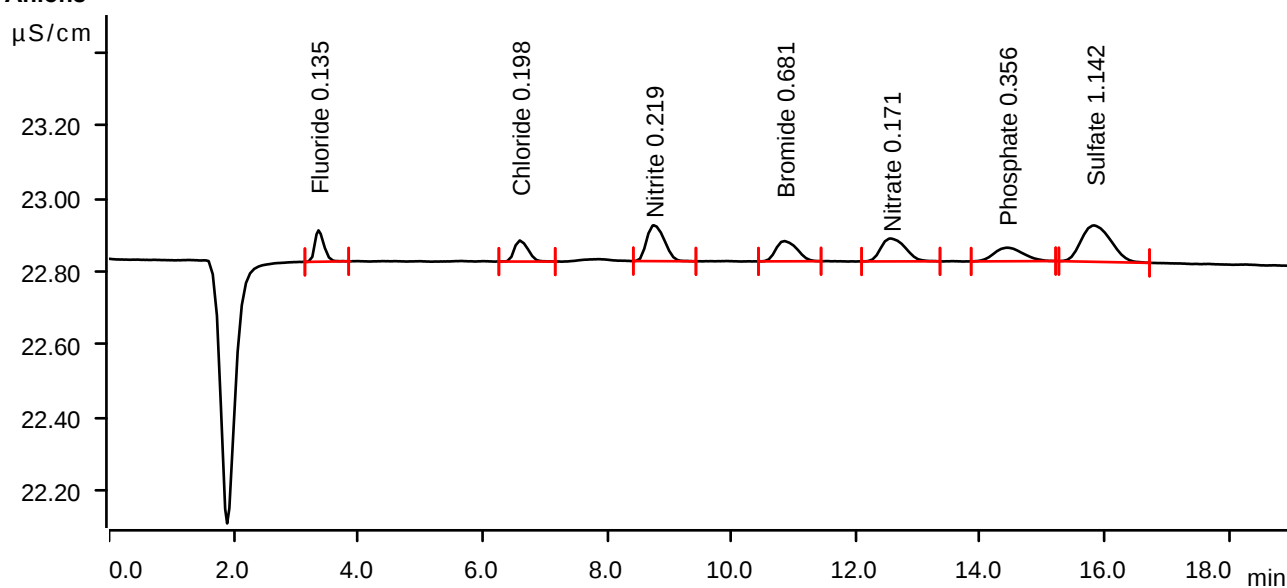

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.367	0.0146	0.086	0.135	Fluoride
2	6.600	0.0149	0.058	0.198	Chloride
3	8.750	0.0324	0.098	0.219	Nitrite
4	10.855	0.0219	0.055	0.681	Bromide
5	12.563	0.0286	0.063	0.171	Nitrate
6	14.428	0.0202	0.037	0.356	Phosphate
7	15.832	0.0553	0.099	1.142	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-10-14 19:21:34 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.56 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

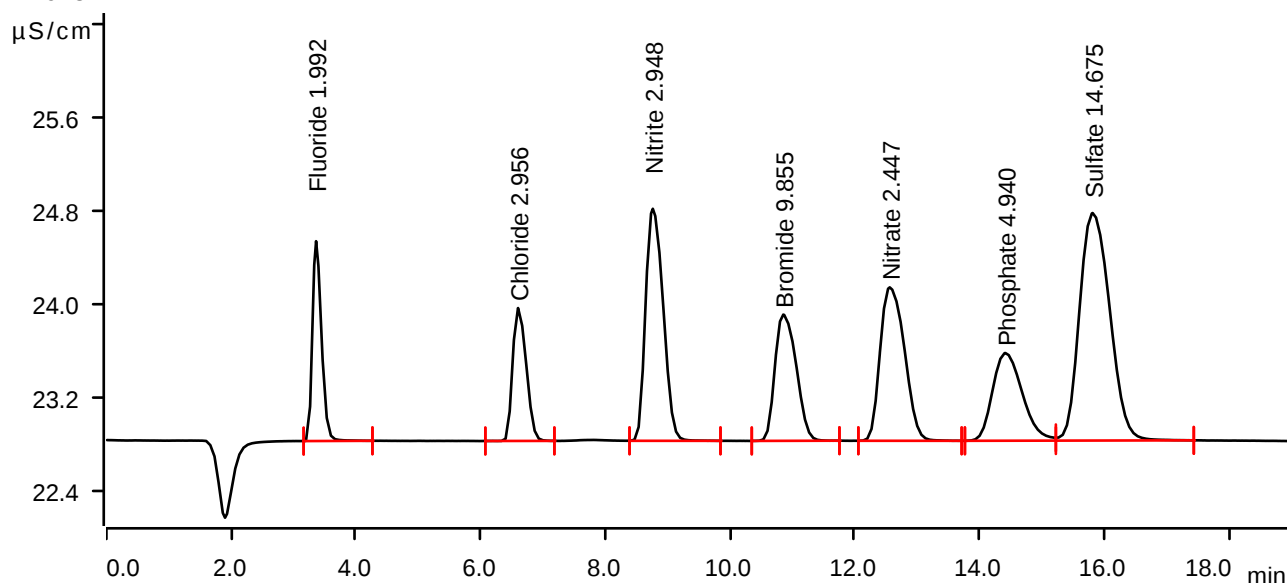

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.363	0.2880	1.717	1.992	Fluoride
2	6.602	0.2885	1.141	2.956	Chloride
3	8.762	0.6520	1.993	2.948	Nitrite
4	10.853	0.4287	1.084	9.855	Bromide
5	12.560	0.5966	1.318	2.447	Nitrate
6	14.413	0.4149	0.753	4.940	Phosphate
7	15.813	1.0998	1.954	14.675	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2024-10-14 19:43:04 UTC-4
Method IC1-091624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

