


LB132994

SFAM01.1

INSTRUMENT ID: CV1

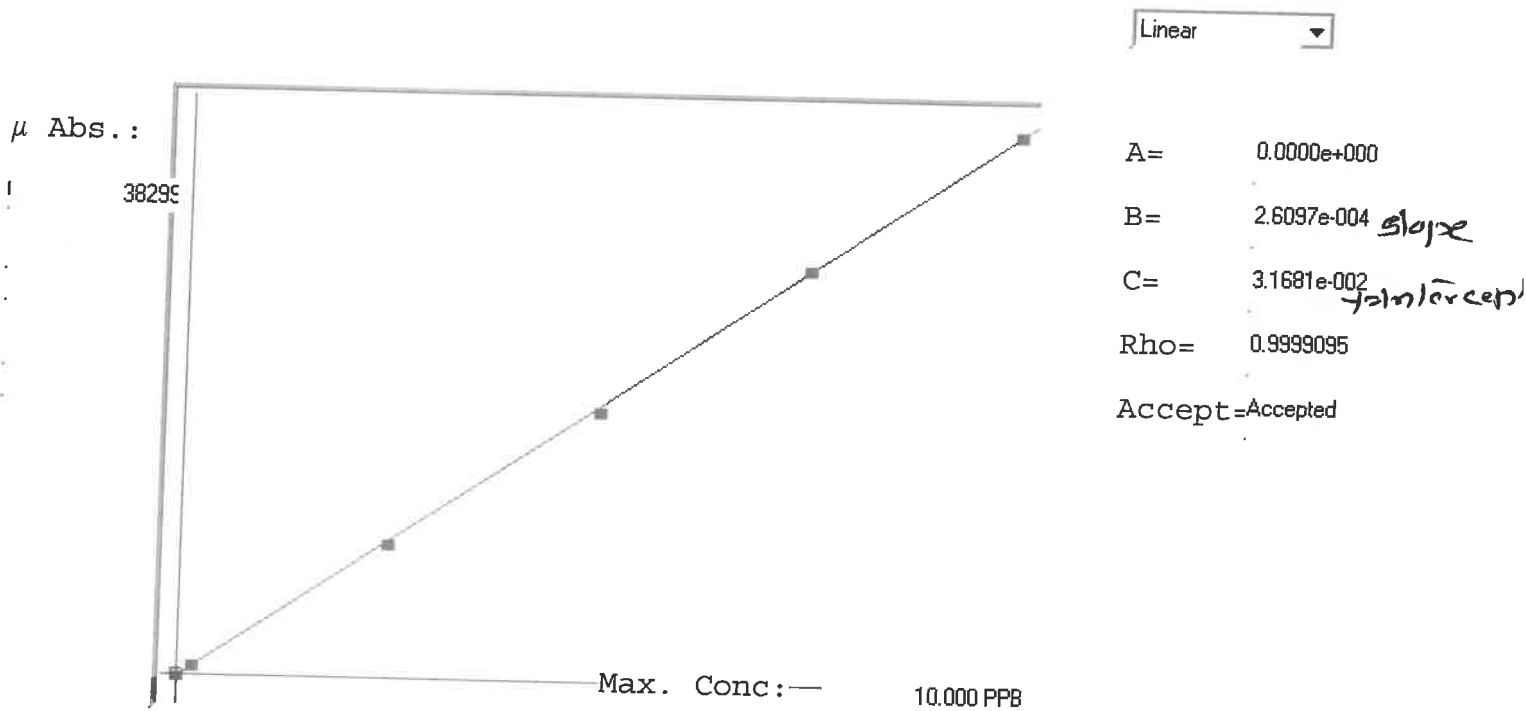

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	g.d.
0.00	0.000	0.037	0.037	19	0.000	19					
0.05	0.050					442					
0.20	0.200	0.234	0.034	775	0.0 %	775	0				
2.50	2.500	2.458	-0.042	9296	0.0 %	9296					
5.00	5.000	4.908	-0.092	18686	0.0 %	18686					
7.50	7.500	7.537	0.037	28759	0.0 %	28759					
10.0	10.000	10.027	0.027	38299	0.0 %	38299					

LB132994

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Stnd Conc	Method	Units	Date	Type
	0 S0	19	-		0 SFAM01.1	PPB	10/18/2024 9:42	Std
	0.2 S01	775	-		0.2 SFAM01.1	PPB	10/18/2024 9:44	Std
	2.5 S02	9296	-		2.5 SFAM01.1	PPB	10/18/2024 9:46	Std
	5 S03	18686	-		5 SFAM01.1	PPB	10/18/2024 9:49	Std
	7.5 S04	28759	-		7.5 SFAM01.1	PPB	10/18/2024 9:51	Std
	10 S05	38299	-		10 SFAM01.1	PPB	10/18/2024 9:56	Std
ICV042	ICV042	15363	4.041 -		SFAM01.1	PPB	10/18/2024 9:59	SMPL
ICB042	ICB042	-54	0.0176 -		SFAM01.1	PPB	10/18/2024 10:04	SMPL
CCV037	CCV037	19597	5.1459 -		SFAM01.1	PPB	10/18/2024 10:06	SMPL
CCB037	CCB037	-55	0.0173 -		SFAM01.1	PPB	10/18/2024 10:14	SMPL
P3391-01	MDL-WATER	65	0.0486 -		SFAM01.1	PPB	10/18/2024 10:25	SMPL
PB164245BL	PBW245	-45	0.0199 -		SFAM01.1	PPB	10/18/2024 10:27	SMPL
CCV038	CCV038	19226	5.0491 -		SFAM01.1	PPB	10/18/2024 10:30	SMPL
CCB038	CCB038	-85	0.0095 -		SFAM01.1	PPB	10/18/2024 10:35	SMPL