


L913362-6

7470A

INSTRUMENT ID: CV1

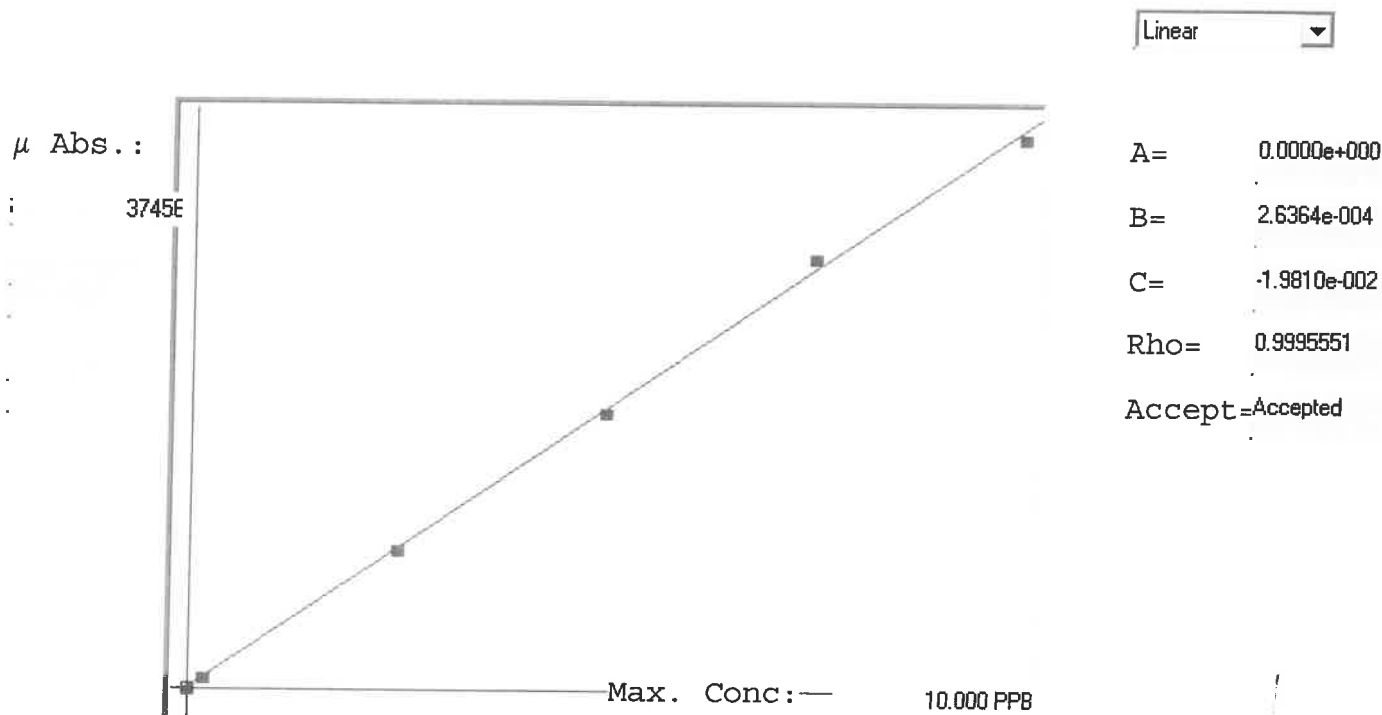

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	Std
0.0	0.000	0.001	0.001	79	0.000	79	0				60
0.2	0.200	0.186	-0.014	781	0.0 %	781					7
2.5	2.500	2.485	-0.015	9501	0.0 %	9501					1
5.0	5.000	4.952	-0.048	18857	0.0 %	18857					1
7.5	7.500	7.721	0.221	29362	0.0 %	29362					3
10.0	10.000	9.855	-0.145	37456	0.0 %	37456					1

LB133026 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 21 Oct 2024 11:15:52

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	79	-	0.0000	7470A	PPB	21 Oct 2024 11:52:43	S	Std
0.2 - 1	50.2	781	-	0.2000	7470A	PPB	21 Oct 2024 11:55:00	S	Std
2.5 - 1	52.5	9501	-	2.5000	7470A	PPB	21 Oct 2024 11:57:17	S	Std
5.0 - 1	55	18857	-	5.0000	7470A	PPB	21 Oct 2024 11:59:34	S	Std
7.5 - 1	57.5	29362	-	7.5000	7470A	PPB	21 Oct 2024 12:01:50	S	Std
10.0 - 1	510	37456	-	10.0000	7470A	PPB	21 Oct 2024 12:04:07	S	Std
ICV45 - 1	ICV45	16274	4.2707	-	7470A	PPB	21 Oct 2024 12:07:09	U	SMPL
ICB45 - 1	ICB45	-131	-0.0543	-	7470A	PPB	21 Oct 2024 12:09:24	U	SMPL
CCV45 - 1	CCV45	20038	5.2630	-	7470A	PPB	21 Oct 2024 12:11:41	U	SMPL
CCB45 - 1	CCB45	-144	-0.0578	-	7470A	PPB	21 Oct 2024 12:13:56	U	SMPL
CRA - 1	CRA	779	0.1856	-	7470A	PPB	21 Oct 2024 12:16:13	U	SMPL
HighStd - 1	HighStd	39293	10.3394	-	7470A	PPB	21 Oct 2024 12:18:27	U	SMPL
PB164290BL - 1	PBW	-65	-0.0369	-	7470A	PPB	21 Oct 2024 12:23:01	U	SMPL
PB164290BS - 1	LCSW	17820	4.6782	-	7470A	PPB	21 Oct 2024 12:25:16	U	SMPL
P4417-03 - 1	HOPPER-A-SOLID	2840	0.7289	-	7470A	PPB	21 Oct 2024 12:27:33	U	SMPL
P4417-06 - 1	HOPPER-B-SOLID	462	0.1020	-	7470A	PPB	21 Oct 2024 12:29:50	U	SMPL
P4417-09 - 1	HOPPER-C-SOLID	873	0.2103	-	7470A	PPB	21 Oct 2024 12:32:10	U	SMPL
P4419-04 - 1	IB-1	80	0.0013	-	7470A	PPB	21 Oct 2024 12:34:28	U	SMPL
P4425-02 - 1	TP-1	17	-0.0153	-	7470A	PPB	21 Oct 2024 12:36:44	U	SMPL
CCV46 - 1	CCV46	20467	5.3761	-	7470A	PPB	21 Oct 2024 12:38:59	U	SMPL
CCB46 - 1	CCB46	-144	-0.0578	-	7470A	PPB	21 Oct 2024 12:41:14	U	SMPL
P4425-04 - 1	TP-2	26	-0.0130	-	7470A	PPB	21 Oct 2024 12:43:31	U	SMPL
P4425-06 - 1	TP-3	30	-0.0119	-	7470A	PPB	21 Oct 2024 12:45:46	U	SMPL
P4425-08 - 1	TP-4	56	-0.0050	-	7470A	PPB	21 Oct 2024 12:48:02	U	SMPL
P4425-10 - 1	TP-5	52	-0.0061	-	7470A	PPB	21 Oct 2024 12:50:17	U	SMPL
P4430-01 - 1	VNJ-209	269	0.0511	-	7470A	PPB	21 Oct 2024 12:52:33	U	SMPL
P4430-01DUP - 1	VNJ-209DUP	66	-0.0024	-	7470A	PPB	21 Oct 2024 12:54:50	U	SMPL
P4430-01MS - 1	VNJ-209MS	16998	4.4615	-	7470A	PPB	21 Oct 2024 13:01:34	U	SMPL
P4430-01MSD - 1	VNJ-209MSD	17190	4.5121	-	7470A	PPB	21 Oct 2024 13:03:51	U	SMPL
PB164291BL - 1	PBW	-200	-0.0725	-	7470A	PPB	21 Oct 2024 13:06:09	U	SMPL
PB164291BS - 1	LCSW	15281	4.0089	-	7470A	PPB	21 Oct 2024 13:11:09	U	SMPL
CCV47 - 1	CCV47	20288	5.3289	-	7470A	PPB	21 Oct 2024 13:13:24	U	SMPL
CCB47 - 1	CCB47	-194	-0.0710	-	7470A	PPB	21 Oct 2024 13:15:41	U	SMPL
P4417-11 - 1	HOPPER-A-WATER	19	-0.0148	-	7470A	PPB	21 Oct 2024 13:17:59	U	SMPL
P4417-13 - 1	HOPPER-B-WATER	10	-0.0172	-	7470A	PPB	21 Oct 2024 13:20:14	U	SMPL
P4417-13DUP - 1	HOPPER-B-WATERDUP	-12	-0.0230	-	7470A	PPB	21 Oct 2024 13:22:30	U	SMPL
P4417-13MS - 1	HOPPER-B-WATERMS	15165	3.9783	-	7470A	PPB	21 Oct 2024 13:27:28	U	SMPL
P4417-13MSD - 1	HOPPER-B-WATERMSD	12392	3.2472	-	7470A	PPB	21 Oct 2024 13:29:44	U	SMPL
PB164195TB - 1	PB164195TB	-158	-0.0615	-	7470A	PPB	21 Oct 2024 13:32:01	U	SMPL
PB164197TB - 1	PB164197TB	-23	-0.0259	-	7470A	PPB	21 Oct 2024 13:34:19	U	SMPL
CCV48 - 1	CCV48	17615	4.6242	-	7470A	PPB	21 Oct 2024 13:36:36	U	SMPL
CCB48 - 1	CCB48	-134	-0.0551	-	7470A	PPB	21 Oct 2024 13:38:53	U	SMPL
P4430-01LX5 - 1		-15	-0.0238	-	7470A	PPB	21 Oct 2024 13:41:10	U	SMPL
P4430-01A - 1		16696	4.3819	-	7470A	PPB	21 Oct 2024 13:43:25	U	SMPL
P4417-13LX5 - 1		-172	-0.0652	-	7470A	PPB	21 Oct 2024 13:45:41	U	SMPL
P4417-13A - 1		16836	4.4188	-	7470A	PPB	21 Oct 2024 13:47:58	U	SMPL
CHK STD - 1	CHK STD	27099	7.1246	-	7470A	PPB	21 Oct 2024 13:50:13	U	SMPL
CCV49 - 1	CCV49	20241	5.3165	-	7470A	PPB	21 Oct 2024 13:55:06	U	SMPL
CCB49 - 1	CCB49	-234	-0.0815	-	7470A	PPB	21 Oct 2024 13:57:22	U	SMPL