


LB13303)

SFAM01.1

INSTRUMENT ID: CV1

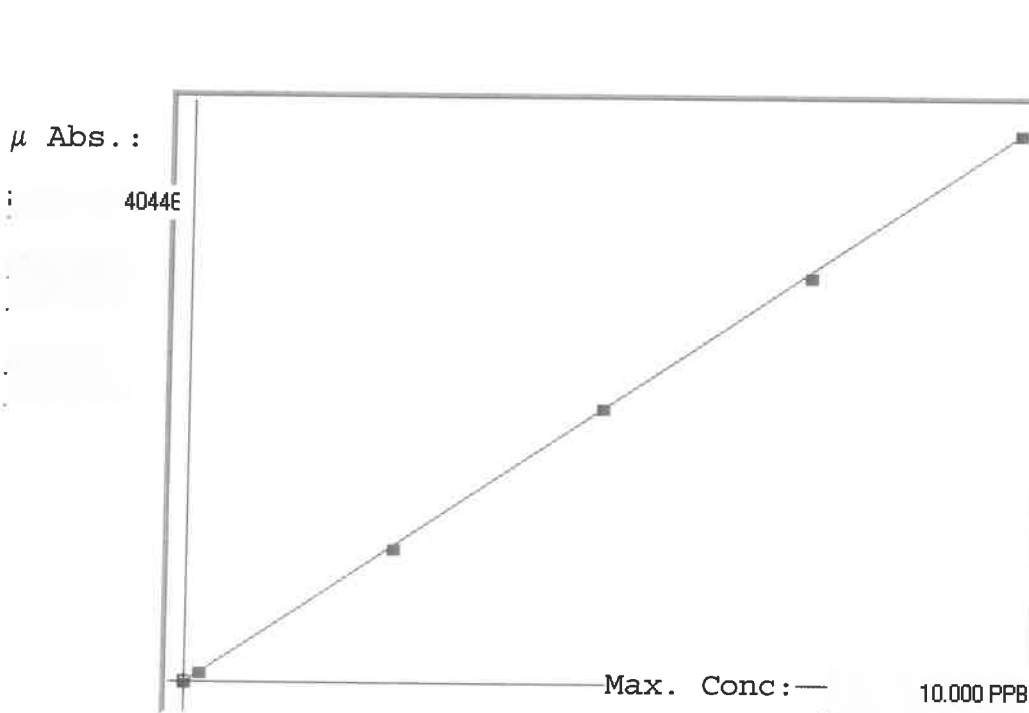

Linear

A= 0.0000e+000

B= 2.4799e-004 slope

C= 1.2468e-002 y-intercept

Rho= 0.9999336

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/00
0.00	0.000	0.003	0.003	-39	0.000	-39					
0.05	0.050										
0.20	0.200	0.213	0.013	809	0.0 %	809					
2.50	2.500	2.478	-0.022	9943	0.0 %	9943					
5.00	5.000	5.044	0.044	20289	0.0 %	20289					
7.50	7.500	7.420	-0.080	29869	0.0 %	29869					
10.0	10.000	10.043	0.043	40446	0.0 %	40446					

LB133031

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	-39	-		0 SFAM01.1	PPB	10/21/2024 15:34	Std
	0.2 S01	809	-		0.2 SFAM01.1	PPB	10/21/2024 15:37	Std
	2.5 S02	9943	-		2.5 SFAM01.1	PPB	10/21/2024 15:39	Std
	5 S03	20289	-		5 SFAM01.1	PPB	10/21/2024 15:41	Std
	7.5 S04	29869	-		7.5 SFAM01.1	PPB	10/21/2024 15:44	Std
	10 S05	40446	-		10 SFAM01.1	PPB	10/21/2024 15:46	Std
ICV046	ICV046	16281	4.0499 -		SFAM01.1	PPB	10/21/2024 15:49	SMPL
ICB046	ICB046	-40	0.0025 -		SFAM01.1	PPB	10/21/2024 16:02	SMPL
CCV050	CCV050	20627	5.1277 -		SFAM01.1	PPB	10/21/2024 16:04	SMPL
CCB050	CCB050	-36	0.0035 -		SFAM01.1	PPB	10/21/2024 16:09	SMPL
PB164305BL	PBW305	29	0.0197 -		SFAM01.1	PPB	10/21/2024 16:11	SMPL
P3391-02	MDL-WATER	137	0.0464 -		SFAM01.1	PPB	10/21/2024 16:13	SMPL
CCV051	CCV051	20642	5.1314 -		SFAM01.1	PPB	10/21/2024 16:15	SMPL
CCB051	CCB051	17	0.0167 -		SFAM01.1	PPB	10/21/2024 16:20	SMPL