


LB133160

7471B

INSTRUMENT MD: CV1

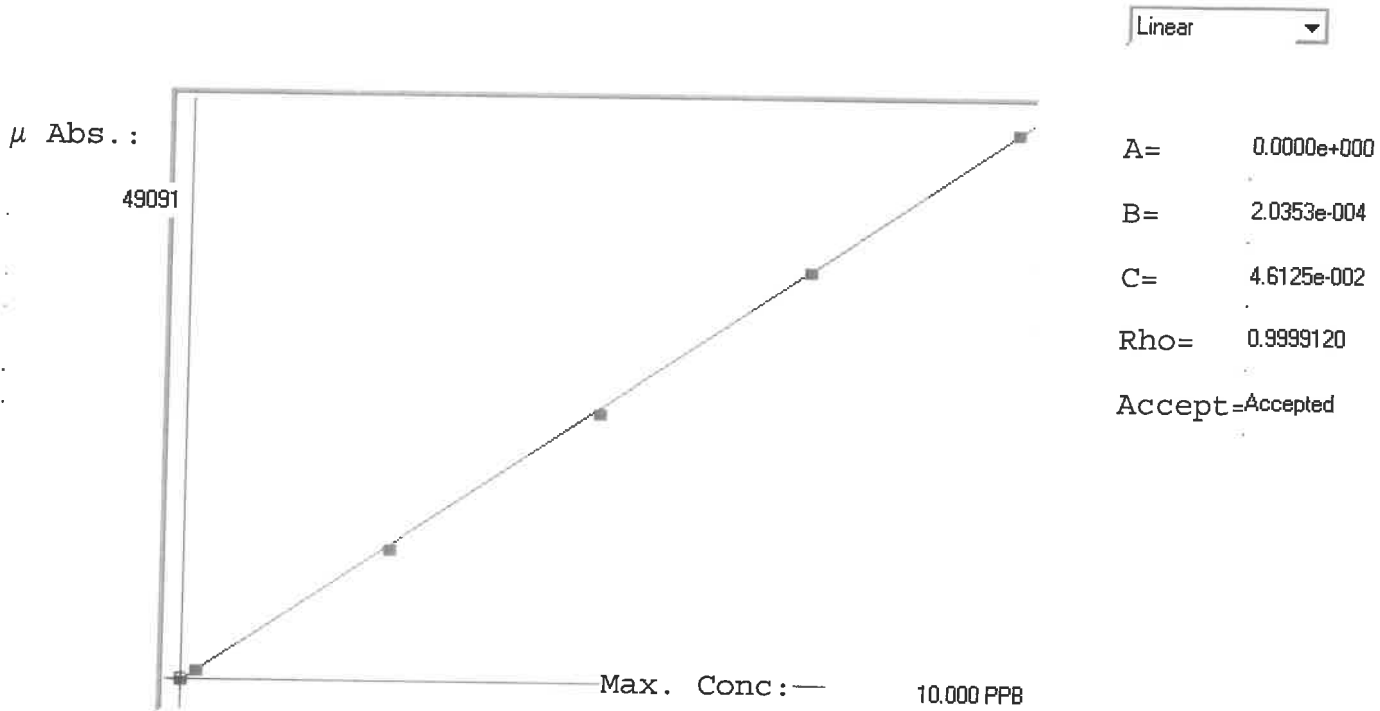

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.049	0.049	14	0.000	14					0
0.2	0.200	0.233	0.033	916	0.0 %	916					17
2.5	2.500	2.437	-0.063	11747	0.0 %	11747					3
5.0	5.000	4.927	-0.073	23983	0.0 %	23983					1
7.5	7.500	7.516	0.016	36702	0.0 %	36702					0
10.0	10.000	10.038	0.038	49091	0.0 %	49091					0

LB133160 INSTRUMENT ID : CV21

Method: 7471B

Operator: Admin

Date of Analysis: 28 Oct 2024 08:06:46

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SP	14	-	0.0000	7471B	PPB	28 Oct 2024 08:44:21	S	Std
0.2 - 1	SP 2	916	-	0.2000	7471B	PPB	28 Oct 2024 08:46:38	S	Std
2.5 - 1	SP 2.5	11747	-	2.5000	7471B	PPB	28 Oct 2024 08:48:55	S	Std
5.0 - 1	SP 5	23983	-	5.0000	7471B	PPB	28 Oct 2024 08:51:12	S	Std
7.5 - 1	SP 7.5	36702	-	7.5000	7471B	PPB	28 Oct 2024 08:53:31	S	Std
10.0 - 1	SP 10	49091	-	10.0000	7471B	PPB	28 Oct 2024 08:55:50	S	Std
ICV54 - 1	ICV54	19148	3.9434	-	7471B	PPB	28 Oct 2024 08:58:52	U	SMPL
ICB54 - 1	ICB54	-312	-0.0174	-	7471B	PPB	28 Oct 2024 09:01:06	U	SMPL
CCV76 - 1	CCV76	24284	4.9887	-	7471B	PPB	28 Oct 2024 09:03:24	U	SMPL
CCB76 - 1	CCB76	-326	-0.0202	-	7471B	PPB	28 Oct 2024 09:05:38	U	SMPL
CRA - 1	CRA	889	0.2271	-	7471B	PPB	28 Oct 2024 09:07:56	U	SMPL
HighStd - 1	HighStd	49505	10.1220	-	7471B	PPB	28 Oct 2024 09:10:10	U	SMPL
ChkStd - 1	ChkStd	34208	7.0086	-	7471B	PPB	28 Oct 2024 09:12:25	U	SMPL
PB164429BL - 1	PBS	-122	0.0213	-	7471B	PPB	28 Oct 2024 09:14:47	U	SMPL
PB164429BS - 1	LCSS	16868	3.4793	-	7471B	PPB	28 Oct 2024 09:17:07	U	SMPL
P4531-01 - 1	OR-03-102424	1262	0.3030	-	7471B	PPB	28 Oct 2024 09:19:23	U	SMPL
P4545-01 - 1	VNJ-215	5343	1.1336	-	7471B	PPB	28 Oct 2024 09:21:42	U	SMPL
P4545-01DUP - 1	VNJ-215DUP	4333	0.9280	-	7471B	PPB	28 Oct 2024 09:24:00	U	SMPL
P4545-01MS - 1	VNJ-215MS	23500	4.8292	-	7471B	PPB	28 Oct 2024 09:26:20	U	SMPL
P4545-01MSD - 1	VNJ-215MSD	20716	4.2625	-	7471B	PPB	28 Oct 2024 09:28:37	U	SMPL
CCV77 - 1	CCV77	24141	4.9596	-	7471B	PPB	28 Oct 2024 09:30:58	U	SMPL
CCB77 - 1	CCB77	-305	-0.0160	-	7471B	PPB	28 Oct 2024 09:33:19	U	SMPL
P4547-01 - 1	BP-F-21	299	0.1070	-	7471B	PPB	28 Oct 2024 09:35:37	U	SMPL
P4547-05 - 1	BP-F-20	113	0.0691	-	7471B	PPB	28 Oct 2024 09:37:52	U	SMPL
P4561-01 - 1	BP-F-19	81	0.0626	-	7471B	PPB	28 Oct 2024 09:40:08	U	SMPL
P4561-05 - 1	BP-F-18	534	0.1548	-	7471B	PPB	28 Oct 2024 09:42:23	U	SMPL
P4566-01 - 1	HD-01-102524	1903	0.4334	-	7471B	PPB	28 Oct 2024 09:44:39	U	SMPL
P4567-01 - 1	WC-1	2824	0.6209	-	7471B	PPB	28 Oct 2024 09:46:55	U	SMPL
P4567-05 - 1	WC-2	2864	0.6290	-	7471B	PPB	28 Oct 2024 09:49:12	U	SMPL
P4567-09 - 1	WC-3	3507	0.7599	-	7471B	PPB	28 Oct 2024 09:51:29	U	SMPL
P4545-01LX5 - 1		1113	0.2727	-	7471B	PPB	28 Oct 2024 09:53:47	U	SMPL
P4545-01A - 1		22294	4.5837	-	7471B	PPB	28 Oct 2024 09:56:03	U	SMPL
CCV78 - 1	CCV78	24747	5.0830	-	7471B	PPB	28 Oct 2024 09:58:18	U	SMPL
CCB78 - 1	CCB78	-279	-0.0107	-	7471B	PPB	28 Oct 2024 10:00:37	U	SMPL