

66133212

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

10/30/2024 13:52

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.003	0.0	0.112	
ICB1	-0.005	0.0	0.011	
CCV1	1.002	0.0	0.112	
CCB1	-0.004	0.0	0.011	
PB164502BS	0.993	0.0	0.111	
P4368-03	0.022	0.0	0.014	
PB164504BL	-0.003	0.0	0.012	
PB164504BS	1.005	0.0	0.112	
P4368-09	0.022	0.0	0.014	
PB164502BL	-0.009	0.0	0.011	
CCV2	1.006	0.0	0.112	
CCB2	0.006	0.0	0.012	

N	12
Mean	0.420
SD	0.5138
CV%	122.38

Aquakem v. 7.2AQ1

Results from time period:

Wed Oct 30 12:30:06 2024

Wed Oct 30 13:45:38 2024

Sample Id	Sam/Ctr/c/	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.0092	mg/l	10/30/2024 12:30:06	
0.05PPM	A	Phenolics-	P	0.0497	mg/l	10/30/2024 12:30:07	
0.1PPM	A	Phenolics-	P	0.0996	mg/l	10/30/2024 12:30:08	
0.25PPM	A	Phenolics-	P	0.256	mg/l	10/30/2024 12:30:09	
0.50PPM	A	Phenolics-	P	0.5035	mg/l	10/30/2024 12:30:10	
1.0PPM	A	Phenolics-	P	1.004	mg/l	10/30/2024 12:30:11	
2.0PPM	A	Phenolics-	P	1.9964	mg/l	10/30/2024 12:30:12	
ICV1	S	Phenolics-	P	1.0026	mg/l	10/30/2024 13:18:38	
ICB1	S	Phenolics-	P	-0.0046	mg/l	10/30/2024 13:18:41	
CCV1	S	Phenolics-	P	1.002	mg/l	10/30/2024 13:18:42	
CCB1	S	Phenolics-	P	-0.0043	mg/l	10/30/2024 13:18:44	
PB164502BS	S	Phenolics-	P	0.9934	mg/l	10/30/2024 13:18:48	
P4368-03	S	Phenolics-	P	0.0223	mg/l	10/30/2024 13:28:40	
PB164504BL	S	Phenolics-	P	-0.0035	mg/l	10/30/2024 13:28:43	
PB164504BS	S	Phenolics-	P	1.0052	mg/l	10/30/2024 13:28:45	
P4368-09	S	Phenolics-	P	0.022	mg/l	10/30/2024 13:28:46	
PB164502BL	S	Phenolics-	P	-0.0091	mg/l	10/30/2024 13:45:35	
CCV2	S	Phenolics-	P	1.0056	mg/l	10/30/2024 13:45:37	
CCB2	S	Phenolics-	P	0.0063	mg/l	10/30/2024 13:45:38	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM Instrument ID : Konelab

10/30/2024 12:34


Test Phenolics-

Accepted 10/30/2024 12:34

Factor 10.05
Bias 0.012

Coeff. of det. 0.999949

Errors

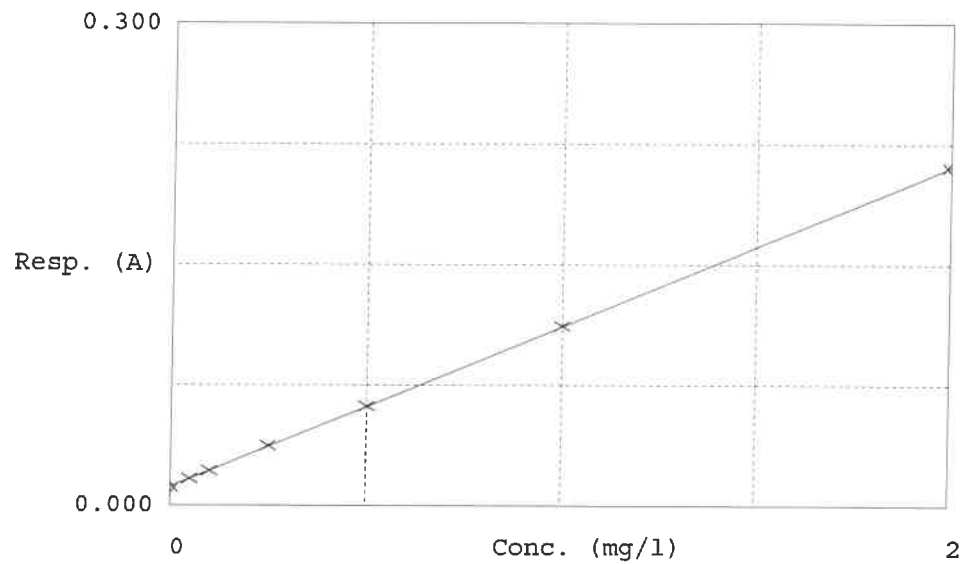

	Calibrator	Response	Calc. con.	Conc.	Re Errors
1	0.00PPM	0.011	-0.0092	0.0000	~
2	Phenol-2	0.017	0.0497	0.0500	-0.6
3	Phenol-2	0.022	0.0996	0.1000	-0.4
4	Phenol-2	0.037	0.2560	0.2500	2.4
5	Phenol-2	0.062	0.5035	0.5000	0.7
6	Phenol-2	0.112	1.0040	1.0000	0.4
7	Phenol-2	0.210	1.9964	2.0000	-0.2

10/30/2024

RM