

LB133307

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : NF Instrument ID : Konelab

11/11/2024 11:16

Test: CNEPA-NEW

Sample Id	Result	Dil. 1 +	Response	Errors
ICV001 ICV001	92.374	0.0	0.085	
ICB001 ICB001	0.361	0.0	0.001	
CCV001 CCV001	241.604	0.0	0.221	
CCB001 CCB001	0.515	0.0	0.001	
P B164689BL PBW689	-0.336	0.0	0.000	
P B164689TB LEB689	0.238	0.0	0.001	
P4623-01 MBH6M7	-0.209	0.0	0.001	
P4623-02 MBH6M8	0.364	0.0	0.001	
P4623-03 MBH6M9	0.453	0.0	0.001	
P4623-04 MBH6N0	0.210	0.0	0.001	
P4623-05 MBH6N1	0.462	0.0	0.001	
P4623-06 MBH6M6	0.456	0.0	0.001	
P4623-07 MBH6N2	-0.553	0.0	0.000	
P4623-08 MBH6N3	0.316	0.0	0.001	
P4623-09 MBH6N4	-0.754	0.0	0.000	
P4623-10 MBH6N5	-1.976	0.0	-0.001	
P4623-11 MBH6N6	-0.466	0.0	0.000	
P4623-12 MBH6N6D	-0.626	0.0	0.000	
P4623-13 MBH6N6S	94.802	0.0	0.087	
P4623-14 MBH6N7	-0.114	0.0	0.001	
CCV002 CCV002	253.680	0.0	0.232	
CCB002 CCB002	-0.090	0.0	0.001	

N	22
Mean	30.941
SD	75.3377
CV%	243.48

NF
11.11.2024 P

Aquakem v. 7.2AQ1

Results from time period:

Mon Nov 11 09:50:10 2024

Mon Nov 11 11:14:00 2024

Sample Id	Sam/Ct	Test short name	Test type	Result	Result unit	Result date and time
S0.0	A	CNEPA-NEW	P	0.0262	µg/l	11/11/2024 10:08:43
S5.0	A	CNEPA-NEW	P	4.256	µg/l	11/11/2024 10:08:44
S10.0	A	CNEPA-NEW	P	10.4544	µg/l	11/11/2024 10:08:45
S100.0	A	CNEPA-NEW	P	97.6177	µg/l	11/11/2024 10:08:46
S250.0	A	CNEPA-NEW	P	254.3418	µg/l	11/11/2024 10:08:47
S500.0	A	CNEPA-NEW	P	498.304	µg/l	11/11/2024 10:08:48
ICV001 ICV001	S	CNEPA-NEW	P	92.3738	µg/l	11/11/2024 10:39:05
ICB001 ICB001	S	CNEPA-NEW	P	0.3612	µg/l	11/11/2024 10:39:06
CCV001 CCV001	S	CNEPA-NEW	P	241.6038	µg/l	11/11/2024 10:39:08
CCB001 CCB001	S	CNEPA-NEW	P	0.5154	µg/l	11/11/2024 10:39:10
PB164689BL PBW689	S	CNEPA-NEW	P	-0.3362	µg/l	11/11/2024 10:39:12
PB164689TB LEB689	S	CNEPA-NEW	P	0.2383	µg/l	11/11/2024 10:39:14
P4623-01 MBH6M7	S	CNEPA-NEW	P	-0.2092	µg/l	11/11/2024 10:46:40
P4623-02 MBH6M8	S	CNEPA-NEW	P	0.3638	µg/l	11/11/2024 10:46:41
P4623-03 MBH6M9	S	CNEPA-NEW	P	0.4528	µg/l	11/11/2024 10:46:42
P4623-04 MBH6N0	S	CNEPA-NEW	P	0.2104	µg/l	11/11/2024 10:46:43
P4623-05 MBH6N1	S	CNEPA-NEW	P	0.4617	µg/l	11/11/2024 10:46:44
P4623-06 MBH6M6	S	CNEPA-NEW	P	0.4559	µg/l	11/11/2024 10:46:45
P4623-07 MBH6N2	S	CNEPA-NEW	P	-0.5525	µg/l	11/11/2024 10:46:46
P4623-08 MBH6N3	S	CNEPA-NEW	P	0.3164	µg/l	11/11/2024 10:46:47
P4623-09 MBH6N4	S	CNEPA-NEW	P	-0.7541	µg/l	11/11/2024 10:46:48
P4623-10 MBH6N5	S	CNEPA-NEW	P	-1.9761	µg/l	11/11/2024 10:46:49
P4623-11 MBH6N6	S	CNEPA-NEW	P	-0.4662	µg/l	11/11/2024 10:52:50
P4623-12 MBH6N6D	S	CNEPA-NEW	P	-0.6259	µg/l	11/11/2024 10:52:51
P4623-13 MBH6N6S	S	CNEPA-NEW	P	94.8024	µg/l	11/11/2024 11:13:57
P4623-14 MBH6N7	S	CNEPA-NEW	P	-0.1141	µg/l	11/11/2024 11:13:58
CCV002 CCV002	S	CNEPA-NEW	P	253.6804	µg/l	11/11/2024 11:13:59
CCB002 CCB002	S	CNEPA-NEW	P	-0.0896	µg/l	11/11/2024 11:14:00

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : NF Instrument ID : Konelab

11/11/2024 10:09

Test CNEPA-NEW


Accepted 11/11/2024 10:09

~~Factor~~ Slope ~~1096~~ 0.000 913
~~Bias~~ Intercept 0.001

NF
11.11.2024

Coeff. of det. 0.999858

Errors

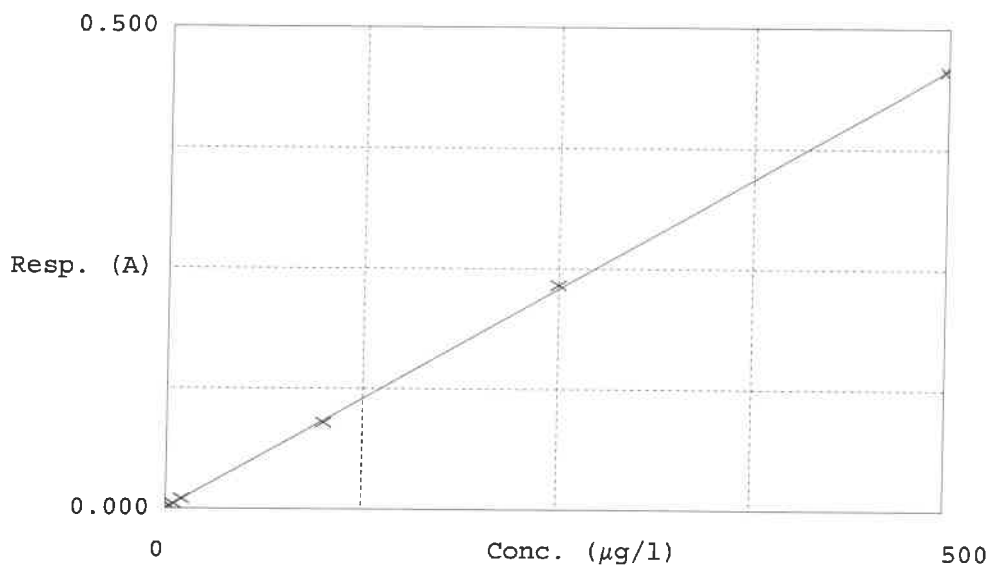

Calibrator	Response	Calc. con.	Conc.	Re Errors	
150.0 0.0PPBCN	0.001	0.0262	0.0000		
255.0 5.0PPBCN	0.005	4.2560	5.0000	-14.9	
3910.0 10PPBCN	0.010	10.4544	10.0000	4.5	
49100.0 100PPBCN	0.090	97.6177	100.0000	-2.4	NF
56250.0 250PPBCN	0.233	254.3418	250.0000	1.7	
65000.0 500PPBCN	0.456	498.3040	500.0000	-0.3	11.11.2024