


LB1933T2

7470A

INSTRUMENT ID: CV1

Linear

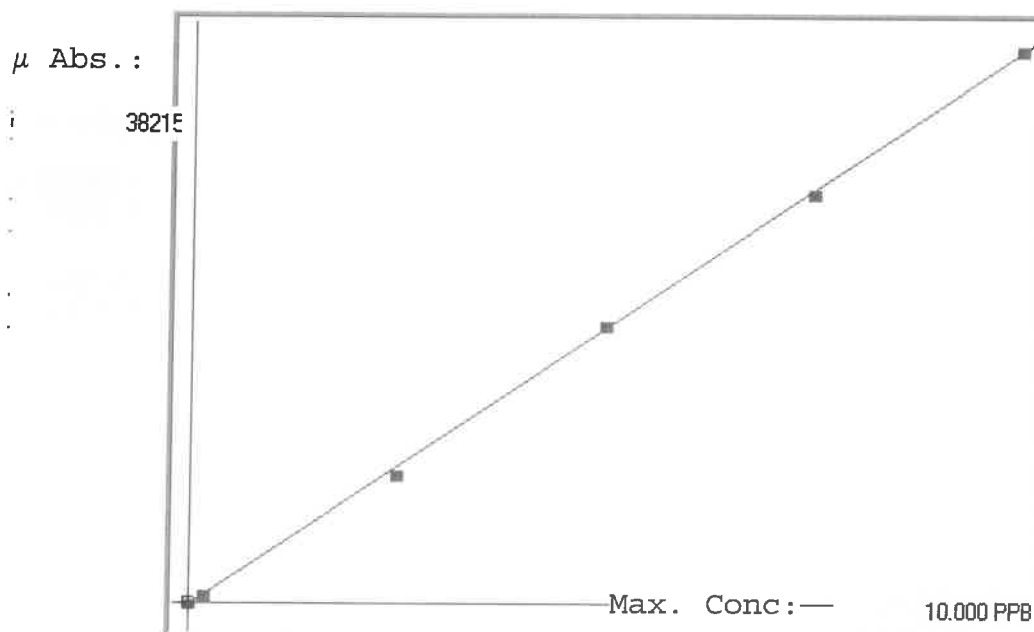

A= 0.0000e+000

B= 2.6139e-004

C= 4.2402e-002

Rho= 0.9998343

Accept=Accepted

| Std ID | Conc.  | Calc.  | Dev.   | Mean  | SD or %RSD | Rep 1 | Rep 2 | Rep 3 | Rep 4 | Rep 5 | %D |
|--------|--------|--------|--------|-------|------------|-------|-------|-------|-------|-------|----|
| 0.0    | 0.000  | 0.067  | 0.067  | 93    | 0.000      | 93    | 0     |       |       |       | 1  |
| 0.2    | 0.200  | 0.203  | 0.003  | 614   | 0.0 %      | 614   |       |       |       |       | 2  |
| 2.5    | 2.500  | 2.382  | -0.118 | 8950  | 0.0 %      | 8950  |       |       |       |       | 5  |
| 5.0    | 5.000  | 5.070  | 0.070  | 19234 | 0.0 %      | 19234 |       |       |       |       | 1  |
| 7.5    | 7.500  | 7.447  | -0.053 | 28329 | 0.0 %      | 28329 |       |       |       |       | 1  |
| 10.0   | 10.000 | 10.031 | 0.031  | 38215 | 0.0 %      | 38215 |       |       |       |       | 0  |

## LB133352 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 08 Nov 2024 09:40:21

| Sample ID       | Extended ID      | µ Abs. | Conc.   | Std Conc | Method | Units | Date                 | Type | Type |
|-----------------|------------------|--------|---------|----------|--------|-------|----------------------|------|------|
| 0.0 - 1         | 50               | 93     | -       | 0.0000   | 7470A  | PPB   | 08 Nov 2024 10:04:53 | S    | Std  |
| 0.2 - 1         | 50.2             | 614    | -       | 0.2000   | 7470A  | PPB   | 08 Nov 2024 10:07:10 | S    | Std  |
| 2.5 - 1         | 52.7             | 8950   | -       | 2.5000   | 7470A  | PPB   | 08 Nov 2024 10:09:27 | S    | Std  |
| 5.0 - 1         | 55               | 19234  | -       | 5.0000   | 7470A  | PPB   | 08 Nov 2024 10:11:43 | S    | Std  |
| 7.5 - 1         | 57.5             | 28329  | -       | 7.5000   | 7470A  | PPB   | 08 Nov 2024 10:13:59 | S    | Std  |
| 10.0 - 1        | 510              | 38215  | -       | 10.0000  | 7470A  | PPB   | 08 Nov 2024 10:16:17 | S    | Std  |
| ICV75 - 1       | ICV75            | 13850  | 3.6626  | -        | 7470A  | PPB   | 08 Nov 2024 10:19:04 | U    | SMPL |
| ICB75 - 1       | ICB75            | -223   | -0.0159 | -        | 7470A  | PPB   | 08 Nov 2024 10:21:18 | U    | SMPL |
| CCV51 - 1       | CCV51            | 19260  | 5.0767  | -        | 7470A  | PPB   | 08 Nov 2024 10:23:35 | U    | SMPL |
| CCB51 - 1       | CCB51            | -209   | -0.0122 | -        | 7470A  | PPB   | 08 Nov 2024 10:25:49 | U    | SMPL |
| CRA - 1         | CRA              | 564    | 0.1898  | -        | 7470A  | PPB   | 08 Nov 2024 10:28:06 | U    | SMPL |
| HighStd - 1     | HighStd          | 36747  | 9.6476  | -        | 7470A  | PPB   | 08 Nov 2024 10:30:21 | U    | SMPL |
| ChkStd - 1      | ChkStd           | 25382  | 6.6770  | -        | 7470A  | PPB   | 08 Nov 2024 10:35:46 | U    | SMPL |
| PB164791BL - 1  | PBW              | -362   | -0.0522 | -        | 7470A  | PPB   | 08 Nov 2024 10:38:01 | U    | SMPL |
| PB164791BS - 1  | LCSW             | 15875  | 4.1919  | -        | 7470A  | PPB   | 08 Nov 2024 10:40:19 | U    | SMPL |
| P4718-03 - 1    | WB-307-SB02      | -255   | -0.0243 | -        | 7470A  | PPB   | 08 Nov 2024 10:42:34 | U    | SMPL |
| P4718-03DUP - 1 | WB-307-SB02DUP   | -92    | 0.0184  | -        | 7470A  | PPB   | 08 Nov 2024 10:44:52 | U    | SMPL |
| P4718-03MS - 1  | WB-307-SB02MS    | 12687  | 3.3586  | -        | 7470A  | PPB   | 08 Nov 2024 10:47:09 | U    | SMPL |
| P4718-03MSD - 1 | WB-307-SB02MSD   | 15411  | 4.0707  | -        | 7470A  | PPB   | 08 Nov 2024 10:49:26 | U    | SMPL |
| P4719-03 - 1    | BAYAVE-STOCKPILE | -195   | -0.0086 | -        | 7470A  | PPB   | 08 Nov 2024 10:51:42 | U    | SMPL |
| CCV52 - 1       | CCV52            | 18837  | 4.9662  | -        | 7470A  | PPB   | 08 Nov 2024 10:53:59 | U    | SMPL |
| CCB52 - 1       | CCB52            | -279   | -0.0305 | -        | 7470A  | PPB   | 08 Nov 2024 10:56:15 | U    | SMPL |
| P4720-05 - 1    | JC-701-COMP-01   | -108   | 0.0142  | -        | 7470A  | PPB   | 08 Nov 2024 10:58:31 | U    | SMPL |
| P4722-04 - 1    | WC-1(0-6)        | -61    | 0.0265  | -        | 7470A  | PPB   | 08 Nov 2024 11:00:46 | U    | SMPL |
| P4722-09 - 1    | WC-2(0-6)        | -98    | 0.0168  | -        | 7470A  | PPB   | 08 Nov 2024 11:03:02 | U    | SMPL |
| P4722-14 - 1    | WC-3(0-6)        | -42    | 0.0314  | -        | 7470A  | PPB   | 08 Nov 2024 11:05:18 | U    | SMPL |
| P4732-02 - 1    | PPE-COMP         | 94     | 0.0670  | -        | 7470A  | PPB   | 08 Nov 2024 11:07:33 | U    | SMPL |
| P4738-02 - 1    | 72-12018         | -10    | 0.0398  | -        | 7470A  | PPB   | 08 Nov 2024 11:09:50 | U    | SMPL |
| P4739-04 - 1    | TP-14            | 65     | 0.0594  | -        | 7470A  | PPB   | 08 Nov 2024 11:12:06 | U    | SMPL |
| P4739-08 - 1    | BP-G2            | 157    | 0.0834  | -        | 7470A  | PPB   | 08 Nov 2024 11:14:23 | U    | SMPL |
| P4739-12 - 1    | BP-B2            | -254   | -0.0240 | -        | 7470A  | PPB   | 08 Nov 2024 11:16:40 | U    | SMPL |
| P4739-16 - 1    | TP-11            | 9      | 0.0448  | -        | 7470A  | PPB   | 08 Nov 2024 11:18:57 | U    | SMPL |
| CCV53 - 1       | CCV53            | 17701  | 4.6692  | -        | 7470A  | PPB   | 08 Nov 2024 11:21:12 | U    | SMPL |
| CCB53 - 1       | CCB53            | -253   | -0.0237 | -        | 7470A  | PPB   | 08 Nov 2024 11:23:27 | U    | SMPL |
| PB164694TB - 1  | PB164694TB       | -114   | 0.0126  | -        | 7470A  | PPB   | 08 Nov 2024 11:25:44 | U    | SMPL |
| P4718-03LX5 - 1 |                  | -90    | 0.0189  | -        | 7470A  | PPB   | 08 Nov 2024 11:28:00 | U    | SMPL |
| P4718-03A - 1   |                  | 14079  | 3.7225  | -        | 7470A  | PPB   | 08 Nov 2024 11:30:15 | U    | SMPL |
| CCV54 - 1       | CCV54            | 17291  | 4.5621  | -        | 7470A  | PPB   | 08 Nov 2024 11:32:30 | U    | SMPL |
| CCB54 - 1       | CCB54            | -218   | -0.0146 | -        | 7470A  | PPB   | 08 Nov 2024 11:34:48 | U    | SMPL |