


Clear table

Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A

ident	concentratio tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio n HPO4	concentratio on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-101624	10/16/2024 10:55	10	NF/IZ
STD2	0.424	0.632	0.639	2.106	0.535	1.072	3.276	IC1-101624	10/16/2024 11:17	10	NF/IZ
STD3	0.796	1.206	1.205	4.013	1.000	2.000	6.052	IC1-101624	10/16/2024 11:38	10	NF/IZ
STD4	1.032	1.537	1.531	5.116	1.277	2.557	7.662	IC1-101624	10/16/2024 11:59	10	NF/IZ
STD5	1.966	2.927	2.921	9.77	2.439	4.871	14.51	IC1-101624	10/16/2024 12:21	10	NF/IZ
STD6	3.88	5.901	5.91	19.683	4.912	9.831	29.286	IC1-101624	10/16/2024 12:42	10	NF/IZ
STD7	5.102	7.598	7.593	25.312	6.337	12.67	37.714	IC1-101624	10/16/2024 13:04	10	NF/IZ
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4				
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000				
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000				
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000				
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000				
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000				
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000				
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000				
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4				
STD1											
STD2	6.0000	5.3333	6.5000	5.3000	7.0000	7.2000	9.2000				
STD3	-0.5000	0.5000	0.4167	0.3250	0.0000	0.0000	0.8667				
STD4	3.2000	2.4667	2.0667	2.3200	2.1600	2.2800	2.1600				
STD5	-1.7000	-2.4333	-2.6333	-2.3000	-2.4400	-2.5800	-3.2667				
STD6	-3.0000	-1.6500	-1.5000	-1.5850	-1.7600	-1.6900	-2.3800				
STD7	2.0400	1.3067	1.2400	1.2480	1.3920	1.3600	1.9297				

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

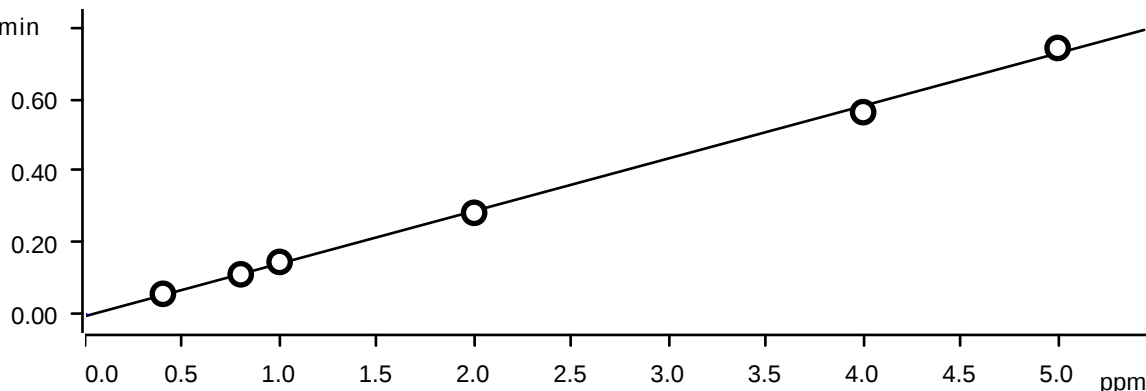

Function: $A = -5.06114\text{E-}3 + 0.0146570 \times Q$


Relative standard deviation 3.824450 %

Correlation coefficient 0.999229

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-10-16 10:55:46 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.057	STD2	2024-10-16 11:17:08 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.112	STD3	2024-10-16 11:38:32 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.146	STD4	2024-10-16 11:59:57 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.283	STD5	2024-10-16 12:21:22 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.564	STD6	2024-10-16 12:42:48 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.743	STD7	2024-10-16 13:04:15 UTC-4	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

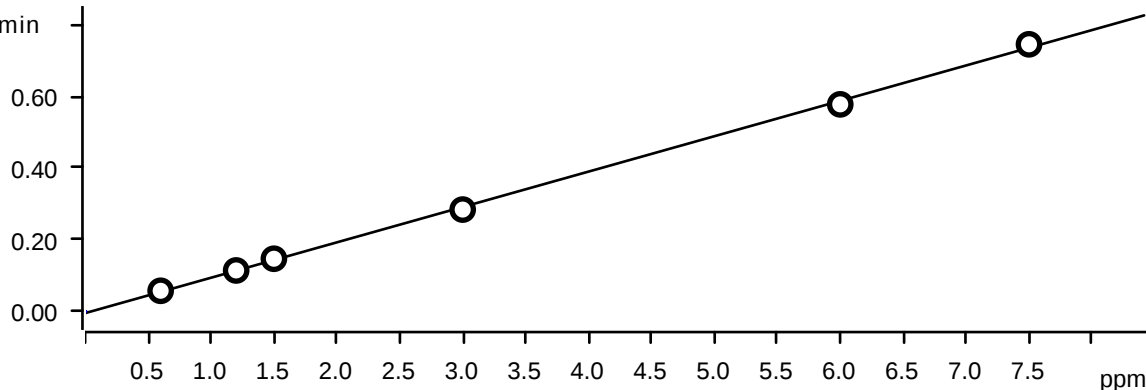

Function: $A = -4.66155\text{E-}3 + 9.86442\text{E-}3 \times Q$


Relative standard deviation 2.532075 %

Correlation coefficient 0.999661

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-10-16 10:55:46 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.058	STD2	2024-10-16 11:17:08 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.114	STD3	2024-10-16 11:38:32 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.147	STD4	2024-10-16 11:59:57 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.284	STD5	2024-10-16 12:21:22 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.577	STD6	2024-10-16 12:42:48 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.745	STD7	2024-10-16 13:04:15 UTC-4	used

Nitrite (Anions)


(μS/cm) x min

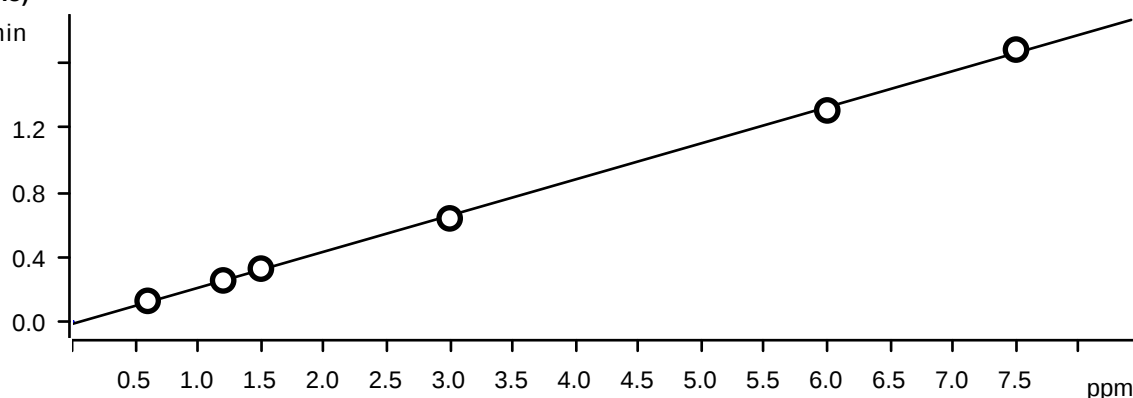Function: $A = -0.0158639 + 0.0223869 \times Q$

Relative standard deviation 2.476730 %

Correlation coefficient 0.999680


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-10-16 10:55:46 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.127	STD2	2024-10-16 11:17:08 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.254	STD3	2024-10-16 11:38:32 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.327	STD4	2024-10-16 11:59:57 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.638	STD5	2024-10-16 12:21:22 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.307	STD6	2024-10-16 12:42:48 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.684	STD7	2024-10-16 13:04:15 UTC-4	used

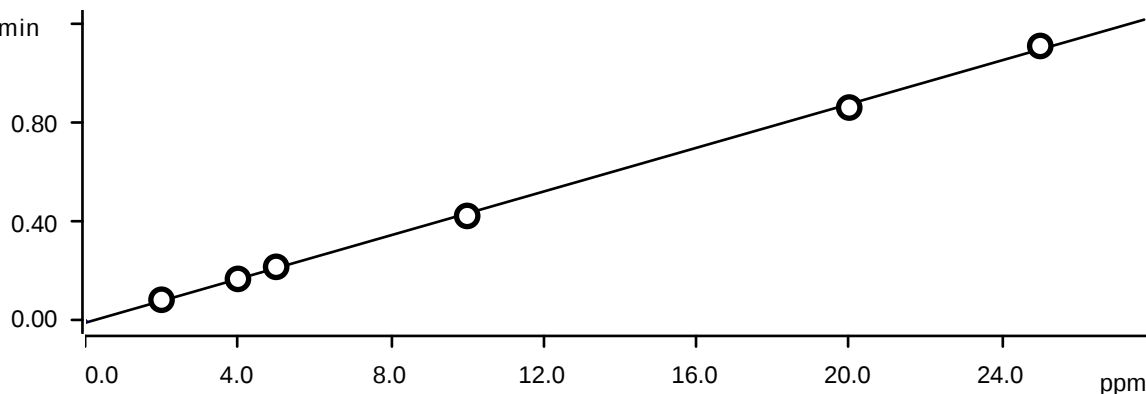Bromide (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -7.83486E-3 + 4.40426E-3 \times Q$

Relative standard deviation 2.425045 %

Correlation coefficient 0.999690


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-10-16 10:55:46 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.085	STD2	2024-10-16 11:17:08 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.169	STD3	2024-10-16 11:38:32 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.217	STD4	2024-10-16 11:59:57 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.422	STD5	2024-10-16 12:21:22 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.859	STD6	2024-10-16 12:42:48 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.107	STD7	2024-10-16 13:04:15 UTC-4	used

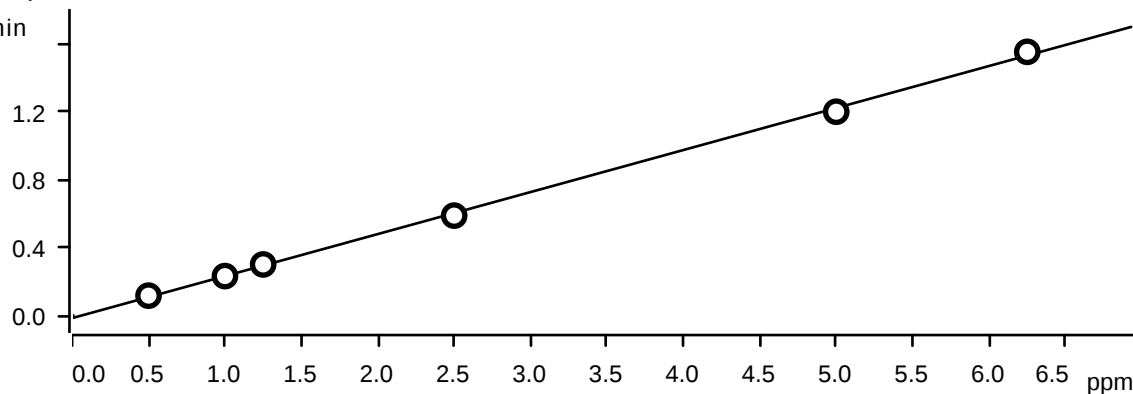Nitrate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0159932 + 0.0247327 \times Q$

Relative standard deviation 2.693966 %

Correlation coefficient 0.999623


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-10-16 10:55:46 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.116	STD2	2024-10-16 11:17:08 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.231	STD3	2024-10-16 11:38:32 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.300	STD4	2024-10-16 11:59:57 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.587	STD5	2024-10-16 12:21:22 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.199	STD6	2024-10-16 12:42:48 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.551	STD7	2024-10-16 13:04:15 UTC-4	used

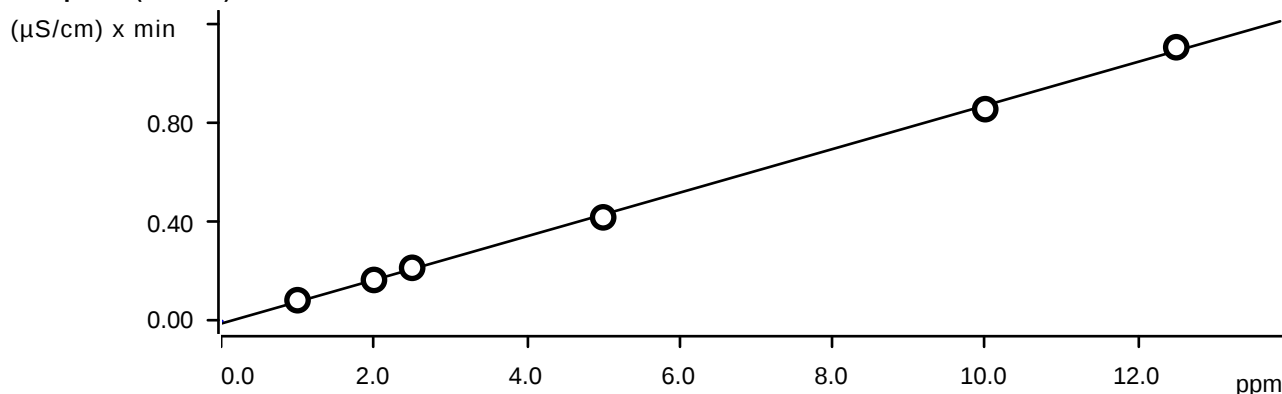Phosphate (Anions)Function: $A = -9.96170E-3 + 8.78405E-3 \times Q$

Relative standard deviation 2.667639 %

Correlation coefficient 0.999628

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-10-16 10:55:46 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.084	STD2	2024-10-16 11:17:08 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.166	STD3	2024-10-16 11:38:32 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.215	STD4	2024-10-16 11:59:57 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.418	STD5	2024-10-16 12:21:22 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.854	STD6	2024-10-16 12:42:48 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.103	STD7	2024-10-16 13:04:15 UTC-4	used

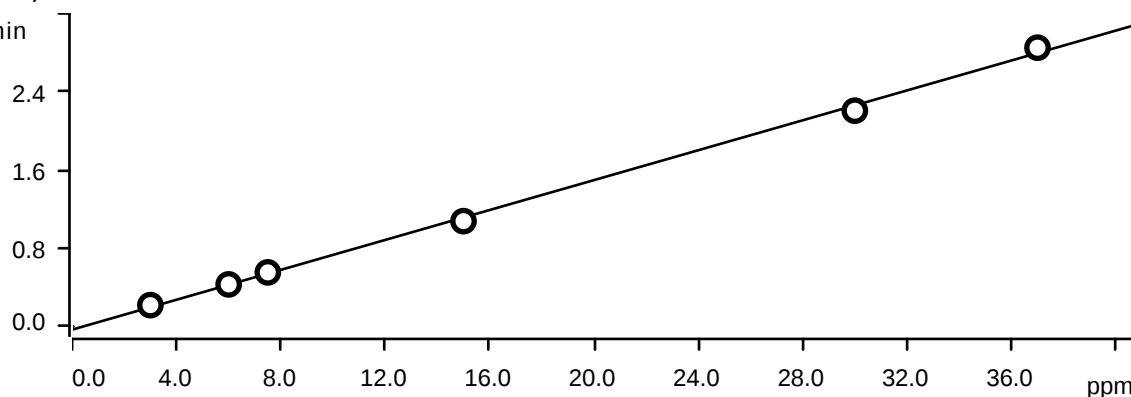Sulfate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0322401 + 7.64234E-3 \times Q$

Relative standard deviation 3.651427 %

Correlation coefficient 0.999303


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-10-16 10:55:46 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.218	STD2	2024-10-16 11:17:08 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.430	STD3	2024-10-16 11:38:32 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.553	STD4	2024-10-16 11:59:57 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.077	STD5	2024-10-16 12:21:22 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.206	STD6	2024-10-16 12:42:48 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.850	STD7	2024-10-16 13:04:15 UTC-4	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2024-10-16 10:55:46 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.33 MPa
Maximum pressure monitored yes
Temperature ---- °C

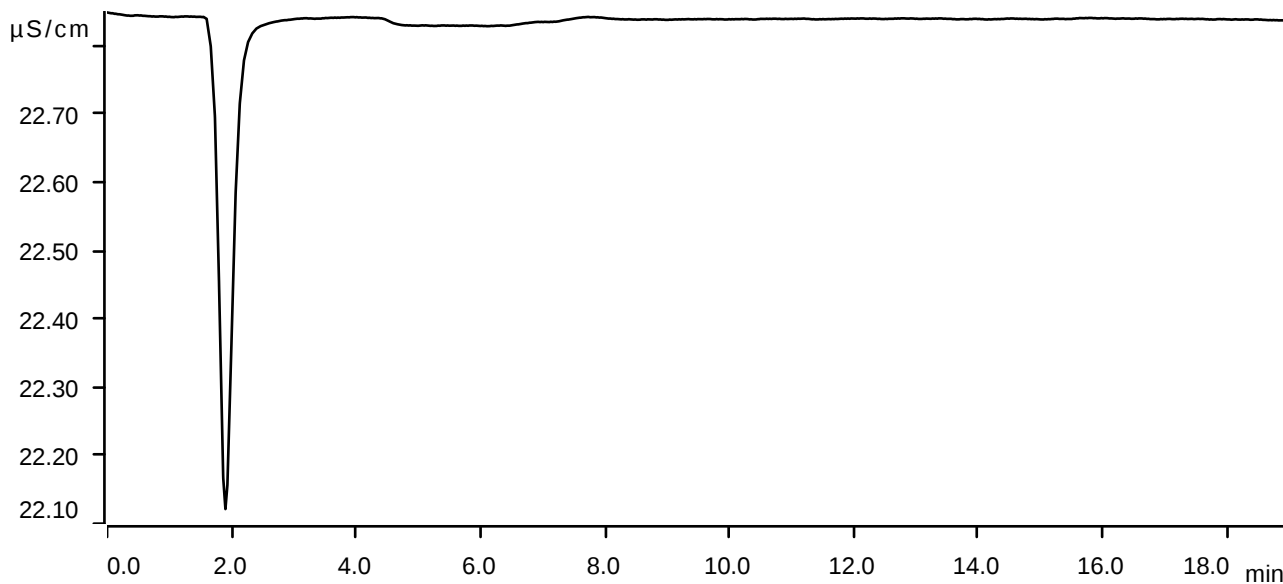Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2024-10-16 11:17:08 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.56 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

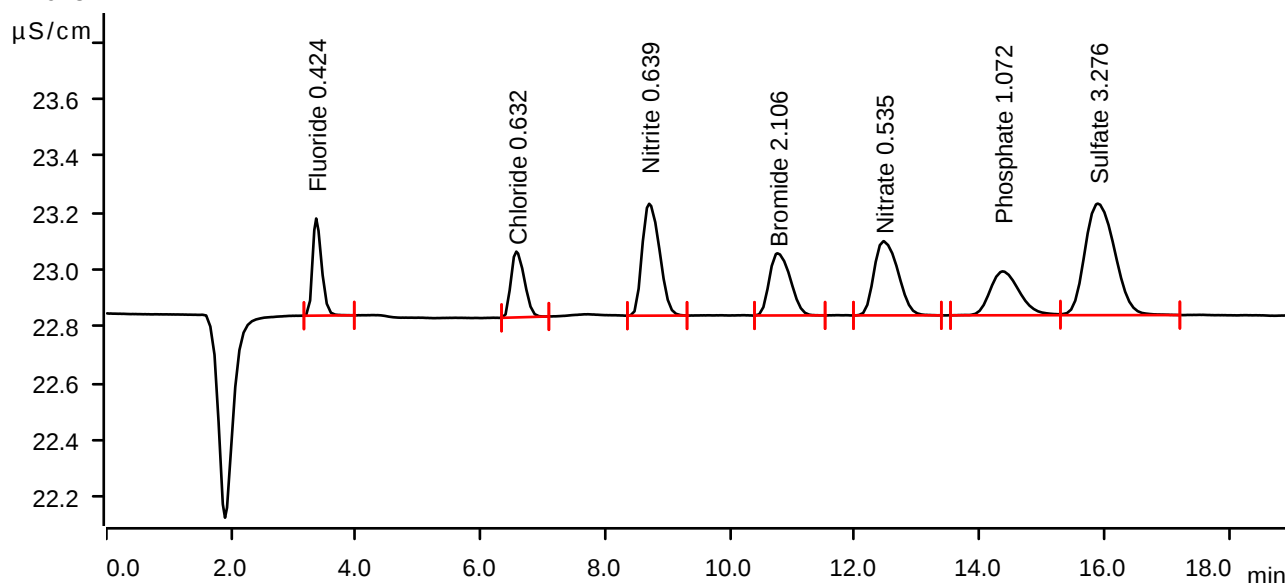

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.365	0.0571	0.341	0.424	Fluoride
2	6.573	0.0576	0.231	0.632	Chloride
3	8.703	0.1273	0.393	0.639	Nitrite
4	10.758	0.0849	0.219	2.106	Bromide
5	12.458	0.1163	0.261	0.535	Nitrate
6	14.368	0.0842	0.154	1.072	Phosphate
7	15.893	0.2181	0.392	3.276	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2024-10-16 11:38:32 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

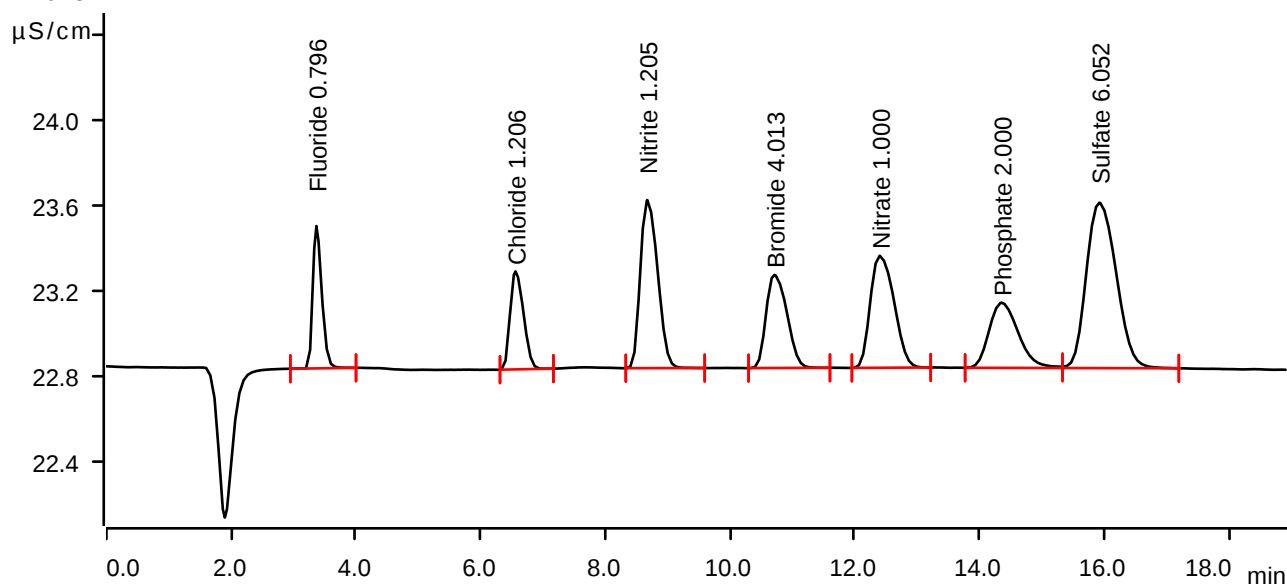

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.368	0.1116	0.667	0.796	Fluoride
2	6.560	0.1143	0.459	1.206	Chloride
3	8.673	0.2538	0.788	1.205	Nitrite
4	10.712	0.1689	0.436	4.013	Bromide
5	12.398	0.2314	0.525	1.000	Nitrate
6	14.353	0.1657	0.305	2.000	Phosphate
7	15.922	0.4302	0.775	6.052	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2024-10-16 11:59:57 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

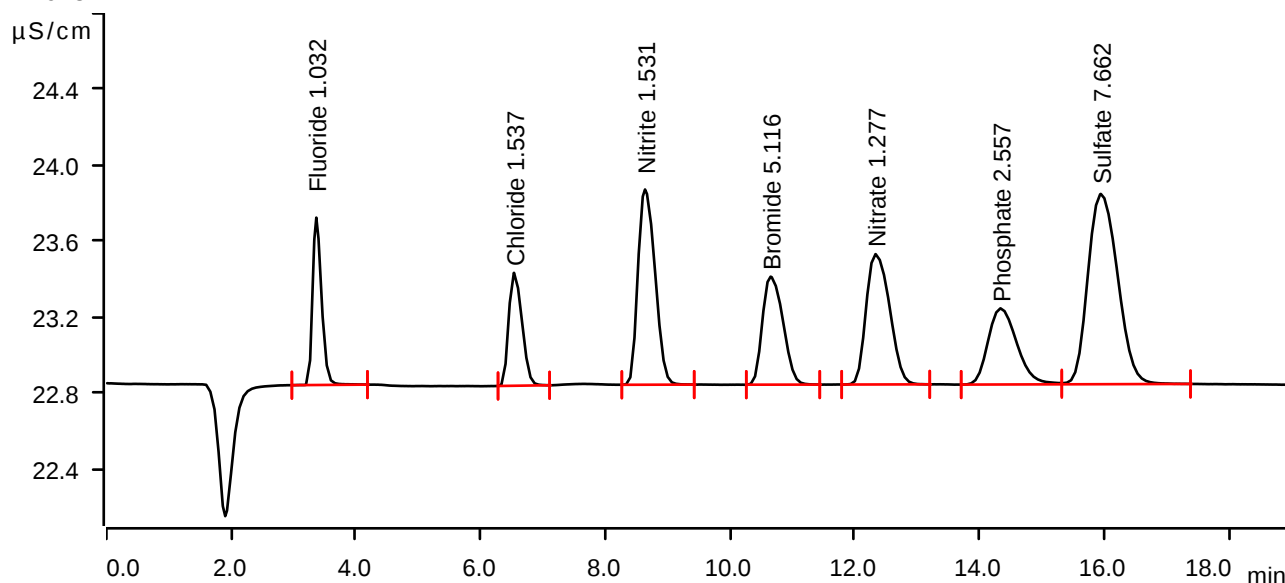

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.367	0.1462	0.882	1.032	Fluoride
2	6.537	0.1469	0.595	1.537	Chloride
3	8.637	0.3270	1.029	1.531	Nitrite
4	10.650	0.2175	0.569	5.116	Bromide
5	12.332	0.2999	0.687	1.277	Nitrate
6	14.337	0.2147	0.401	2.557	Phosphate
7	15.945	0.5533	1.003	7.662	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2024-10-16 12:21:22 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

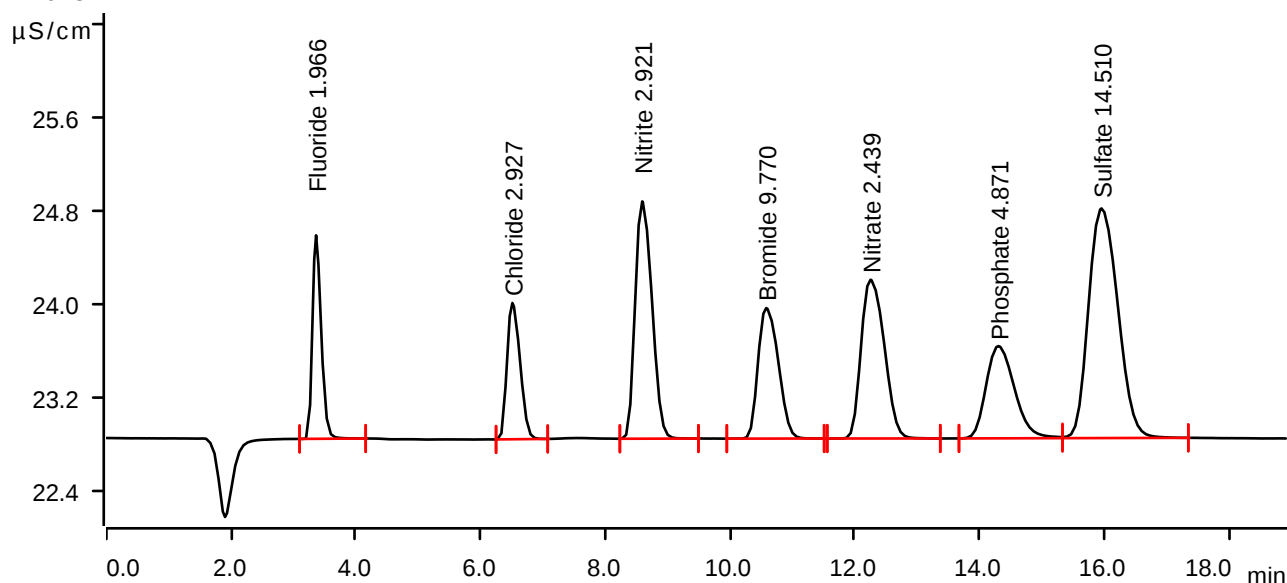

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.363	0.2831	1.748	1.966	Fluoride
2	6.510	0.2841	1.170	2.927	Chloride
3	8.592	0.6381	2.038	2.921	Nitrite
4	10.580	0.4225	1.121	9.770	Bromide
5	12.252	0.5873	1.364	2.439	Nitrate
6	14.302	0.4179	0.793	4.871	Phosphate
7	15.955	1.0767	1.972	14.510	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2024-10-16 12:42:48 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

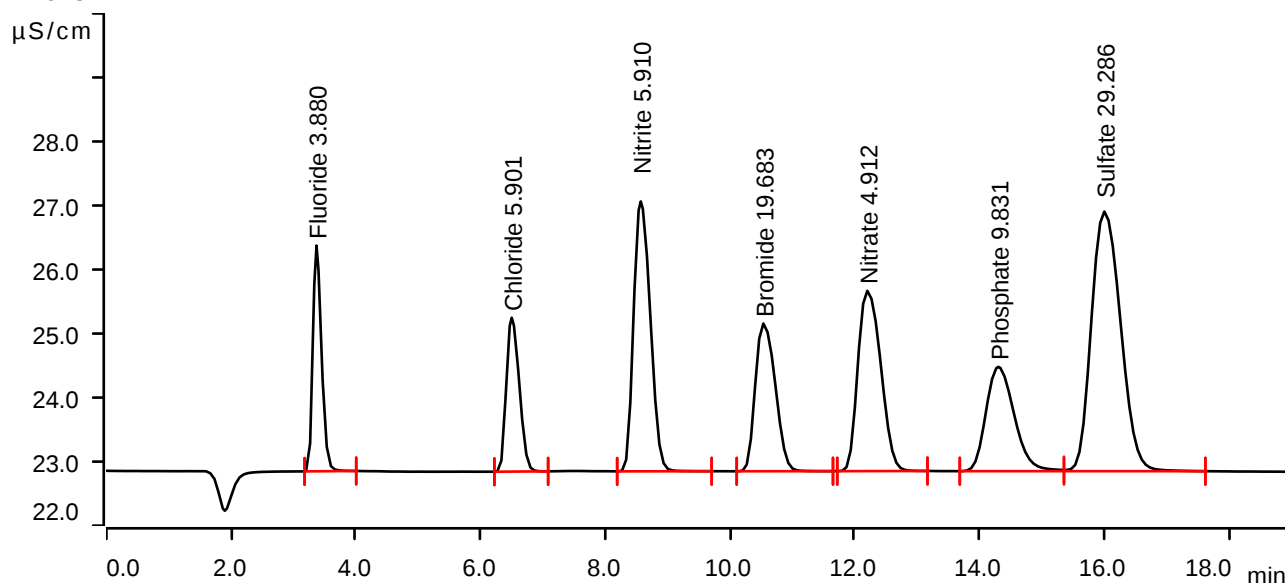

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.370	0.5637	3.525	3.880	Fluoride
2	6.500	0.5774	2.404	5.901	Chloride
3	8.568	1.3072	4.215	5.910	Nitrite
4	10.535	0.8590	2.306	19.683	Bromide
5	12.202	1.1988	2.815	4.912	Nitrate
6	14.302	0.8536	1.629	9.831	Phosphate
7	16.002	2.2059	4.054	29.286	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2024-10-16 13:04:15 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

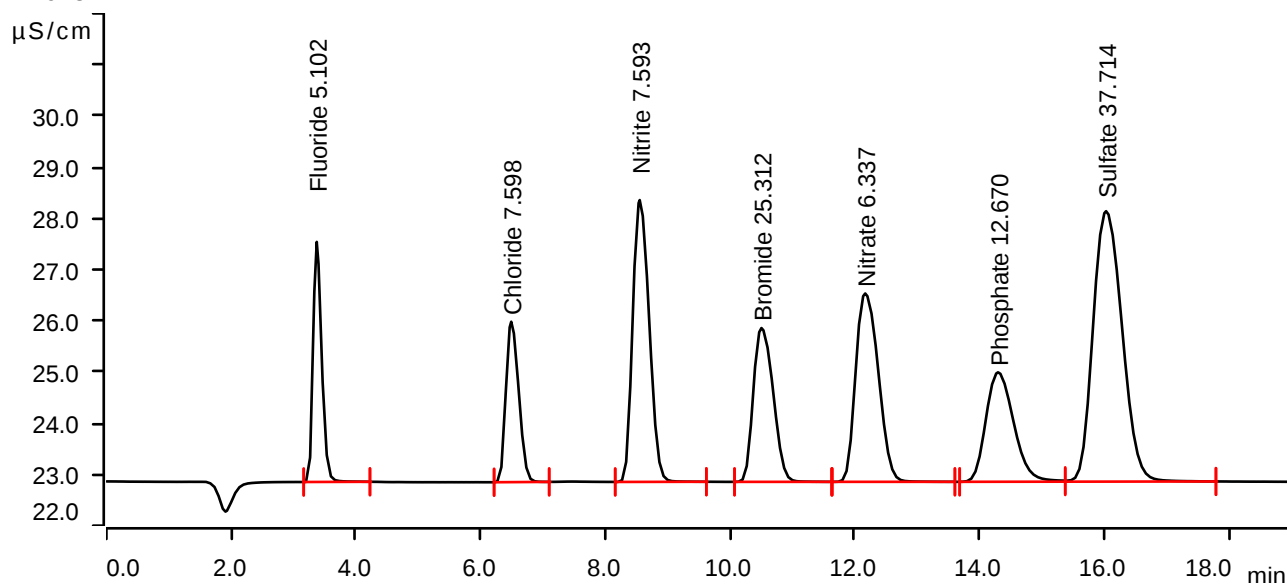

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.373	0.7427	4.687	5.102	Fluoride
2	6.492	0.7448	3.132	7.598	Chloride
3	8.552	1.6841	5.502	7.593	Nitrite
4	10.503	1.1070	3.003	25.312	Bromide
5	12.167	1.5512	3.678	6.337	Nitrate
6	14.297	1.1030	2.137	12.670	Phosphate
7	16.028	2.8500	5.280	37.714	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2024-10-16 13:37:49 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

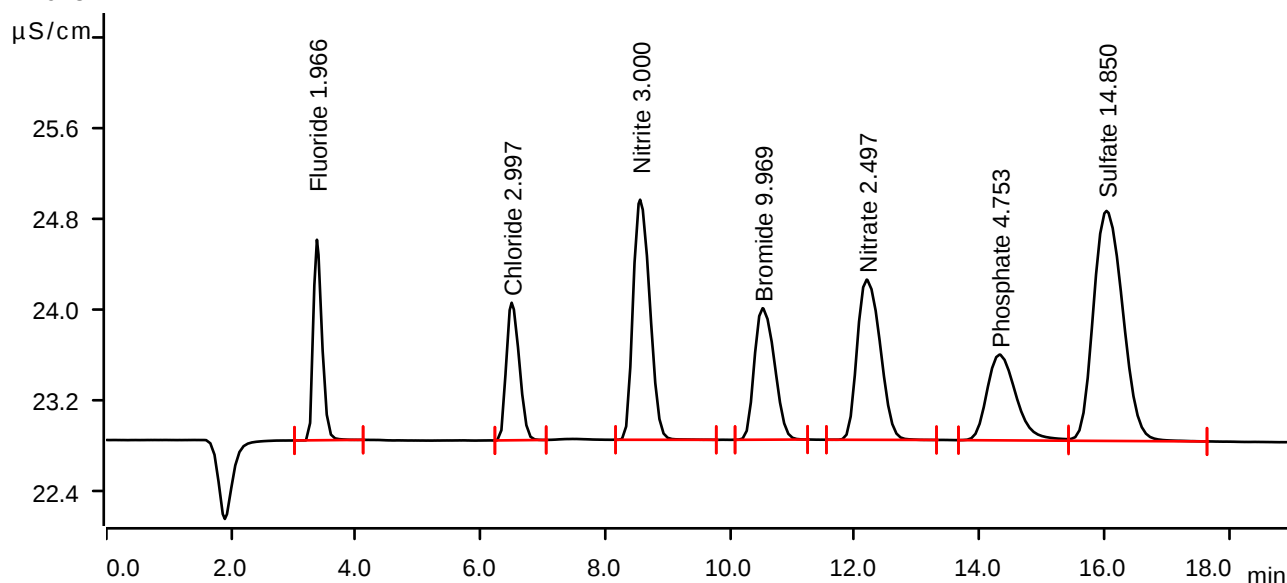


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.377	0.2830	1.762	1.966	Fluoride
2	6.498	0.2910	1.209	2.997	Chloride
3	8.558	0.6557	2.109	3.000	Nitrite
4	10.522	0.4312	1.155	9.969	Bromide
5	12.190	0.6017	1.407	2.497	Nitrate
6	14.320	0.4076	0.753	4.753	Phosphate
7	16.035	1.1027	2.020	14.850	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2024-10-16 13:59:18 UTC-4
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

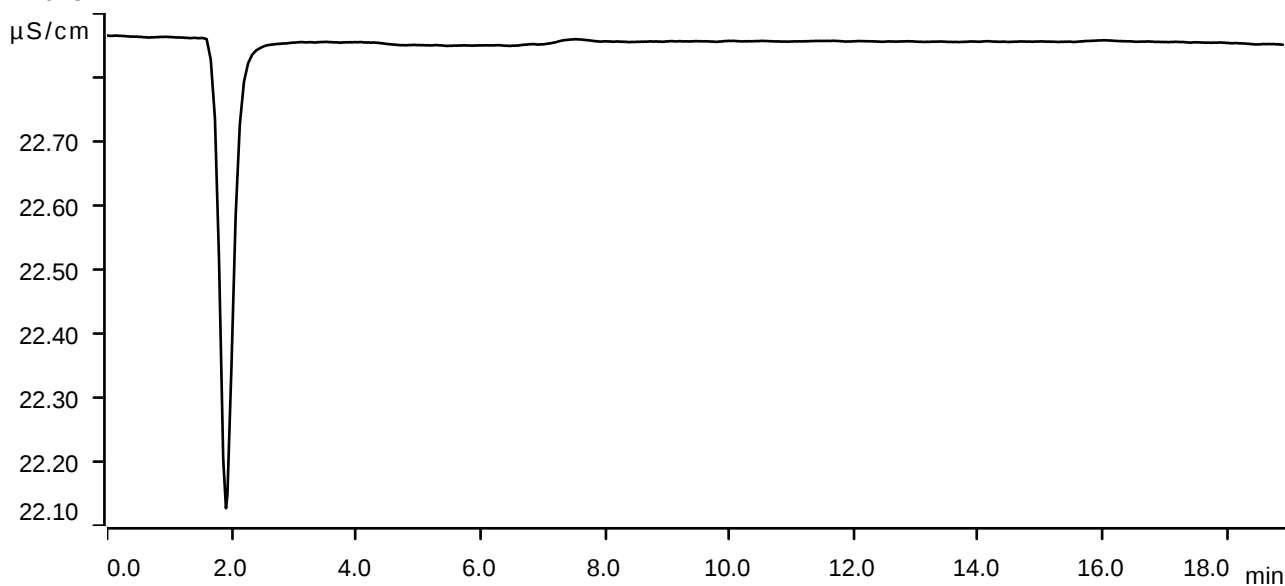Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-11-08 20:40:34 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

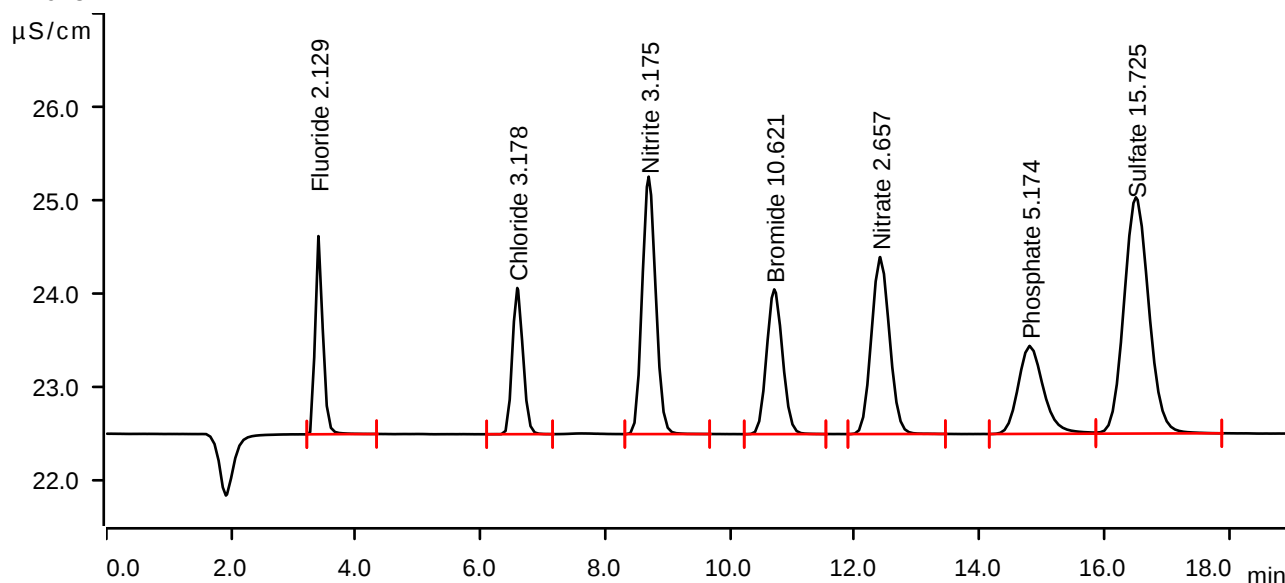

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.400	0.3069	2.128	2.129	Fluoride
2	6.588	0.3088	1.570	3.178	Chloride
3	8.695	0.6949	2.765	3.175	Nitrite
4	10.708	0.4599	1.554	10.621	Bromide
5	12.407	0.6410	1.900	2.657	Nitrate
6	14.803	0.4445	0.945	5.174	Phosphate
7	16.507	1.1695	2.537	15.725	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2024-11-08 21:02:10 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

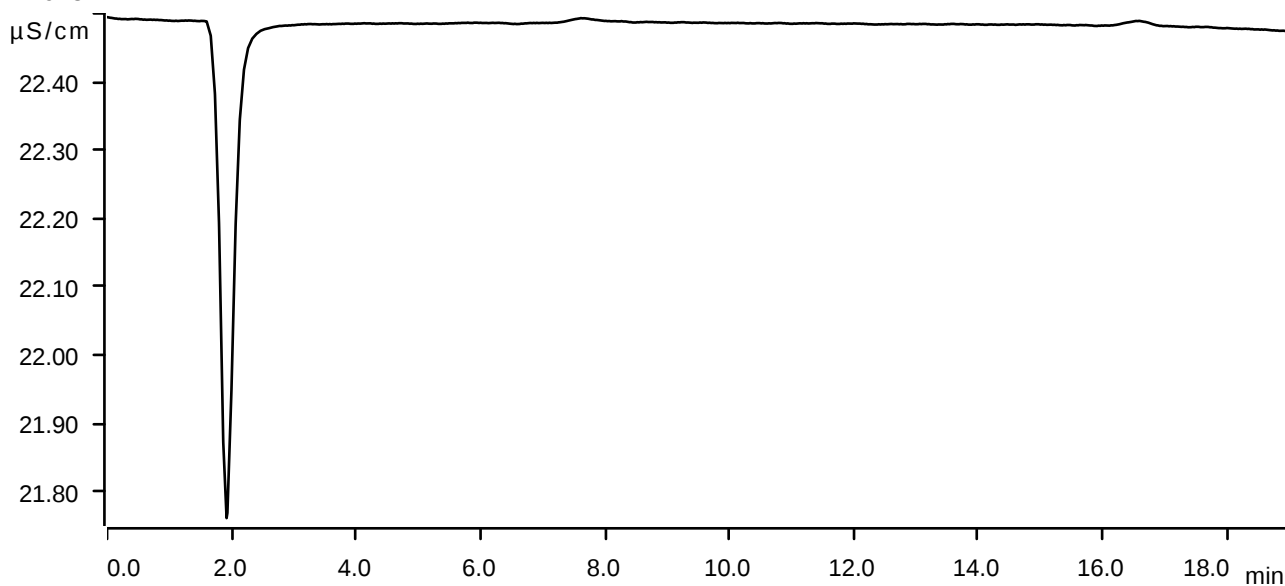


Sample data

Ident LB133371BLW
Sample type Sample
Determination start 2024-11-08 21:23:44 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

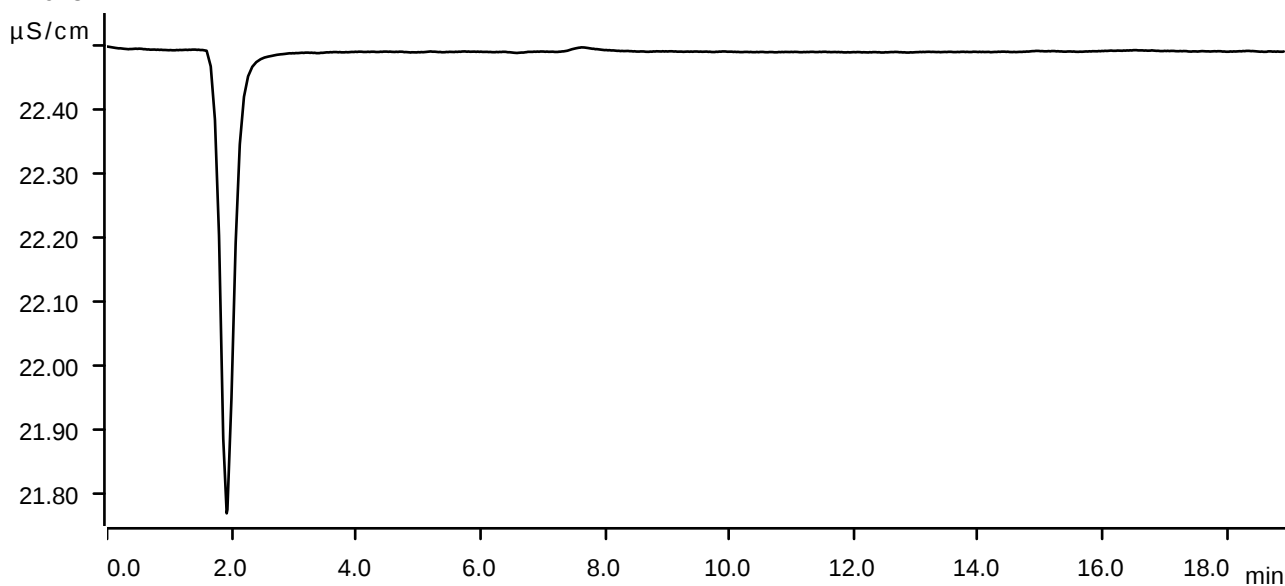


Sample data

Ident LB133371BSW
Sample type Check standard 1
Determination start 2024-11-08 21:45:15 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

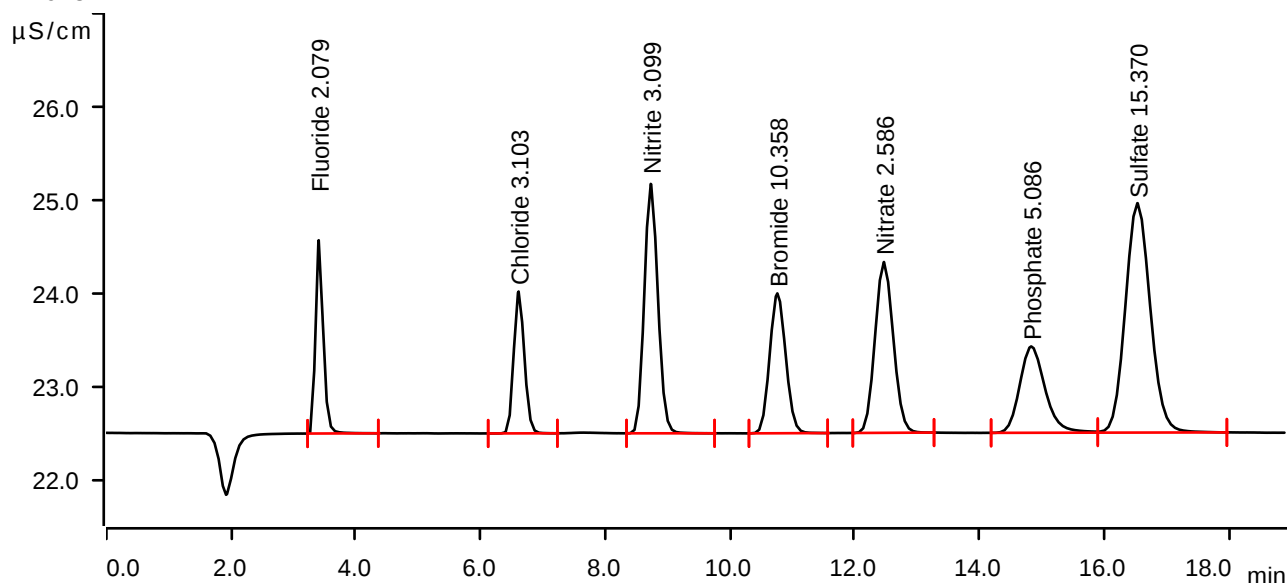

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.405	0.2997	2.075	2.079	Fluoride
2	6.610	0.3014	1.523	3.103	Chloride
3	8.728	0.6780	2.678	3.099	Nitrite
4	10.758	0.4484	1.502	10.358	Bromide
5	12.465	0.6237	1.834	2.586	Nitrate
6	14.828	0.4368	0.927	5.086	Phosphate
7	16.530	1.1424	2.463	15.370	Sulfate


Sample data

Ident P4791-02
Sample type Sample
Determination start 2024-11-08 22:49:54 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

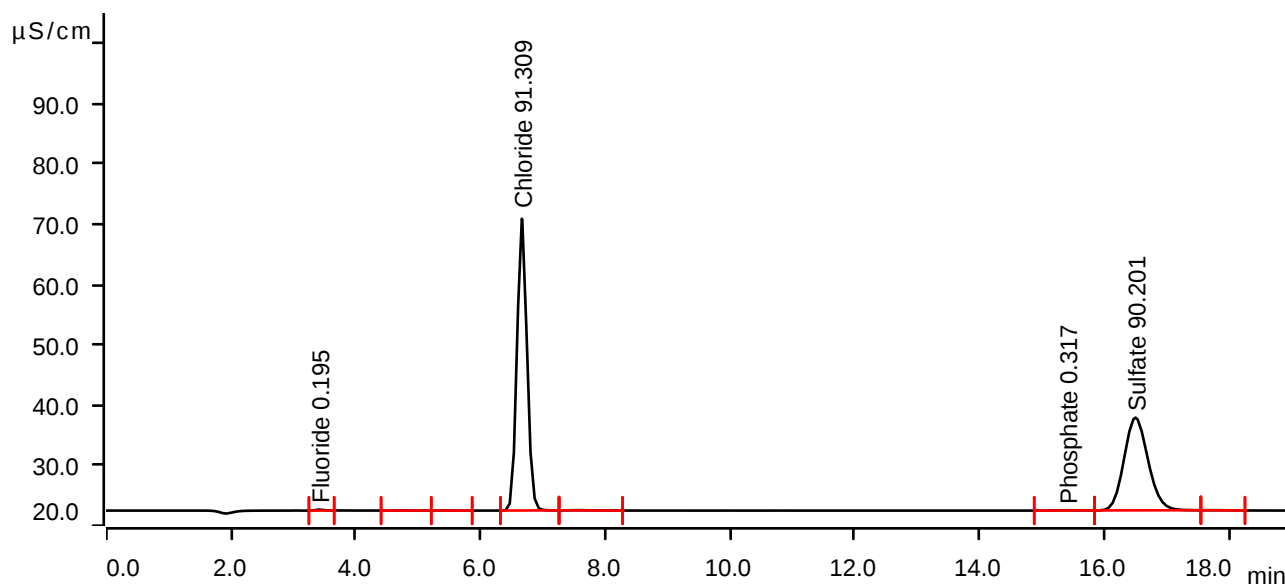

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.410	0.0235	0.160	0.195	Fluoride
2	4.748	0.0062	0.026	invalid	
3	5.435	0.0046	0.017	invalid	
4	6.662	9.0025	48.430	91.309	Chloride
5	7.568	0.0190	0.043	invalid	
6	15.452	0.0179	0.036	0.317	Phosphate
7	16.500	6.8612	15.392	90.201	Sulfate
8	17.767	0.0072	0.017	invalid	


Sample data

Ident P4791-02MS
Sample type Sample
Determination start 2024-11-08 23:32:58 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

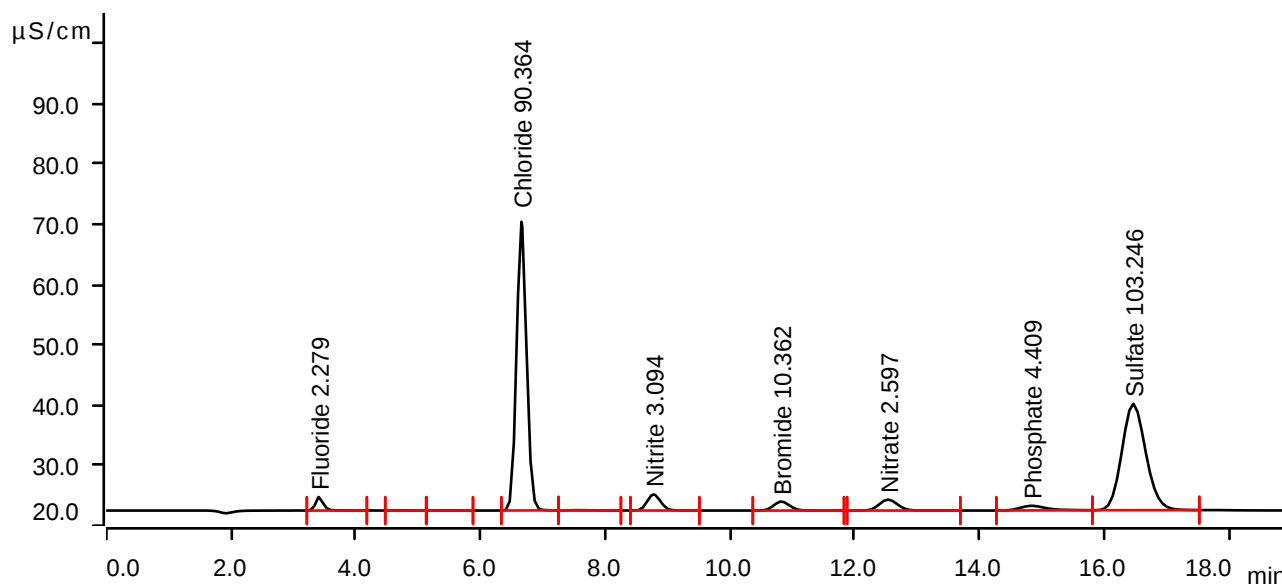

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.405	0.3290	2.244	2.279	Fluoride
2	4.745	0.0055	0.026	invalid	
3	5.445	0.0044	0.016	invalid	
4	6.655	8.9093	47.899	90.364	Chloride
5	7.565	0.0182	0.042	invalid	
6	8.773	0.6768	2.676	3.094	Nitrite
7	10.822	0.4485	1.492	10.362	Bromide
8	12.533	0.6264	1.823	2.597	Nitrate
9	14.835	0.3773	0.767	4.409	Phosphate
10	16.463	7.8582	17.652	103.246	Sulfate


Sample data

Ident P4791-02MSD
Sample type Sample
Determination start 2024-11-08 23:54:32 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

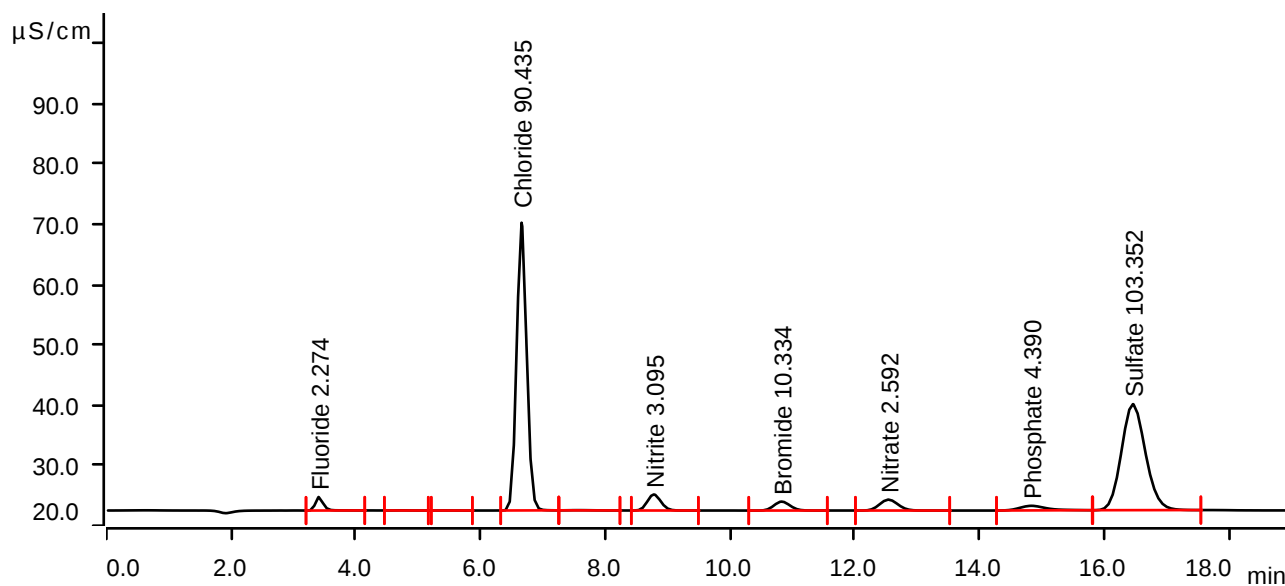

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.405	0.3283	2.235	2.274	Fluoride
2	4.743	0.0053	0.025	invalid	
3	5.432	0.0042	0.016	invalid	
4	6.657	8.9163	47.750	90.435	Chloride
5	7.567	0.0180	0.041	invalid	
6	8.777	0.6771	2.664	3.095	Nitrite
7	10.827	0.4473	1.483	10.334	Bromide
8	12.540	0.6252	1.813	2.592	Nitrate
9	14.830	0.3757	0.765	4.390	Phosphate
10	16.458	7.8663	17.596	103.352	Sulfate


Sample data

Ident P4792-04
Sample type Sample
Determination start 2024-11-09 00:37:40 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

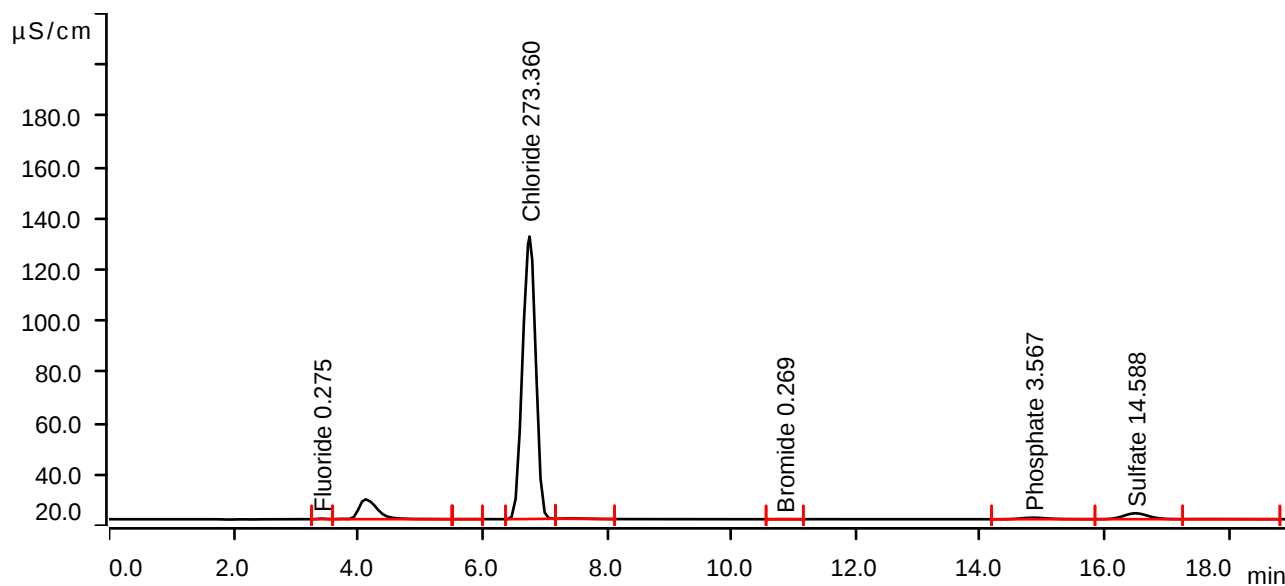

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.410	0.0353	0.223	0.275	Fluoride
2	4.120	2.6745	7.730	invalid	
3	5.742	0.0026	0.011	invalid	
4	6.758	26.9608	110.292	273.360	Chloride
5	7.413	0.0692	0.157	invalid	
6	10.875	0.0040	0.015	0.269	Bromide
7	14.852	0.3033	0.599	3.567	Phosphate
8	16.493	1.0826	2.312	14.588	Sulfate
9	17.672	0.0446	0.052	invalid	


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-11-09 01:20:46 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

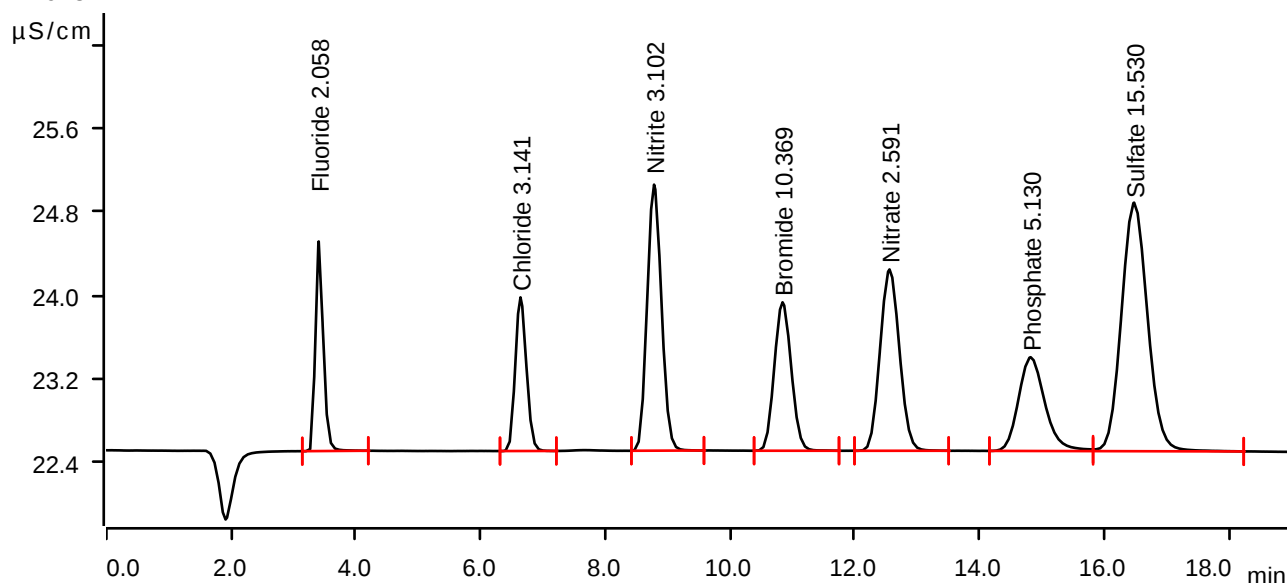

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.405	0.2966	2.005	2.058	Fluoride
2	6.640	0.3052	1.470	3.141	Chloride
3	8.782	0.6785	2.545	3.102	Nitrite
4	10.842	0.4488	1.420	10.369	Bromide
5	12.557	0.6249	1.735	2.591	Nitrate
6	14.820	0.4407	0.897	5.130	Phosphate
7	16.478	1.1546	2.378	15.530	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2024-11-09 01:42:17 UTC-5
Method IC1-101624
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

