


LB133456

7471B

INSTRUMENT (AIR ID): CV1

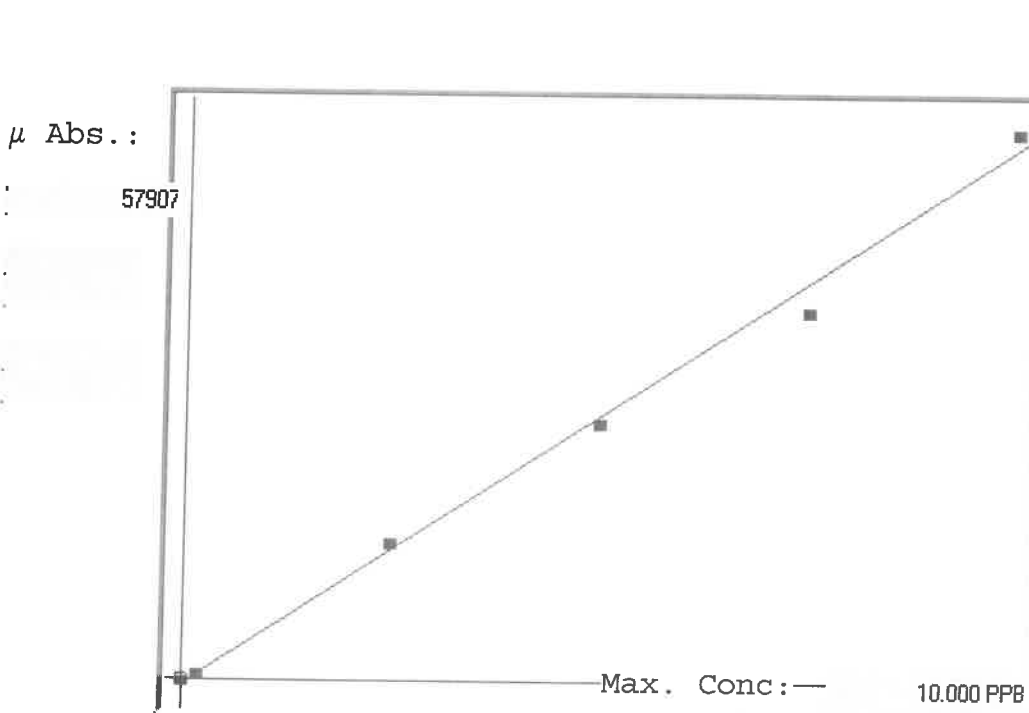

Linear

A= 0.0000e+000

B= 1.7688e-004

C= 9.2714e-002

Rho= 0.9975908

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	$\sigma/01$
0.0	0.000	0.078	0.078	-85	0.000	-85					-
0.2	0.200	0.211	0.011	669	0.0 %	669					5
2.5	2.500	2.665	0.165	14545	0.0 %	14545					7
5.0	5.000	4.897	-0.103	27158	0.0 %	27158					-2
7.5	7.500	7.014	-0.486	39128	0.0 %	39128					-6
10.0	10.000	10.335	0.335	57907	0.0 %	57907					3

LB133456 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 14 Nov 2024 16:05:56

Sample ID	Extended ID	μ Abs.	Conc.	Std Cond	Method	Units	Date	Type	Type
0.0 - 1	50	-85	-	0.0000	7471B	PPB	14 Nov 2024 16:14:56	S	Std
0.2 - 1	50.2	669	-	0.2000	7471B	PPB	14 Nov 2024 16:17:12	S	Std
2.5 - 1	52.5	14545	-	2.5000	7471B	PPB	14 Nov 2024 16:19:29	S	Std
5.0 - 1	55	27158	-	5.0000	7471B	PPB	14 Nov 2024 16:21:46	S	Std
7.5 - 1	57.5	39128	-	7.5000	7471B	PPB	14 Nov 2024 16:24:05	S	Std
10.0 - 1	50	57907	-	10.0000	7471B	PPB	14 Nov 2024 16:35:30	S	Std
ICV86 - 1	ICV86	19915	3.6153	-	7471B	PPB	14 Nov 2024 16:38:16	U	SMPL
ICB86 - 1	ICB86	-46	0.0846	-	7471B	PPB	14 Nov 2024 16:45:43	U	SMPL
CCV89 - 1	CCV89	27380	4.9358	-	7471B	PPB	14 Nov 2024 16:47:57	U	SMPL
CCB89 - 1	CCB89	-207	0.0561	-	7471B	PPB	14 Nov 2024 16:50:12	U	SMPL
CRA - 1	CRA	590	0.1971	-	7471B	PPB	14 Nov 2024 16:52:33	U	SMPL
HighStd - 1	HighStd	58161	10.3804	-	7471B	PPB	14 Nov 2024 16:54:48	U	SMPL
ChkStd - 1	ChkStd	35662	6.4007	-	7471B	PPB	14 Nov 2024 16:57:03	U	SMPL
PB164984BL - 1	PBS	-263	0.0462	-	7471B	PPB	14 Nov 2024 16:59:29	U	SMPL
PB164984BS - 1	LCSS	22303	4.0377	-	7471B	PPB	14 Nov 2024 17:01:54	U	SMPL
P4824-01 - 1	T-20	1748	0.4019	-	7471B	PPB	14 Nov 2024 17:04:10	U	SMPL
P4825-01 - 1	STOCK-PILE	5909	1.1379	-	7471B	PPB	14 Nov 2024 17:06:31	U	SMPL
P4833-01 - 1	MH-731	7431	1.4071	-	7471B	PPB	14 Nov 2024 17:08:50	U	SMPL
P4833-05 - 1	TP-2	3968	0.7946	-	7471B	PPB	14 Nov 2024 17:11:09	U	SMPL
P4833-05DUP - 1	TP-2DUP	3044	0.6311	-	7471B	PPB	14 Nov 2024 17:13:26	U	SMPL
CCV90 - 1	CCV90	27427	4.9441	-	7471B	PPB	14 Nov 2024 17:15:43	U	SMPL
CCB90 - 1	CCB90	-304	0.0389	-	7471B	PPB	14 Nov 2024 17:18:00	U	SMPL
P4833-05MS - 1	TP-2MS	23244	4.2042	-	7471B	PPB	14 Nov 2024 17:20:20	U	SMPL
P4833-05MSD - 1	TP-2MSD	21591	3.9118	-	7471B	PPB	14 Nov 2024 17:22:34	U	SMPL
P4834-03 - 1	SLP-1-STONE	3455	0.7038	-	7471B	PPB	14 Nov 2024 17:24:56	U	SMPL
P4835-03 - 1	345-2-STONE	7634	1.4430	-	7471B	PPB	14 Nov 2024 17:27:16	U	SMPL
P4836-03 - 1	T3-STONE	2205	0.4827	-	7471B	PPB	14 Nov 2024 17:29:33	U	SMPL
P4837-03 - 1	3TRK-STONE	1267	0.3168	-	7471B	PPB	14 Nov 2024 17:31:51	U	SMPL
P4838-03 - 1	T1-STONE	906	0.2530	-	7471B	PPB	14 Nov 2024 17:34:08	U	SMPL
P4833-05LX5 - 1		264	0.1394	-	7471B	PPB	14 Nov 2024 17:36:25	U	SMPL
P4833-05 - 1		23142	4.1861	-	7471B	PPB	14 Nov 2024 17:38:42	U	SMPL
CCV91 - 1	CCV91	28091	5.0615	-	7471B	PPB	14 Nov 2024 17:40:57	U	SMPL
CCB91 - 1	CCB91	-292	0.0411	-	7471B	PPB	14 Nov 2024 17:43:16	U	SMPL