


LB133490

7470A

INSTRUMENT ID: CY2

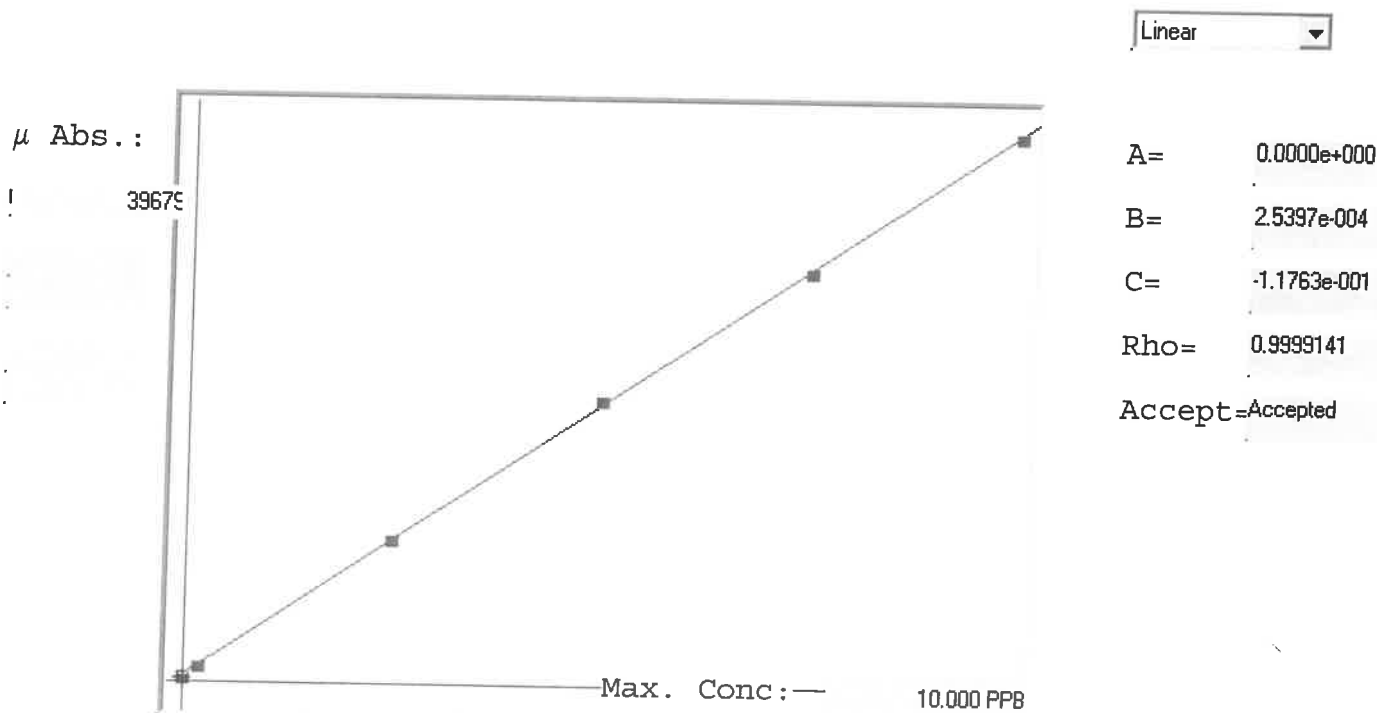

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.042	-0.042	298	0.000	298	0				
0.2	0.200	0.191	-0.009	1216	0.0 %	1216					
2.5	2.500	2.508	0.008	10338	0.0 %	10338					
5.0	5.000	5.101	0.101	20548	0.0 %	20548					
7.5	7.500	7.482	-0.018	29924	0.0 %	29924					
10.0	10.000	9.960	-0.040	39679	0.0 %	39679					

15
002000

LB133490 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 18 Nov 2024 12:50:35

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	298	-	0.0000	7470A	PPB	18 Nov 2024 13:23:28	S	Std
0.2 - 1	50.2	1216	-	0.2000	7470A	PPB	18 Nov 2024 13:25:44	S	Std
2.5 - 1	52.5	10338	-	2.5000	7470A	PPB	18 Nov 2024 13:28:01	S	Std
5.0 - 1	55	20548	-	5.0000	7470A	PPB	18 Nov 2024 13:30:17	S	Std
7.5 - 1	57.5	29924	-	7.5000	7470A	PPB	18 Nov 2024 13:32:33	S	Std
10.0 - 1	518	39679	-	10.0000	7470A	PPB	18 Nov 2024 13:43:15	S	Std
ICB89 - 1	ICB89	15193	3.7409	-	7470A	PPB	18 Nov 2024 13:46:07	U	SMPL
ICB89 - 1	ICB89	91	-0.0945	-	7470A	PPB	18 Nov 2024 13:48:22	U	SMPL
CCV01 - 1	CCV01	19919	4.9412	-	7470A	PPB	18 Nov 2024 13:53:37	U	SMPL
CCB01 - 1	CCB01	135	-0.0833	-	7470A	PPB	18 Nov 2024 13:58:36	U	SMPL
CRA - 1	CRA	1138	0.1714	-	7470A	PPB	18 Nov 2024 14:00:51	U	SMPL
HighStd - 1	HighStd	38800	9.7364	-	7470A	PPB	18 Nov 2024 14:03:06	U	SMPL
ChkStd - 1	ChkStd	28923	6.7200	-	7470A	PPB	18 Nov 2024 14:05:21	U	SMPL
PB165041BL - 1	PBW	585	0.0309	-	7470A	PPB	18 Nov 2024 14:07:39	U	SMPL
PB165041BS - 1	LCSW	17477	4.3210	-	7470A	PPB	18 Nov 2024 14:12:49	U	SMPL
P4821-04 - 1	BP-F-24	531	0.0172	-	7470A	PPB	18 Nov 2024 14:15:06	U	SMPL
P4821-08 - 1	BP-F-2	455	-0.0021	-	7470A	PPB	18 Nov 2024 14:17:25	U	SMPL
P4823-04 - 1	MH-4	440	-0.0059	-	7470A	PPB	18 Nov 2024 14:19:43	U	SMPL
P4833-04 - 1	MH-731	652	0.0480	-	7470A	PPB	18 Nov 2024 14:21:59	U	SMPL
P4833-08 - 1	TP-2	696	0.0591	-	7470A	PPB	18 Nov 2024 14:24:14	U	SMPL
CCV02 - 1	CCV02	19977	4.9559	-	7470A	PPB	18 Nov 2024 14:26:30	U	SMPL
CCB02 - 1	CCB02	70	-0.0998	-	7470A	PPB	18 Nov 2024 14:28:48	U	SMPL
P4833-08DUP - 1	TP-2DUP	657	0.0492	-	7470A	PPB	18 Nov 2024 14:31:07	U	SMPL
P4833-08MS - 1	TP-2MS	16649	4.1107	-	7470A	PPB	18 Nov 2024 14:33:22	U	SMPL
P4833-08MSD - 1	TP-2MSD	15995	3.9446	-	7470A	PPB	18 Nov 2024 14:38:15	U	SMPL
PB165066BL - 1	PBW	546	0.0210	-	7470A	PPB	18 Nov 2024 14:43:20	U	SMPL
PB165066BS - 1	LCSW	13940	3.4227	-	7470A	PPB	18 Nov 2024 14:45:35	U	SMPL
P4867-02 - 1	TT-070-IDWGW-20241113	11	-0.1148	-	7470A	PPB	18 Nov 2024 14:47:51	U	SMPL
P4867-03 - 1	TT-071-IDWGW-20241113	741	0.0706	-	7470A	PPB	18 Nov 2024 14:50:08	U	SMPL
P4867-04 - 1	TT-072-IDWGW-20241113	89	-0.0950	-	7470A	PPB	18 Nov 2024 14:52:27	U	SMPL
P4867-04DUP - 1	TT-072-IDWGW-20241113DUP	163	-0.0762	-	7470A	PPB	18 Nov 2024 14:54:45	U	SMPL
P4867-04MS - 1	TT-072-IDWGW-20241113MS	17552	4.3401	-	7470A	PPB	18 Nov 2024 14:57:01	U	SMPL
CCV03 - 1	CCV03	20602	5.1147	-	7470A	PPB	18 Nov 2024 14:59:16	U	SMPL
CCB03 - 1	CCB03	339	-0.0315	-	7470A	PPB	18 Nov 2024 15:01:33	U	SMPL
P4867-04MSD - 1	TT-072-IDWGW-20241113MSD	16166	3.9881	-	7470A	PPB	18 Nov 2024 15:03:50	U	SMPL
P4868-01 - 1	RW5-SP100-20241114	-36	-0.1268	-	7470A	PPB	18 Nov 2024 15:06:05	U	SMPL
P4868-03 - 1	RW5-SP303-20241114	90	-0.0948	-	7470A	PPB	18 Nov 2024 15:08:23	U	SMPL
PB164944TB - 1	PB164944TB	678	0.0546	-	7470A	PPB	18 Nov 2024 15:10:38	U	SMPL
P4833-08LX5 - 1		32	-0.1095	-	7470A	PPB	18 Nov 2024 15:12:54	U	SMPL
P4833-08A - 1		15896	3.9195	-	7470A	PPB	18 Nov 2024 15:15:10	U	SMPL
P4867-04LX5 - 1		-131	-0.1509	-	7470A	PPB	18 Nov 2024 15:17:26	U	SMPL
P4867-04A - 1		16978	4.1943	-	7470A	PPB	18 Nov 2024 15:19:44	U	SMPL
CCV04 - 1	CCV04	20196	5.0116	-	7470A	PPB	18 Nov 2024 15:22:01	U	SMPL
CCB04 - 1	CCB04	815	0.0894	-	7470A	PPB	18 Nov 2024 15:24:19	U	SMPL