


LB133516

7471B

INSTRUMENT ID: CV1

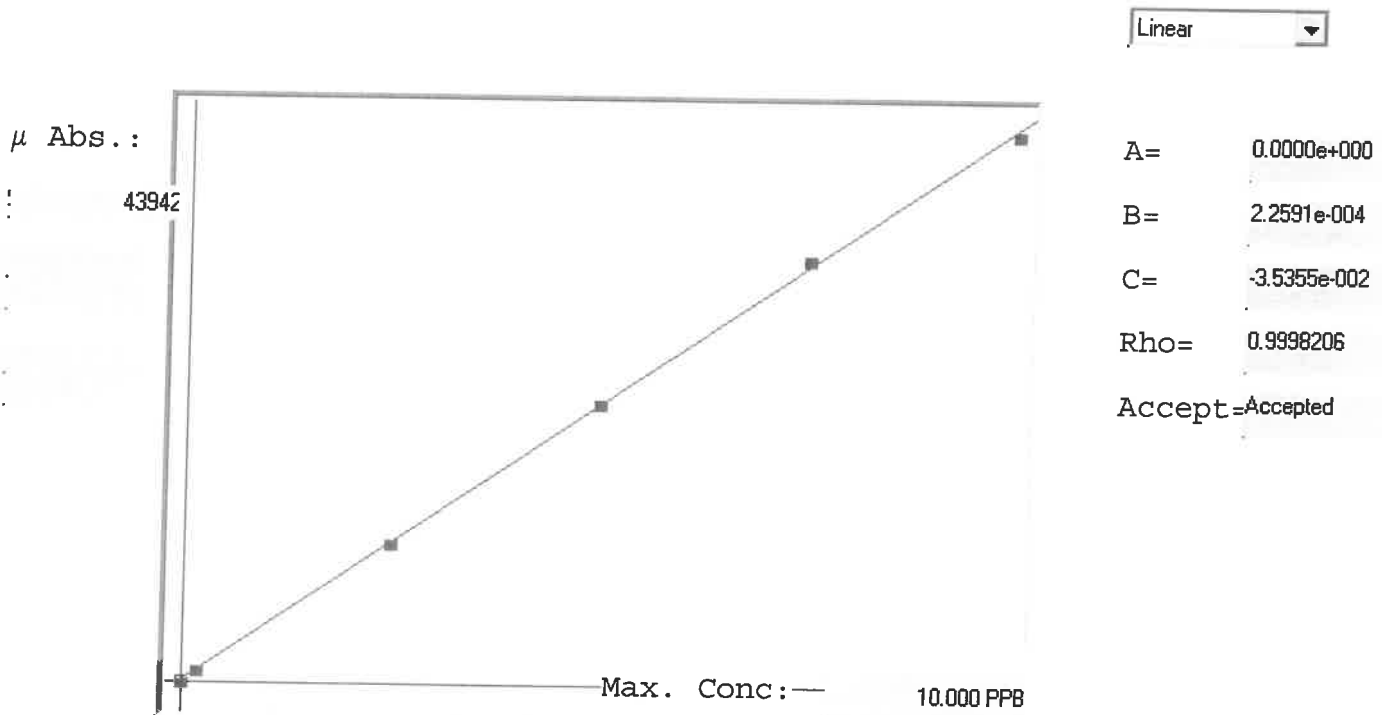

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	4/6/11
0.0	0.000	-0.035	-0.035	1	0.000	1					
0.2	0.200	0.198	-0.002	1031	0.0 %	1031					
2.5	2.500	2.494	-0.006	11197	0.0 %	11197					
5.0	5.000	5.027	0.027	22411	0.0 %	22411					
7.5	7.500	7.624	0.124	33907	0.0 %	33907					
10.0	10.000	9.891	-0.109	43942	0.0 %	43942					

LB133516 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 19 Nov 2024 14:37:52

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	1	-	0.0000	7471B	PPB	19 Nov 2024 15:10:33	S	Std
0.2 - 1	50-2	1031	-	0.2000	7471B	PPB	19 Nov 2024 15:12:50	S	Std
2.5 - 1	52-5	11197	-	2.5000	7471B	PPB	19 Nov 2024 15:15:07	S	Std
5.0 - 1	55	22411	-	5.0000	7471B	PPB	19 Nov 2024 15:17:24	S	Std
7.5 - 1	57-5	33907	-	7.5000	7471B	PPB	19 Nov 2024 15:19:42	S	Std
10.0 - 1	510	43942	-	10.0000	7471B	PPB	19 Nov 2024 15:24:58	S	Std
ICV91 - 1	ICV91	16581	3.7104	-	7471B	PPB	19 Nov 2024 15:27:43	U	SMPL
ICB91 - 1	ICB91	-56	-0.0480	-	7471B	PPB	19 Nov 2024 15:32:37	U	SMPL
CCV10 - 1	CCV10	22483	5.0437	-	7471B	PPB	19 Nov 2024 15:34:51	U	SMPL
CCB10 - 1	CCB10	35	-0.0274	-	7471B	PPB	19 Nov 2024 15:39:45	U	SMPL
CRA - 1	CRA	1086	0.2100	-	7471B	PPB	19 Nov 2024 15:42:00	U	SMPL
HighStd - 1	HighStd	43937	9.8904	-	7471B	PPB	19 Nov 2024 15:44:15	U	SMPL
ChkStd - 1	ChkStd	32320	7.2660	-	7471B	PPB	19 Nov 2024 15:46:29	U	SMPL
PB165113BL - 1	PBS	-161	-0.0717	-	7471B	PPB	19 Nov 2024 15:48:54	U	SMPL
PB165113BS - 1	LCSS	18476	4.1385	-	7471B	PPB	19 Nov 2024 15:51:15	U	SMPL
P4869-01 - 1	EO-02-11152024	5872	1.2912	-	7471B	PPB	19 Nov 2024 15:53:32	U	SMPL
P4887-01 - 1	MH-739	790	0.1431	-	7471B	PPB	19 Nov 2024 15:55:51	U	SMPL
P4887-05 - 1	MH-760	1450	0.2922	-	7471B	PPB	19 Nov 2024 15:58:12	U	SMPL
P4889-01 - 1	VNJ-228	2574	0.5461	-	7471B	PPB	19 Nov 2024 16:00:31	U	SMPL
P4889-01DUP - 1	VNJ-228DUP	2822	0.6022	-	7471B	PPB	19 Nov 2024 16:02:47	U	SMPL
CCV11 - 1	CCV11	22744	5.1027	-	7471B	PPB	19 Nov 2024 16:05:04	U	SMPL
CCB11 - 1	CCB11	-199	-0.0803	-	7471B	PPB	19 Nov 2024 16:07:23	U	SMPL
P4889-01MS - 1	VNJ-228MS	22116	4.9608	-	7471B	PPB	19 Nov 2024 16:09:41	U	SMPL
P4889-01MSD - 1	VNJ-228MSD	21796	4.8885	-	7471B	PPB	19 Nov 2024 16:15:23	U	SMPL
P4889-03 - 1	#72-11978	6384	1.4068	-	7471B	PPB	19 Nov 2024 16:17:38	U	SMPL
P4889-05 - 1	#72-11930	5345	1.1721	-	7471B	PPB	19 Nov 2024 16:19:56	U	SMPL
P4892-01 - 1	WB-310-TOP	226945	51.2333	-	7471B	PPB	19 Nov 2024 16:22:14	U	SMPL
P4892-02 - 1	WB-310-BOT	596	0.0993	-	7471B	PPB	19 Nov 2024 16:28:09	U	SMPL
P4893-01 - 1	MH-763	316	0.0360	-	7471B	PPB	19 Nov 2024 16:30:25	U	SMPL
P4893-05 - 1	MH-762	557	0.0905	-	7471B	PPB	19 Nov 2024 16:32:42	U	SMPL
P4908-01 - 1	SP-1	1114	0.2163	-	7471B	PPB	19 Nov 2024 16:34:59	U	SMPL
P4908-03 - 1	SP-2	1326	0.2642	-	7471B	PPB	19 Nov 2024 16:37:14	U	SMPL
CCV12 - 1	CCV12	22922	5.1429	-	7471B	PPB	19 Nov 2024 16:39:29	U	SMPL
CCB12 - 1	CCB12	-189	-0.0781	-	7471B	PPB	19 Nov 2024 16:41:45	U	SMPL
P4909-01 - 1	BU-02-111824	1191	0.2337	-	7471B	PPB	19 Nov 2024 16:44:04	U	SMPL
P4910-01 - 1	MH-COTTAGE	697	0.1221	-	7471B	PPB	19 Nov 2024 16:46:20	U	SMPL
P4910-05 - 1	MH-759	749	0.1338	-	7471B	PPB	19 Nov 2024 16:48:35	U	SMPL
P4889-01LX5 - 1		495	0.0765	-	7471B	PPB	19 Nov 2024 16:50:50	U	SMPL
P4889-01A - 1		22005	4.9357	-	7471B	PPB	19 Nov 2024 16:56:14	U	SMPL
P4992-01DLX10 - 1		22883	5.1341	-	7471B	PPB	19 Nov 2024 17:03:49	U	SMPL
CCV13 - 1	CCV13	23362	5.2423	-	7471B	PPB	19 Nov 2024 17:06:06	U	SMPL
CCB13 - 1	CCB13	-183	-0.0767	-	7471B	PPB	19 Nov 2024 17:08:25	U	SMPL