


LB133599

7470A

INSTRUMENT ID: CV1

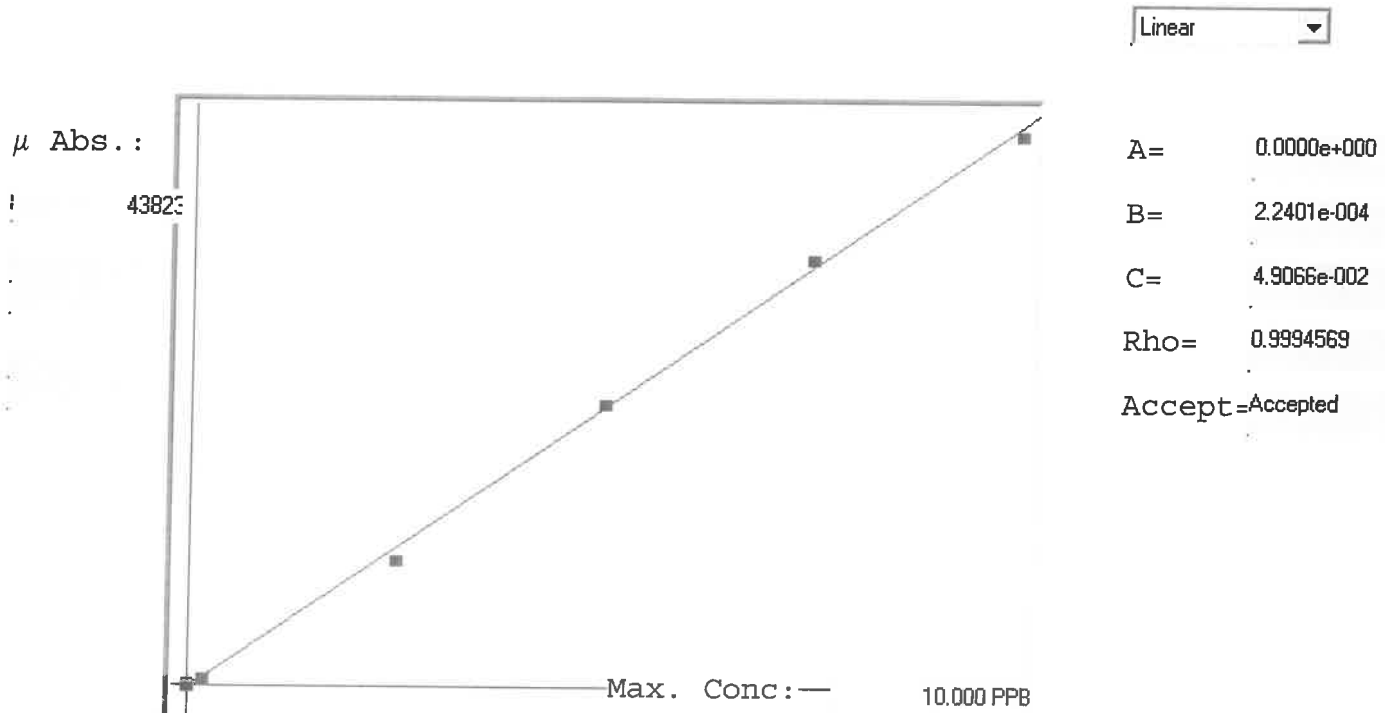

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.060	0.060	48	0.000	48	0				-
0.2	0.200	0.193	-0.007	641	0.0 %	641					-4
2.5	2.500	2.323	-0.177	10150	0.0 %	10150					-7
5.0	5.000	5.098	0.098	22538	0.0 %	22538					2
7.5	7.500	7.661	0.161	33983	0.0 %	33983					2
10.0	10.000	9.866	-0.134	43823	0.0 %	43823					-1

LB133599 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 25 Nov 2024 11:13:24

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	48	-	0.0000	7470A	PPB	25 Nov 2024 11:21:40	S	Std
0.2 - 1	50.2	641	-	0.2000	7470A	PPB	25 Nov 2024 11:23:57	S	Std
2.5 - 1	52.5	10150	-	2.5000	7470A	PPB	25 Nov 2024 11:26:14	S	Std
5.0 - 1	55	22538	-	5.0000	7470A	PPB	25 Nov 2024 11:31:07	S	Std
7.5 - 1	57.5	33983	-	7.5000	7470A	PPB	25 Nov 2024 11:43:03	S	Std
10.0 - 1	510	43823	-	10.0000	7470A	PPB	25 Nov 2024 11:45:18	S	Std
ICV100 - 1	ICV100	18944	4.2926	-	7470A	PPB	25 Nov 2024 11:50:44	U	SMPL
ICB100 - 1	ICB100	-181	0.0085	-	7470A	PPB	25 Nov 2024 11:52:59	U	SMPL
CCV46 - 1	CCV46	22780	5.1519	-	7470A	PPB	25 Nov 2024 11:55:16	U	SMPL
CCB46 - 1	CCB46	-189	0.0067	-	7470A	PPB	25 Nov 2024 11:57:31	U	SMPL
CRA - 1	CRA	659	0.1967	-	7470A	PPB	25 Nov 2024 11:59:48	U	SMPL
HighStd - 1	HighStd	44506	10.0187	-	7470A	PPB	25 Nov 2024 12:02:03	U	SMPL
ChkStd - 1	ChkStd	32229	7.2685	-	7470A	PPB	25 Nov 2024 12:04:18	U	SMPL
PB165227BL - 1	PBW	-520	-0.0674	-	7470A	PPB	25 Nov 2024 12:06:37	U	SMPL
PB165227BS - 1	LCSW	16808	3.8142	-	7470A	PPB	25 Nov 2024 12:08:55	U	SMPL
P4947-01 - 1	A3988	-222	-0.0007	-	7470A	PPB	25 Nov 2024 12:11:11	U	SMPL
P4947-01DUP - 1	A3988DUP	-42	0.0397	-	7470A	PPB	25 Nov 2024 12:13:30	U	SMPL
P4947-01MS - 1	A3988MS	15727	3.5720	-	7470A	PPB	25 Nov 2024 12:18:32	U	SMPL
P4947-01MSD - 1	A3988MSD	15095	3.4304	-	7470A	PPB	25 Nov 2024 12:20:49	U	SMPL
P4949-01 - 1	REACTOR-SUMP	348	0.1270	-	7470A	PPB	25 Nov 2024 12:23:07	U	SMPL
CCV47 - 1	CCV47	21640	4.8965	-	7470A	PPB	25 Nov 2024 12:40:14	U	SMPL
CCB47 - 1	CCB47	-258	-0.0087	-	7470A	PPB	25 Nov 2024 12:42:29	U	SMPL
P4972-05 - 1	628-F	4725	1.1075	-	7470A	PPB	25 Nov 2024 12:44:47	U	SMPL
P4947-01LX5 - 1		-730	-0.1145	-	7470A	PPB	25 Nov 2024 12:47:02	U	SMPL
P4947-01A - 1		14631	3.3265	-	7470A	PPB	25 Nov 2024 12:49:21	U	SMPL
CCV48 - 1	CCV48	20445	4.6289	-	7470A	PPB	25 Nov 2024 12:55:36	U	SMPL
CCB48 - 1	CCB48	-108	0.0249	-	7470A	PPB	25 Nov 2024 12:57:51	U	SMPL