


LB133732

SFAM01.1 INSTRUMENT ID: CV1

Linear

μ Abs.:

40692

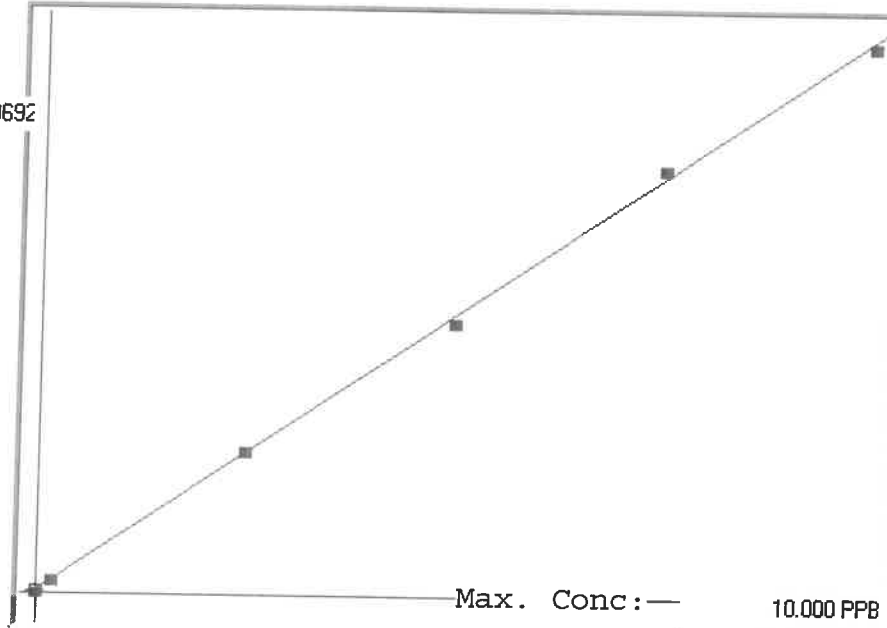

A= 0.0000e+000

B= 2.4470e-004 *slope*

C= -5.4586e-002 *y-intercept*

Rho= 0.9996141

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	<i>o/d</i>
0.00	0.000	-0.017	-0.017	153	0.000	153	0				<i>=</i>
0.05	0.050					442	0				<i>67</i>
0.20	0.200	0.213	0.013	1095	0.0 %	1095					<i>12/5/21</i>
2.50	2.500	2.532	0.032	10569	0.0 %	10569					<i>1</i>
5.00	5.000	4.877	-0.123	20154	0.0 %	20154					<i>-2</i>
7.50	7.500	7.692	0.192	31659	0.0 %	31659					<i>3</i>
10.0	10.000	9.903	-0.097	40692	0.0 %	40692					<i>-1</i>

LB133732

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	153	-		0 SFAM01.1	PPB	12/4/2024 13:15	Std
	0.2 S01	1095	-		0.2 SFAM01.1	PPB	12/4/2024 13:17	Std
	2.5 S02	10569	-		2.5 SFAM01.1	PPB	12/4/2024 13:20	Std
	5 S03	20154	-		5 SFAM01.1	PPB	12/4/2024 13:24	Std
	7.5 S04	31659	-		7.5 SFAM01.1	PPB	12/4/2024 13:26	Std
	10 S05	40692	-		10 SFAM01.1	PPB	12/4/2024 13:31	Std
ICV006	ICV006	16620	4.0123 -		SFAM01.1	PPB	12/4/2024 13:34	SMPL
ICB006	ICB006	85	-0.0338 -		SFAM01.1	PPB	12/4/2024 13:36	SMPL
CCV083	CCV083	19882	4.8105 -		SFAM01.1	PPB	12/4/2024 13:38	SMPL
CCB083	CCB083	48	-0.0428 -		SFAM01.1	PPB	12/4/2024 13:41	SMPL
PB165376BL	PBS376	168	-0.0135 -		SFAM01.1	PPB	12/4/2024 13:43	SMPL
P4776-03	MDL-SOIL	371	0.0362 -		SFAM01.1	PPB	12/4/2024 14:00	SMPL
CCV084	CCV084	19787	4.7873 -		SFAM01.1	PPB	12/4/2024 14:02	SMPL
CCB084	CCB084	13	-0.0514 -		SFAM01.1	PPB	12/4/2024 14:05	SMPL