

| Instrument IIC |        | IC-1    | Analyst: |         | NF      | Method: 00.0/9056A |         | Method name |  | date time        | il wt/Fin | Analyst |
|----------------|--------|---------|----------|---------|---------|--------------------|---------|-------------|--|------------------|-----------|---------|
| Ident          | Con F- | Con CL- | Con NO2  | Con BR- | Con NO3 | Con HPO4           | Con SO4 |             |  |                  |           |         |
| STD1           | 0      | 0       | 0        | 0       | 0       | 0                  | 0       | IC1-111824  |  | 11/18/2024 11:24 | 10        | NF/IZ   |
| STD2           | 0.402  | 0.571   | 0.601    | 1.961   | 0.489   | 1.025              | 3.062   | IC1-111824  |  | 11/18/2024 11:46 | 10        | NF/IZ   |
| STD3           | 0.794  | 1.185   | 1.175    | 3.939   | 0.997   | 1.928              | 6.062   | IC1-111824  |  | 11/18/2024 12:07 | 10        | NF/IZ   |
| STD4           | 1.023  | 1.554   | 1.535    | 5.128   | 1.284   | 2.665              | 7.843   | IC1-111824  |  | 11/18/2024 12:29 | 10        | NF/IZ   |
| STD5           | 1.997  | 3.009   | 2.993    | 9.997   | 2.488   | 4.96               | 14.679  | IC1-111824  |  | 11/18/2024 12:50 | 10        | NF/IZ   |
| STD6           | 3.936  | 5.952   | 5.978    | 19.928  | 4.964   | 9.645              | 28.993  | IC1-111824  |  | 11/18/2024 13:11 | 10        | NF/IZ   |
| STD7           | 5.049  | 7.529   | 7.517    | 25.045  | 6.279   | 12.776             | 37.863  | IC1-111824  |  | 11/18/2024 13:33 | 10        | NF/IZ   |
| ICV            | 1.966  | 3.006   | 2.997    | 9.98    | 2.49    | 4.979              | 14.594  | IC1-111824  |  | 11/18/2024 13:54 | 10        | NF/IZ   |
| ICB            | 0      | 0       | 0        | 0       | 0       | 0                  | 0       | IC1-111824  |  | 11/18/2024 14:16 | 10        | NF/IZ   |
| CCV            | 1.973  | 2.997   | 3.032    | 10.094  | 2.498   | 4.705              | 14.554  | IC1-111824  |  | 12/6/2024 10:41  | 10        | NF/IZ   |
| CCB            | 0      | 0       | 0        | 0       | 0       | 0                  | 0       | IC1-111824  |  | 12/6/2024 11:02  | 10        | NF/IZ   |
| LB133778BLW    | 0      | 0       | 0        | 0       | 0       | 0                  | 0       | IC1-111824  |  | 12/6/2024 11:24  | 10        | NF/IZ   |
| LB133778BSW    | 1.989  | 3.007   | 3.041    | 10.128  | 2.507   | 4.927              | 14.566  | IC1-111824  |  | 12/6/2024 11:45  | 10        | NF/IZ   |
| P5145-01       | 0.136  | 6.785   | 0.048    | 0       | 0.215   | 0                  | 13.49   | IC1-111824  |  | 12/6/2024 12:07  | 10        | NF/IZ   |
| P5145-01MS     | 2.16   | 9.662   | 3.123    | 10.329  | 2.771   | 4.92               | 28.206  | IC1-111824  |  | 12/6/2024 12:28  | 10        | NF/IZ   |
| P5145-01MSD    | 2.158  | 9.662   | 3.124    | 10.34   | 2.779   | 5.047              | 28.135  | IC1-111824  |  | 12/6/2024 12:50  | 10        | NF/IZ   |
| CCV            | 2.1    | 3.149   | 3.188    | 10.601  | 2.627   | 5.111              | 15.241  | IC1-111824  |  | 12/6/2024 13:12  | 10        | NF/IZ   |
| CCB            | 0      | 0       | 0        | 0       | 0       | 0                  | 0       | IC1-111824  |  | 12/6/2024 13:33  | 10        | NF/IZ   |


Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A

| ident | concentra<br>tion F- | concentratio<br>n CL- | concentrati<br>on NO2 | concentrati<br>on BR- | concentrati<br>on NO3 | concentrati<br>on HPO4 | concentrati<br>on SO4 | file name  | date time        | Initial<br>wt/<br>Final | Analyst |
|-------|----------------------|-----------------------|-----------------------|-----------------------|-----------------------|------------------------|-----------------------|------------|------------------|-------------------------|---------|
| STD1  | 0.000                | 0.000                 | 0.000                 | 0.000                 | 0.000                 | 0.000                  | 0.000                 | IC1-111824 | 11/18/2024 11:24 | 10                      | NF/IZ   |
| STD2  | 0.402                | 0.571                 | 0.601                 | 1.961                 | 0.489                 | 1.025                  | 3.062                 | IC1-111824 | 11/18/2024 11:46 | 10                      | NF/IZ   |
| STD3  | 0.794                | 1.185                 | 1.175                 | 3.939                 | 0.997                 | 1.928                  | 6.062                 | IC1-111824 | 11/18/2024 12:07 | 10                      | NF/IZ   |
| STD4  | 1.023                | 1.554                 | 1.535                 | 5.128                 | 1.284                 | 2.665                  | 7.843                 | IC1-111824 | 11/18/2024 12:29 | 10                      | NF/IZ   |
| STD5  | 1.997                | 3.009                 | 2.993                 | 9.997                 | 2.488                 | 4.960                  | 14.679                | IC1-111824 | 11/18/2024 12:50 | 10                      | NF/IZ   |
| STD6  | 3.936                | 5.952                 | 5.978                 | 19.928                | 4.964                 | 9.645                  | 28.993                | IC1-111824 | 11/18/2024 13:11 | 10                      | NF/IZ   |
| STD7  | 5.049                | 7.529                 | 7.517                 | 25.045                | 6.279                 | 12.776                 | 37.863                | IC1-111824 | 11/18/2024 13:33 | 10                      | NF/IZ   |

| ident | True<br>Value F- | True Value<br>CL- | True Value<br>NO2 | True Value<br>BR- | True Value<br>NO3 | True Value<br>HPO4 | True Value<br>SO4 |
|-------|------------------|-------------------|-------------------|-------------------|-------------------|--------------------|-------------------|
| STD1  | 0.0000           | 0.0000            | 0.0000            | 0.0000            | 0.0000            | 0.0000             | 0.0000            |
| STD2  | 0.4000           | 0.6000            | 0.6000            | 2.0000            | 0.5000            | 1.0000             | 3.0000            |
| STD3  | 0.8000           | 1.2000            | 1.2000            | 4.0000            | 1.0000            | 2.0000             | 6.0000            |
| STD4  | 1.0000           | 1.5000            | 1.5000            | 5.0000            | 1.2500            | 2.5000             | 7.5000            |
| STD5  | 2.0000           | 3.0000            | 3.0000            | 10.0000           | 2.5000            | 5.0000             | 15.0000           |
| STD6  | 4.0000           | 6.0000            | 6.0000            | 20.0000           | 5.0000            | 10.0000            | 30.0000           |
| STD7  | 5.0000           | 7.5000            | 7.5000            | 25.0000           | 6.2500            | 12.5000            | 37.0000           |

| ident | Relative<br>Error F- | Relative<br>Error CL- | Relative<br>Error NO2 | Relative<br>Error BR- | Relative<br>Error NO3 | Relative<br>Error HPO4 | Relative<br>Error SO4 |
|-------|----------------------|-----------------------|-----------------------|-----------------------|-----------------------|------------------------|-----------------------|
| STD1  |                      |                       |                       |                       |                       |                        |                       |
| STD2  | 0.5000               | -4.8333               | 0.1667                | -1.9500               | -2.2000               | 2.5000                 | 2.0667                |
| STD3  | -0.7500              | -1.2500               | -2.0833               | -1.5250               | -0.3000               | -3.6000                | 1.0333                |
| STD4  | 2.3000               | 3.6000                | 2.3333                | 2.5600                | 2.7200                | 6.6000                 | 4.5733                |
| STD5  | -0.1500              | 0.3000                | -0.2333               | -0.0300               | -0.4800               | -0.8000                | -2.1400               |
| STD6  | -1.6000              | -0.8000               | -0.3667               | -0.3600               | -0.7200               | -3.5500                | -3.3567               |
| STD7  | 0.9800               | 0.3667                | 0.2267                | 0.1800                | 0.4640                | 2.2080                 | 2.3324                |

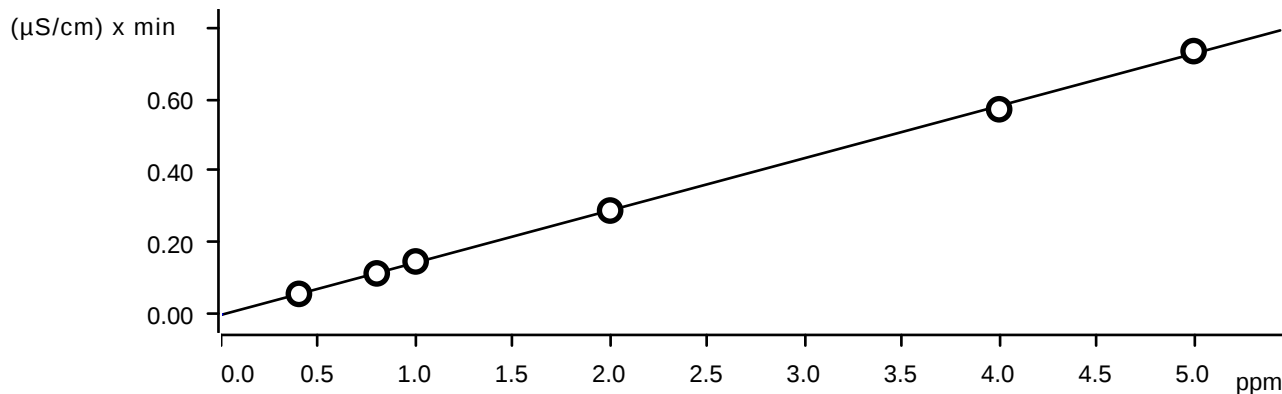
**Fluoride (Anions)**

Function: . . . . .  $A = -1.48773\text{E-}3 + 0.0145652 \times Q$

Relative standard deviation . . . . . 1.923523 %

Correlation coefficient . . . . . 0.999800


| Sample type | Index | Conc. | Volume | Dilution | Sample amount | Area  | Ident | Date                      | Used |
|-------------|-------|-------|--------|----------|---------------|-------|-------|---------------------------|------|
| Standard 1  | 1     | 0.000 | 10.0   | 1.0      | 1.0           | n. d. | STD1  | 2024-11-18 11:24:52 UTC-5 | used |
| Standard 2  | 1     | 0.400 | 10.0   | 1.0      | 1.0           | 0.057 | STD2  | 2024-11-18 11:46:16 UTC-5 | used |
| Standard 3  | 1     | 0.800 | 10.0   | 1.0      | 1.0           | 0.114 | STD3  | 2024-11-18 12:07:40 UTC-5 | used |
| Standard 4  | 1     | 1.000 | 10.0   | 1.0      | 1.0           | 0.147 | STD4  | 2024-11-18 12:29:05 UTC-5 | used |
| Standard 5  | 1     | 2.000 | 10.0   | 1.0      | 1.0           | 0.289 | STD5  | 2024-11-18 12:50:30 UTC-5 | used |
| Standard 6  | 1     | 4.000 | 10.0   | 1.0      | 1.0           | 0.572 | STD6  | 2024-11-18 13:11:57 UTC-5 | used |
| Standard 7  | 1     | 5.000 | 10.0   | 1.0      | 1.0           | 0.734 | STD7  | 2024-11-18 13:33:24 UTC-5 | used |

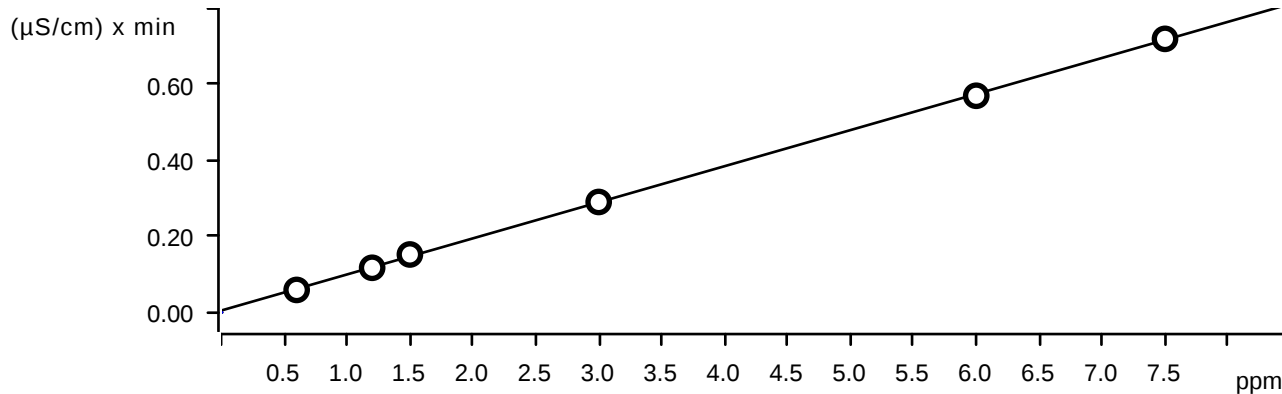**Chloride (Anions)**

Function: . . . . .  $A = 4.85841\text{E-}3 + 9.50243\text{E-}3 \times Q$

Relative standard deviation . . . . . 1.265280 %  
Correlation coefficient . . . . . 0.999910

| Sample type | Index | Conc. | Volume | Dilution | Sample amount | Area  | Ident | Date                      | Used |
|-------------|-------|-------|--------|----------|---------------|-------|-------|---------------------------|------|
| Standard 1  | 1     | 0.000 | 10.0   | 1.0      | 1.0           | n. d. | STD1  | 2024-11-18 11:24:52 UTC-5 | used |
| Standard 2  | 1     | 0.600 | 10.0   | 1.0      | 1.0           | 0.059 | STD2  | 2024-11-18 11:46:16 UTC-5 | used |
| Standard 3  | 1     | 1.200 | 10.0   | 1.0      | 1.0           | 0.117 | STD3  | 2024-11-18 12:07:40 UTC-5 | used |
| Standard 4  | 1     | 1.500 | 10.0   | 1.0      | 1.0           | 0.153 | STD4  | 2024-11-18 12:29:05 UTC-5 | used |
| Standard 5  | 1     | 3.000 | 10.0   | 1.0      | 1.0           | 0.291 | STD5  | 2024-11-18 12:50:30 UTC-5 | used |
| Standard 6  | 1     | 6.000 | 10.0   | 1.0      | 1.0           | 0.570 | STD6  | 2024-11-18 13:11:57 UTC-5 | used |
| Standard 7  | 1     | 7.500 | 10.0   | 1.0      | 1.0           | 0.720 | STD7  | 2024-11-18 13:33:24 UTC-5 | used |

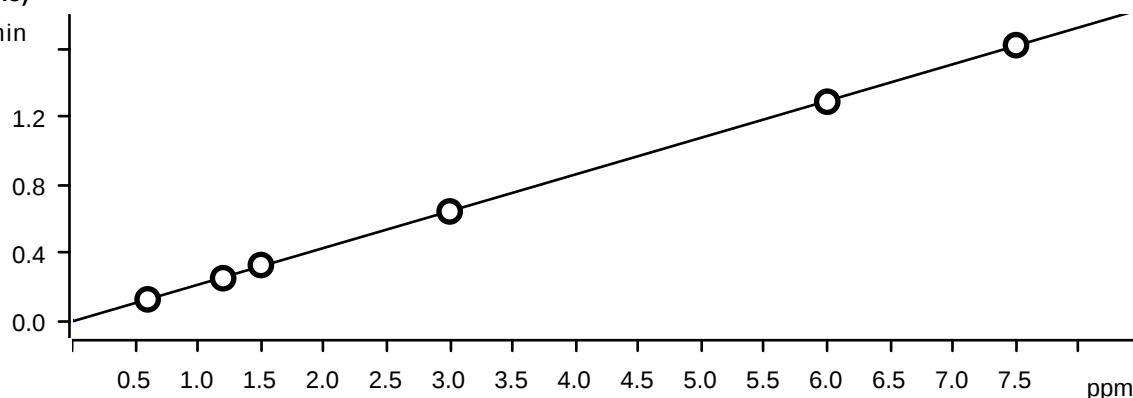
**Nitrite (Anions)** $(\mu\text{S/cm}) \times \text{min}$ 

Function: . . . . .  $A = -5.27414E-3 + 0.0216316 \times Q$   
Relative standard deviation . . . . . 0.783603 %  
Correlation coefficient . . . . . 0.999967

| Sample type | Index | Conc. | Volume | Dilution | Sample amount | Area  | Ident | Date                      | Used |
|-------------|-------|-------|--------|----------|---------------|-------|-------|---------------------------|------|
| Standard 1  | 1     | 0.000 | 10.0   | 1.0      | 1.0           | n. d. | STD1  | 2024-11-18 11:24:52 UTC-5 | used |
| Standard 2  | 1     | 0.600 | 10.0   | 1.0      | 1.0           | 0.125 | STD2  | 2024-11-18 11:46:16 UTC-5 | used |
| Standard 3  | 1     | 1.200 | 10.0   | 1.0      | 1.0           | 0.249 | STD3  | 2024-11-18 12:07:40 UTC-5 | used |
| Standard 4  | 1     | 1.500 | 10.0   | 1.0      | 1.0           | 0.327 | STD4  | 2024-11-18 12:29:05 UTC-5 | used |
| Standard 5  | 1     | 3.000 | 10.0   | 1.0      | 1.0           | 0.642 | STD5  | 2024-11-18 12:50:30 UTC-5 | used |
| Standard 6  | 1     | 6.000 | 10.0   | 1.0      | 1.0           | 1.288 | STD6  | 2024-11-18 13:11:57 UTC-5 | used |
| Standard 7  | 1     | 7.500 | 10.0   | 1.0      | 1.0           | 1.621 | STD7  | 2024-11-18 13:33:24 UTC-5 | used |

# Bromide (Anions)

( $\mu\text{S}/\text{cm}$ )  $\times$  min

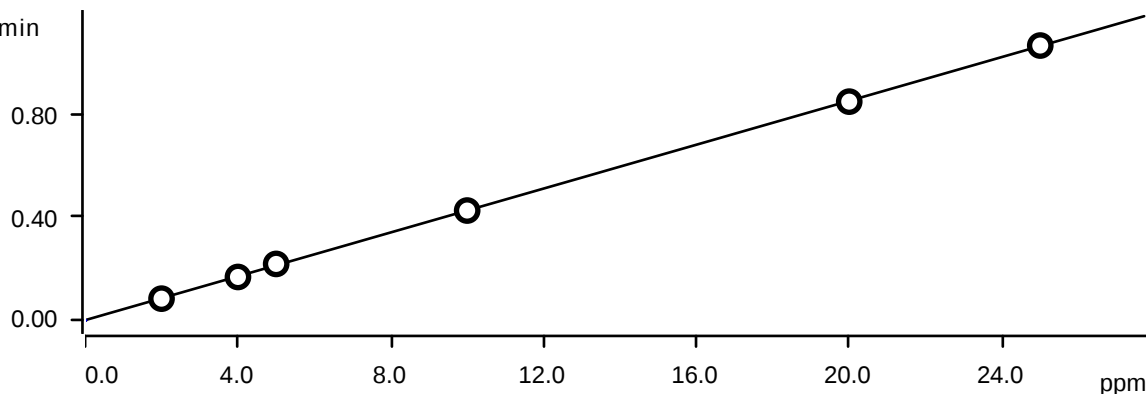

Function: . . . . .  $A = 7.64331E-4 + 4.24604E-3 \times Q$


Relative standard deviation . . . . . 0.771268 %

Correlation coefficient . . . . . 0.999967

| Sample type | Index | Conc.  | Volume | Dilution | Sample amount | Area  | Ident | Date                      | Used |
|-------------|-------|--------|--------|----------|---------------|-------|-------|---------------------------|------|
| Standard 1  | 1     | 0.000  | 10.0   | 1.0      | 1.0           | n. d. | STD1  | 2024-11-18 11:24:52 UTC-5 | used |
| Standard 2  | 1     | 2.000  | 10.0   | 1.0      | 1.0           | 0.084 | STD2  | 2024-11-18 11:46:16 UTC-5 | used |
| Standard 3  | 1     | 4.000  | 10.0   | 1.0      | 1.0           | 0.168 | STD3  | 2024-11-18 12:07:40 UTC-5 | used |
| Standard 4  | 1     | 5.000  | 10.0   | 1.0      | 1.0           | 0.219 | STD4  | 2024-11-18 12:29:05 UTC-5 | used |
| Standard 5  | 1     | 10.000 | 10.0   | 1.0      | 1.0           | 0.425 | STD5  | 2024-11-18 12:50:30 UTC-5 | used |
| Standard 6  | 1     | 20.000 | 10.0   | 1.0      | 1.0           | 0.847 | STD6  | 2024-11-18 13:11:57 UTC-5 | used |
| Standard 7  | 1     | 25.000 | 10.0   | 1.0      | 1.0           | 1.064 | STD7  | 2024-11-18 13:33:24 UTC-5 | used |

# Nitrate (Anions)

( $\mu\text{S}/\text{cm}$ )  $\times$  min

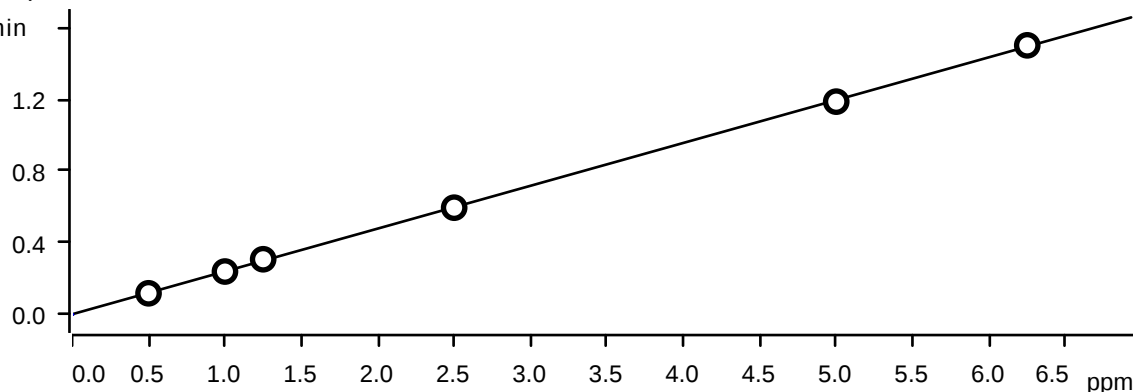


Function: . . . . .  $A = 1.14484E-3 + 0.0238833 \times Q$

Relative standard deviation . . . . . 1.085494 %

Correlation coefficient . . . . . 0.999936

| Sample type | Index | Conc. | Volume | Dilution | Sample amount | Area  | Ident | Date                      | Used |
|-------------|-------|-------|--------|----------|---------------|-------|-------|---------------------------|------|
| Standard 1  | 1     | 0.000 | 10.0   | 1.0      | 1.0           | n. d. | STD1  | 2024-11-18 11:24:52 UTC-5 | used |
| Standard 2  | 1     | 0.500 | 10.0   | 1.0      | 1.0           | 0.118 | STD2  | 2024-11-18 11:46:16 UTC-5 | used |
| Standard 3  | 1     | 1.000 | 10.0   | 1.0      | 1.0           | 0.239 | STD3  | 2024-11-18 12:07:40 UTC-5 | used |
| Standard 4  | 1     | 1.250 | 10.0   | 1.0      | 1.0           | 0.308 | STD4  | 2024-11-18 12:29:05 UTC-5 | used |
| Standard 5  | 1     | 2.500 | 10.0   | 1.0      | 1.0           | 0.595 | STD5  | 2024-11-18 12:50:30 UTC-5 | used |
| Standard 6  | 1     | 5.000 | 10.0   | 1.0      | 1.0           | 1.187 | STD6  | 2024-11-18 13:11:57 UTC-5 | used |
| Standard 7  | 1     | 6.250 | 10.0   | 1.0      | 1.0           | 1.501 | STD7  | 2024-11-18 13:33:24 UTC-5 | used |

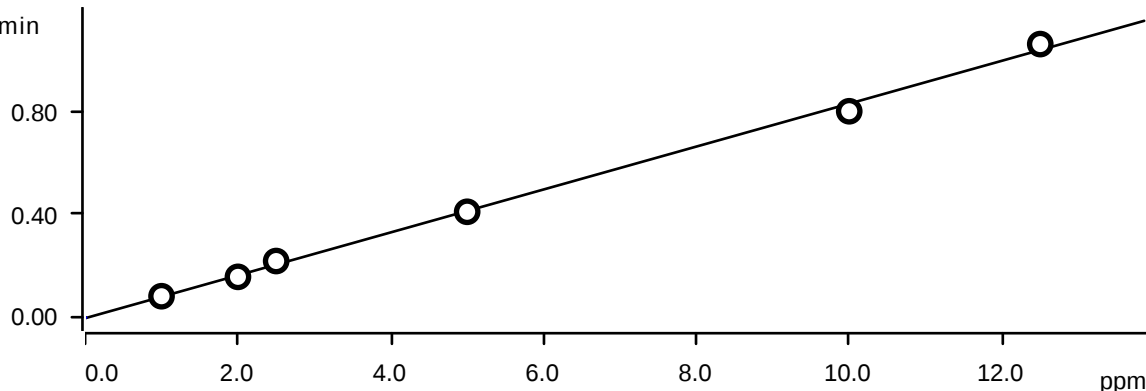
**Phosphate (Anions)** $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: . . . . .  $A = -2.33576E-3 + 8.30878E-3 \times Q$ 

Relative standard deviation . . . . . 4.444706 %

Correlation coefficient . . . . . 0.998936

| Sample type | Index | Conc.  | Volume | Dilution | Sample amount | Area  | Ident | Date                      | Used |
|-------------|-------|--------|--------|----------|---------------|-------|-------|---------------------------|------|
| Standard 1  | 1     | 0.000  | 10.0   | 1.0      | 1.0           | n. d. | STD1  | 2024-11-18 11:24:52 UTC-5 | used |
| Standard 2  | 1     | 1.000  | 10.0   | 1.0      | 1.0           | 0.083 | STD2  | 2024-11-18 11:46:16 UTC-5 | used |
| Standard 3  | 1     | 2.000  | 10.0   | 1.0      | 1.0           | 0.158 | STD3  | 2024-11-18 12:07:40 UTC-5 | used |
| Standard 4  | 1     | 2.500  | 10.0   | 1.0      | 1.0           | 0.219 | STD4  | 2024-11-18 12:29:05 UTC-5 | used |
| Standard 5  | 1     | 5.000  | 10.0   | 1.0      | 1.0           | 0.410 | STD5  | 2024-11-18 12:50:30 UTC-5 | used |
| Standard 6  | 1     | 10.000 | 10.0   | 1.0      | 1.0           | 0.799 | STD6  | 2024-11-18 13:11:57 UTC-5 | used |
| Standard 7  | 1     | 12.500 | 10.0   | 1.0      | 1.0           | 1.059 | STD7  | 2024-11-18 13:33:24 UTC-5 | used |

## Sulfate (Anions)

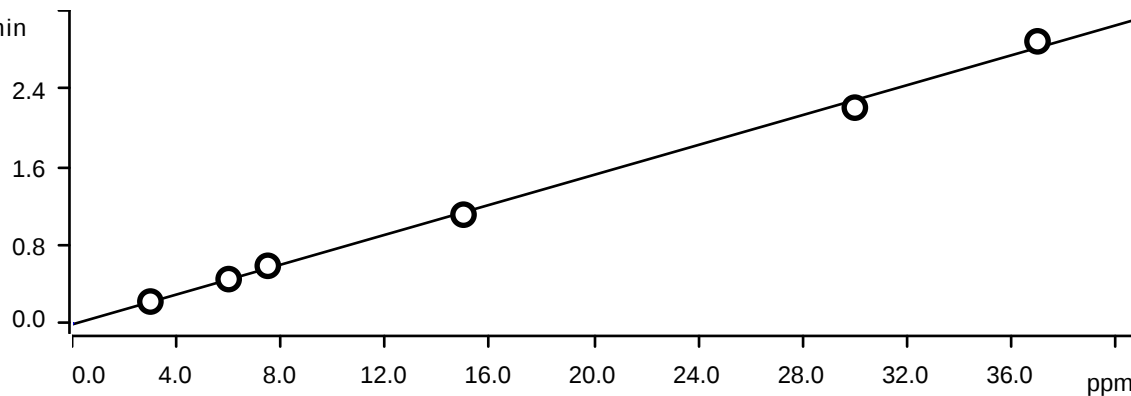 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: . . . . .  $A = -9.71222\text{E-}3 + 7.64397\text{E-}3 \times Q$ 

Relative standard deviation . . . . . 4.327283 %

Correlation coefficient . . . . . 0.998986


| Sample type | Index | Conc.  | Volume | Dilution | Sample amount | Area  | Ident | Date                      | Used |
|-------------|-------|--------|--------|----------|---------------|-------|-------|---------------------------|------|
| Standard 1  | 1     | 0.000  | 10.0   | 1.0      | 1.0           | n. d. | STD1  | 2024-11-18 11:24:52 UTC-5 | used |
| Standard 2  | 1     | 3.000  | 10.0   | 1.0      | 1.0           | 0.224 | STD2  | 2024-11-18 11:46:16 UTC-5 | used |
| Standard 3  | 1     | 6.000  | 10.0   | 1.0      | 1.0           | 0.454 | STD3  | 2024-11-18 12:07:40 UTC-5 | used |
| Standard 4  | 1     | 7.500  | 10.0   | 1.0      | 1.0           | 0.590 | STD4  | 2024-11-18 12:29:05 UTC-5 | used |
| Standard 5  | 1     | 15.000 | 10.0   | 1.0      | 1.0           | 1.112 | STD5  | 2024-11-18 12:50:30 UTC-5 | used |
| Standard 6  | 1     | 30.000 | 10.0   | 1.0      | 1.0           | 2.206 | STD6  | 2024-11-18 13:11:57 UTC-5 | used |
| Standard 7  | 1     | 37.000 | 10.0   | 1.0      | 1.0           | 2.884 | STD7  | 2024-11-18 13:33:24 UTC-5 | used |

**Sample data**

Ident . . . . . STD1  
Sample type . . . . . Standard 1  
Determination start . . . . . 2024-11-18 11:24:52 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

**Anions**

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.60 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

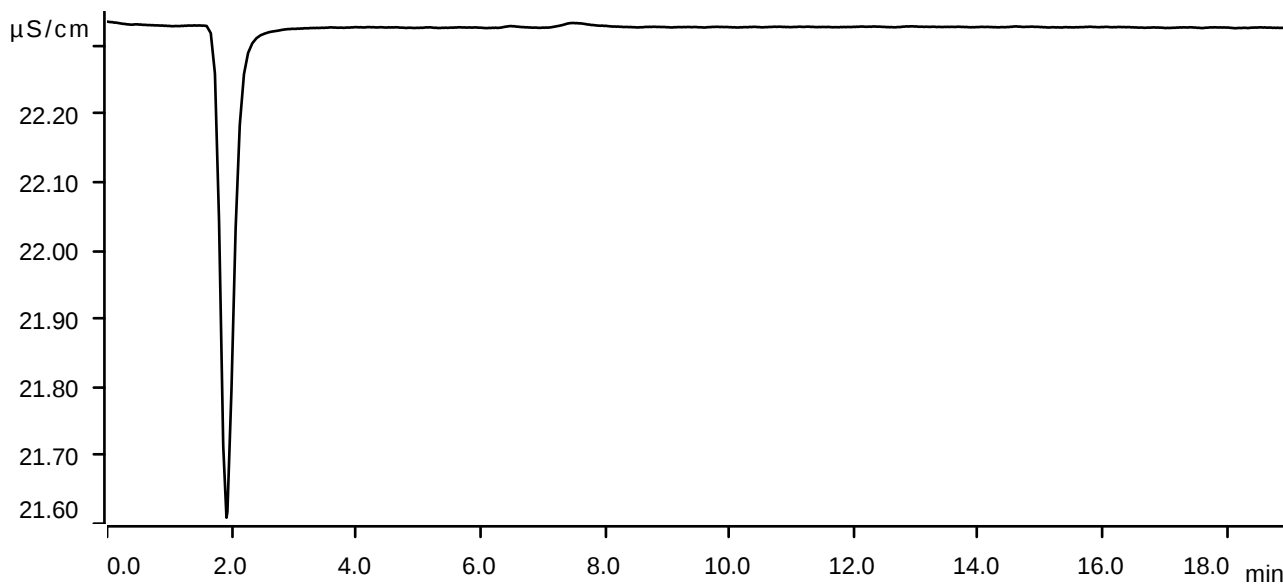**Anions**


## Sample data

Ident . . . . . STD2  
Sample type . . . . . Standard 2  
Determination start . . . . . 2024-11-18 11:46:16 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.54 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

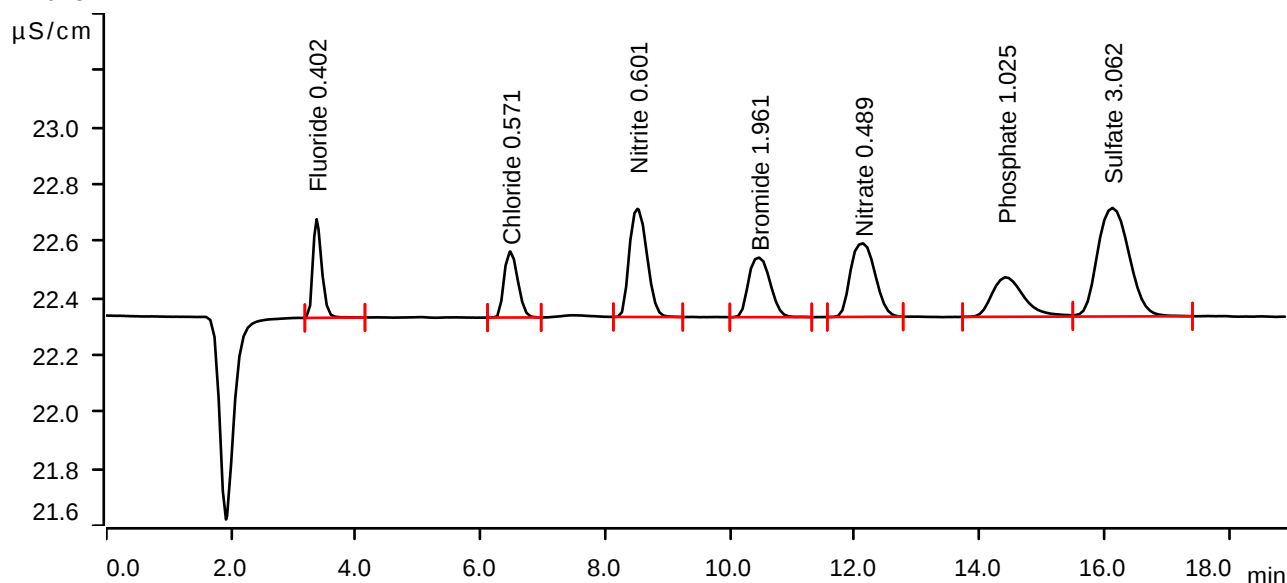

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.372                 | 0.0570                | 0.347           | 0.402                | Fluoride       |
| 2           | 6.477                 | 0.0592                | 0.232           | 0.571                | Chloride       |
| 3           | 8.515                 | 0.1247                | 0.380           | 0.601                | Nitrite        |
| 4           | 10.463                | 0.0840                | 0.209           | 1.961                | Bromide        |
| 5           | 12.127                | 0.1179                | 0.258           | 0.489                | Nitrate        |
| 6           | 14.418                | 0.0829                | 0.139           | 1.025                | Phosphate      |
| 7           | 16.130                | 0.2243                | 0.381           | 3.062                | Sulfate        |


## Sample data

Ident . . . . . STD3  
Sample type . . . . . Standard 3  
Determination start . . . . . 2024-11-18 12:07:40 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.37 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

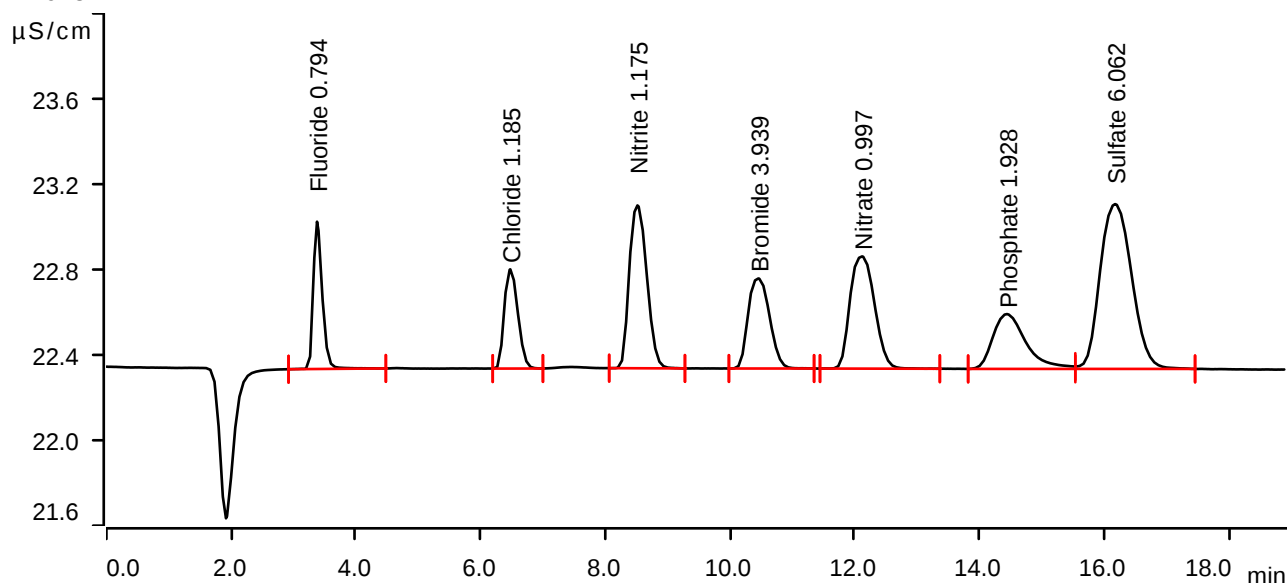

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.378                 | 0.1141                | 0.690           | 0.794                | Fluoride       |
| 2           | 6.478                 | 0.1175                | 0.465           | 1.185                | Chloride       |
| 3           | 8.515                 | 0.2490                | 0.763           | 1.175                | Nitrite        |
| 4           | 10.453                | 0.1680                | 0.422           | 3.939                | Bromide        |
| 5           | 12.117                | 0.2394                | 0.526           | 0.997                | Nitrate        |
| 6           | 14.440                | 0.1579                | 0.257           | 1.928                | Phosphate      |
| 7           | 16.173                | 0.4537                | 0.772           | 6.062                | Sulfate        |


## Sample data

Ident . . . . . STD4  
Sample type . . . . . Standard 4  
Determination start . . . . . 2024-11-18 12:29:05 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.32 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

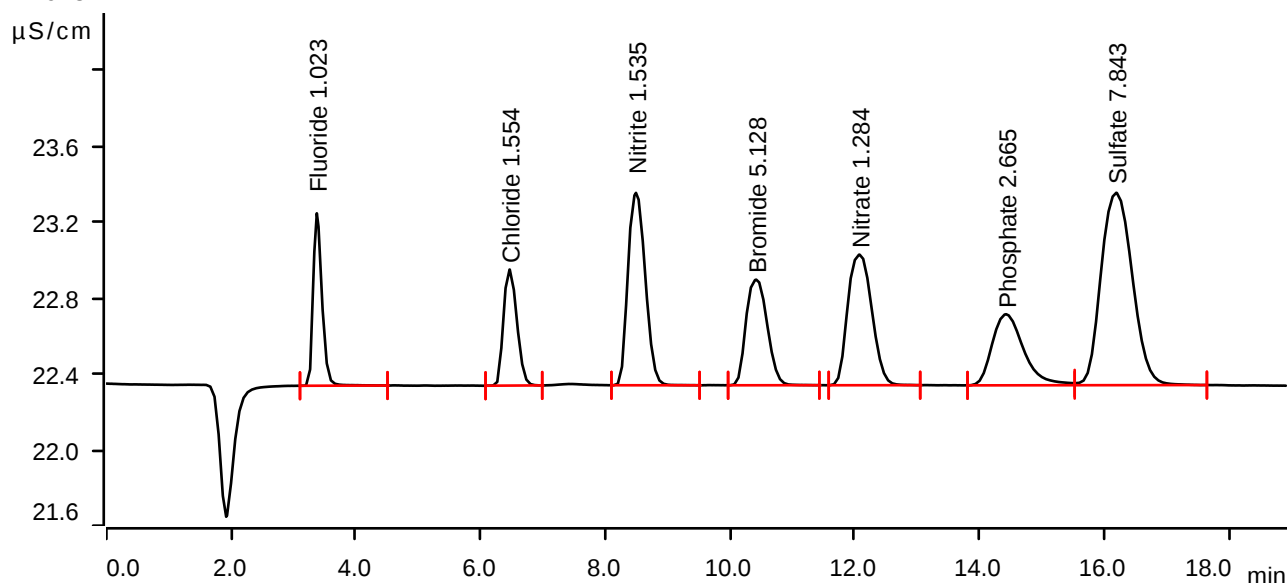

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.375                 | 0.1475                | 0.909           | 1.023                | Fluoride       |
| 2           | 6.465                 | 0.1525                | 0.612           | 1.554                | Chloride       |
| 3           | 8.493                 | 0.3268                | 1.014           | 1.535                | Nitrite        |
| 4           | 10.420                | 0.2185                | 0.557           | 5.128                | Bromide        |
| 5           | 12.077                | 0.3078                | 0.689           | 1.284                | Nitrate        |
| 6           | 14.427                | 0.2191                | 0.375           | 2.665                | Phosphate      |
| 7           | 16.192                | 0.5898                | 1.014           | 7.843                | Sulfate        |


## Sample data

Ident . . . . . STD5  
Sample type . . . . . Standard 5  
Determination start . . . . . 2024-11-18 12:50:30 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.26 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

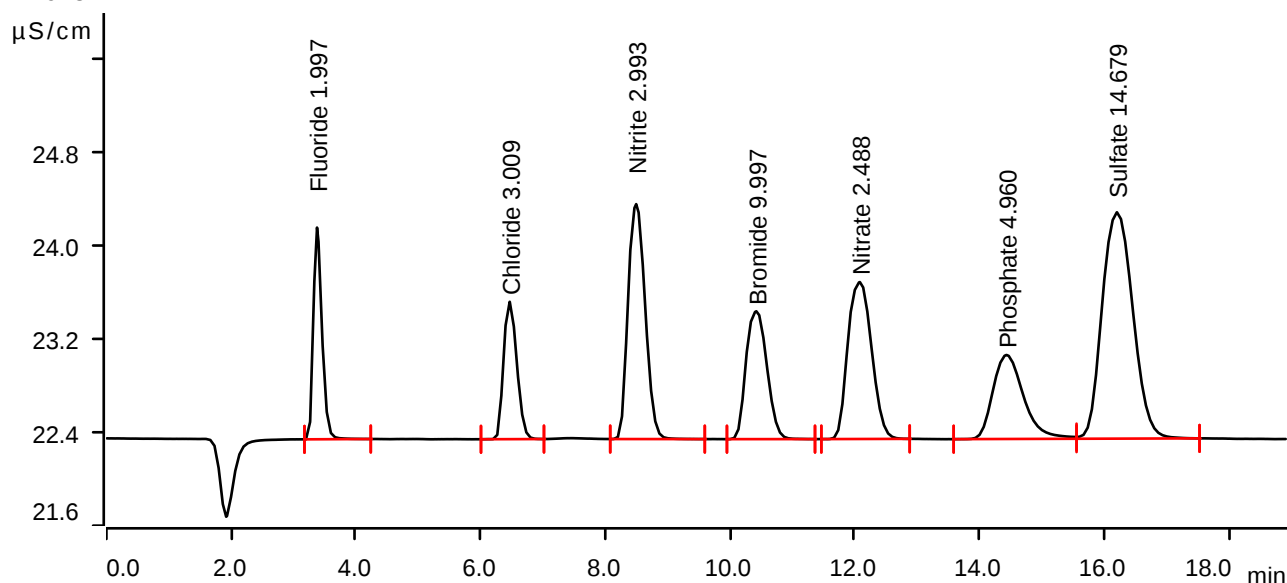

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.378                 | 0.2894                | 1.819           | 1.997                | Fluoride       |
| 2           | 6.467                 | 0.2908                | 1.180           | 3.009                | Chloride       |
| 3           | 8.495                 | 0.6422                | 2.018           | 2.993                | Nitrite        |
| 4           | 10.422                | 0.4253                | 1.098           | 9.997                | Bromide        |
| 5           | 12.082                | 0.5953                | 1.348           | 2.488                | Nitrate        |
| 6           | 14.432                | 0.4098                | 0.722           | 4.960                | Phosphate      |
| 7           | 16.203                | 1.1123                | 1.944           | 14.679               | Sulfate        |


## Sample data

Ident . . . . . STD6  
Sample type . . . . . Standard 6  
Determination start . . . . . 2024-11-18 13:11:57 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.37 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

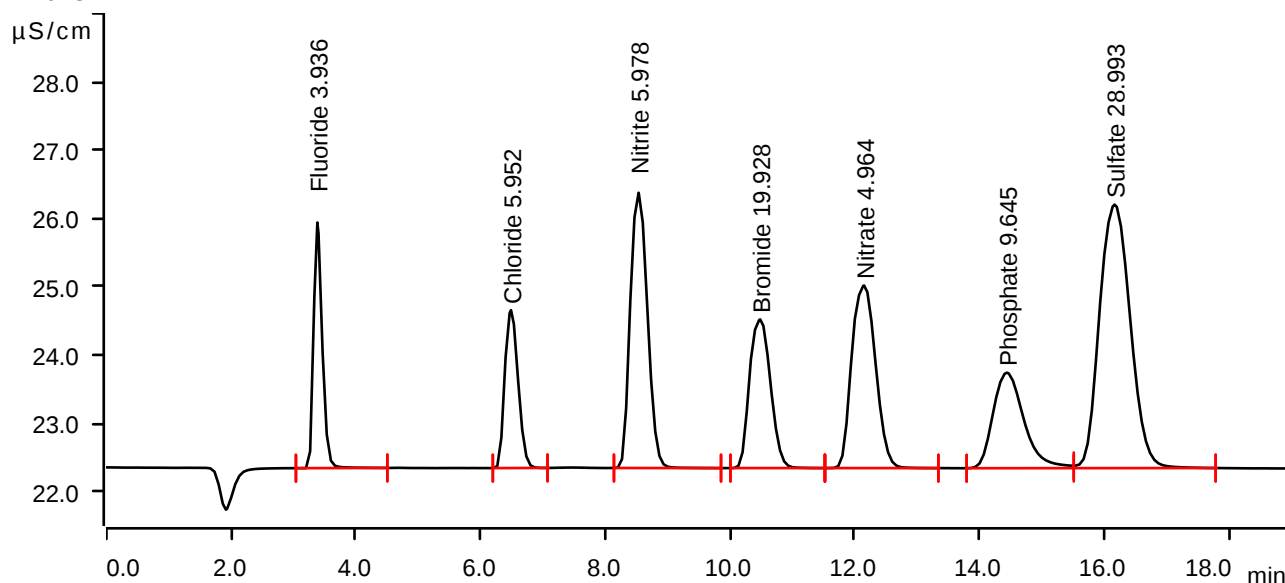

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.383                 | 0.5717                | 3.596           | 3.936                | Fluoride       |
| 2           | 6.488                 | 0.5704                | 2.311           | 5.952                | Chloride       |
| 3           | 8.533                 | 1.2879                | 4.031           | 5.978                | Nitrite        |
| 4           | 10.483                | 0.8469                | 2.176           | 19.928               | Bromide        |
| 5           | 12.148                | 1.1866                | 2.673           | 4.964                | Nitrate        |
| 6           | 14.438                | 0.7991                | 1.399           | 9.645                | Phosphate      |
| 7           | 16.165                | 2.2065                | 3.859           | 28.993               | Sulfate        |


## Sample data

Ident . . . . . STD7  
Sample type . . . . . Standard 7  
Determination start . . . . . 2024-11-18 13:33:24 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.54 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

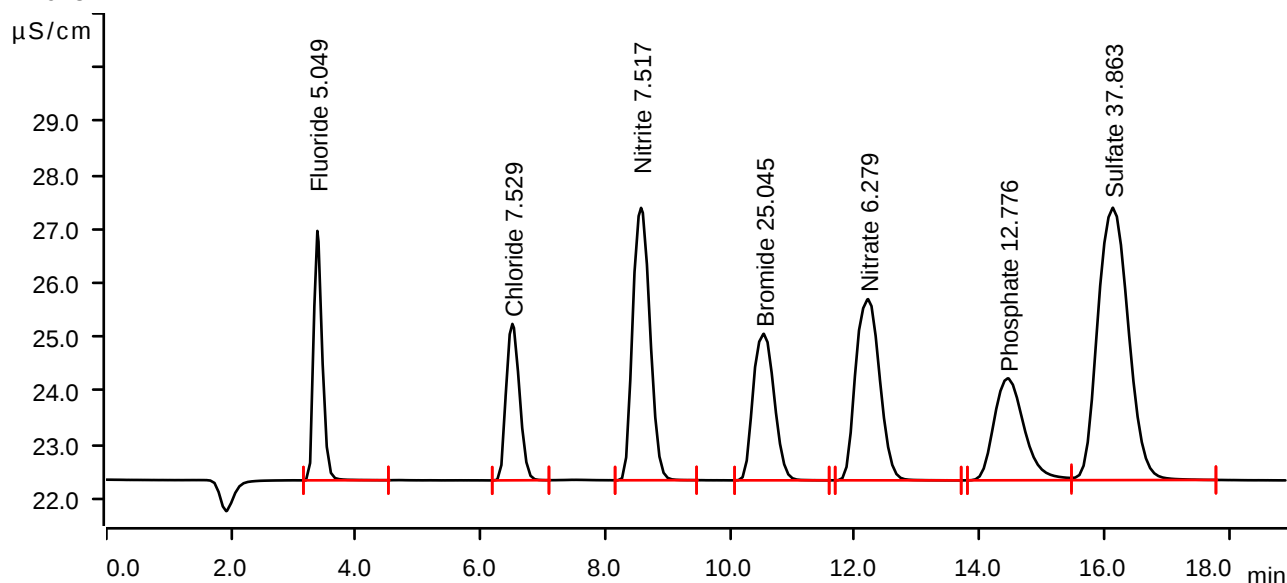

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.383                 | 0.7339                | 4.626           | 5.049                | Fluoride       |
| 2           | 6.510                 | 0.7203                | 2.901           | 7.529                | Chloride       |
| 3           | 8.573                 | 1.6208                | 5.052           | 7.517                | Nitrite        |
| 4           | 10.542                | 1.0642                | 2.717           | 25.045               | Bromide        |
| 5           | 12.213                | 1.5007                | 3.361           | 6.279                | Nitrate        |
| 6           | 14.452                | 1.0592                | 1.891           | 12.776               | Phosphate      |
| 7           | 16.138                | 2.8845                | 5.052           | 37.863               | Sulfate        |


## Sample data

Ident . . . . . ICV  
Sample type . . . . . Check standard 1  
Determination start . . . . . 2024-11-18 13:54:44 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.66 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

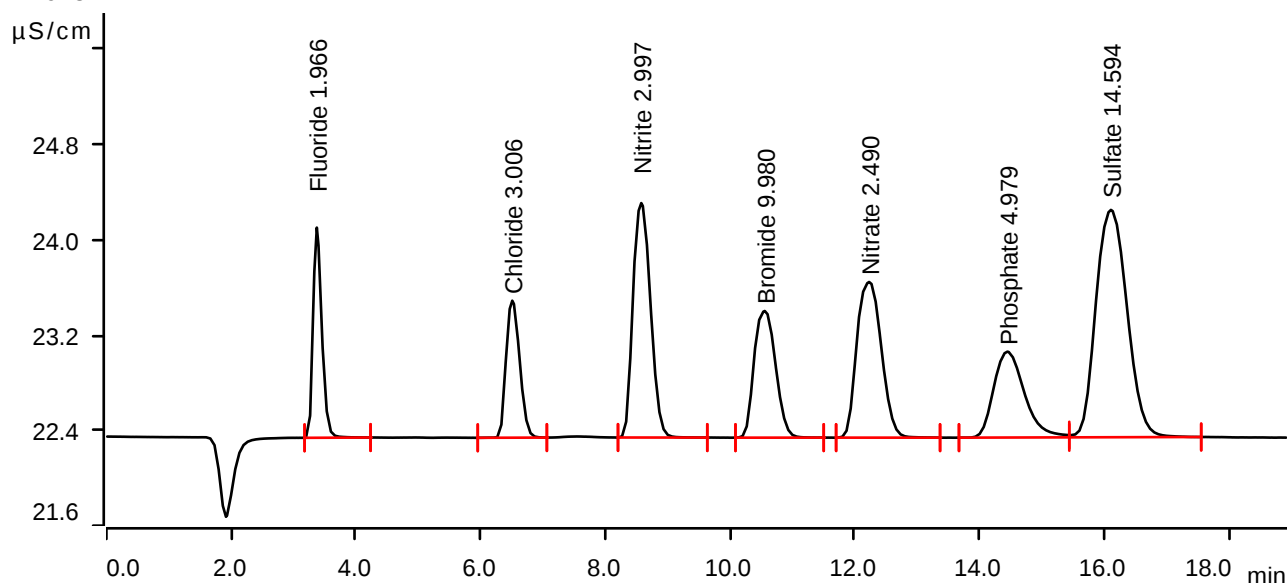


| Peak number | Retention time | Area          | Height | Concentration | Component name |
|-------------|----------------|---------------|--------|---------------|----------------|
|             | min            | (µS/cm) x min | µS/cm  | ppm           |                |
| 1           | 3.375          | 0.2848        | 1.764  | 1.966         | Fluoride       |
| 2           | 6.508          | 0.2905        | 1.150  | 3.006         | Chloride       |
| 3           | 8.577          | 0.6430        | 1.968  | 2.997         | Nitrite        |
| 4           | 10.557         | 0.4245        | 1.063  | 9.980         | Bromide        |
| 5           | 12.230         | 0.5959        | 1.307  | 2.490         | Nitrate        |
| 6           | 14.447         | 0.4114        | 0.721  | 4.979         | Phosphate      |
| 7           | 16.107         | 1.1058        | 1.909  | 14.594        | Sulfate        |

**Sample data**

Ident . . . . . ICB  
Sample type . . . . . Sample  
Determination start . . . . . 2024-11-18 14:16:12 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

**Anions**

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.66 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

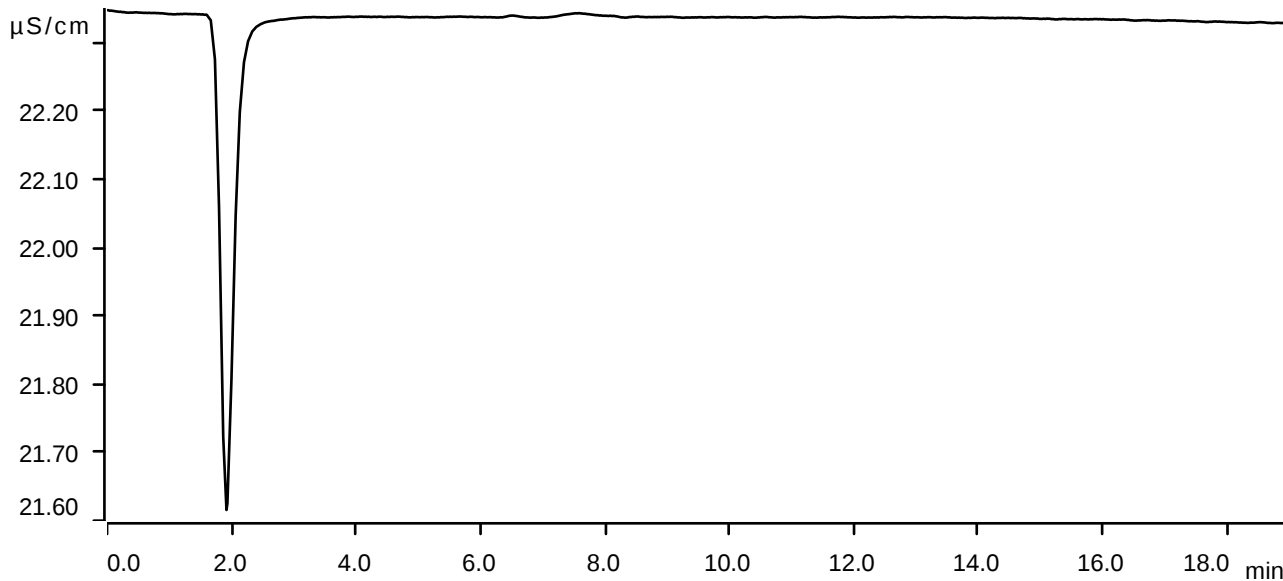**Anions**


## Sample data

Ident . . . . . CCV  
Sample type . . . . . Check standard 1  
Determination start . . . . . 2024-12-06 10:41:24 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 13.06 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

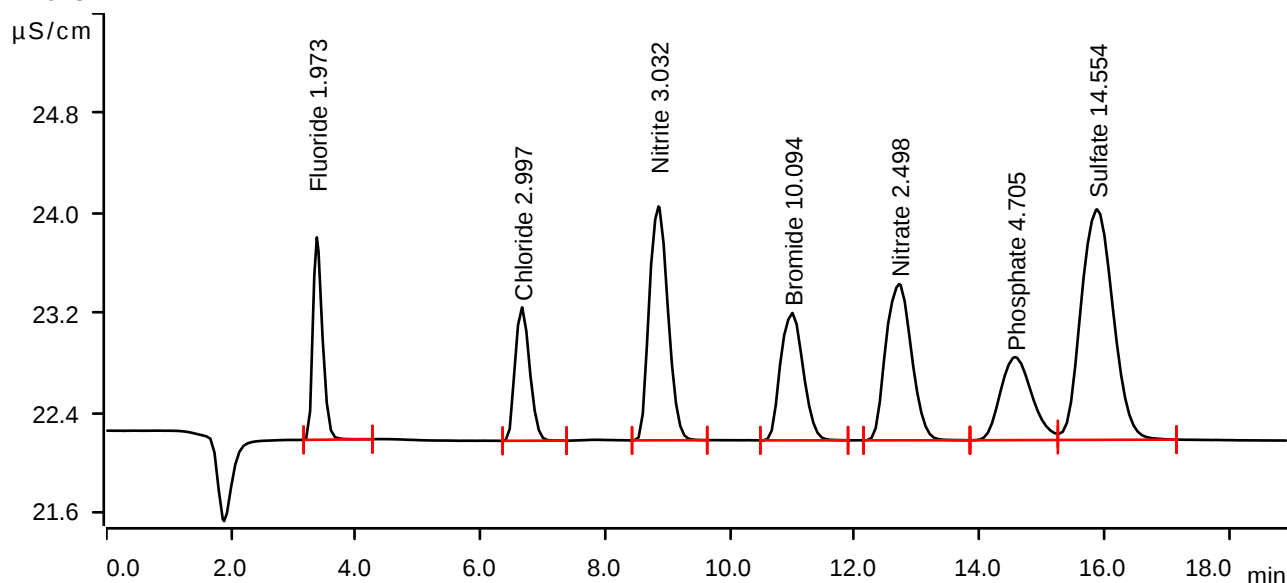


| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.375                 | 0.2858                | 1.620           | 1.973                | Fluoride       |
| 2           | 6.665                 | 0.2896                | 1.068           | 2.997                | Chloride       |
| 3           | 8.853                 | 0.6506                | 1.872           | 3.032                | Nitrite        |
| 4           | 10.998                | 0.4294                | 1.020           | 10.094               | Bromide        |
| 5           | 12.712                | 0.5978                | 1.251           | 2.498                | Nitrate        |
| 6           | 14.568                | 0.3886                | 0.665           | 4.705                | Phosphate      |
| 7           | 15.883                | 1.1028                | 1.845           | 14.554               | Sulfate        |

**Sample data**

Ident . . . . . CCB  
Sample type . . . . . Sample  
Determination start . . . . . 2024-12-06 11:02:54 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

**Anions**

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 13.06 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

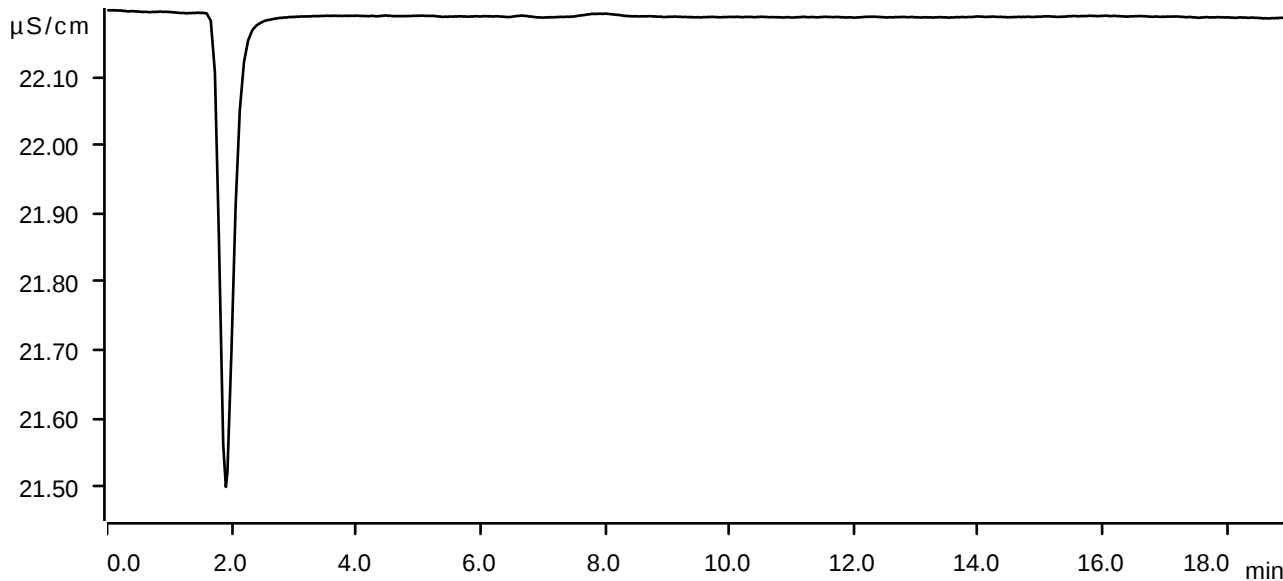**Anions**


## Sample data

Ident . . . . . LB133778BLW  
 Sample type . . . . . Sample  
 Determination start . . . . . 2024-12-06 11:24:23 UTC-5  
 Method . . . . . IC1-111824  
 Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
 Channel . . . . . Conductivity  
 Recording time . . . . . 19.0 min  
 Integration . . . . . Automatically  
 Column type . . . . . Metrosep A Supp 19 - 150/4.0  
 Eluent composition . . . . . not defined  
 Flow . . . . . 0.700 mL/min  
 Maximum flow monitored . . . . . yes  
 Pressure . . . . . 13.01 MPa  
 Maximum pressure monitored . . . . . yes  
 Temperature . . . . . ---- °C

## Anions

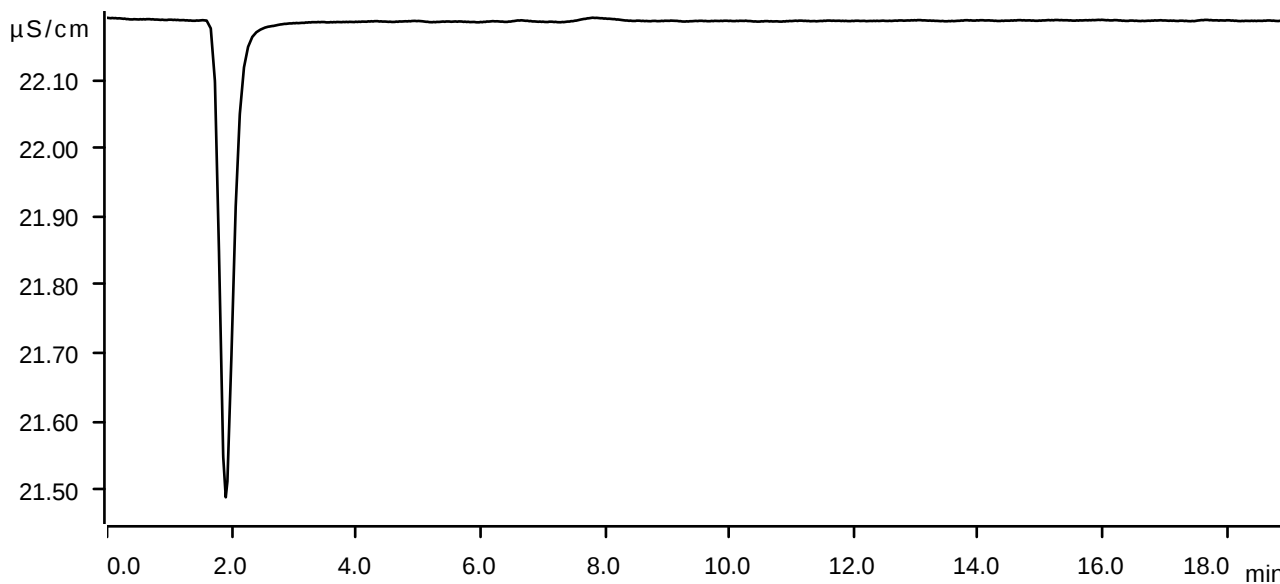


## Sample data

Ident . . . . . LB133778BSW  
Sample type . . . . . Check standard 1  
Determination start . . . . . 2024-12-06 11:45:54 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 12.95 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

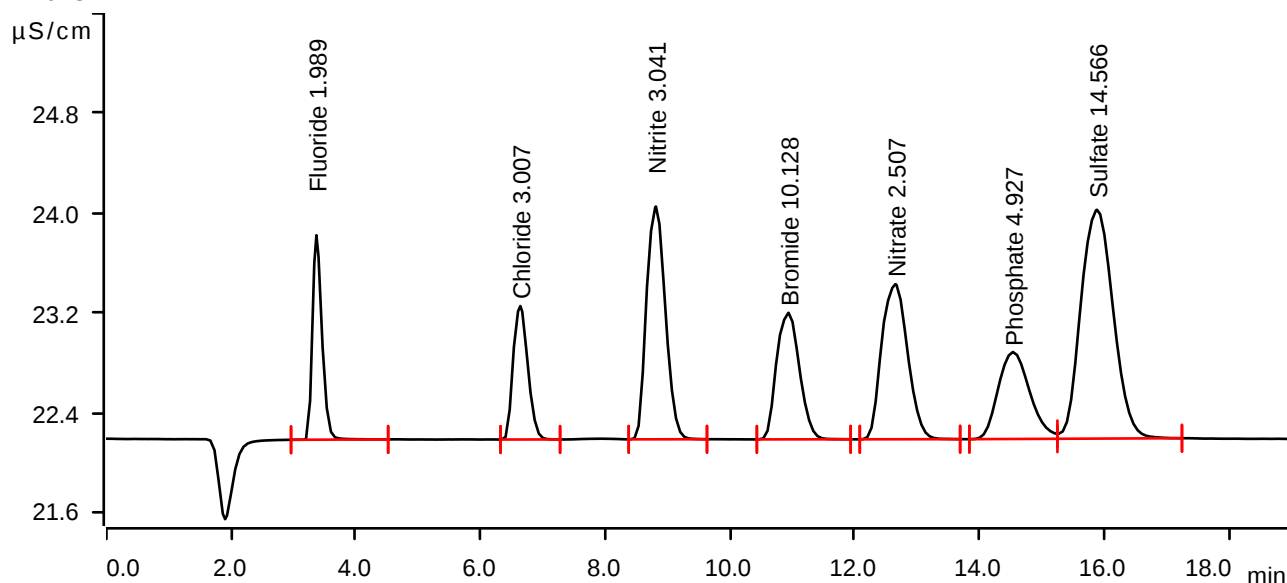

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.368                 | 0.2883                | 1.636           | 1.989                | Fluoride       |
| 2           | 6.637                 | 0.2906                | 1.068           | 3.007                | Chloride       |
| 3           | 8.812                 | 0.6526                | 1.863           | 3.041                | Nitrite        |
| 4           | 10.938                | 0.4308                | 1.013           | 10.128               | Bromide        |
| 5           | 12.650                | 0.5999                | 1.242           | 2.507                | Nitrate        |
| 6           | 14.535                | 0.4070                | 0.696           | 4.927                | Phosphate      |
| 7           | 15.883                | 1.1037                | 1.832           | 14.566               | Sulfate        |


## Sample data

Ident . . . . . P5145-01  
Sample type . . . . . Sample  
Determination start . . . . . 2024-12-06 12:07:26 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 12.95 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

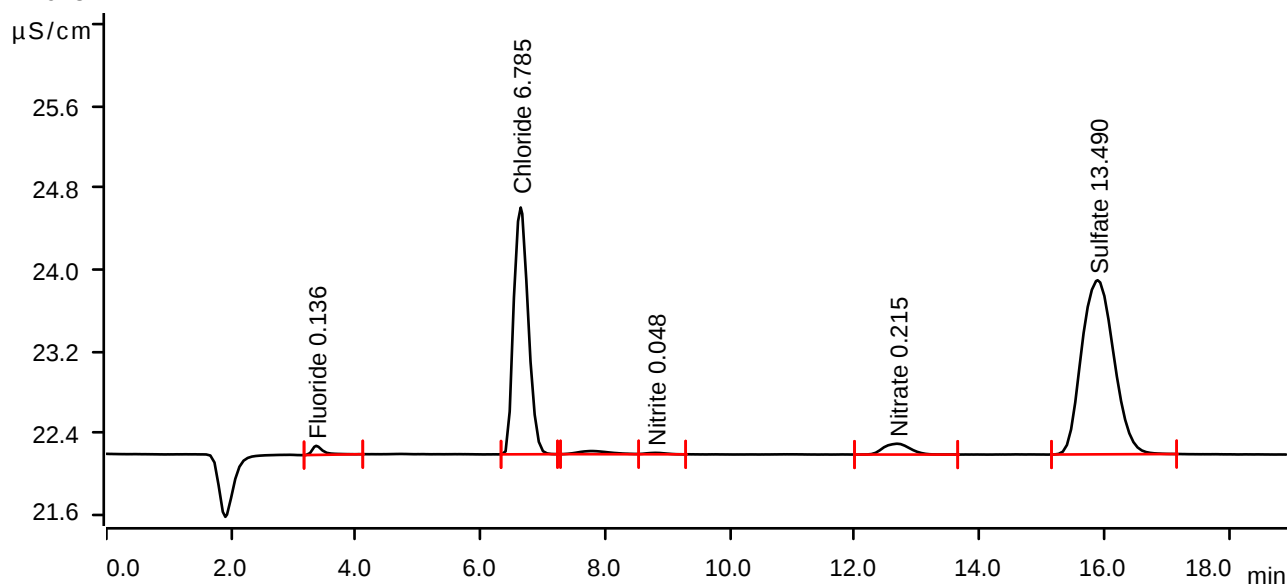

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.365                 | 0.0183                | 0.089           | 0.136                | Fluoride       |
| 2           | 6.643                 | 0.6496                | 2.409           | 6.785                | Chloride       |
| 3           | 7.772                 | 0.0185                | 0.031           | invalid              |                |
| 4           | 8.805                 | 0.0051                | 0.014           | 0.048                | Nitrite        |
| 5           | 12.683                | 0.0524                | 0.106           | 0.215                | Nitrate        |
| 6           | 15.893                | 1.0215                | 1.699           | 13.490               | Sulfate        |


**Sample data**

Ident . . . . . P5145-01MS  
Sample type . . . . . Sample  
Determination start . . . . . 2024-12-06 12:28:58 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

**Anions**

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 12.95 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

Anions

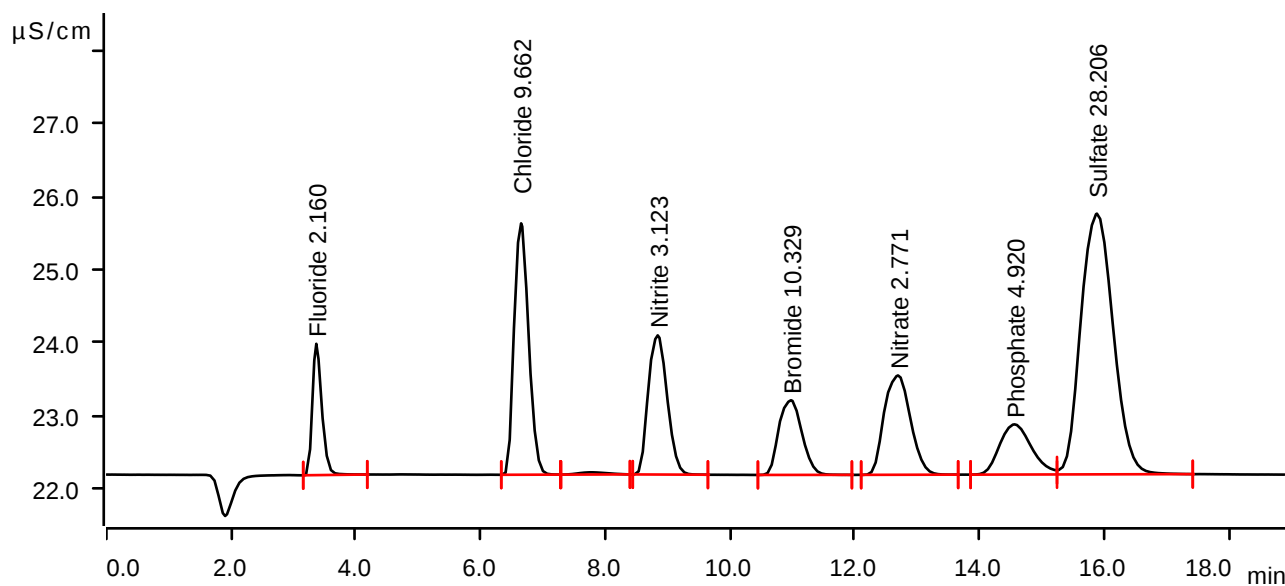

| Peak number | Retention time<br>min | Area<br>( $\mu\text{S/cm}$ ) x min | Height<br>$\mu\text{S/cm}$ | Concentration<br>ppm | Component name |
|-------------|-----------------------|------------------------------------|----------------------------|----------------------|----------------|
| 1           | 3.367                 | 0.3131                             | 1.795                      | 2.160                | Fluoride       |
| 2           | 6.650                 | 0.9230                             | 3.435                      | 9.662                | Chloride       |
| 3           | 7.760                 | 0.0160                             | 0.030                      | invalid              |                |
| 4           | 8.840                 | 0.6702                             | 1.902                      | 3.123                | Nitrite        |
| 5           | 10.977                | 0.4393                             | 1.021                      | 10.329               | Bromide        |
| 6           | 12.693                | 0.6630                             | 1.357                      | 2.771                | Nitrate        |
| 7           | 14.562                | 0.4065                             | 0.685                      | 4.920                | Phosphate      |
| 8           | 15.882                | 2.1464                             | 3.563                      | 28.206               | Sulfate        |


**Sample data**

Ident . . . . . P5145-01MSD  
Sample type . . . . . Sample  
Determination start . . . . . 2024-12-06 12:50:32 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

**Anions**

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 13.06 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

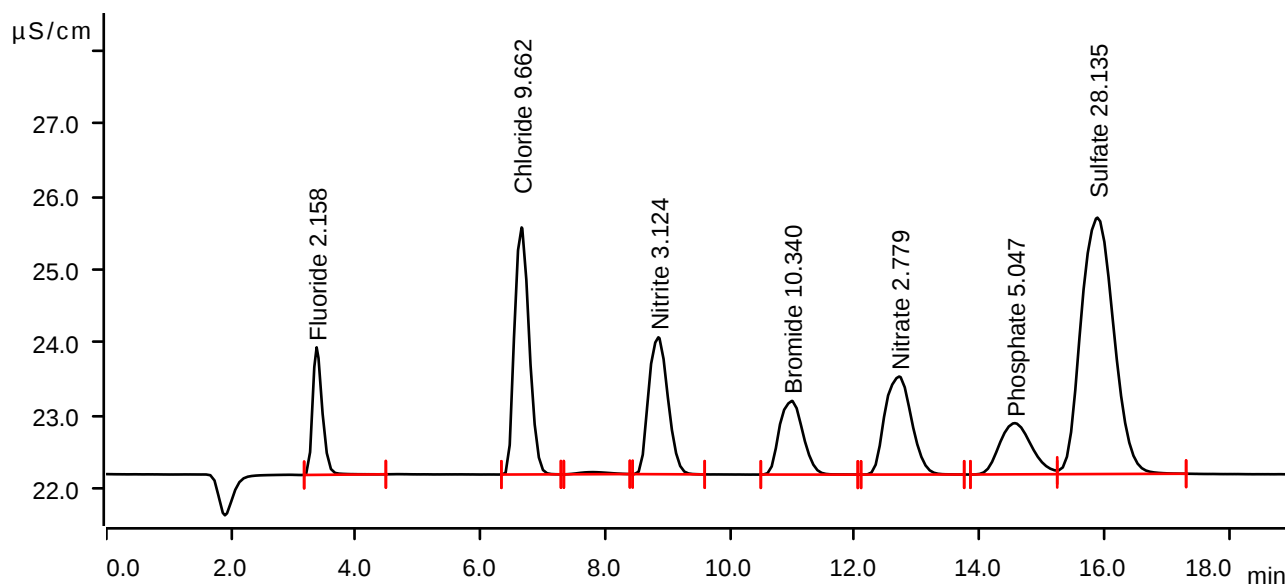

| Peak number | Retention time<br>min | Area<br>( $\mu\text{S/cm}$ ) x min | Height<br>$\mu\text{S/cm}$ | Concentration<br>ppm | Component name |
|-------------|-----------------------|------------------------------------|----------------------------|----------------------|----------------|
| 1           | 3.372                 | 0.3128                             | 1.743                      | 2.158                | Fluoride       |
| 2           | 6.658                 | 0.9230                             | 3.376                      | 9.662                | Chloride       |
| 3           | 7.805                 | 0.0156                             | 0.029                      | invalid              |                |
| 4           | 8.850                 | 0.6705                             | 1.871                      | 3.124                | Nitrite        |
| 5           | 10.990                | 0.4398                             | 1.007                      | 10.340               | Bromide        |
| 6           | 12.712                | 0.6648                             | 1.341                      | 2.779                | Nitrate        |
| 7           | 14.567                | 0.4170                             | 0.700                      | 5.047                | Phosphate      |
| 8           | 15.890                | 2.1409                             | 3.504                      | 28.135               | Sulfate        |


## Sample data

Ident . . . . . CCV  
Sample type . . . . . Check standard 1  
Determination start . . . . . 2024-12-06 13:12:05 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 13.06 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

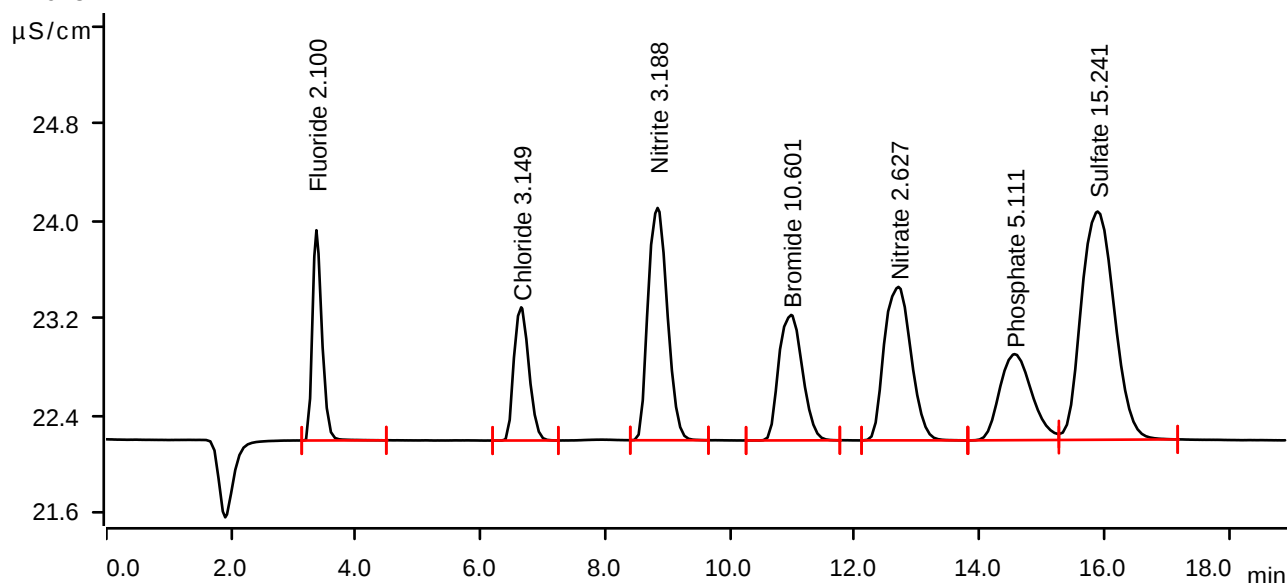

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.368                 | 0.3043                | 1.724           | 2.100                | Fluoride       |
| 2           | 6.652                 | 0.3041                | 1.092           | 3.149                | Chloride       |
| 3           | 8.838                 | 0.6844                | 1.905           | 3.188                | Nitrite        |
| 4           | 10.980                | 0.4509                | 1.029           | 10.601               | Bromide        |
| 5           | 12.700                | 0.6284                | 1.259           | 2.627                | Nitrate        |
| 6           | 14.560                | 0.4223                | 0.705           | 5.111                | Phosphate      |
| 7           | 15.893                | 1.1553                | 1.871           | 15.241               | Sulfate        |

## Sample data

Ident . . . . . CCB  
Sample type . . . . . Sample  
Determination start . . . . . 2024-12-06 13:33:35 UTC-5  
Method . . . . . IC1-111824  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 13.01 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

