

Ident	Instrument IC-1			Analyst : NF		Method: 300.0 / 9056A		date time	Initial Analyst	
	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4			Method name
STD1	0	0	0	0	0	0	0	0 IC1-111824	11/18/2024 11:24	10 NF/IZ
STD2	0.402	0.571	0.601	1.961	0.489	1.025	3.062	IC1-111824	11/18/2024 11:46	10 NF/IZ
STD3	0.794	1.185	1.175	3.939	0.997	1.928	6.062	IC1-111824	11/18/2024 12:07	10 NF/IZ
STD4	1.023	1.554	1.535	5.128	1.284	2.665	7.843	IC1-111824	11/18/2024 12:29	10 NF/IZ
STD5	1.997	3.009	2.993	9.997	2.488	4.96	14.679	IC1-111824	11/18/2024 12:50	10 NF/IZ
STD6	3.936	5.952	5.978	19.928	4.964	9.645	28.993	IC1-111824	11/18/2024 13:11	10 NF/IZ
STD7	5.049	7.529	7.517	25.045	6.279	12.776	37.863	IC1-111824	11/18/2024 13:33	10 NF/IZ
ICV	1.966	3.006	2.997	9.98	2.49	4.979	14.594	IC1-111824	11/18/2024 13:54	10 NF/IZ
ICB	0	0	0	0	0	0	0	IC1-111824	11/18/2024 14:16	10 NF/IZ
CCV	1.986	3.023	3.05	10.179	2.515	5.026	14.318	IC1-111824	12/16/2024 12:15	10 NF/IZ
CCB	0	0	0	0	0	0	0	IC1-111824	12/16/2024 12:37	10 NF/IZ
LB133970BLW	0	0	0	0	0	0	0	IC1-111824	12/16/2024 12:58	10 NF/IZ
LB133970BSW	1.99	3.025	3.062	10.186	2.518	5.028	14.35	IC1-111824	12/16/2024 13:20	10 NF/IZ
P5291-01	0.026	91.525	0	0.104	0.603	0	7.176	IC1-111824	12/16/2024 13:42	10 NF/IZ
P5291-02	0.068	171.027	0.042	0.241	6.115	0	22.697	IC1-111824	12/16/2024 14:03	10 NF/IZ
P5291-03	0.08	796.103	0.055	0.424	3.597	0	29.313	IC1-111824	12/16/2024 14:25	10 NF/IZ
P5291-04	0.039	153.496	0.048	0	0.602	0	19.076	IC1-111824	12/16/2024 14:46	10 NF/IZ
P5291-05	0.098	222.207	0.07	0.262	0.079	0	7.135	IC1-111824	12/16/2024 15:08	10 NF/IZ
P5291-06	0.091	439.641	0	0.466	0.95	0	33.078	IC1-111824	12/16/2024 15:29	10 NF/IZ
P5291-07	0.059	596.295	0.172	0.492	1.398	0	36.912	IC1-111824	12/16/2024 15:51	10 NF/IZ
P5291-08MS	2.03	570.007	3.166	10.565	3.973	5.024	50.444	IC1-111824	12/16/2024 16:12	10 NF/IZ
CCV	2.017	3.045	3.077	10.268	2.539	5.23	14.651	IC1-111824	12/16/2024 16:34	10 NF/IZ
CCB	0	0	0	0	0	0	0	IC1-111824	12/16/2024 16:55	10 NF/IZ
P5291-09MSD	2.032	569.688	3.204	10.614	3.89	5.016	50.478	IC1-111824	12/16/2024 17:17	10 NF/IZ
P5291-10	0.062	549.888	0.153	0.428	1.385	0	38.804	IC1-111824	12/16/2024 17:38	10 NF/IZ
P5291-11	0	-0.011	0	0	0	0	0	IC1-111824	12/16/2024 17:50	10 NF/IZ
CCV	2.027	3.048	3.086	10.294	2.545	5.232	14.66	IC1-111824	12/16/2024 18:00	10 NF/IZ
CCB	0	0	0	0	0	0	0	IC1-111824	12/16/2024 18:21	10 NF/IZ
CCV	2.017	3.064	3.096	10.342	2.558	5.1	14.715	IC1-111824	12/16/2024 18:43	10 NF/IZ
									12/17/2024 9:51	10 NF/IZ

CCB	0	0	0	0	0	0	0	IC1-111824	12/17/2024 10:12	10 NF/IZ
LB133970BLW2	0	0	0	0	0	0	0	IC1-111824	12/17/2024 10:34	10 NF/IZ
LB133970BSW2	2.038	3.103	3.132	10.466	2.579	5.181	14.697	IC1-111824	12/17/2024 10:55	10 NF/IZ
P5291-10DLX2	0.031	258.001	0.059	0.401	0.697	0	19.373	IC1-111824	12/17/2024 11:17	10 NF/IZ
CCV	2.004	3.056	3.08	10.283	2.533	5.1	14.497	IC1-111824	12/17/2024 11:38	10 NF/IZ
CCB	0	0	0	0	0	0	0	IC1-111824	12/17/2024 12:00	10 NF/IZ

Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A


ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-111824	11/18/2024 11:24	10	NF/IZ
STD2	0.402	0.571	0.601	1.961	0.489	1.025	3.062	IC1-111824	11/18/2024 11:46	10	NF/IZ
STD3	0.794	1.185	1.175	3.939	0.997	1.928	6.062	IC1-111824	11/18/2024 12:07	10	NF/IZ
STD4	1.023	1.554	1.535	5.128	1.284	2.665	7.843	IC1-111824	11/18/2024 12:29	10	NF/IZ
STD5	1.997	3.009	2.993	9.997	2.488	4.960	14.679	IC1-111824	11/18/2024 12:50	10	NF/IZ
STD6	3.936	5.952	5.978	19.928	4.964	9.645	28.993	IC1-111824	11/18/2024 13:11	10	NF/IZ
STD7	5.049	7.529	7.517	25.045	6.279	12.776	37.863	IC1-111824	11/18/2024 13:33	10	NF/IZ

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1							
STD2	0.5000	-4.8333	0.1667	-1.9500	-2.2000	2.5000	2.0667
STD3	-0.7500	-1.2500	-2.0833	-1.5250	-0.3000	-3.6000	1.0333
STD4	2.3000	3.6000	2.3333	2.5600	2.7200	6.6000	4.5733
STD5	-0.1500	0.3000	-0.2333	-0.0300	-0.4800	-0.8000	-2.1400
STD6	-1.6000	-0.8000	-0.3667	-0.3600	-0.7200	-3.5500	-3.3567
STD7	0.9800	0.3667	0.2267	0.1800	0.4640	2.2080	2.3324

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

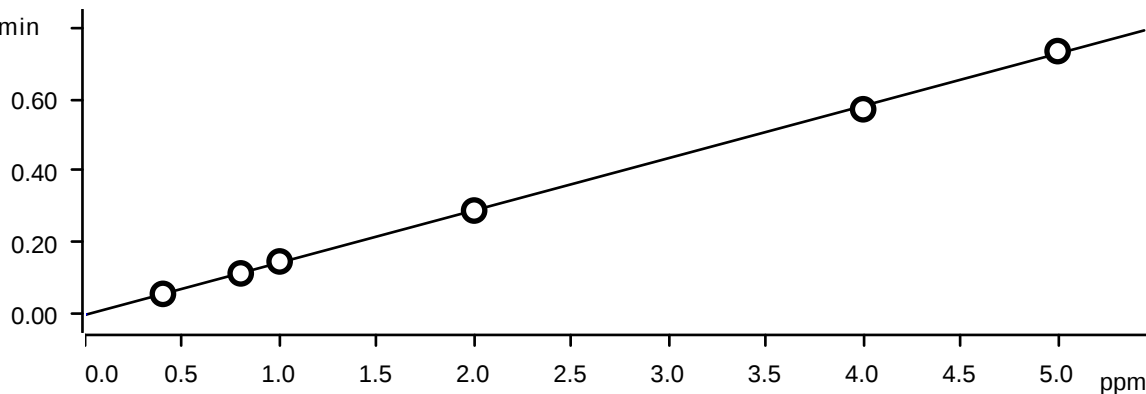

Function: $A = -1.48773\text{E-}3 + 0.0145652 \times Q$


Relative standard deviation 1.923523 %

Correlation coefficient 0.999800

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-11-18 11:24:52 UTC-5	used
Standard 2	1	0.400	10.0	1.0	1.0	0.057	STD2	2024-11-18 11:46:16 UTC-5	used
Standard 3	1	0.800	10.0	1.0	1.0	0.114	STD3	2024-11-18 12:07:40 UTC-5	used
Standard 4	1	1.000	10.0	1.0	1.0	0.147	STD4	2024-11-18 12:29:05 UTC-5	used
Standard 5	1	2.000	10.0	1.0	1.0	0.289	STD5	2024-11-18 12:50:30 UTC-5	used
Standard 6	1	4.000	10.0	1.0	1.0	0.572	STD6	2024-11-18 13:11:57 UTC-5	used
Standard 7	1	5.000	10.0	1.0	1.0	0.734	STD7	2024-11-18 13:33:24 UTC-5	used

Chloride (Anions)


($\mu\text{S}/\text{cm}$) x min

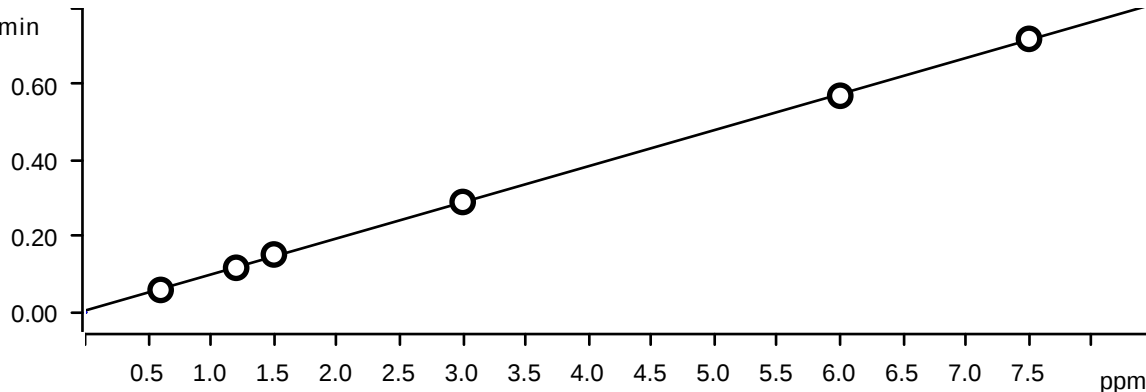

Function: $A = 4.85841\text{E-}3 + 9.50243\text{E-}3 \times Q$

Relative standard deviation 1.265280 %
Correlation coefficient 0.999910

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-11-18 11:24:52 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.059	STD2	2024-11-18 11:46:16 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.117	STD3	2024-11-18 12:07:40 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.153	STD4	2024-11-18 12:29:05 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.291	STD5	2024-11-18 12:50:30 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	0.570	STD6	2024-11-18 13:11:57 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	0.720	STD7	2024-11-18 13:33:24 UTC-5	used

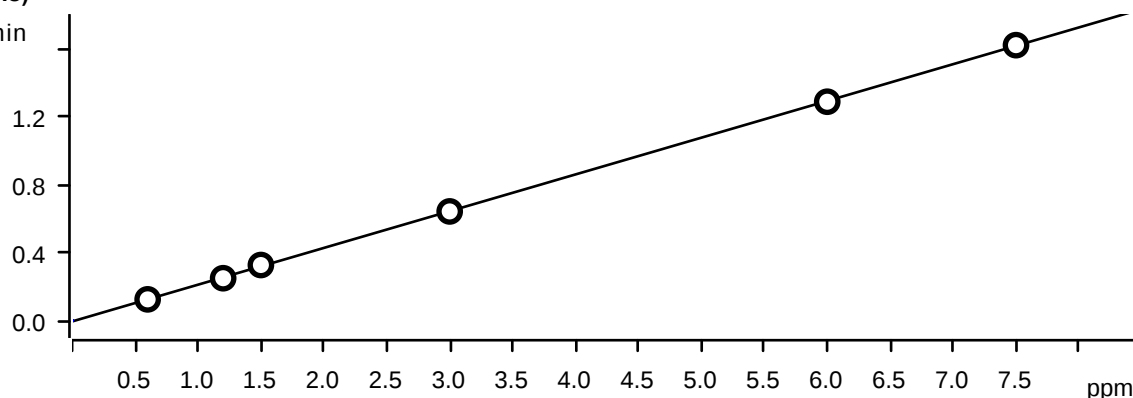
Nitrite (Anions) $(\mu\text{S/cm}) \times \text{min}$ 

Function: $A = -5.27414E-3 + 0.0216316 \times Q$
Relative standard deviation 0.783603 %
Correlation coefficient 0.999967

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-11-18 11:24:52 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.125	STD2	2024-11-18 11:46:16 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.249	STD3	2024-11-18 12:07:40 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.327	STD4	2024-11-18 12:29:05 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.642	STD5	2024-11-18 12:50:30 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	1.288	STD6	2024-11-18 13:11:57 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	1.621	STD7	2024-11-18 13:33:24 UTC-5	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

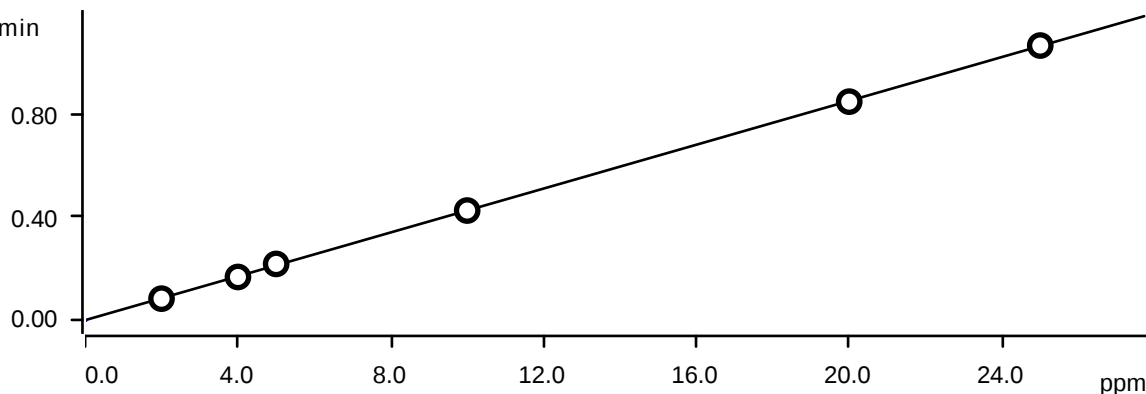

Function: $A = 7.64331E-4 + 4.24604E-3 \times Q$


Relative standard deviation 0.771268 %

Correlation coefficient 0.999967

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-11-18 11:24:52 UTC-5	used
Standard 2	1	2.000	10.0	1.0	1.0	0.084	STD2	2024-11-18 11:46:16 UTC-5	used
Standard 3	1	4.000	10.0	1.0	1.0	0.168	STD3	2024-11-18 12:07:40 UTC-5	used
Standard 4	1	5.000	10.0	1.0	1.0	0.219	STD4	2024-11-18 12:29:05 UTC-5	used
Standard 5	1	10.000	10.0	1.0	1.0	0.425	STD5	2024-11-18 12:50:30 UTC-5	used
Standard 6	1	20.000	10.0	1.0	1.0	0.847	STD6	2024-11-18 13:11:57 UTC-5	used
Standard 7	1	25.000	10.0	1.0	1.0	1.064	STD7	2024-11-18 13:33:24 UTC-5	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

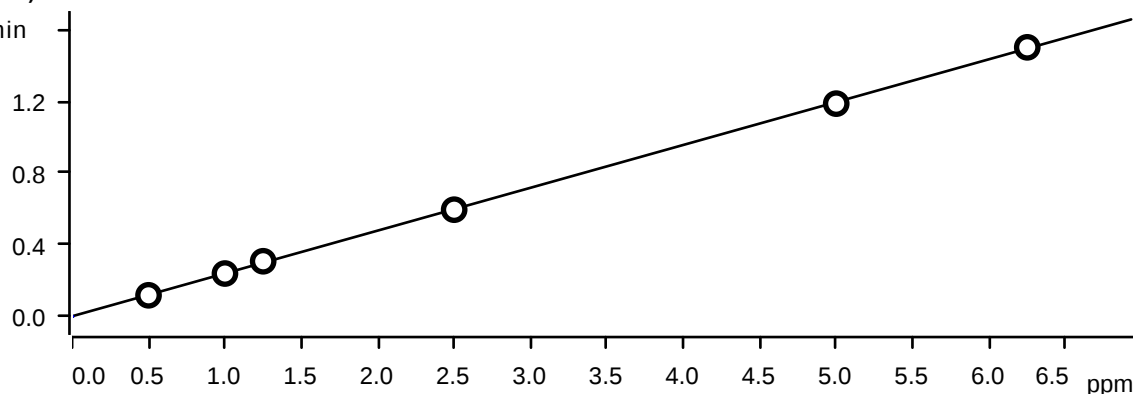


Function: $A = 1.14484E-3 + 0.0238833 \times Q$

Relative standard deviation 1.085494 %

Correlation coefficient 0.999936

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-11-18 11:24:52 UTC-5	used
Standard 2	1	0.500	10.0	1.0	1.0	0.118	STD2	2024-11-18 11:46:16 UTC-5	used
Standard 3	1	1.000	10.0	1.0	1.0	0.239	STD3	2024-11-18 12:07:40 UTC-5	used
Standard 4	1	1.250	10.0	1.0	1.0	0.308	STD4	2024-11-18 12:29:05 UTC-5	used
Standard 5	1	2.500	10.0	1.0	1.0	0.595	STD5	2024-11-18 12:50:30 UTC-5	used
Standard 6	1	5.000	10.0	1.0	1.0	1.187	STD6	2024-11-18 13:11:57 UTC-5	used
Standard 7	1	6.250	10.0	1.0	1.0	1.501	STD7	2024-11-18 13:33:24 UTC-5	used

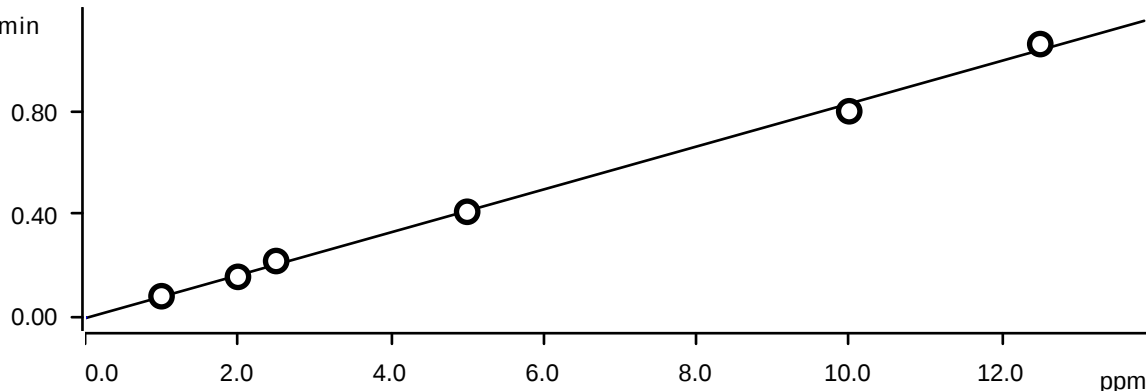
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -2.33576E-3 + 8.30878E-3 \times Q$

Relative standard deviation 4.444706 %

Correlation coefficient 0.998936

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-11-18 11:24:52 UTC-5	used
Standard 2	1	1.000	10.0	1.0	1.0	0.083	STD2	2024-11-18 11:46:16 UTC-5	used
Standard 3	1	2.000	10.0	1.0	1.0	0.158	STD3	2024-11-18 12:07:40 UTC-5	used
Standard 4	1	2.500	10.0	1.0	1.0	0.219	STD4	2024-11-18 12:29:05 UTC-5	used
Standard 5	1	5.000	10.0	1.0	1.0	0.410	STD5	2024-11-18 12:50:30 UTC-5	used
Standard 6	1	10.000	10.0	1.0	1.0	0.799	STD6	2024-11-18 13:11:57 UTC-5	used
Standard 7	1	12.500	10.0	1.0	1.0	1.059	STD7	2024-11-18 13:33:24 UTC-5	used

Sulfate (Anions)

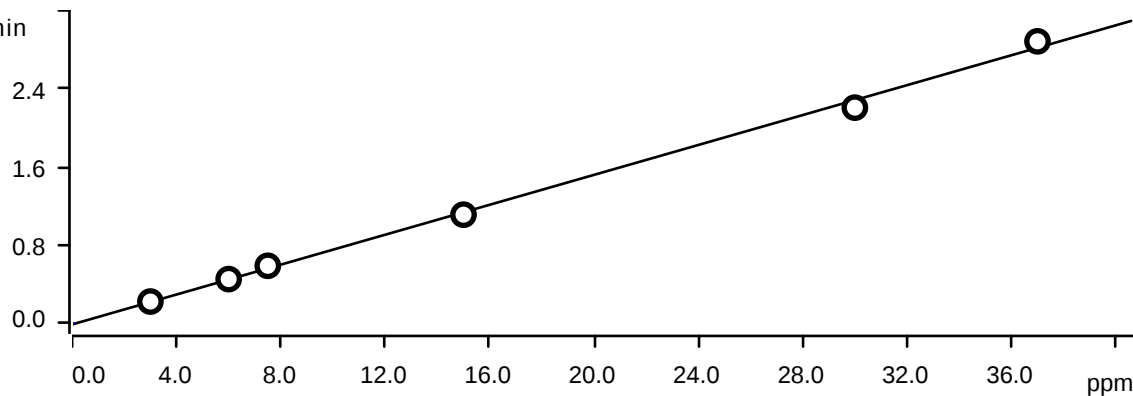 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -9.71222\text{E-}3 + 7.64397\text{E-}3 \times Q$

Relative standard deviation 4.327283 %

Correlation coefficient 0.998986

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-11-18 11:24:52 UTC-5	used
Standard 2	1	3.000	10.0	1.0	1.0	0.224	STD2	2024-11-18 11:46:16 UTC-5	used
Standard 3	1	6.000	10.0	1.0	1.0	0.454	STD3	2024-11-18 12:07:40 UTC-5	used
Standard 4	1	7.500	10.0	1.0	1.0	0.590	STD4	2024-11-18 12:29:05 UTC-5	used
Standard 5	1	15.000	10.0	1.0	1.0	1.112	STD5	2024-11-18 12:50:30 UTC-5	used
Standard 6	1	30.000	10.0	1.0	1.0	2.206	STD6	2024-11-18 13:11:57 UTC-5	used
Standard 7	1	37.000	10.0	1.0	1.0	2.884	STD7	2024-11-18 13:33:24 UTC-5	used


Sample data

Ident STD1
Sample type Standard 1
Determination start 2024-11-18 11:24:52 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

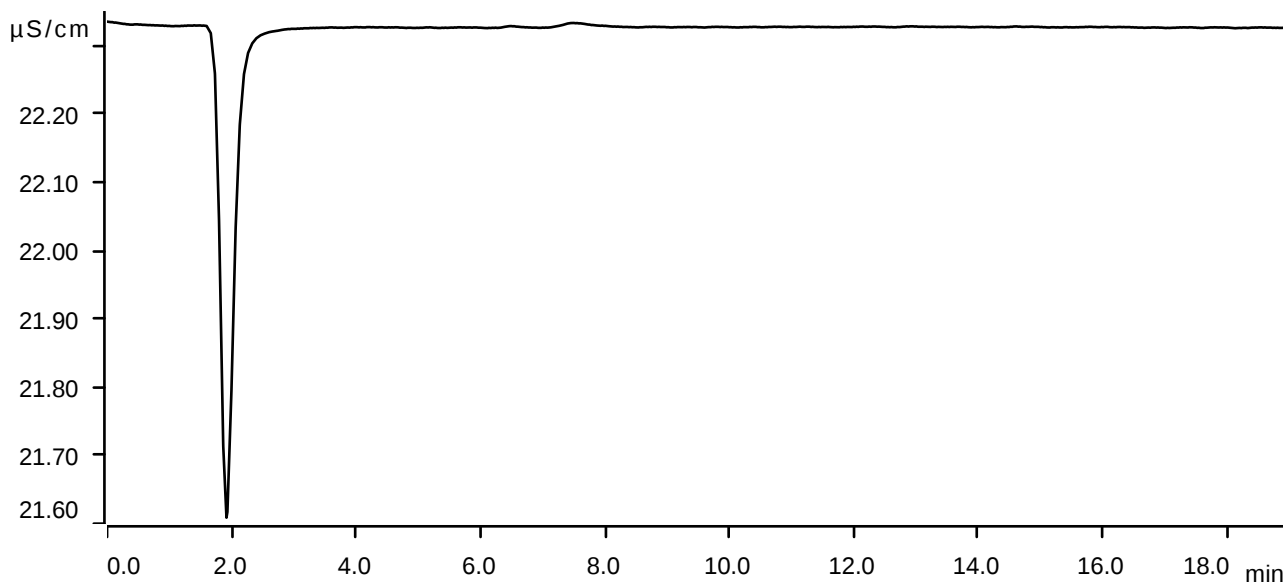


Sample data

Ident STD2
Sample type Standard 2
Determination start 2024-11-18 11:46:16 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

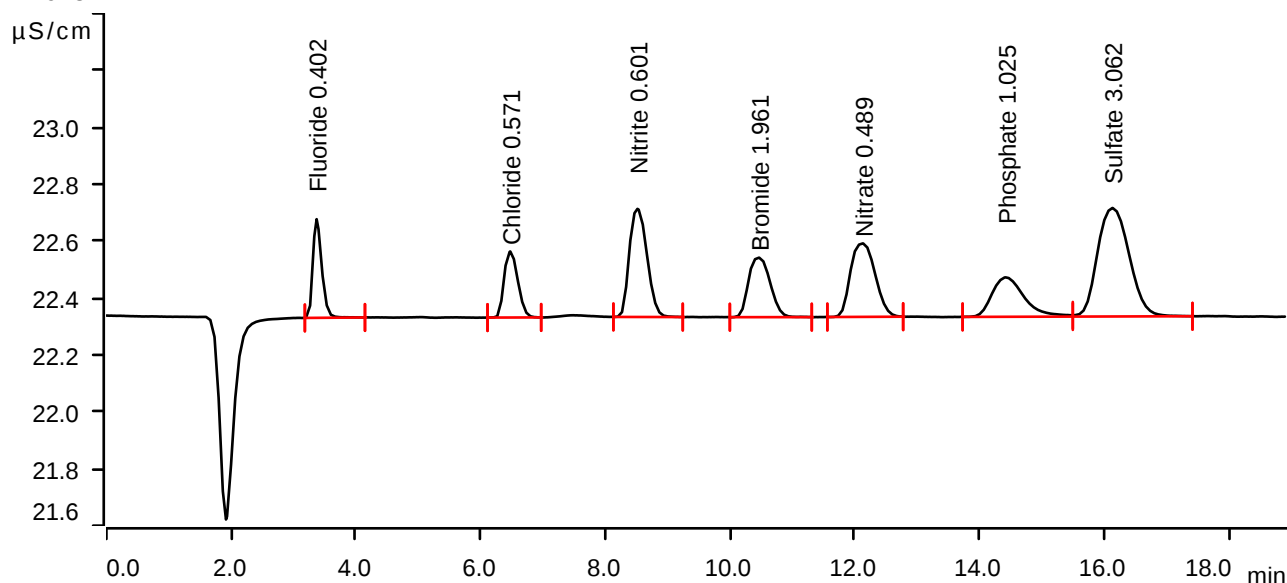

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.372	0.0570	0.347	0.402	Fluoride
2	6.477	0.0592	0.232	0.571	Chloride
3	8.515	0.1247	0.380	0.601	Nitrite
4	10.463	0.0840	0.209	1.961	Bromide
5	12.127	0.1179	0.258	0.489	Nitrate
6	14.418	0.0829	0.139	1.025	Phosphate
7	16.130	0.2243	0.381	3.062	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2024-11-18 12:07:40 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

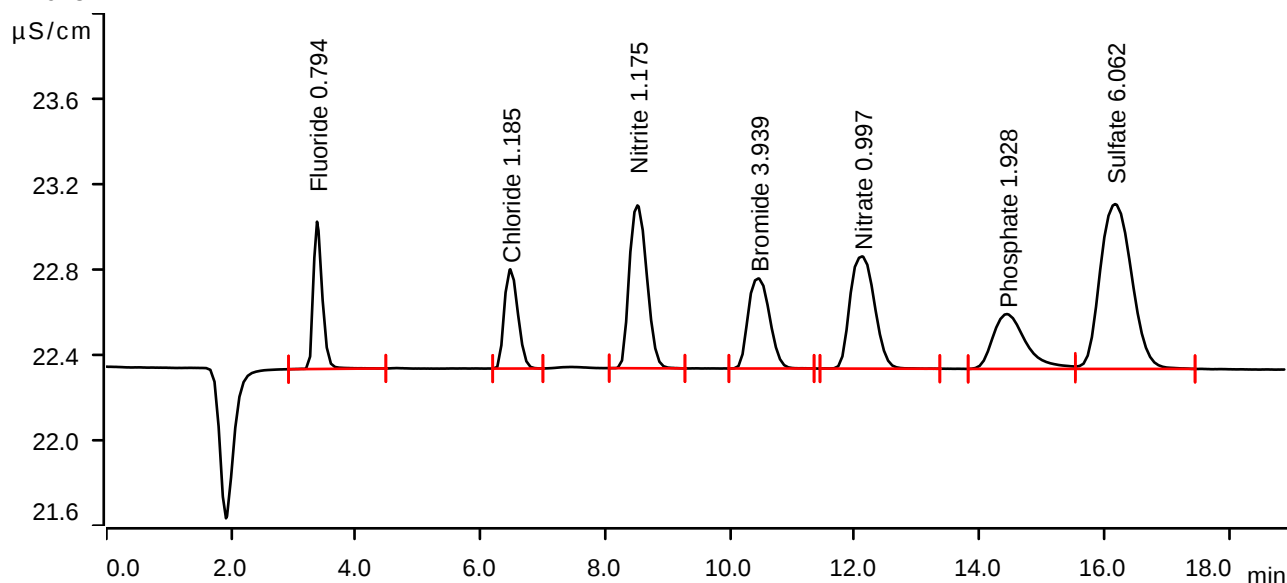

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.378	0.1141	0.690	0.794	Fluoride
2	6.478	0.1175	0.465	1.185	Chloride
3	8.515	0.2490	0.763	1.175	Nitrite
4	10.453	0.1680	0.422	3.939	Bromide
5	12.117	0.2394	0.526	0.997	Nitrate
6	14.440	0.1579	0.257	1.928	Phosphate
7	16.173	0.4537	0.772	6.062	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2024-11-18 12:29:05 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

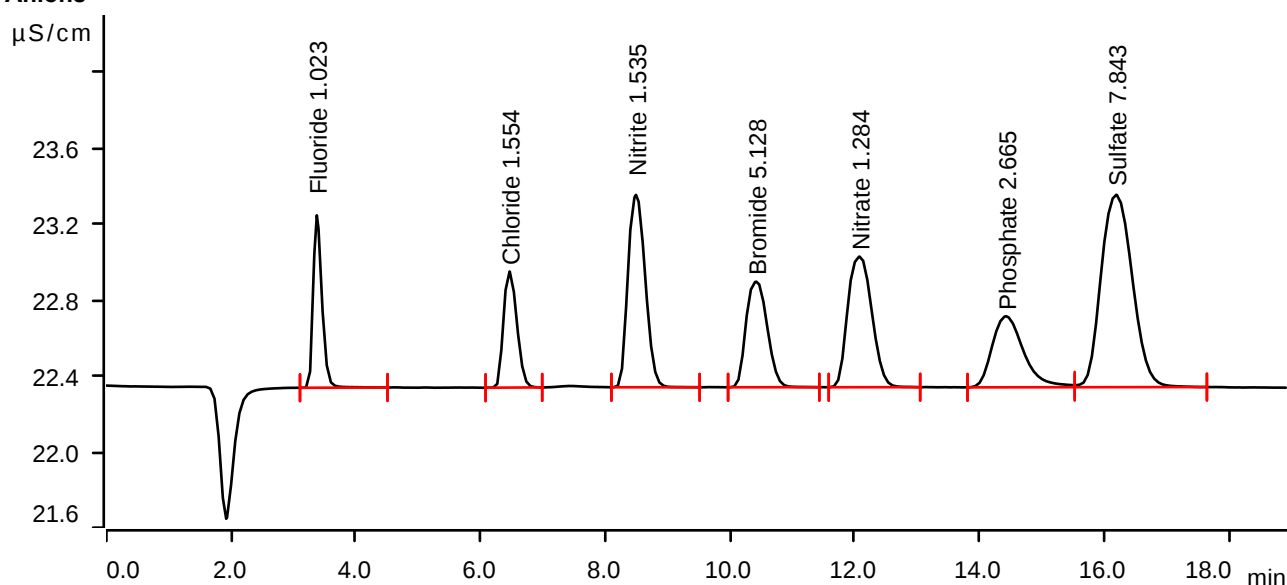

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.375	0.1475	0.909	1.023	Fluoride
2	6.465	0.1525	0.612	1.554	Chloride
3	8.493	0.3268	1.014	1.535	Nitrite
4	10.420	0.2185	0.557	5.128	Bromide
5	12.077	0.3078	0.689	1.284	Nitrate
6	14.427	0.2191	0.375	2.665	Phosphate
7	16.192	0.5898	1.014	7.843	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2024-11-18 12:50:30 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

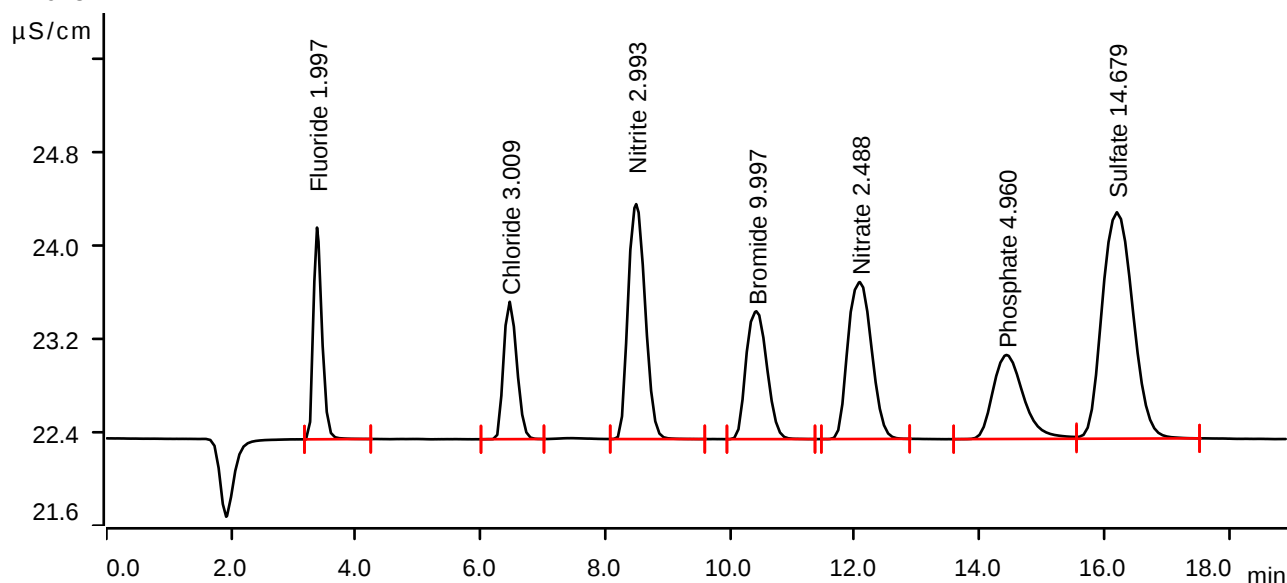

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.378	0.2894	1.819	1.997	Fluoride
2	6.467	0.2908	1.180	3.009	Chloride
3	8.495	0.6422	2.018	2.993	Nitrite
4	10.422	0.4253	1.098	9.997	Bromide
5	12.082	0.5953	1.348	2.488	Nitrate
6	14.432	0.4098	0.722	4.960	Phosphate
7	16.203	1.1123	1.944	14.679	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2024-11-18 13:11:57 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

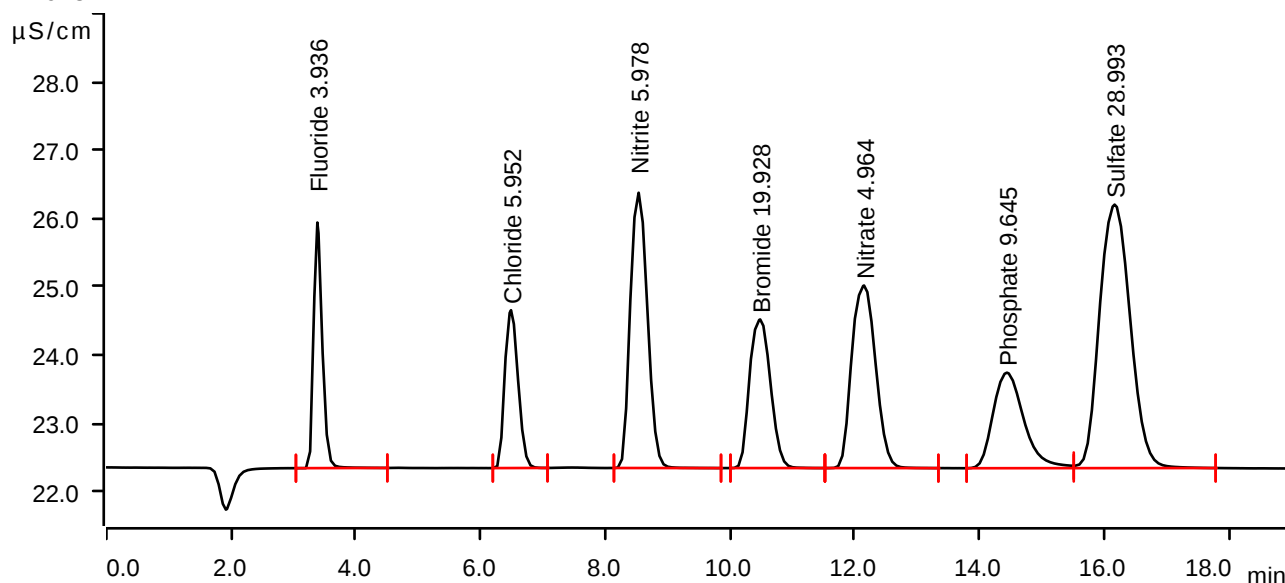

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.383	0.5717	3.596	3.936	Fluoride
2	6.488	0.5704	2.311	5.952	Chloride
3	8.533	1.2879	4.031	5.978	Nitrite
4	10.483	0.8469	2.176	19.928	Bromide
5	12.148	1.1866	2.673	4.964	Nitrate
6	14.438	0.7991	1.399	9.645	Phosphate
7	16.165	2.2065	3.859	28.993	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2024-11-18 13:33:24 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

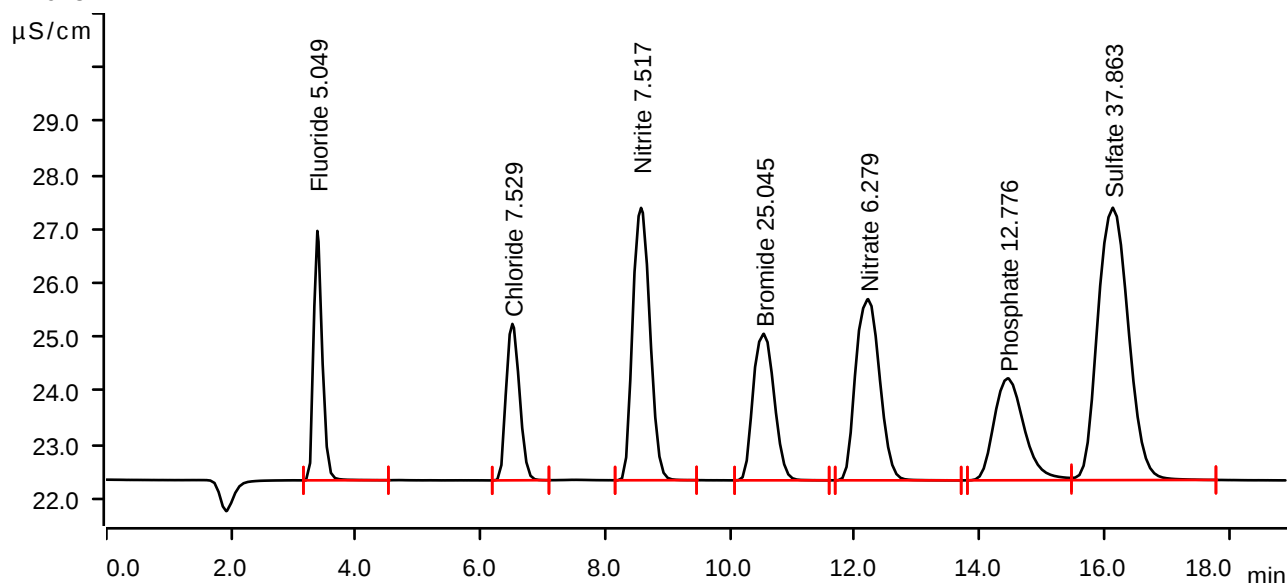

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.383	0.7339	4.626	5.049	Fluoride
2	6.510	0.7203	2.901	7.529	Chloride
3	8.573	1.6208	5.052	7.517	Nitrite
4	10.542	1.0642	2.717	25.045	Bromide
5	12.213	1.5007	3.361	6.279	Nitrate
6	14.452	1.0592	1.891	12.776	Phosphate
7	16.138	2.8845	5.052	37.863	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2024-11-18 13:54:44 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

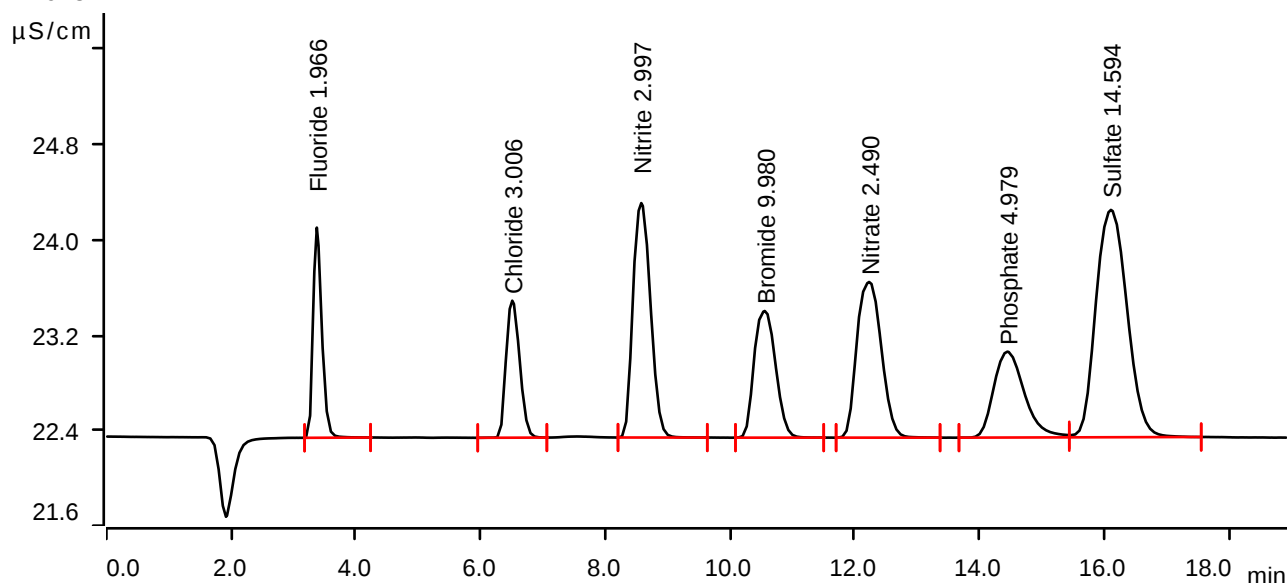

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	3.375	0.2848	1.764	1.966	Fluoride
2	6.508	0.2905	1.150	3.006	Chloride
3	8.577	0.6430	1.968	2.997	Nitrite
4	10.557	0.4245	1.063	9.980	Bromide
5	12.230	0.5959	1.307	2.490	Nitrate
6	14.447	0.4114	0.721	4.979	Phosphate
7	16.107	1.1058	1.909	14.594	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2024-11-18 14:16:12 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

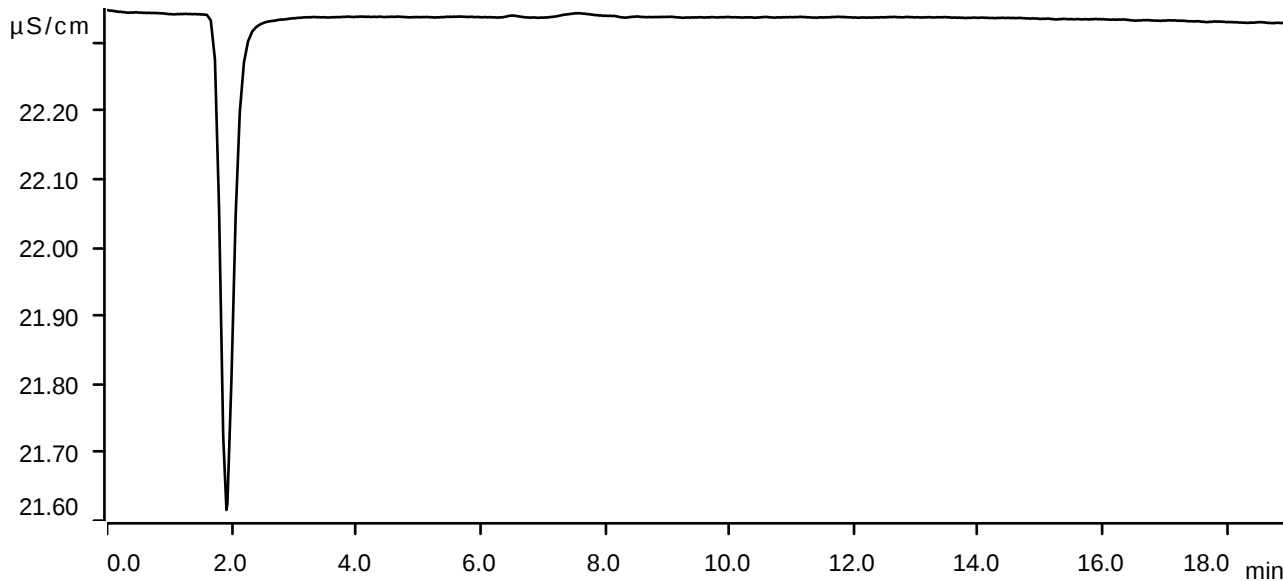


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-12-16 12:15:57 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

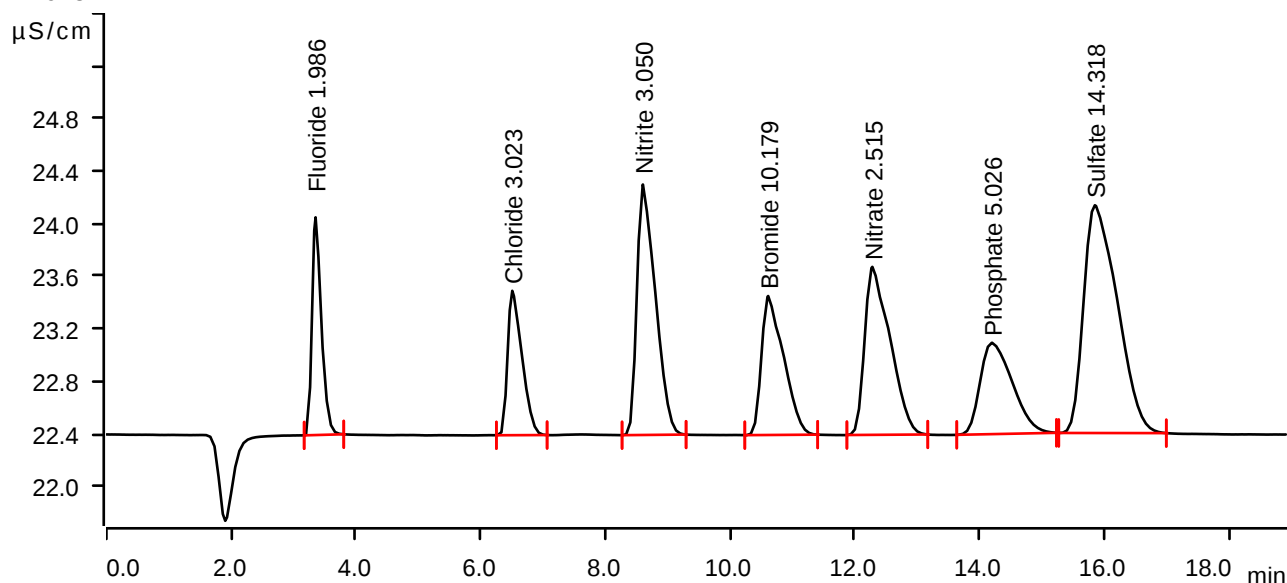


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.2877	1.658	1.986	Fluoride
2	6.508	0.2921	1.099	3.023	Chloride
3	8.603	0.6546	1.907	3.050	Nitrite
4	10.612	0.4330	1.058	10.179	Bromide
5	12.282	0.6019	1.279	2.515	Nitrate
6	14.197	0.4152	0.696	5.026	Phosphate
7	15.848	1.0848	1.734	14.318	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2024-12-16 12:37:27 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

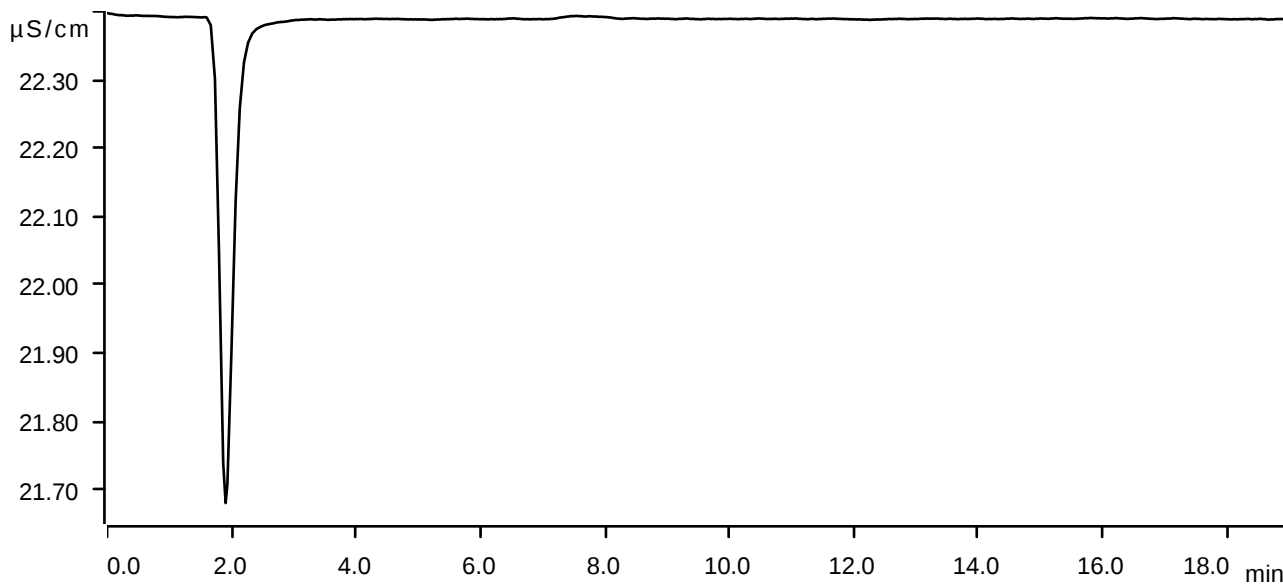Anions


Sample data

Ident LB133970BLW
 Sample type Sample
 Determination start 2024-12-16 12:58:57 UTC-5
 Method IC1-111824
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.99 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

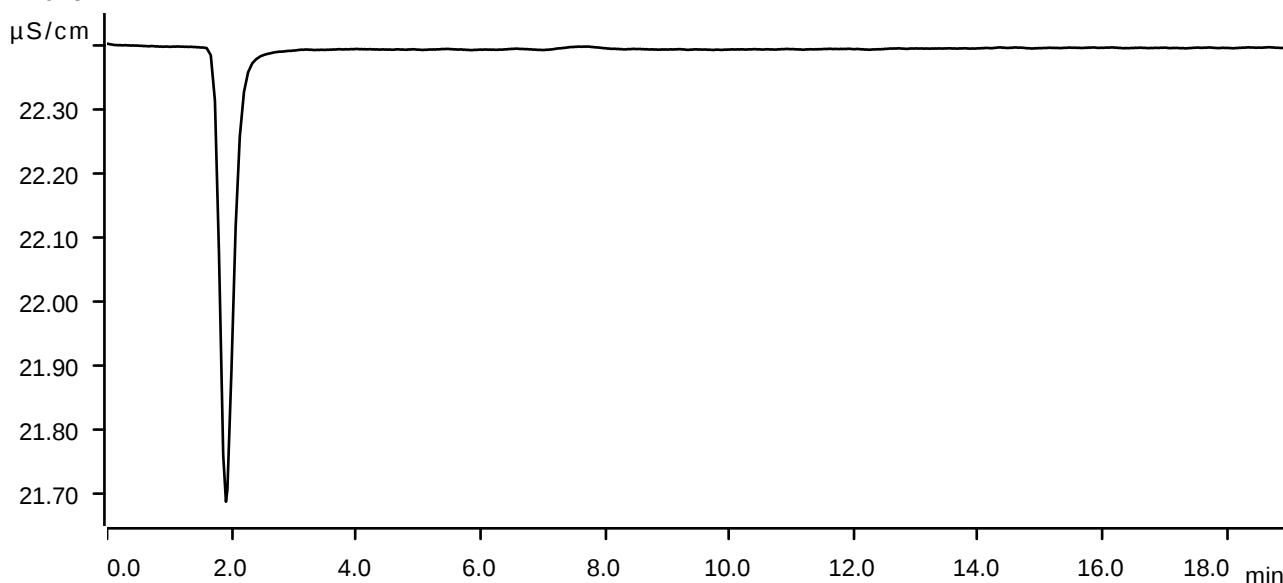


Sample data

Ident LB133970BSW
Sample type Check standard 1
Determination start 2024-12-16 13:20:28 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

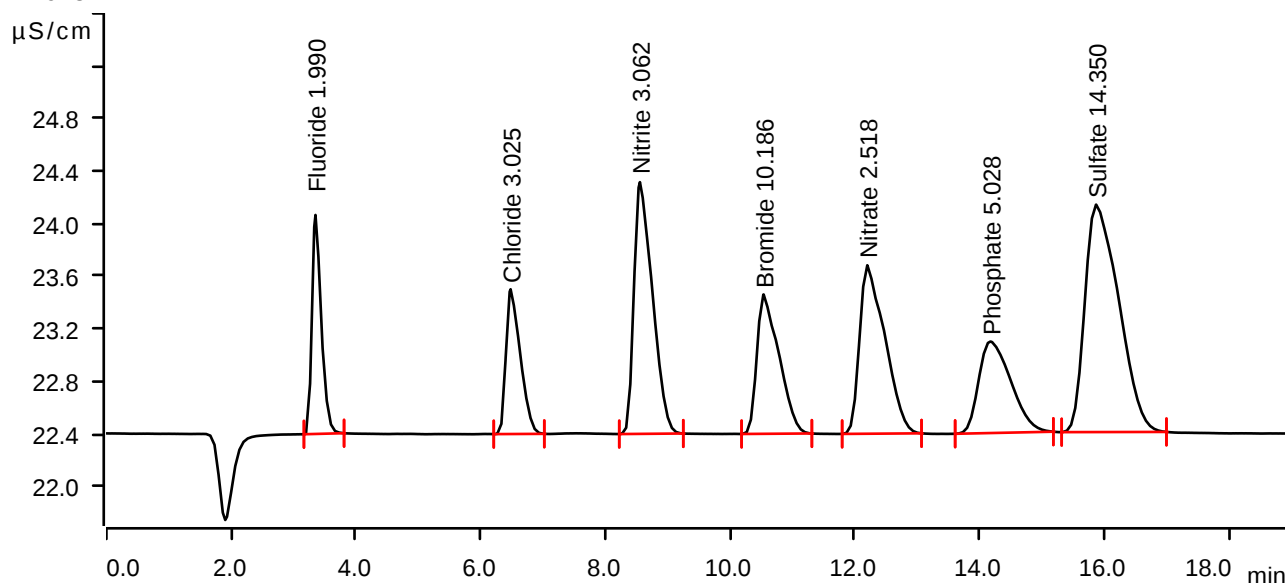

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.2883	1.667	1.990	Fluoride
2	6.482	0.2923	1.102	3.025	Chloride
3	8.555	0.6570	1.917	3.062	Nitrite
4	10.538	0.4333	1.061	10.186	Bromide
5	12.200	0.6026	1.283	2.518	Nitrate
6	14.177	0.4154	0.697	5.028	Phosphate
7	15.870	1.0872	1.732	14.350	Sulfate


Sample data

Ident P5291-01
Sample type Sample
Determination start 2024-12-16 13:42:00 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

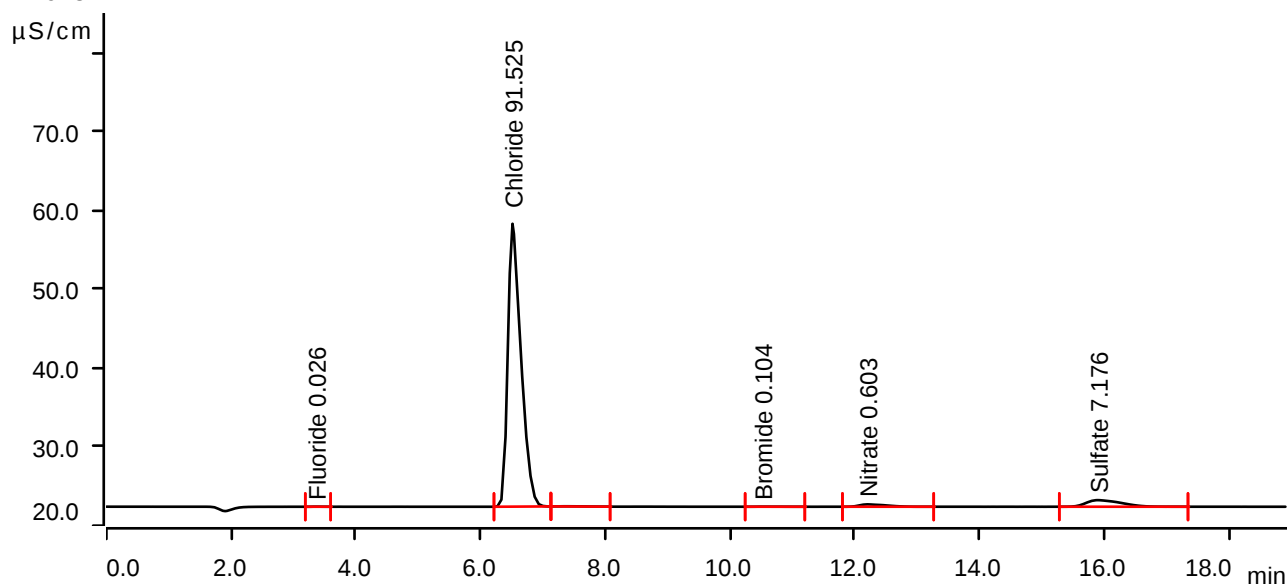

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.362	0.0023	0.014	0.026	Fluoride
2	6.512	8.7019	35.896	91.525	Chloride
3	7.388	0.0110	0.024	invalid	
4	10.517	0.0052	0.012	0.104	Bromide
5	12.200	0.1453	0.303	0.603	Nitrate
6	15.897	0.5388	0.837	7.176	Sulfate


Sample data

Ident P5291-02
Sample type Sample
Determination start 2024-12-16 14:03:33 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

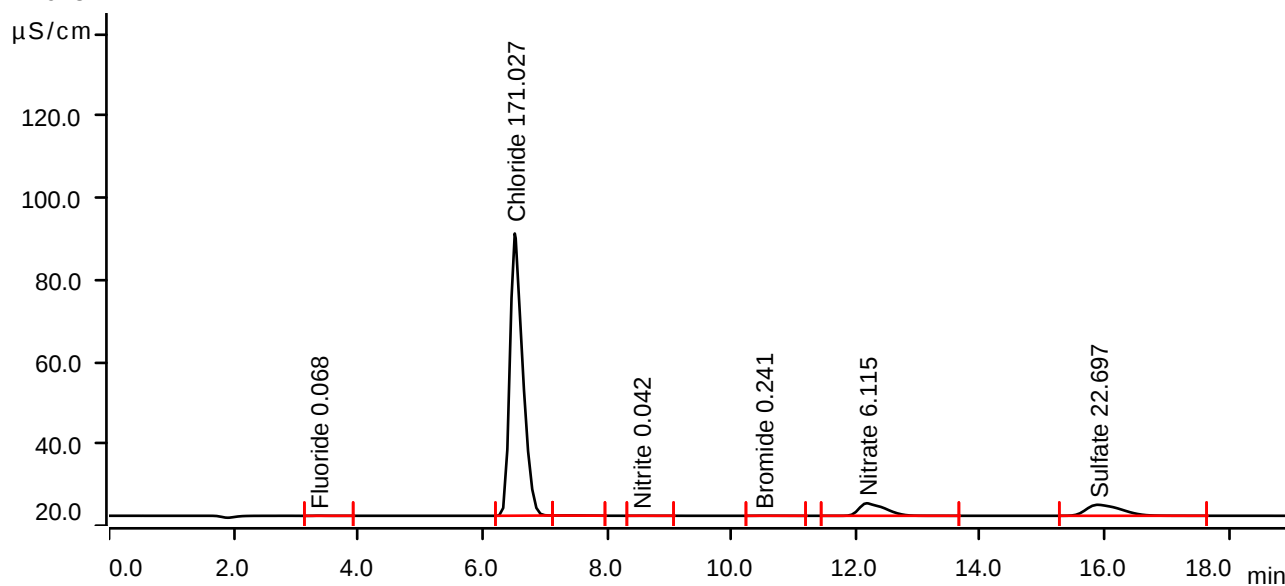

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.0083	0.037	0.068	Fluoride
2	6.520	16.2565	68.870	171.027	Chloride
3	7.352	0.0122	0.028	invalid	
4	8.543	0.0037	0.012	0.042	Nitrite
5	10.512	0.0110	0.026	0.241	Bromide
6	12.177	1.4617	3.059	6.115	Nitrate
7	15.888	1.7252	2.689	22.697	Sulfate


Sample data

Ident P5291-03
Sample type Sample
Determination start 2024-12-16 14:25:06 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

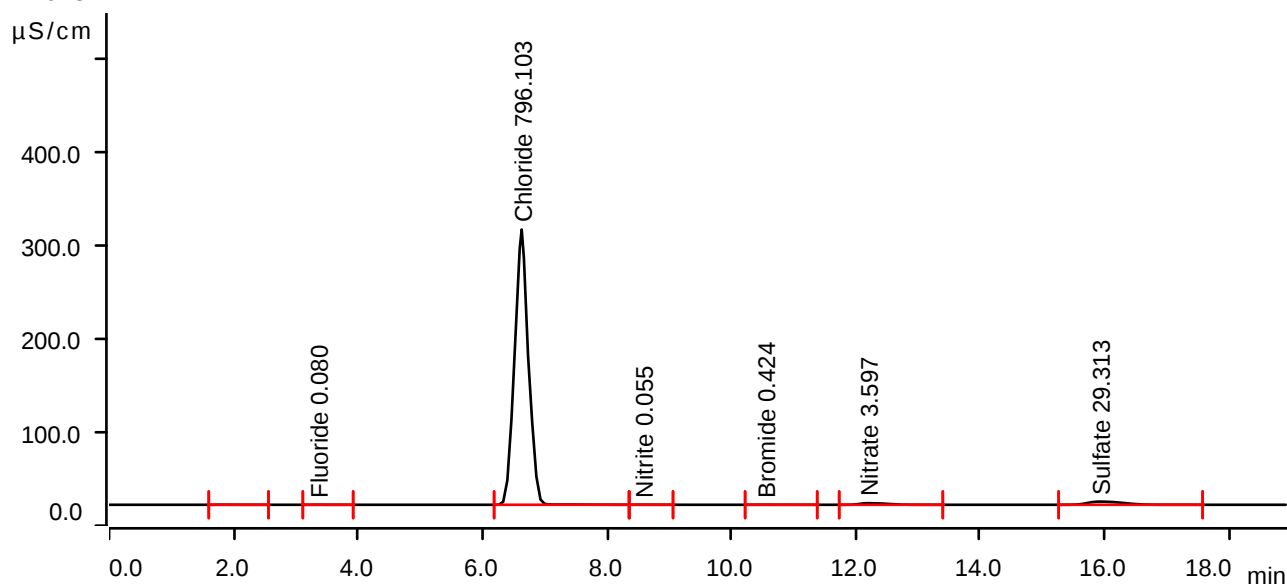

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.880	0.0176	0.071	invalid	
2	3.355	0.0101	0.053	0.080	Fluoride
3	6.632	75.6540	295.528	796.103	Chloride
4	8.573	0.0067	0.020	0.055	Nitrite
5	10.542	0.0188	0.044	0.424	Bromide
6	12.195	0.8602	1.747	3.597	Nitrate
7	15.920	2.2309	3.414	29.313	Sulfate


Sample data

Ident P5291-04
Sample type Sample
Determination start 2024-12-16 14:46:41 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

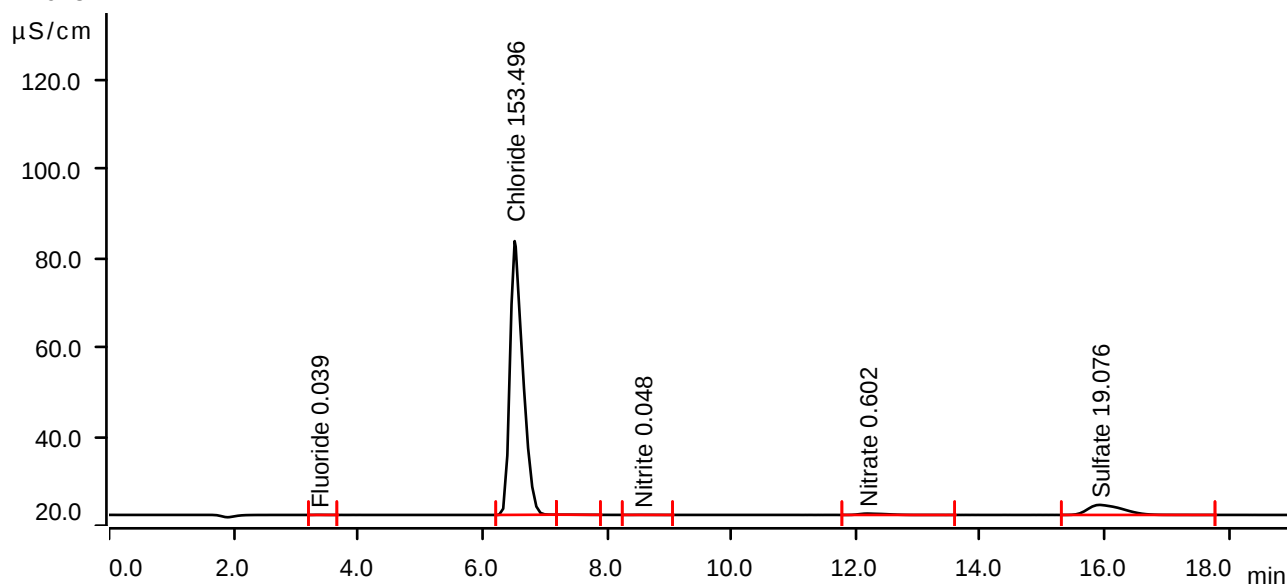

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.368	0.0042	0.024	0.039	Fluoride
2	6.518	14.5907	61.464	153.496	Chloride
3	7.357	0.0049	0.012	invalid	
4	8.563	0.0050	0.014	0.048	Nitrite
5	12.185	0.1448	0.300	0.602	Nitrate
6	15.915	1.4485	2.250	19.076	Sulfate


Sample data

Ident P5291-05
Sample type Sample
Determination start 2024-12-16 15:08:16 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

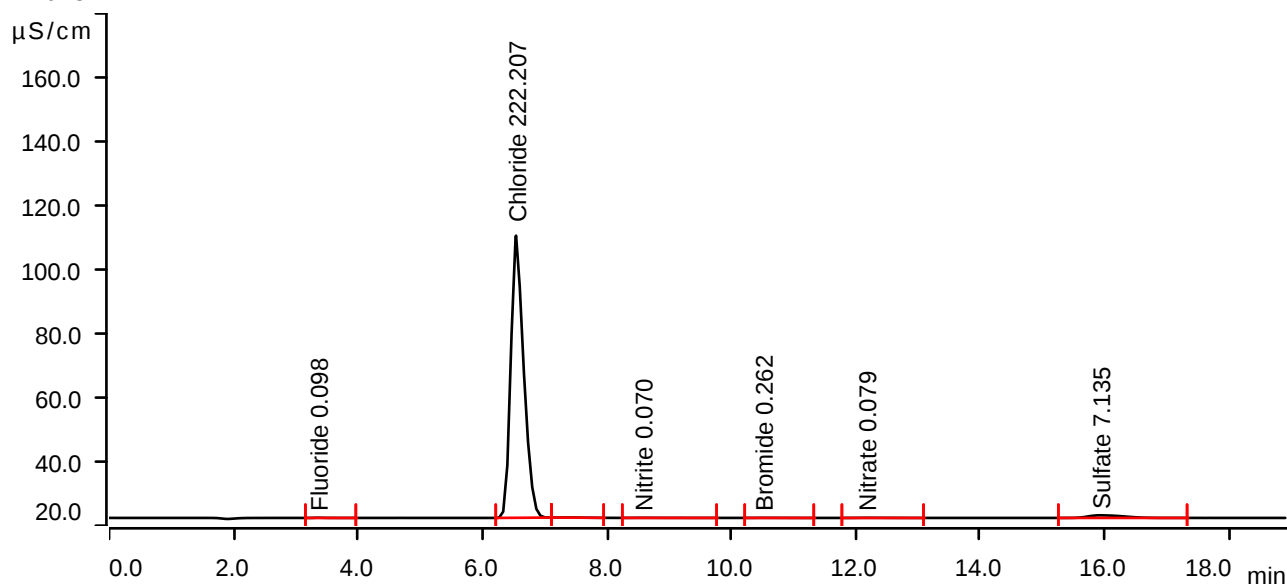

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.0128	0.066	0.098	Fluoride
2	6.542	21.1199	88.152	222.207	Chloride
3	7.315	0.0196	0.045	invalid	
4	8.570	0.0098	0.018	0.070	Nitrite
5	10.528	0.0119	0.028	0.262	Bromide
6	12.168	0.0200	0.041	0.079	Nitrate
7	15.927	0.5357	0.822	7.135	Sulfate


Sample data

Ident P5291-06
Sample type Sample
Determination start 2024-12-16 15:29:50 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

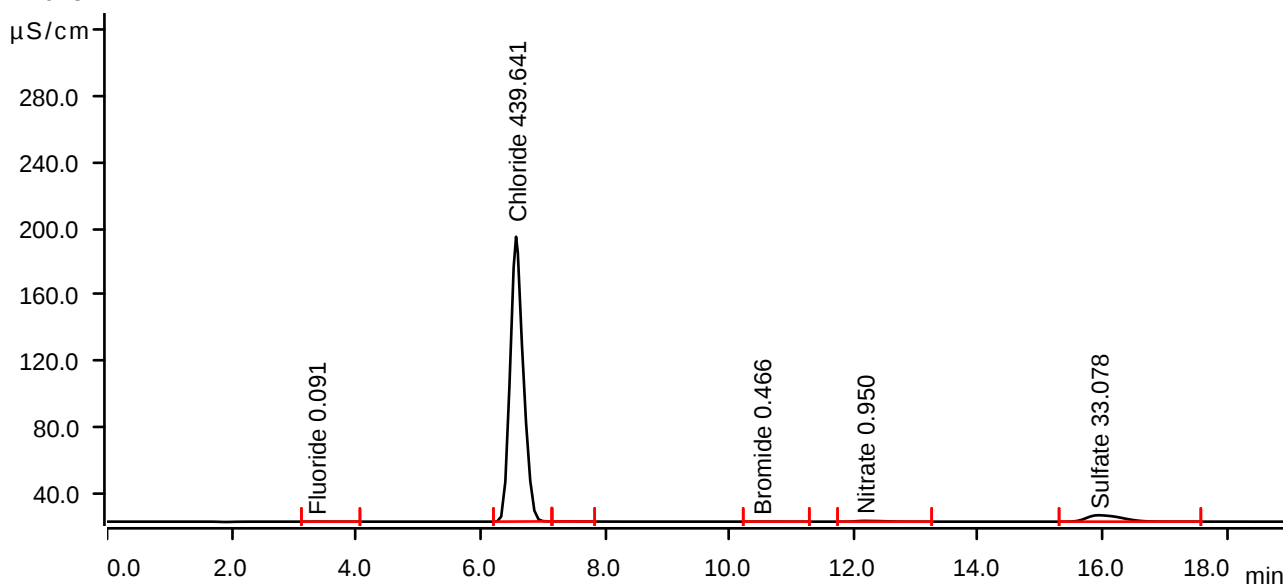

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.0118	0.059	0.091	Fluoride
2	6.573	41.7814	172.377	439.641	Chloride
3	7.288	0.0137	0.031	invalid	
4	10.508	0.0206	0.049	0.466	Bromide
5	12.172	0.2281	0.468	0.950	Nitrate
6	15.933	2.5187	3.896	33.078	Sulfate


Sample data

Ident P5291-07
Sample type Sample
Determination start 2024-12-16 15:51:24 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

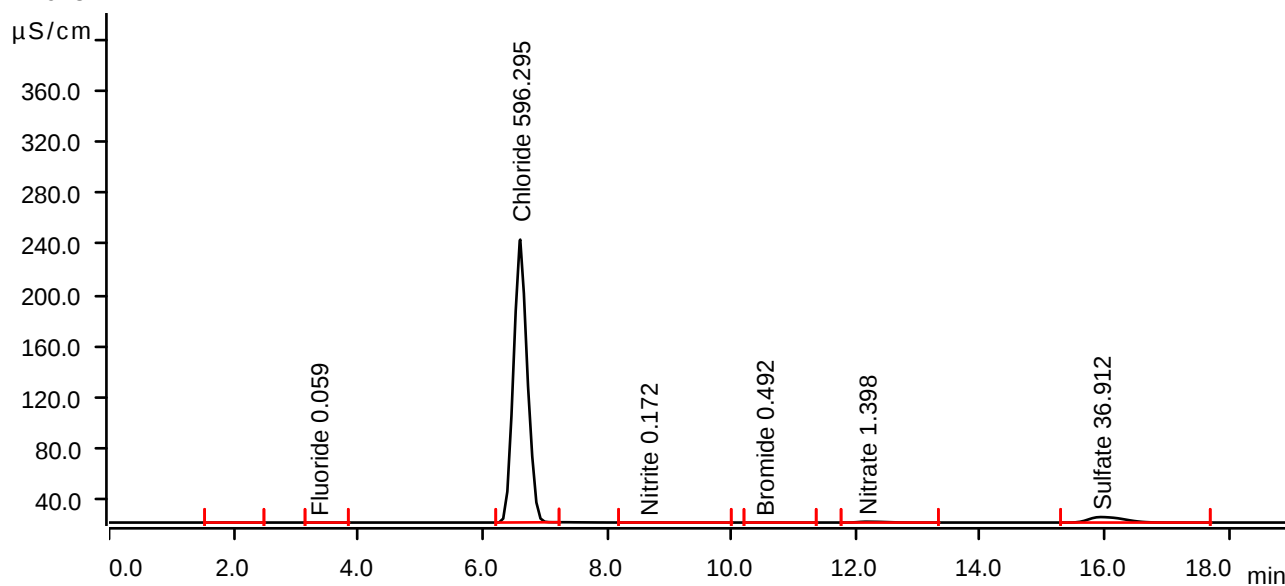

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.880	0.0167	0.067	invalid	
2	3.365	0.0071	0.037	0.059	Fluoride
3	6.608	56.6674	220.861	596.295	Chloride
4	8.613	0.0319	0.048	0.172	Nitrite
5	10.522	0.0217	0.050	0.492	Bromide
6	12.172	0.3350	0.679	1.398	Nitrate
7	15.938	2.8119	4.285	36.912	Sulfate


Sample data

Ident P5291-08MS
Sample type Sample
Determination start 2024-12-16 16:12:56 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

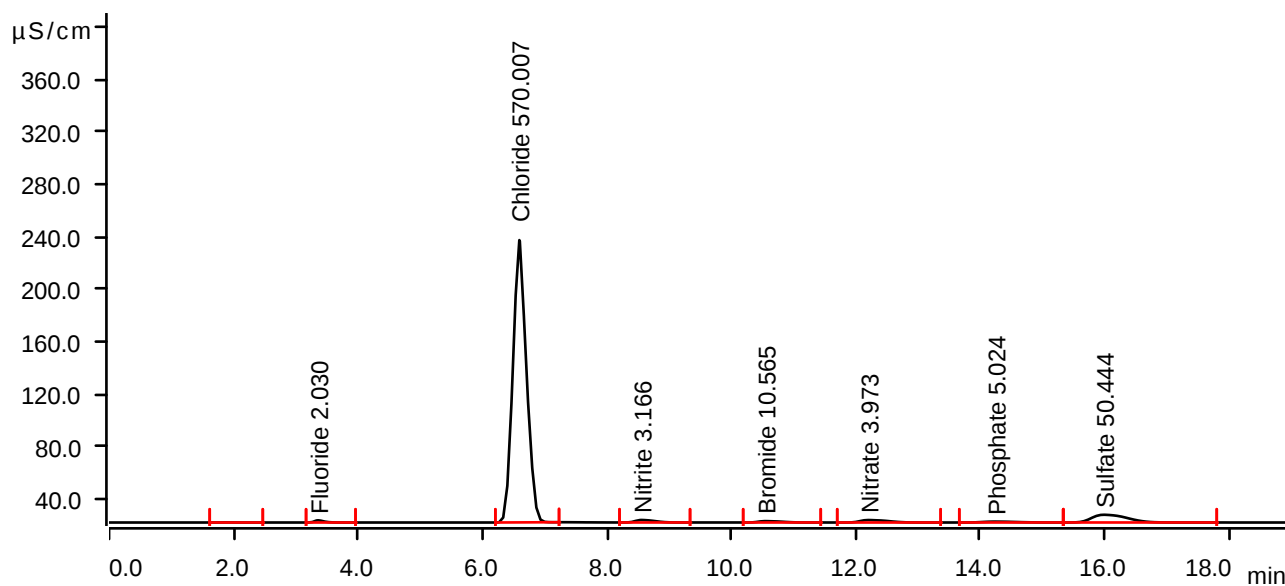

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.890	0.0190	0.078	invalid	
2	3.360	0.2942	1.672	2.030	Fluoride
3	6.593	54.1693	214.946	570.007	Chloride
4	8.558	0.6797	1.900	3.166	Nitrite
5	10.548	0.4494	1.050	10.565	Bromide
6	12.202	0.9501	1.888	3.973	Nitrate
7	14.243	0.4151	0.673	5.024	Phosphate
8	15.987	3.8462	5.885	50.444	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-12-16 16:34:19 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

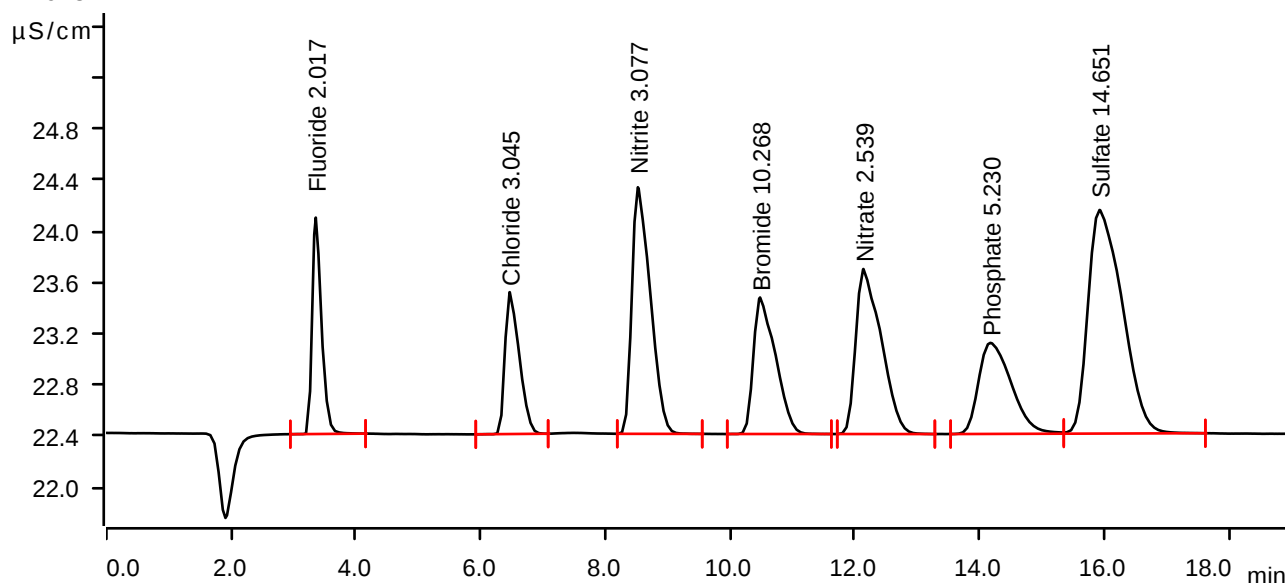

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.2923	1.690	2.017	Fluoride
2	6.465	0.2942	1.108	3.045	Chloride
3	8.522	0.6603	1.926	3.077	Nitrite
4	10.482	0.4367	1.066	10.268	Bromide
5	12.138	0.6075	1.289	2.539	Nitrate
6	14.173	0.4322	0.711	5.230	Phosphate
7	15.923	1.1102	1.746	14.651	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2024-12-16 16:55:50 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

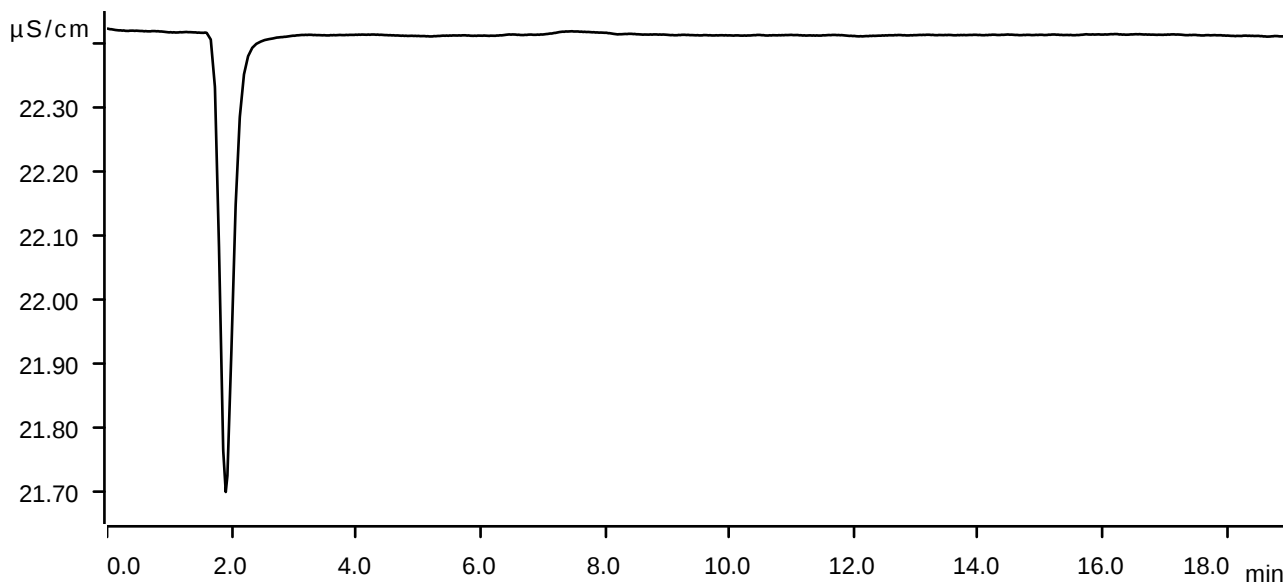


Sample data

Ident P5291-09MSD
Sample type Sample
Determination start 2024-12-16 17:17:20 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

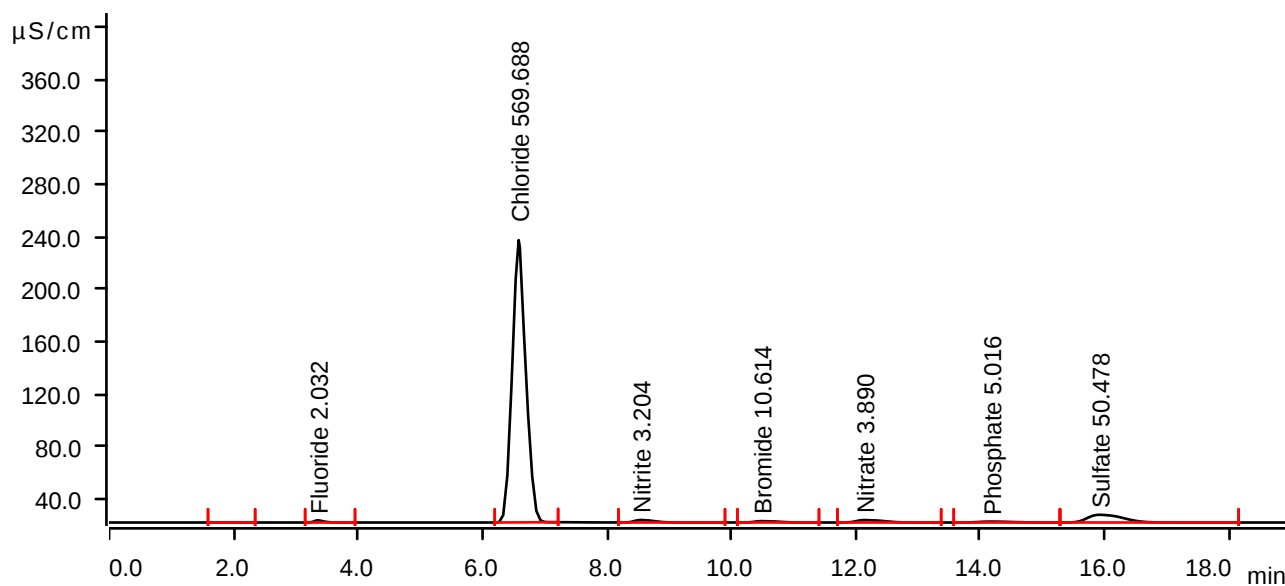

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.883	0.0195	0.079	invalid	
2	3.355	0.2945	1.674	2.032	Fluoride
3	6.583	54.1391	214.945	569.688	Chloride
4	8.542	0.6878	1.901	3.204	Nitrite
5	10.487	0.4514	1.053	10.614	Bromide
6	12.137	0.9302	1.886	3.890	Nitrate
7	14.175	0.4144	0.670	5.016	Phosphate
8	15.917	3.8488	5.871	50.478	Sulfate


Sample data

Ident P5291-10
Sample type Sample
Determination start 2024-12-16 17:38:52 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

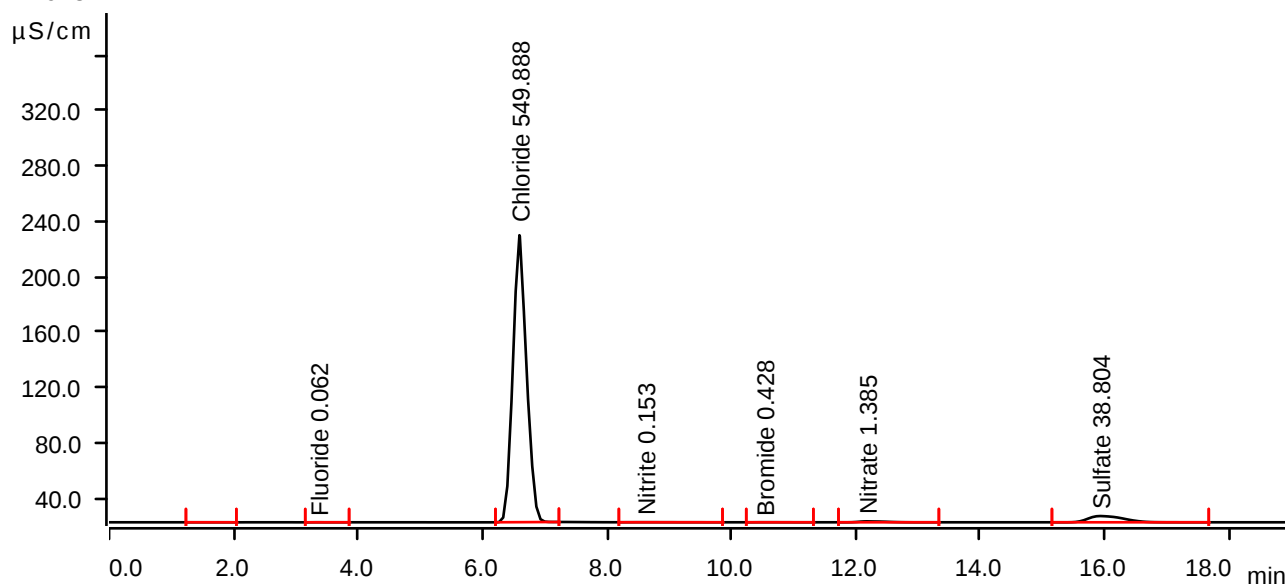

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.857	0.0029	0.012	invalid	
2	3.363	0.0076	0.038	0.062	Fluoride
3	6.595	52.2576	207.296	549.888	Chloride
4	8.613	0.0278	0.044	0.153	Nitrite
5	10.525	0.0190	0.044	0.428	Bromide
6	12.177	0.3319	0.669	1.385	Nitrate
7	15.925	2.9565	4.510	38.804	Sulfate


Sample data

Ident P5291-11
Sample type Sample
Determination start 2024-12-16 18:00:15 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

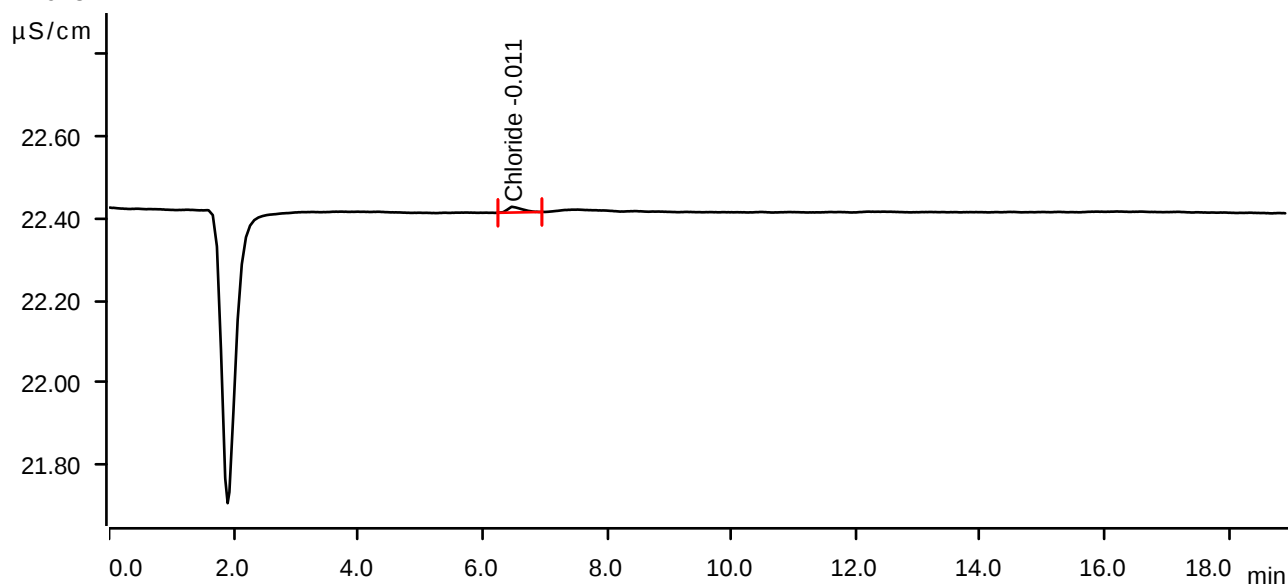

Peak number	Retention time	Area	Height	Concentration	Component name
	min	($\mu\text{S/cm}$) x min	$\mu\text{S/cm}$	ppm	
1	6.475	0.0038	0.014	-0.011	Chloride


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-12-16 18:21:45 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

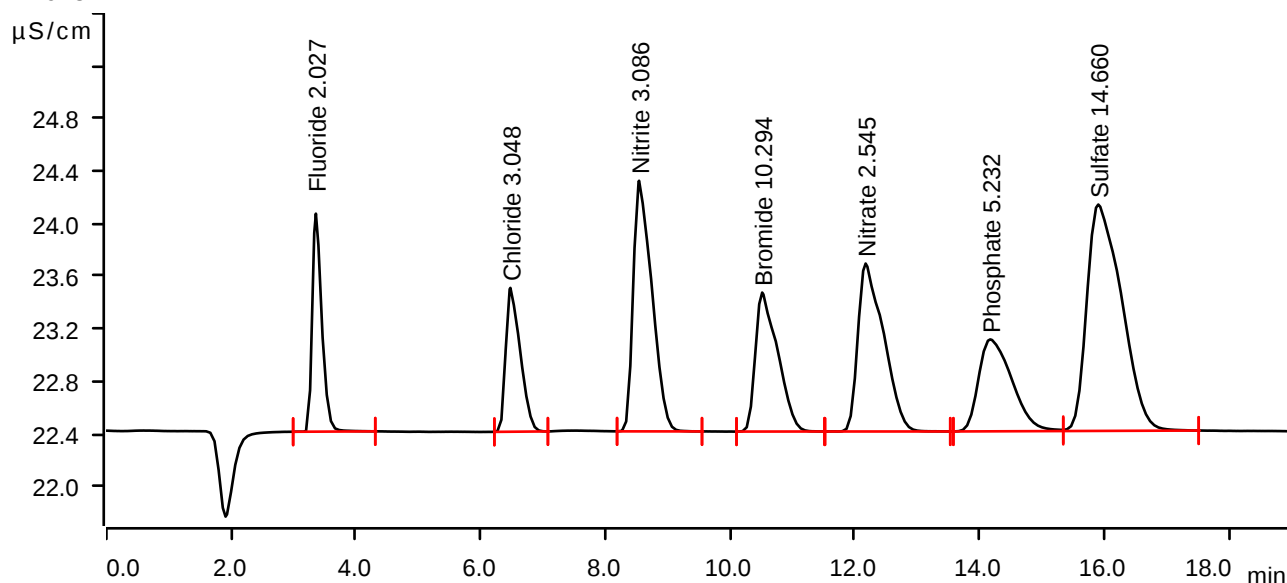

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.360	0.2937	1.660	2.027	Fluoride
2	6.478	0.2945	1.095	3.048	Chloride
3	8.542	0.6623	1.908	3.086	Nitrite
4	10.515	0.4378	1.058	10.294	Bromide
5	12.173	0.6091	1.279	2.545	Nitrate
6	14.172	0.4324	0.700	5.232	Phosphate
7	15.903	1.1109	1.724	14.660	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2024-12-16 18:43:15 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

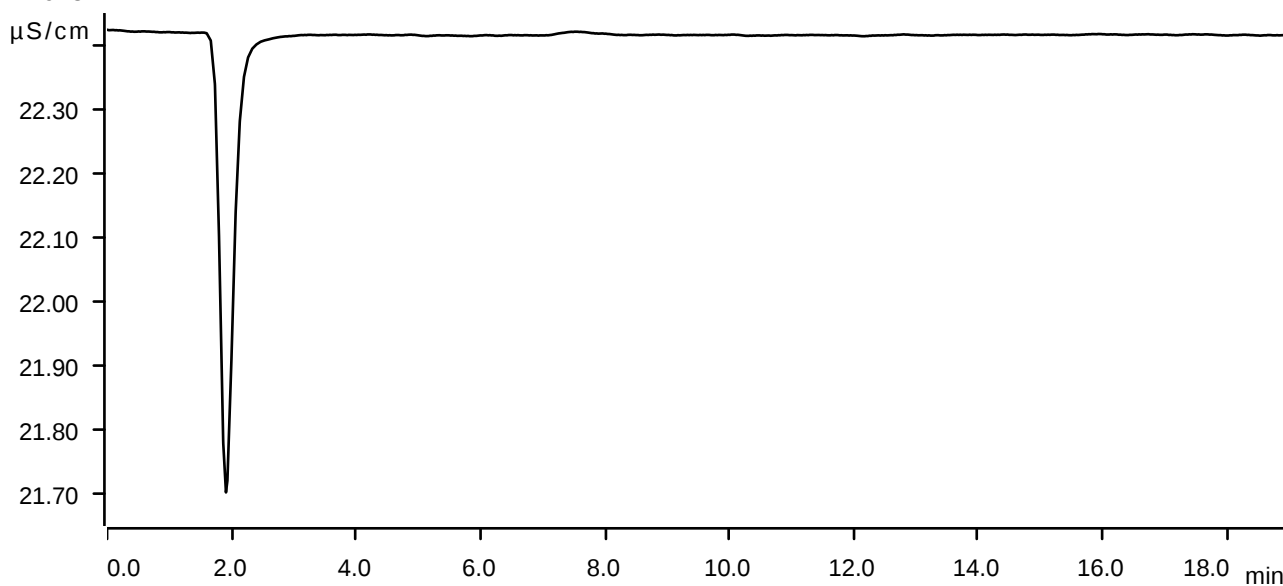


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-12-17 09:51:03 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

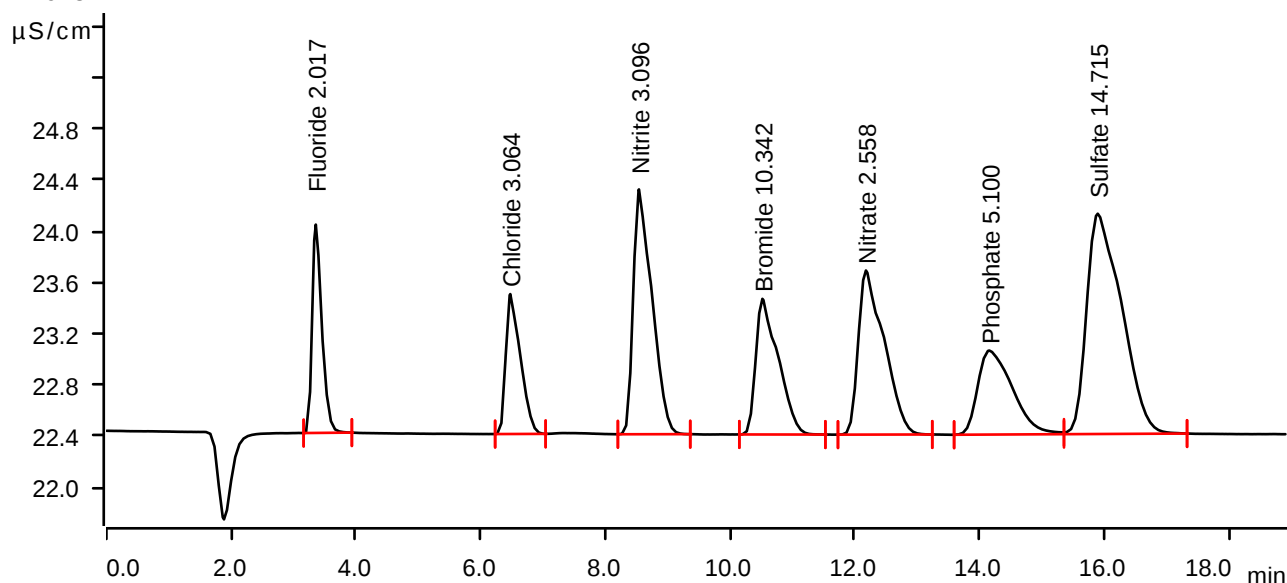

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.2923	1.627	2.017	Fluoride
2	6.477	0.2960	1.093	3.064	Chloride
3	8.540	0.6645	1.912	3.096	Nitrite
4	10.518	0.4399	1.059	10.342	Bromide
5	12.178	0.6120	1.282	2.558	Nitrate
6	14.157	0.4214	0.656	5.100	Phosphate
7	15.895	1.1151	1.720	14.715	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2024-12-17 10:12:33 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

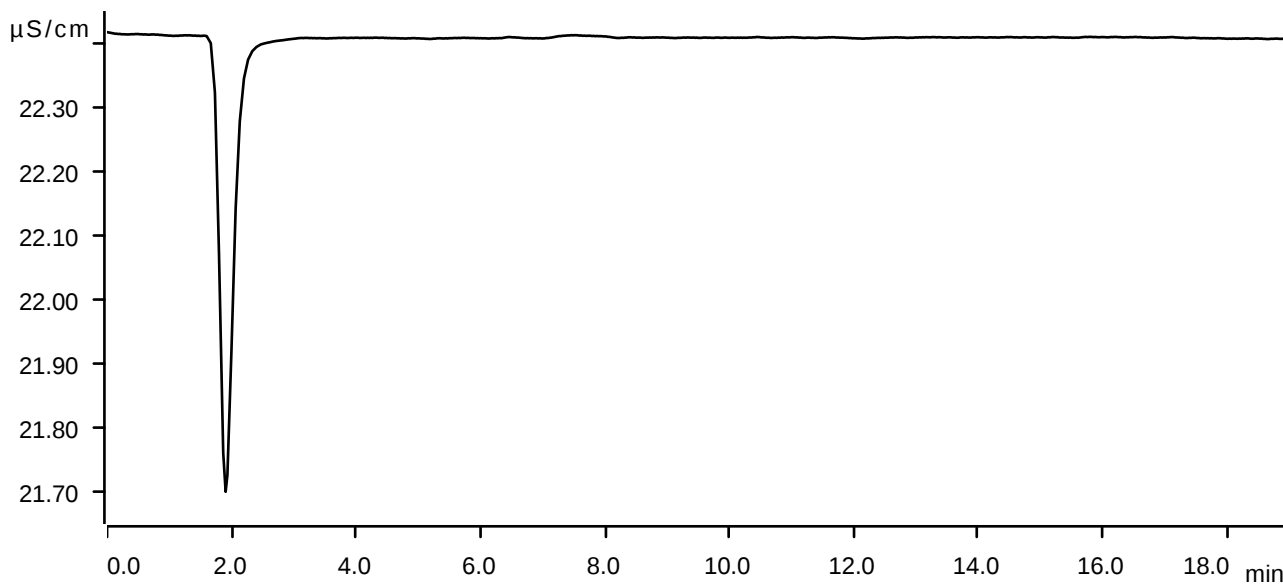


Sample data

Ident LB133970BLW2
Sample type Sample
Determination start 2024-12-17 10:34:03 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

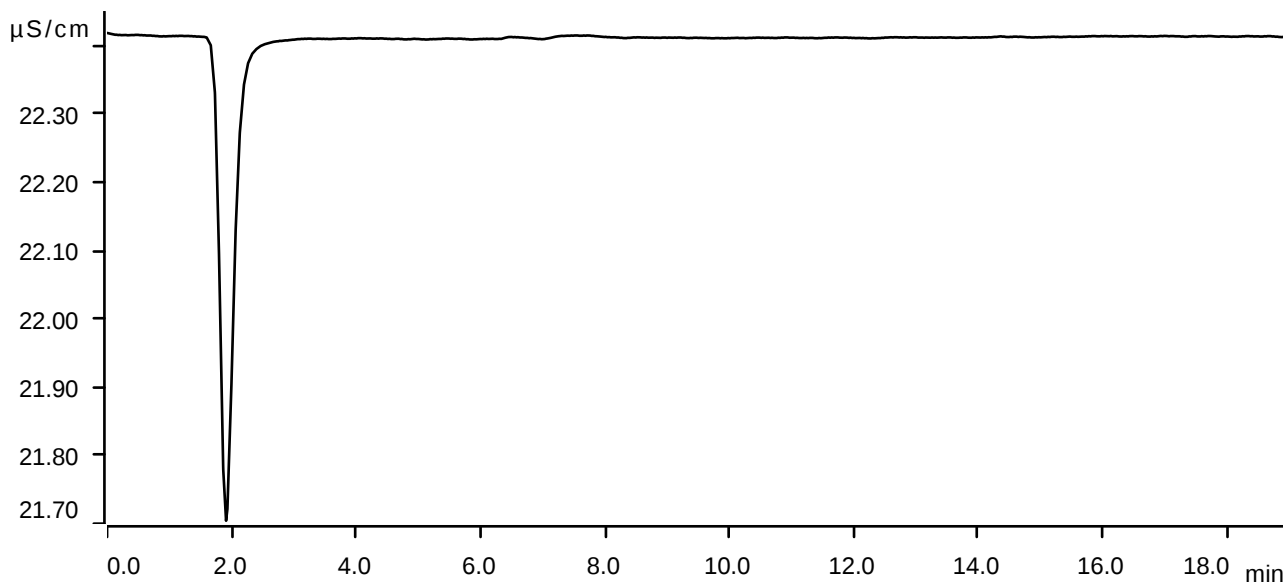


Sample data

Ident LB133970BSW2
Sample type Check standard 1
Determination start 2024-12-17 10:55:35 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

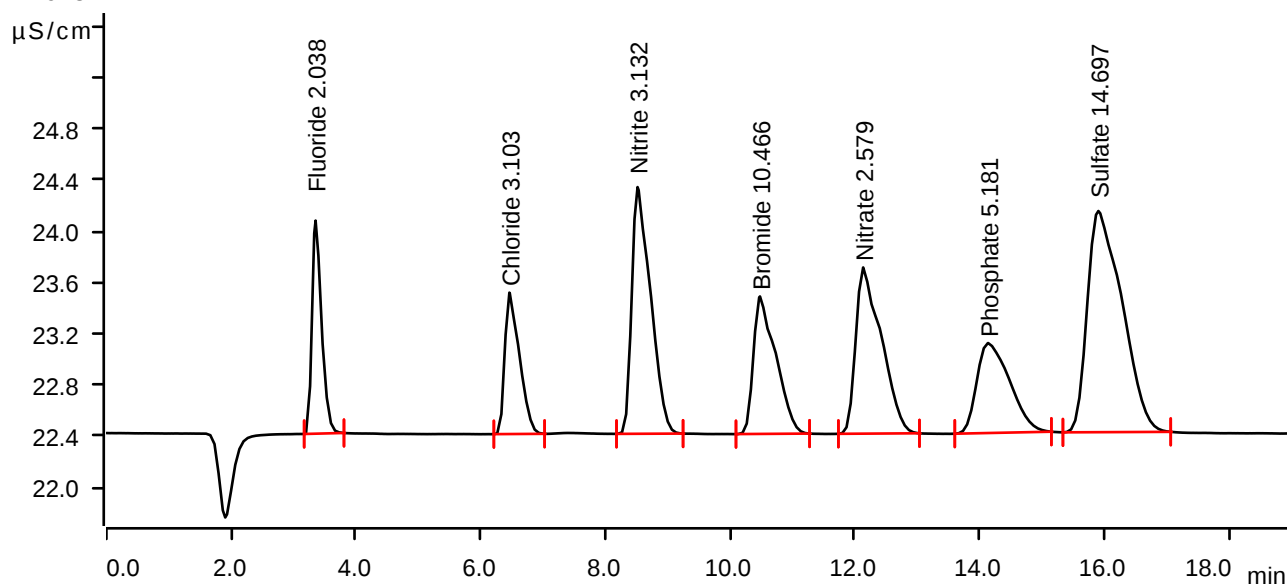

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.2954	1.664	2.038	Fluoride
2	6.462	0.2997	1.104	3.103	Chloride
3	8.517	0.6722	1.927	3.132	Nitrite
4	10.480	0.4451	1.073	10.466	Bromide
5	12.135	0.6171	1.298	2.579	Nitrate
6	14.138	0.4281	0.702	5.181	Phosphate
7	15.905	1.1137	1.727	14.697	Sulfate


Sample data

Ident P5291-10DLX2
Sample type Sample
Determination start 2024-12-17 11:17:07 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

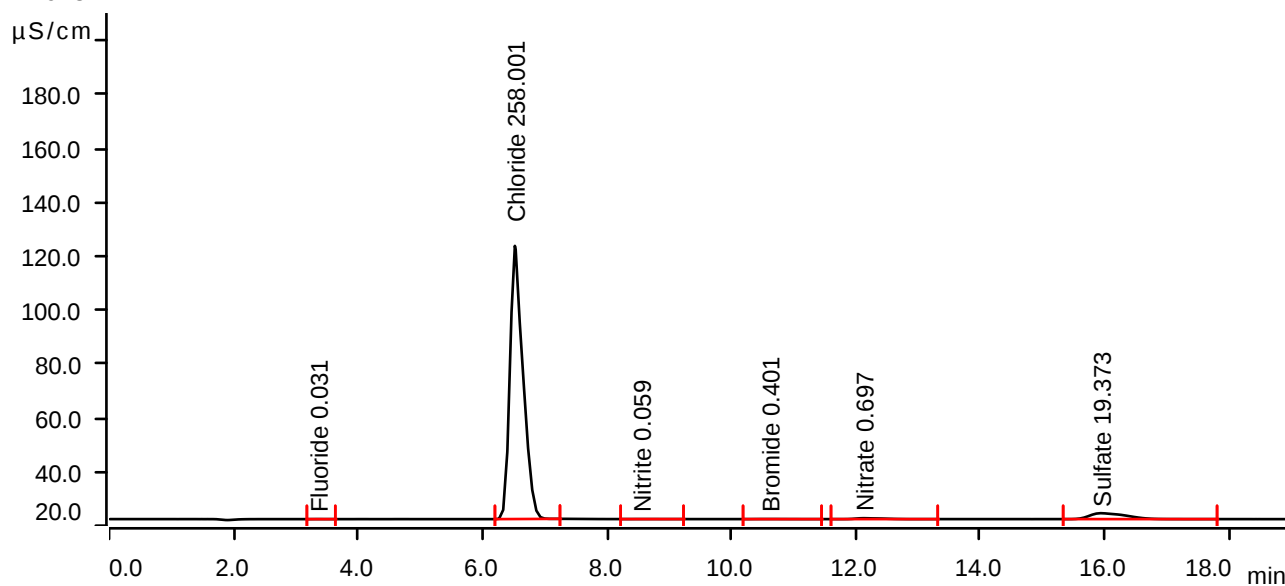

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.0031	0.017	0.031	Fluoride
2	6.522	24.5212	101.322	258.001	Chloride
3	8.545	0.0074	0.015	0.059	Nitrite
4	10.612	0.0178	0.031	0.401	Bromide
5	12.123	0.1677	0.342	0.697	Nitrate
6	15.938	1.4712	2.201	19.373	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-12-17 11:38:37 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

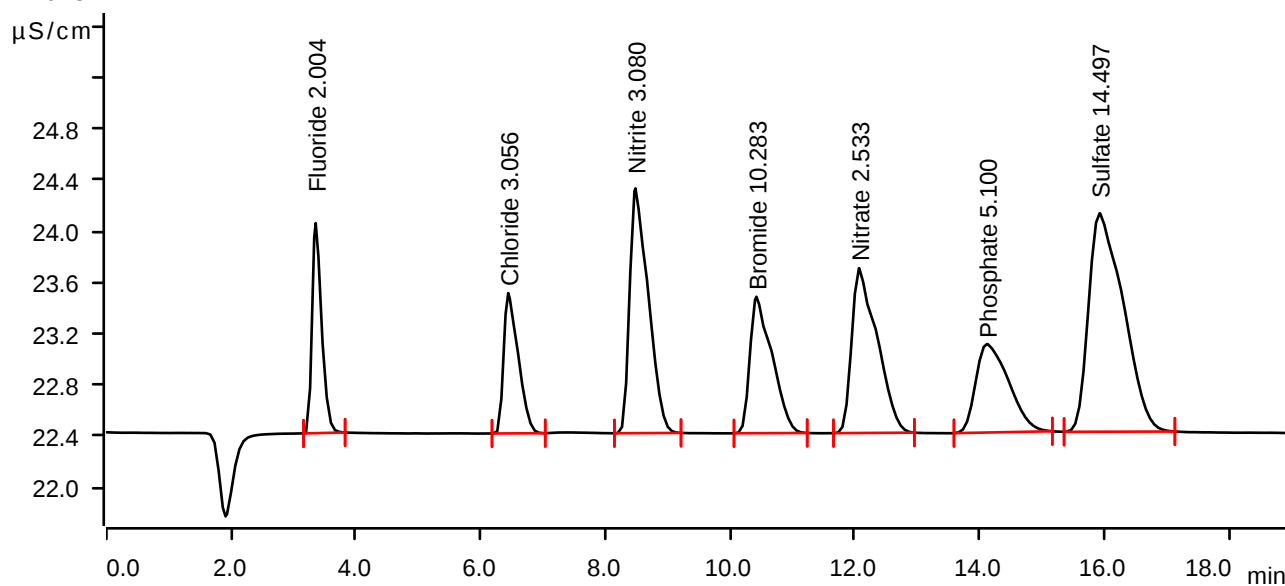

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.2904	1.640	2.004	Fluoride
2	6.443	0.2953	1.096	3.056	Chloride
3	8.483	0.6611	1.912	3.080	Nitrite
4	10.423	0.4374	1.065	10.283	Bromide
5	12.070	0.6062	1.288	2.533	Nitrate
6	14.118	0.4215	0.691	5.100	Phosphate
7	15.925	1.0984	1.706	14.497	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2024-12-17 12:00:07 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

