


LB133975

SFAM01.1

INSTRUMENT ID: CV1

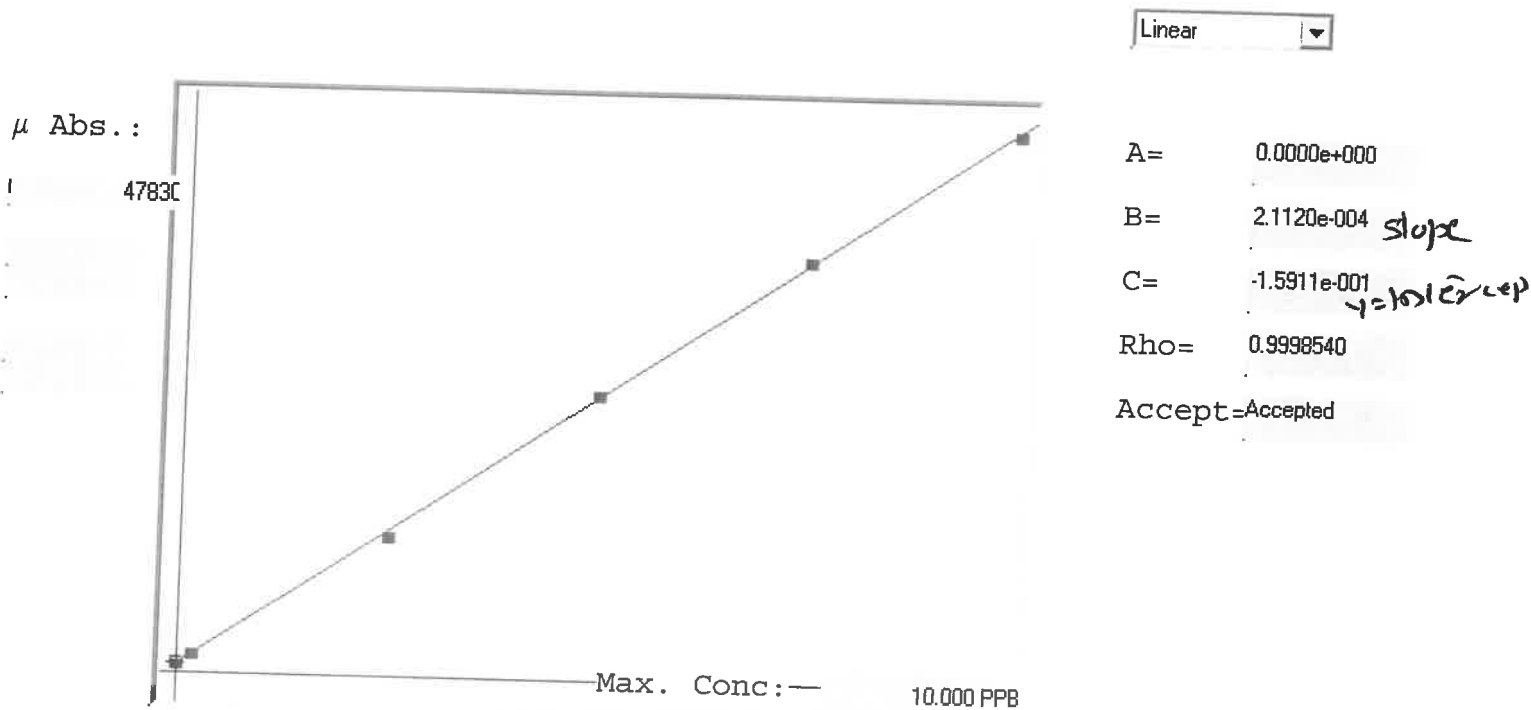

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	Std
0.00	0.000	0.026	0.026	878	0.000	878	0				0.026
0.05	0.050					442	0				1.1
0.20	0.200	0.207	0.007	1735	0.0 %	1735					1.4
2.50	2.500	2.394	-0.106	12087	0.0 %	12087					1.4
5.00	5.000	5.064	0.064	24733	0.0 %	24733					1.4
7.50	7.500	7.566	0.066	36577	0.0 %	36577					1.4
10.0	10.000	9.942	-0.058	47830	0.0 %	47830					1.4

LB133975

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	878	-		0 SFAM01.1	PPB	12/17/2024 14:00	Std
	0.2 S01	1735	-		0.2 SFAM01.1	PPB	12/17/2024 14:02	Std
	2.5 S02	12087	-		2.5 SFAM01.1	PPB	12/17/2024 14:06	Std
	5 S03	24733	-		5 SFAM01.1	PPB	12/17/2024 14:09	Std
	7.5 S04	36577	-		7.5 SFAM01.1	PPB	12/17/2024 14:11	Std
	10 S05	47830	-		10 SFAM01.1	PPB	12/17/2024 14:13	Std
ICV21	ICV21	19166	3.8887 -		SFAM01.1	PPB	12/17/2024 14:22	SMPL
ICB21	ICB21	699	-0.0115 -		SFAM01.1	PPB	12/17/2024 14:25	SMPL
CCV35	CCV35	24642	5.0452 -		SFAM01.1	PPB	12/17/2024 14:27	SMPL
CCB35	CCB35	702	-0.0109 -		SFAM01.1	PPB	12/17/2024 14:29	SMPL
PB165697BL	PBW697	611	-0.0301 -		SFAM01.1	PPB	12/17/2024 14:31	SMPL
PB165541TB	LEB541	494	-0.0548 -		SFAM01.1	PPB	12/17/2024 14:34	SMPL
P5169-01	MJNLH1	416	-0.0713 -		SFAM01.1	PPB	12/17/2024 14:36	SMPL
P5169-02	MJNLH2	481	-0.0575 -		SFAM01.1	PPB	12/17/2024 14:38	SMPL
P5169-03	MJNLH5	4838	0.8627 -		SFAM01.1	PPB	12/17/2024 14:40	SMPL
P5169-04	MJNLH4	1671	0.1938 -		SFAM01.1	PPB	12/17/2024 14:59	SMPL
P5169-05	MJNLH4D	1559	0.1701 -		SFAM01.1	PPB	12/17/2024 15:05	SMPL
P5169-06	MJNLH4S	6464	1.2061 -		SFAM01.1	PPB	12/17/2024 15:07	SMPL
CCV36	CCV36	24438	5.0021 -		SFAM01.1	PPB	12/17/2024 15:09	SMPL
CCB36	CCB36	750	-0.0007 -		SFAM01.1	PPB	12/17/2024 15:12	SMPL