


LB134109

245.1

INSTRUMENT ID: CV1

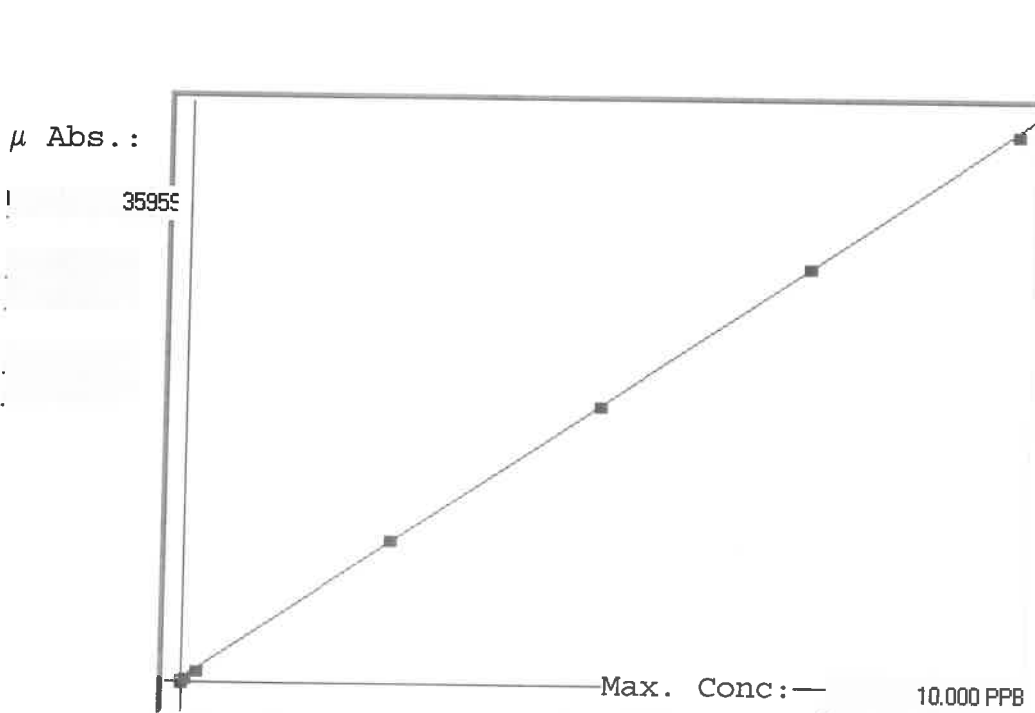

Linear

A= 0.0000e+000

B= 2.7821e-004

C= -5.2546e-002

Rho= 0.9999619

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	-0.020	-0.020	117	0.000	117					41.0
0.05	0.050	0.040	-0.010	332	0.0 %	332					20
0.2	0.200	0.175	-0.025	818	0.0 %	818	0				-13
2.5	2.500	2.548	0.048	9346	0.0 %	9346					2
5.0	5.000	5.023	0.023	18242	0.0 %	18242					0
7.5	7.500	7.533	0.033	27266	0.0 %	27266					0
10.0	10.000	9.952	-0.048	35959	0.0 %	35959					0

LB134109 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 27 Dec 2024 13:29:53

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	117	-	0.0000	245.1	PPB	27 Dec 2024 13:44:00	S	Std
0.05 - 1	50.05	332	-	0.0500	245.1	PPB	27 Dec 2024 13:46:16	S	Std
0.2 - 1	50.2	818	-	0.2000	245.1	PPB	27 Dec 2024 13:48:34	S	Std
2.5 - 1	52.5	9346	-	2.5000	245.1	PPB	27 Dec 2024 13:50:51	S	Std
5.0 - 1	55	18242	-	5.0000	245.1	PPB	27 Dec 2024 13:53:07	S	Std
7.5 - 1	57.5	27266	-	7.5000	245.1	PPB	27 Dec 2024 13:55:23	S	Std
10.0 - 1	510	35959	-	10.0000	245.1	PPB	27 Dec 2024 14:08:25	S	Std
ICV34 - 1	ICV34	15110	4.1512	-245.1		PPB	27 Dec 2024 14:13:58	U	SMPL
ICB34 - 1	ICB34	186	-0.0008	-245.1		PPB	27 Dec 2024 14:18:52	U	SMPL
CCV76 - 1	CCV76	19200	5.2891	-245.1		PPB	27 Dec 2024 14:21:07	U	SMPL
CCB76 - 1	CCB76	74	-0.0320	-245.1		PPB	27 Dec 2024 14:23:22	U	SMPL
CRA - 1	CRA	348	0.0443	-245.1		PPB	27 Dec 2024 14:30:56	U	SMPL
HighStd - 1	HighStd	37082	10.2641	-245.1		PPB	27 Dec 2024 14:33:11	U	SMPL
ChkStd - 1	ChkStd	26822	7.4097	-245.1		PPB	27 Dec 2024 14:35:26	U	SMPL
PB165897BL - 1	PBW	-111	-0.0834	-245.1		PPB	27 Dec 2024 14:47:38	U	SMPL
PB165897BS - 1	LCSW	13885	3.8104	-245.1		PPB	27 Dec 2024 14:55:58	U	SMPL
P4368-12 - 1	MDL-WATER-06-QT4-2024	345	0.0434	-245.1		PPB	27 Dec 2024 15:08:51	U	SMPL
P5297-02 - 1	SEPT-23	810	0.1728	-245.1		PPB	27 Dec 2024 15:11:07	U	SMPL
P5297-02DUP - 1	SEPT-23DUP	531	0.0952	-245.1		PPB	27 Dec 2024 15:16:03	U	SMPL
P5297-02MS - 1	SEPT-23MS	12108	3.3161	-245.1		PPB	27 Dec 2024 15:18:19	U	SMPL
P5297-02MSD - 1	SEPT-23MSD	12061	3.3030	-245.1		PPB	27 Dec 2024 15:20:34	U	SMPL
CCV77 - 1	CCV77	17968	4.9464	-245.1		PPB	27 Dec 2024 15:22:52	U	SMPL
CCB77 - 1	CCB77	42	-0.0409	-245.1		PPB	27 Dec 2024 15:25:09	U	SMPL
P4368-10 - 1	LOD-MDL-WATER-04-QT4-2024	327	0.0384	-245.1		PPB	27 Dec 2024 15:30:00	U	SMPL
P4368-10RE - 1	LOD-MDL-WATER-04-QT4-2024RE	715	0.1464	-245.1		PPB	27 Dec 2024 15:32:16	U	SMPL
P5297-02LX5 - 1		365	0.0490	-245.1		PPB	27 Dec 2024 15:34:32	U	SMPL
P5297-02A - 1		13171	3.6118	-245.1		PPB	27 Dec 2024 15:36:48	U	SMPL
CCV78 - 1	CCV78	17847	4.9127	-245.1		PPB	27 Dec 2024 15:39:03	U	SMPL
CCB78 - 1	CCB78	75	-0.0317	-245.1		PPB	27 Dec 2024 15:43:59	U	SMPL