


Ident	Instrument IC-1				Analyst :	NF	Method:	300.0 / 9056A	Initial \ Analyst			
	Con F-	Con CL-	Con NO2	Con BR-					Con NO3	Con HPO4	Con SO4	Method name
STD1	0	0	0	0	0	0	0	0	IC1-121824	12/18/2024 10:39	10 NF/IZ	
STD2	0.319	0.475	0.485	1.586	0.405	0.794	2.525	2.525	IC1-121824	12/18/2024 11:00	10 NF/IZ	
STD3	0.867	1.29	1.286	4.307	1.073	2.153	6.454	6.454	IC1-121824	12/18/2024 11:22	10 NF/IZ	
STD4	1.065	1.59	1.587	5.29	1.327	2.68	7.947	7.947	IC1-121824	12/18/2024 11:43	10 NF/IZ	
STD5	1.968	2.98	2.975	9.935	2.472	4.928	14.761	14.761	IC1-121824	12/18/2024 12:04	10 NF/IZ	
STD6	3.929	5.897	5.891	19.654	4.906	9.805	29.16	29.16	IC1-121824	12/18/2024 12:26	10 NF/IZ	
STD7	5.052	7.568	7.575	25.229	6.317	12.641	37.652	37.652	IC1-121824	12/18/2024 12:47	10 NF/IZ	
ICV	2.021	3.088	3.087	10.28	2.565	5.117	15.271	15.271	IC1-121824	12/18/2024 13:09	10 NF/IZ	
ICB	0	0	0	0	0	0	0	0	IC1-121824	12/18/2024 13:30	10 NF/IZ	
CCV	2.084	3.09	3.075	10.362	2.571	5.353	15.503	15.503	IC1-121824	1/9/2025 14:07	10 NF/IZ	
CCB	0	0	0	0	0	0	0	0	IC1-121824	1/9/2025 14:29	10 NF/IZ	
LB134228BLW	0	0	0	0	0	0	0	0	IC1-121824	1/9/2025 14:50	10 NF/IZ	
LB134228BSW	2.082	3.081	3.083	10.338	2.566	5.352	15.425	15.425	IC1-121824	1/9/2025 15:12	10 NF/IZ	
Q1049-01	0.429	632.662	0.218	0.667	0.185	0	18.157	18.157	IC1-121824	1/9/2025 15:51	10 NF/IZ	
Q1049-01MS	2.394	604.275	3.138	10.348	2.642	5.104	32.638	32.638	IC1-121824	1/9/2025 16:13	10 NF/IZ	
Q1049-01MSD	2.349	602.093	3.125	10.372	2.621	5.023	32.434	32.434	IC1-121824	1/9/2025 16:34	10 NF/IZ	
CCV	2.098	3.098	3.08	10.261	2.564	5.401	15.431	15.431	IC1-121824	1/9/2025 16:56	10 NF/IZ	
CCB	0	0	0	0	0	0	0	0	IC1-121824	1/9/2025 17:17	10 NF/IZ	

Clear table

Instrument ID: IC-2									
Analyst : IZ				Method: 300.0 / 9056A					
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	Initial wt/ Final
STD1	0	0	0	0	0	0	0	0 IC1-121824	10 NF/IZ
STD2	0.319	0.475	0.485	1.586	0.405	0.794	2.525	IC1-121824	10 NF/IZ
STD3	0.867	1.29	1.286	4.307	1.073	2.153	6.454	IC1-121824	10 NF/IZ
STD4	1.065	1.59	1.587	5.29	1.327	2.68	7.947	IC1-121824	10 NF/IZ
STD5	1.968	2.98	2.975	9.935	2.472	4.928	14.761	IC1-121824	10 NF/IZ
STD6	3.929	5.897	5.891	19.654	4.906	9.805	29.16	IC1-121824	10 NF/IZ
STD7	5.052	7.568	7.575	25.229	6.317	12.641	37.652	IC1-121824	10 NF/IZ
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		date time
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		12/18/2024 10:39
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		12/18/2024 11:00
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		12/18/2024 11:22
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		12/18/2024 11:43
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		12/18/2024 12:04
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		12/18/2024 12:26
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000		12/18/2024 12:47
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4		
STD1									
STD2	-20.2500	-20.8333	-19.1667	-20.7000	-19.0000	-20.6000	-15.8333		
STD3	8.3750	7.5000	7.1667	7.6750	7.3000	7.6500	7.5667		
STD4	6.5000	6.0000	5.8000	5.8000	6.1600	7.2000	5.9600		
STD5	-1.6000	-0.6667	-0.8333	-0.6500	-1.1200	-1.4400	-1.5933		
STD6	-1.7750	-1.7167	-1.8167	-1.7300	-1.8800	-1.9500	-2.8000		
STD7	1.0400	0.9067	1.0000	0.9160	1.0720	1.1280	1.7622		

Fluoride (Anions)

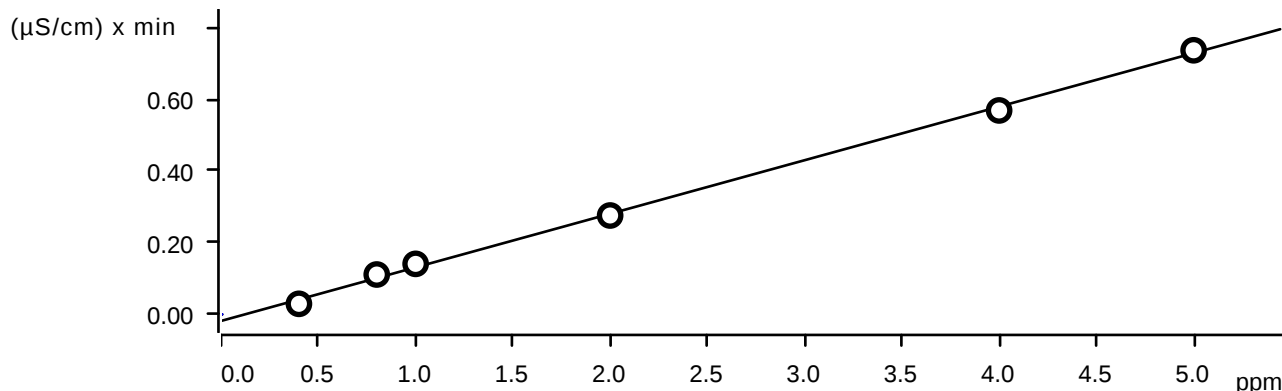


Function: $A = -0.0183596 + 0.0149351 \times Q$

Relative standard deviation 3.731557 %

Correlation coefficient 0.999324

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	0.400	10.0	1.0	1.0	0.029	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	1.000	10.0	1.0	1.0	0.141	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	2.000	10.0	1.0	1.0	0.276	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	4.000	10.0	1.0	1.0	0.568	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	5.000	10.0	1.0	1.0	0.736	STD7	2024-12-18 12:47:45 UTC-5	used

Chloride (Anions)

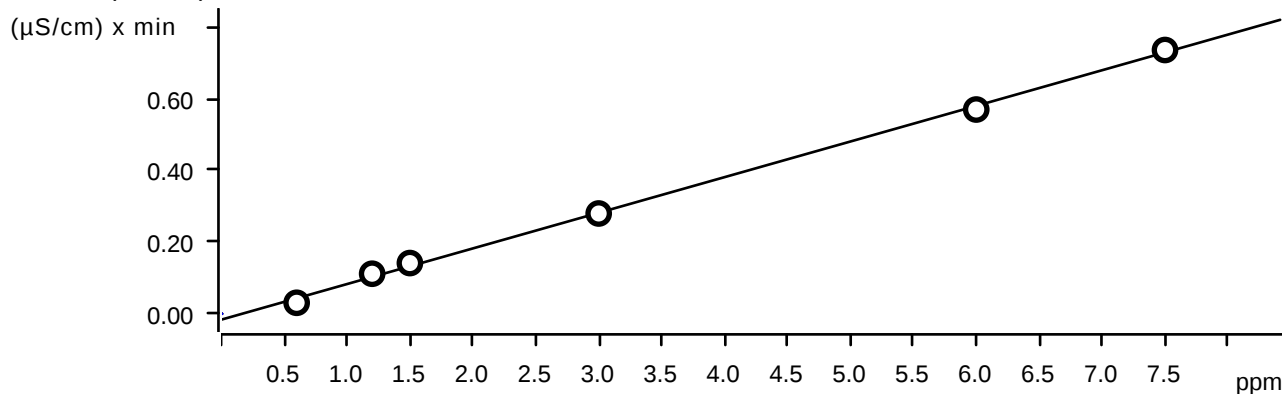


Function: $A = -0.0165562 + 9.93613E-3 \times Q$

Relative standard deviation 3.466087 %

Correlation coefficient 0.999410


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	0.600	10.0	1.0	1.0	0.031	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.112	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.141	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.280	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	0.569	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	0.735	STD7	2024-12-18 12:47:45 UTC-5	used

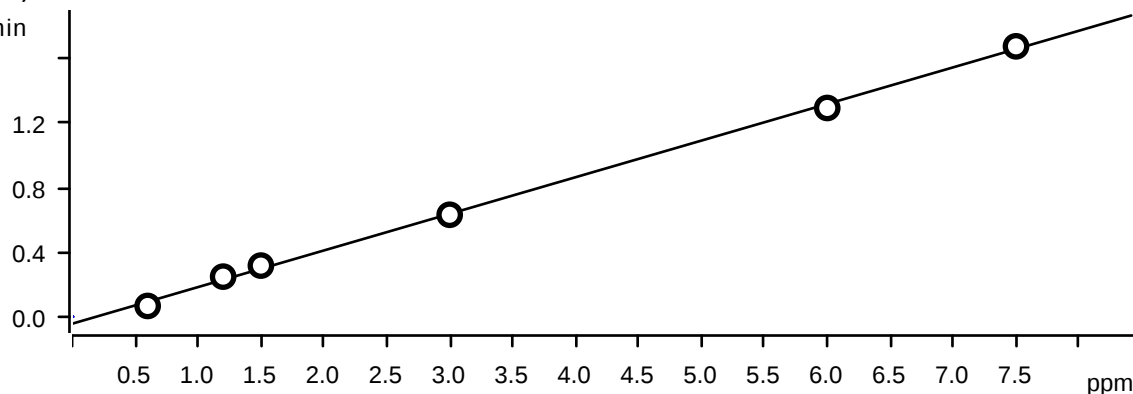Nitrite (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0434679 + 0.0226901 \times Q$

Relative standard deviation 3.455351 %

Correlation coefficient 0.999423

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	0.600	10.0	1.0	1.0	0.067	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.248	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.317	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.632	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	1.293	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	1.675	STD7	2024-12-18 12:47:45 UTC-5	used

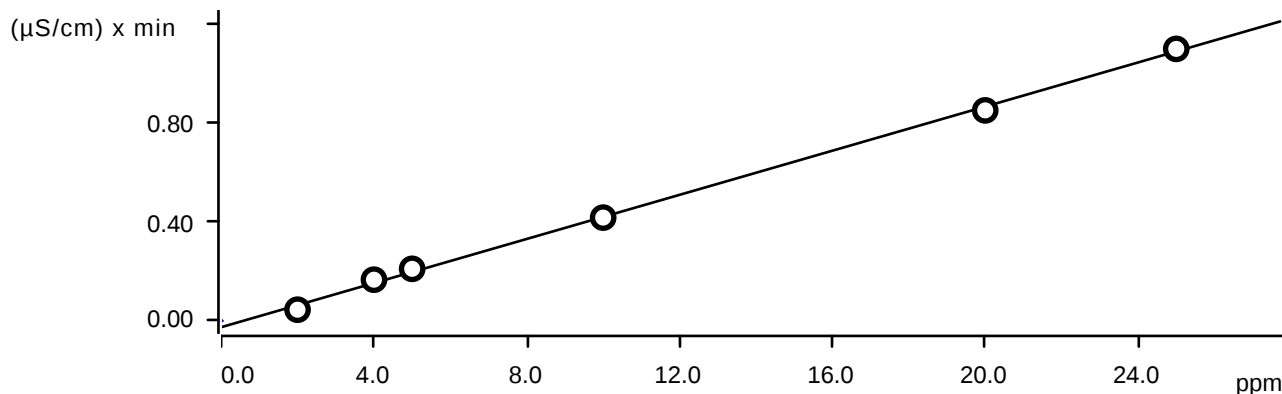
Bromide (Anions)

Function: $A = -0.0255661 + 4.44233E-3 \times Q$

Relative standard deviation 3.478545 %

Correlation coefficient 0.999408

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	2.000	10.0	1.0	1.0	0.045	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	4.000	10.0	1.0	1.0	0.166	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	5.000	10.0	1.0	1.0	0.209	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	10.000	10.0	1.0	1.0	0.416	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	20.000	10.0	1.0	1.0	0.848	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	25.000	10.0	1.0	1.0	1.095	STD7	2024-12-18 12:47:45 UTC-5	used

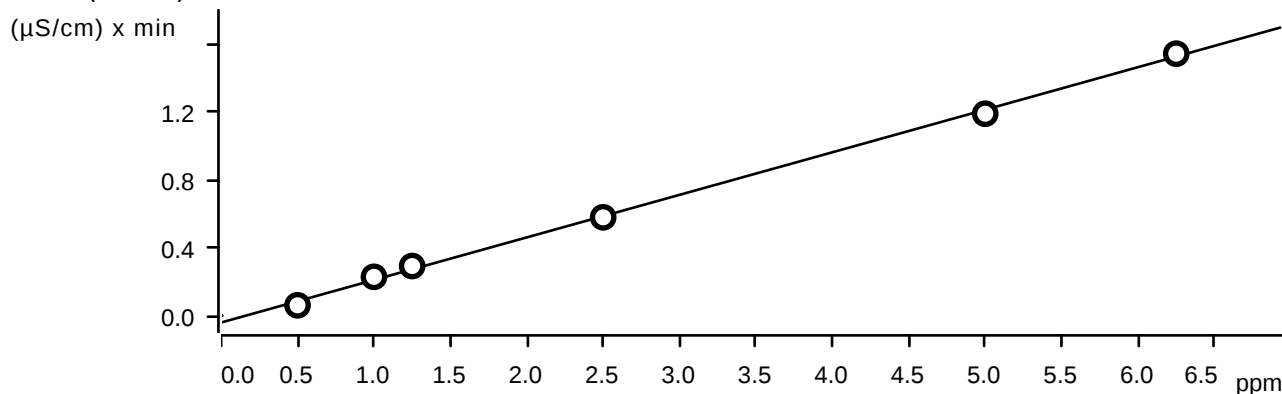Nitrate (Anions)


Function: $A = -0.0400484 + 0.0250507 \times Q$

Relative standard deviation 3.586984 %

Correlation coefficient 0.999378

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	0.500	10.0	1.0	1.0	0.061	STD2	2024-12-18 11:00:37 UTC-5	used

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 3	1	1.000	10.0	1.0	1.0	0.229	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	1.250	10.0	1.0	1.0	0.292	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	2.500	10.0	1.0	1.0	0.579	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	5.000	10.0	1.0	1.0	1.189	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	6.250	10.0	1.0	1.0	1.542	STD7	2024-12-18 12:47:45 UTC-5	used

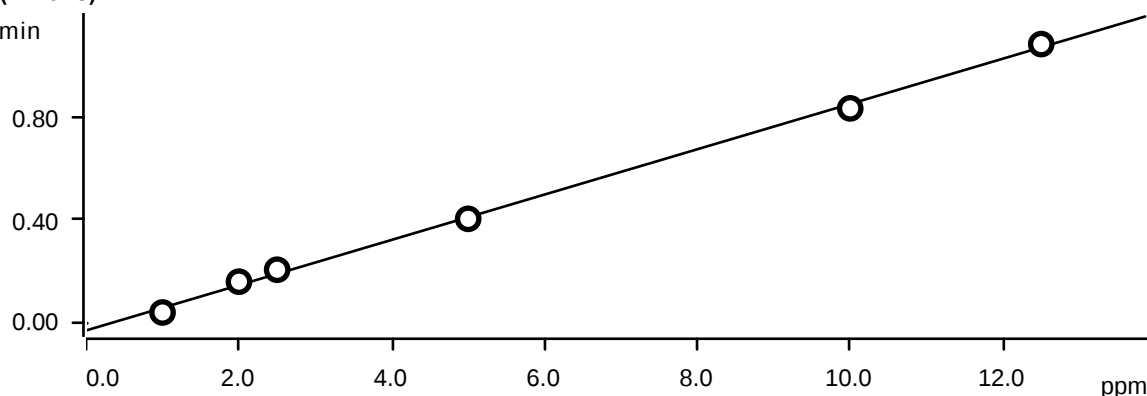
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0282076 + 8.77175E-3 \times Q$

Relative standard deviation 3.880200 %

Correlation coefficient 0.999273

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	1.000	10.0	1.0	1.0	0.041	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	2.000	10.0	1.0	1.0	0.161	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	2.500	10.0	1.0	1.0	0.207	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	5.000	10.0	1.0	1.0	0.404	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	10.000	10.0	1.0	1.0	0.832	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	12.500	10.0	1.0	1.0	1.081	STD7	2024-12-18 12:47:45 UTC-5	used

Sulfate (Anions)

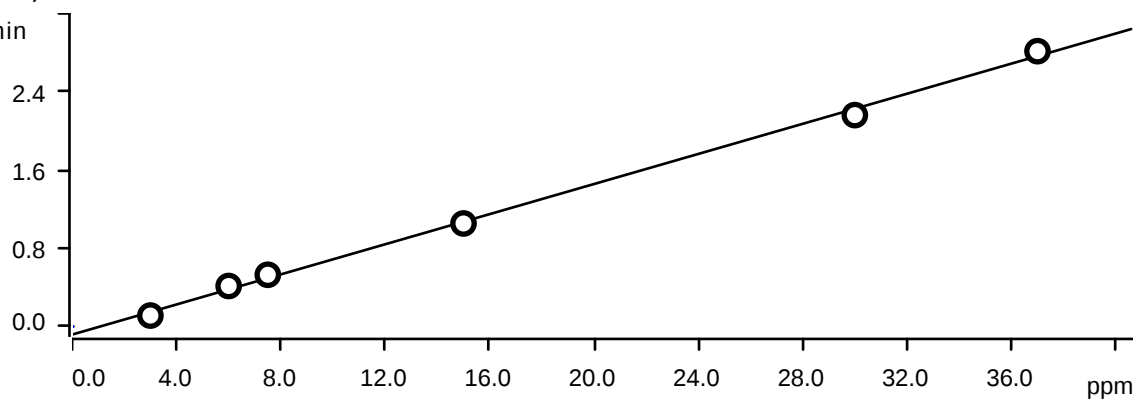 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0827937 + 7.69466E-3 \times Q$

Relative standard deviation 4.394299 %

Correlation coefficient 0.999072


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	3.000	10.0	1.0	1.0	0.112	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	6.000	10.0	1.0	1.0	0.414	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	7.500	10.0	1.0	1.0	0.529	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	15.000	10.0	1.0	1.0	1.053	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	30.000	10.0	1.0	1.0	2.161	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	37.000	10.0	1.0	1.0	2.814	STD7	2024-12-18 12:47:45 UTC-5	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2024-12-18 10:39:14 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

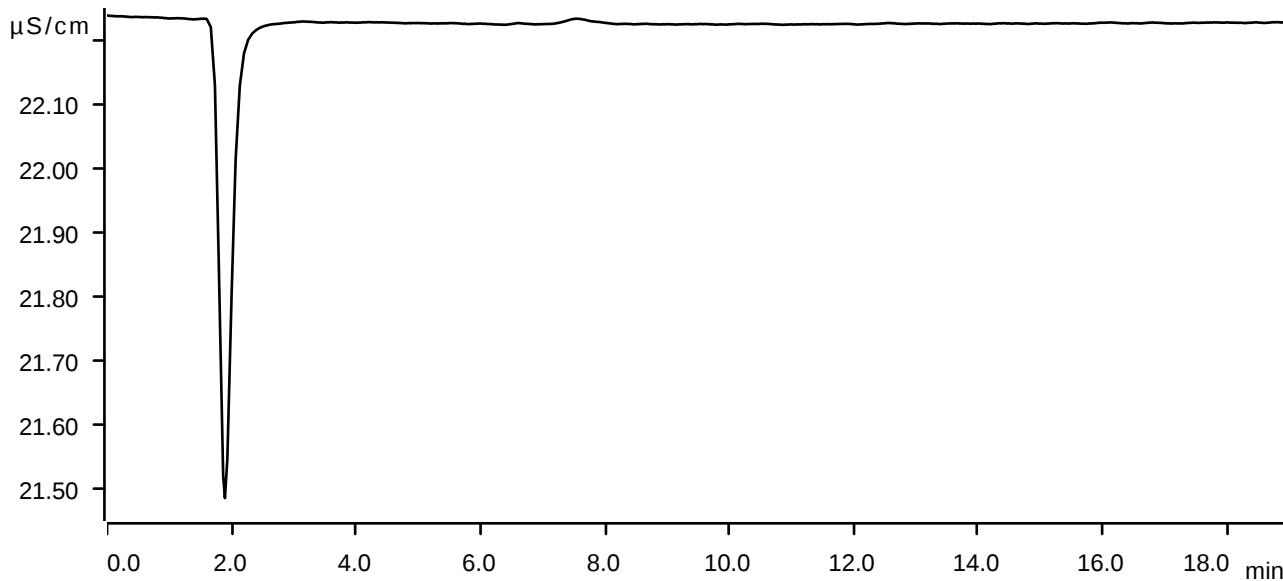Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2024-12-18 11:00:37 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

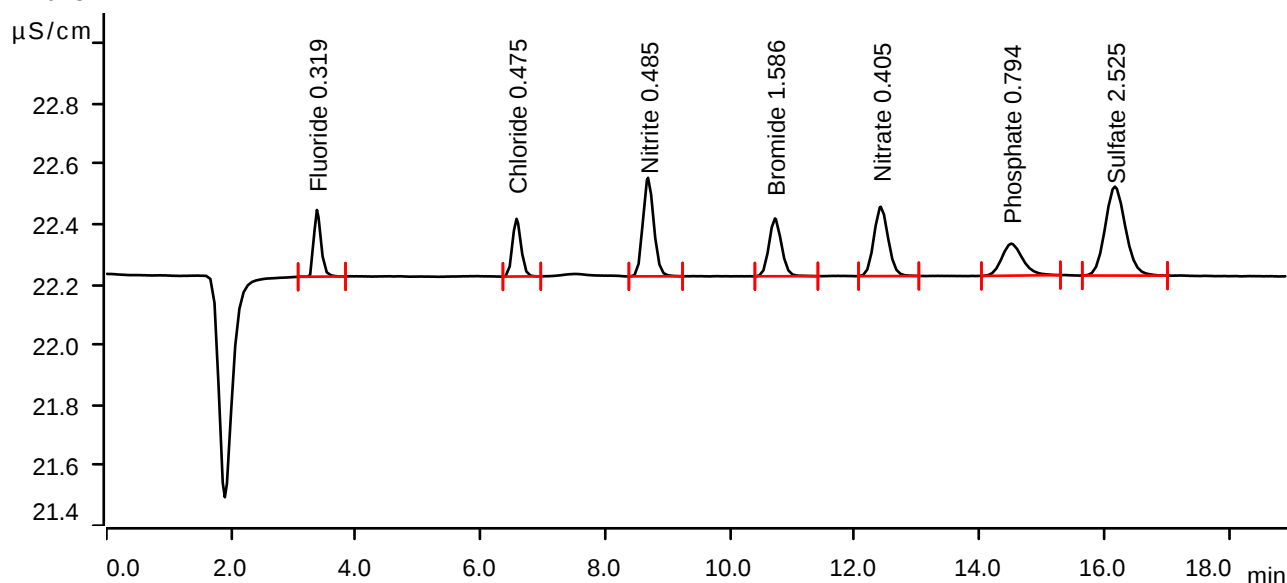

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.377	0.0293	0.221	0.319	Fluoride
2	6.577	0.0307	0.191	0.475	Chloride
3	8.685	0.0666	0.327	0.485	Nitrite
4	10.720	0.0449	0.192	1.586	Bromide
5	12.415	0.0613	0.230	0.405	Nitrate
6	14.510	0.0414	0.106	0.794	Phosphate
7	16.170	0.1115	0.295	2.525	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2024-12-18 11:22:01 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.09 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

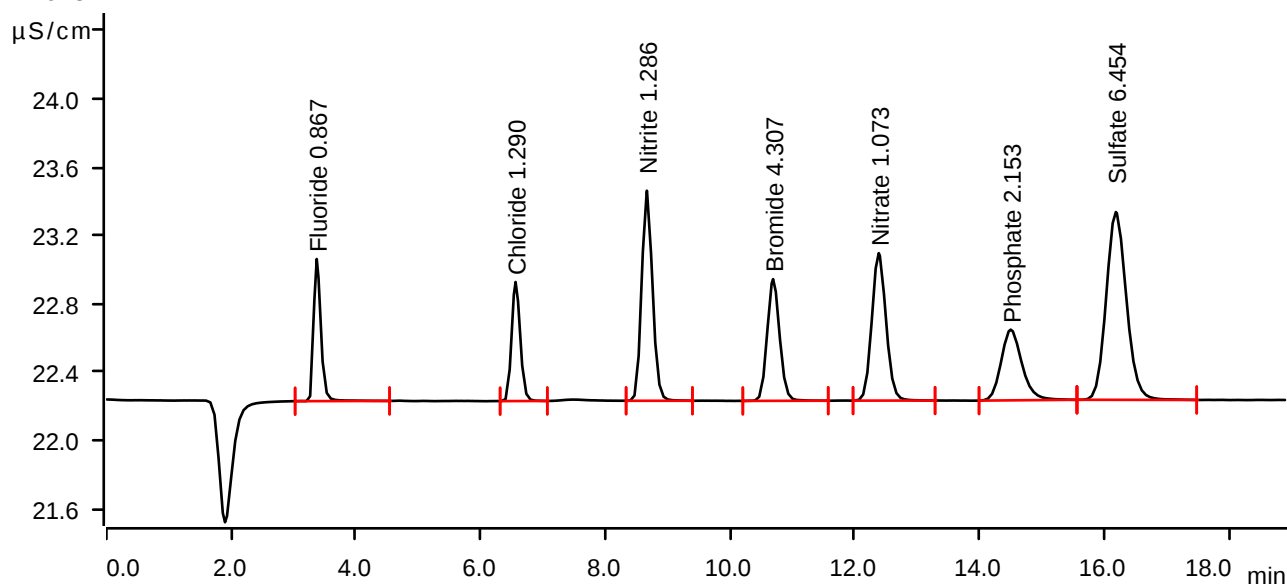

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.373	0.1111	0.832	0.867	Fluoride
2	6.562	0.1116	0.697	1.290	Chloride
3	8.665	0.2483	1.230	1.286	Nitrite
4	10.690	0.1658	0.713	4.307	Bromide
5	12.383	0.2288	0.864	1.073	Nitrate
6	14.500	0.1606	0.414	2.153	Phosphate
7	16.185	0.4138	1.100	6.454	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2024-12-18 11:43:26 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.87 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

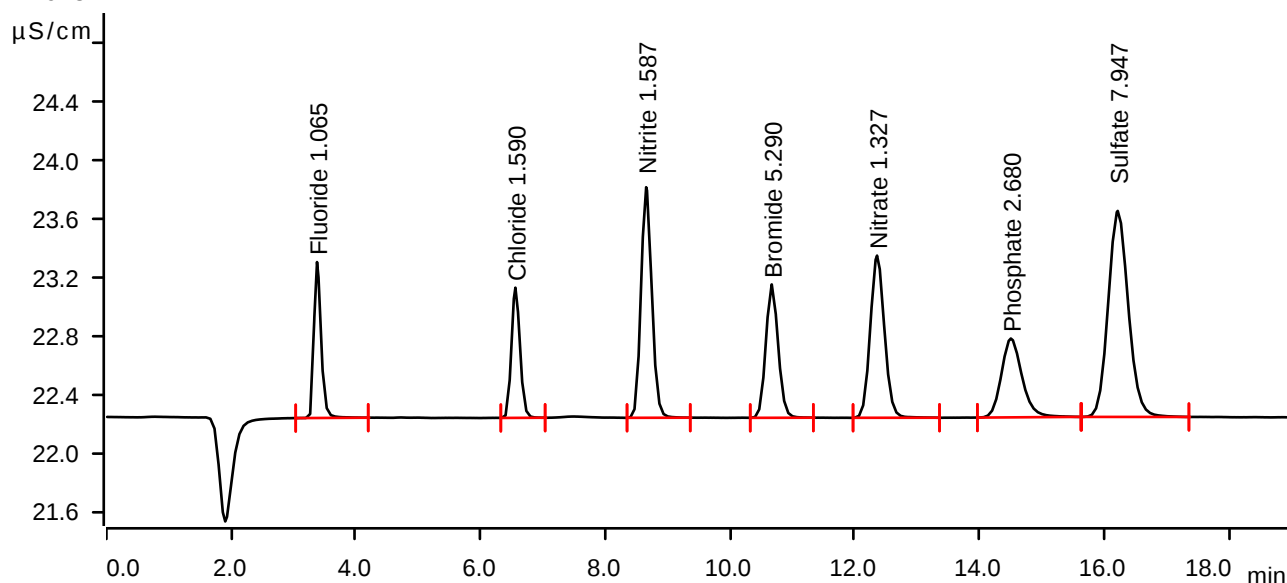

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.378	0.1407	1.065	1.065	Fluoride
2	6.558	0.1414	0.890	1.590	Chloride
3	8.655	0.3167	1.575	1.587	Nitrite
4	10.668	0.2094	0.911	5.290	Bromide
5	12.357	0.2924	1.108	1.327	Nitrate
6	14.502	0.2069	0.539	2.680	Phosphate
7	16.215	0.5287	1.408	7.947	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2024-12-18 12:04:52 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.04 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

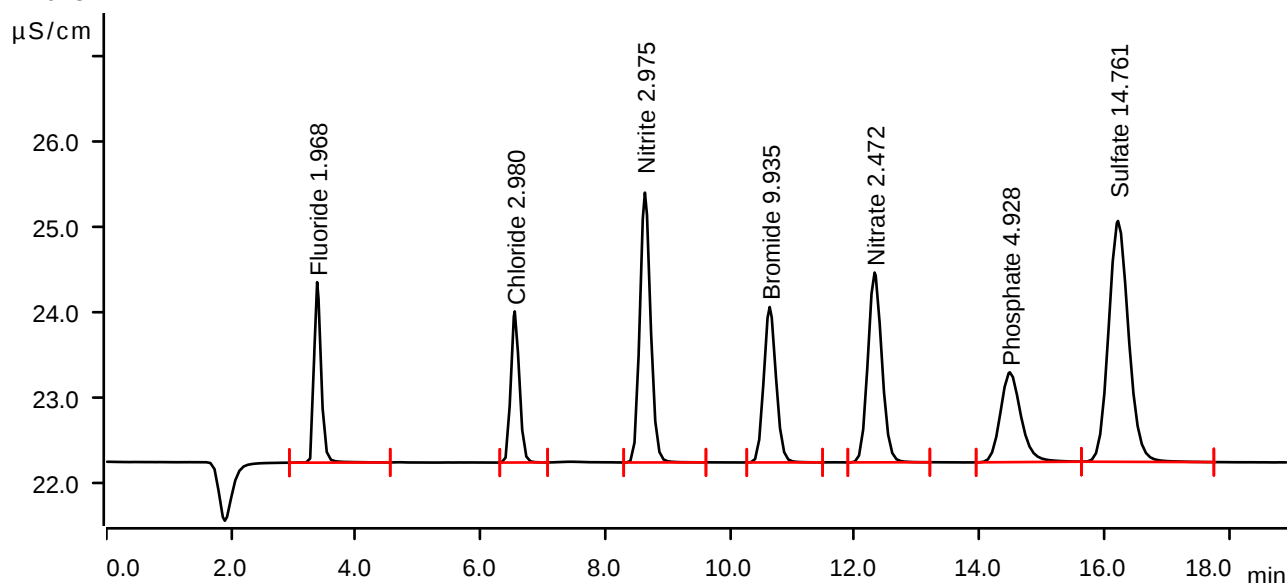

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.380	0.2755	2.114	1.968	Fluoride
2	6.548	0.2796	1.770	2.980	Chloride
3	8.635	0.6316	3.161	2.975	Nitrite
4	10.635	0.4158	1.820	9.935	Bromide
5	12.317	0.5791	2.223	2.472	Nitrate
6	14.485	0.4040	1.052	4.928	Phosphate
7	16.220	1.0530	2.822	14.761	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2024-12-18 12:26:18 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.98 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

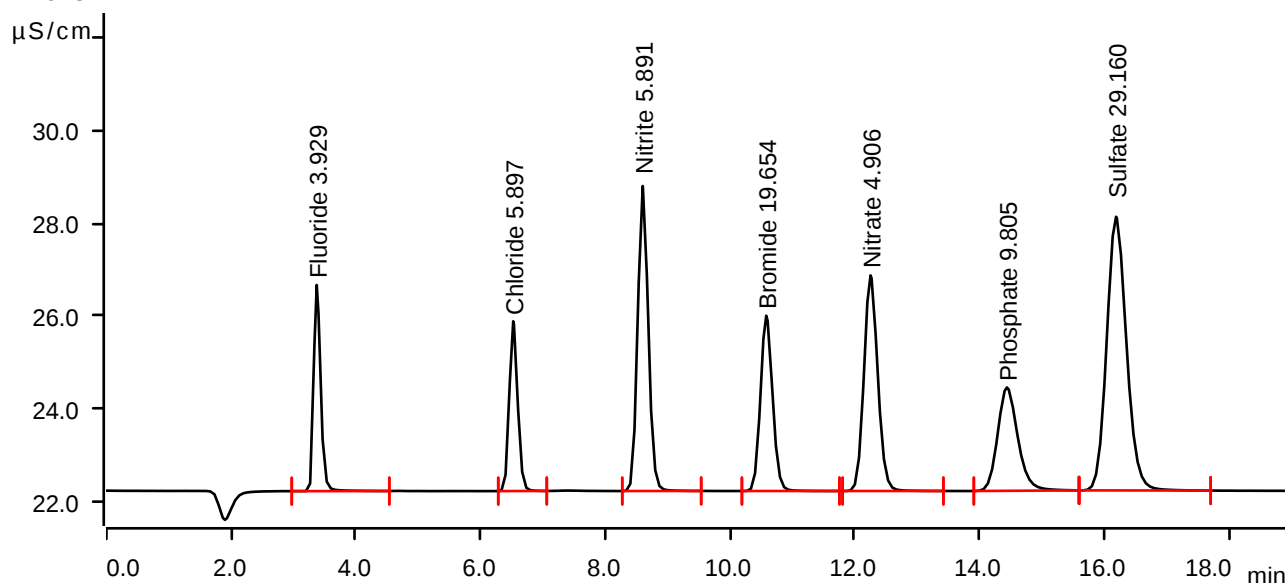

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.373	0.5685	4.427	3.929	Fluoride
2	6.523	0.5694	3.646	5.897	Chloride
3	8.602	1.2933	6.549	5.891	Nitrite
4	10.580	0.8475	3.765	19.654	Bromide
5	12.252	1.1889	4.631	4.906	Nitrate
6	14.438	0.8318	2.220	9.805	Phosphate
7	16.188	2.1610	5.877	29.160	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2024-12-18 12:47:45 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.75 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

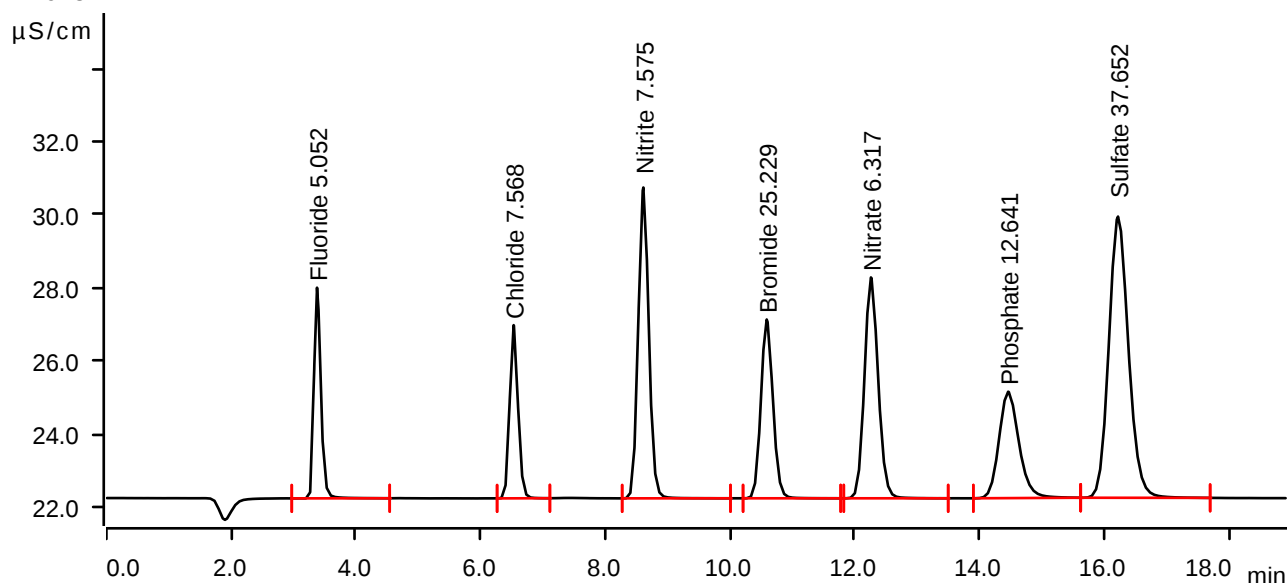

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.378	0.7362	5.758	5.052	Fluoride
2	6.530	0.7354	4.734	7.568	Chloride
3	8.610	1.6752	8.496	7.575	Nitrite
4	10.587	1.0952	4.888	25.229	Bromide
5	12.258	1.5424	6.037	6.317	Nitrate
6	14.458	1.0806	2.908	12.641	Phosphate
7	16.220	2.8144	7.686	37.652	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2024-12-18 13:09:13 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.87 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

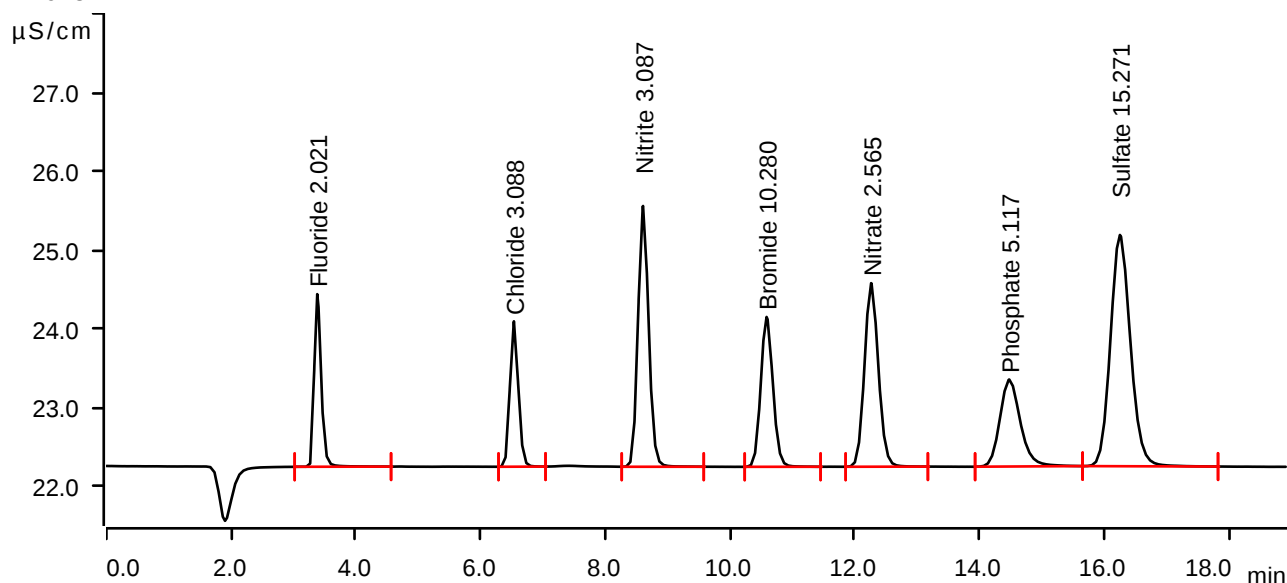

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.382	0.2835	2.190	2.021	Fluoride
2	6.533	0.2903	1.845	3.088	Chloride
3	8.605	0.6571	3.309	3.087	Nitrite
4	10.585	0.4311	1.902	10.280	Bromide
5	12.262	0.6024	2.329	2.565	Nitrate
6	14.477	0.4207	1.104	5.117	Phosphate
7	16.250	1.0923	2.934	15.271	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2024-12-18 13:30:41 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.64 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

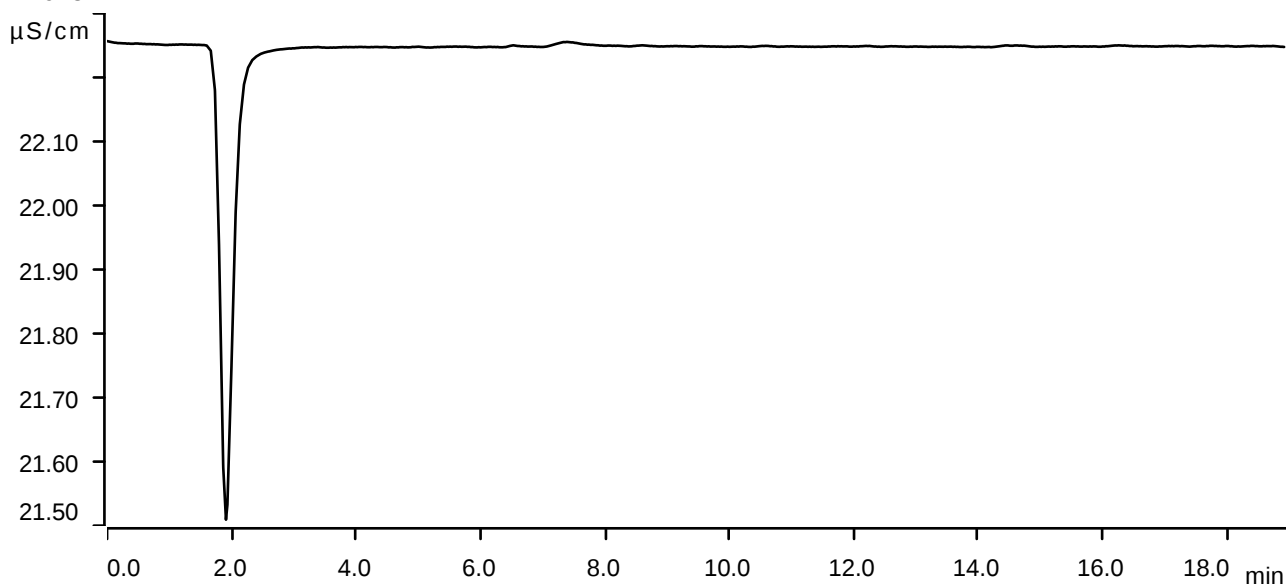


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-01-09 14:07:42 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

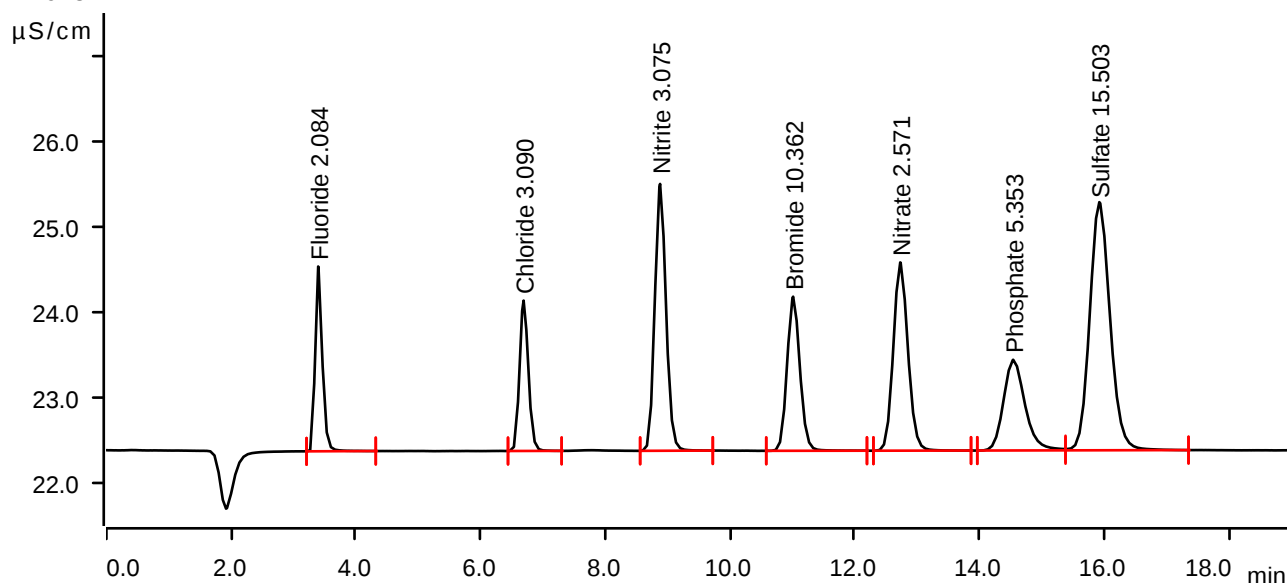


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.397	0.2880	2.165	2.084	Fluoride
2	6.690	0.2895	1.761	3.090	Chloride
3	8.878	0.6508	3.125	3.075	Nitrite
4	11.012	0.4313	1.805	10.362	Bromide
5	12.728	0.5995	2.205	2.571	Nitrate
6	14.540	0.4234	1.062	5.353	Phosphate
7	15.920	1.0984	2.907	15.503	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-01-09 14:29:12 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

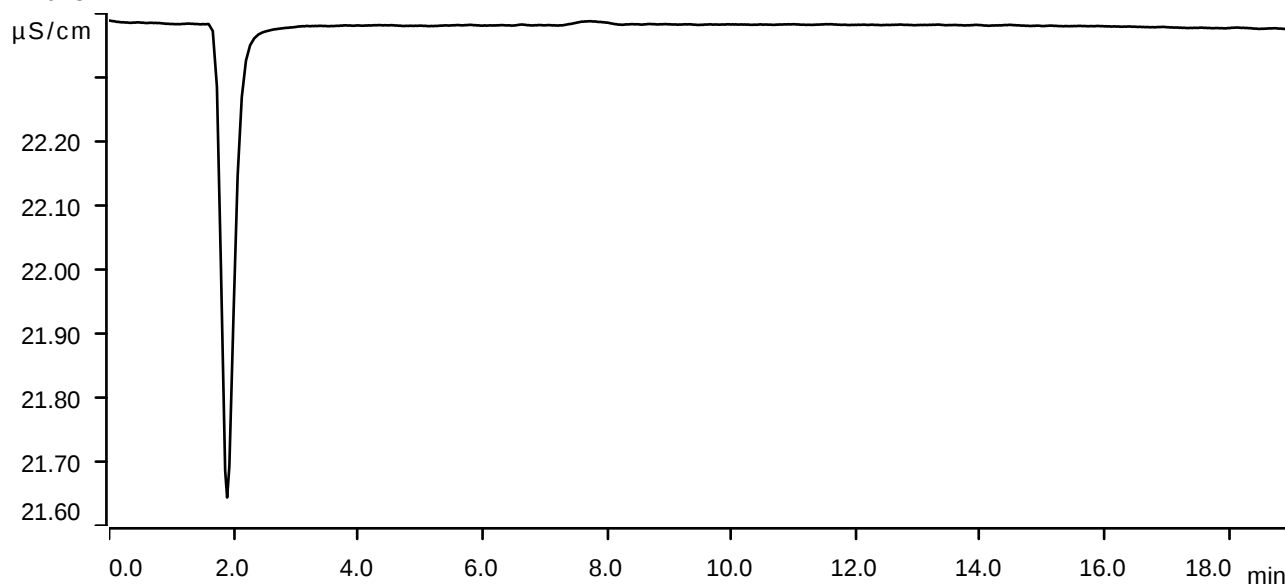
Anions

Sample data

Ident LB134228BLW
Sample type Sample
Determination start 2025-01-09 14:50:42 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

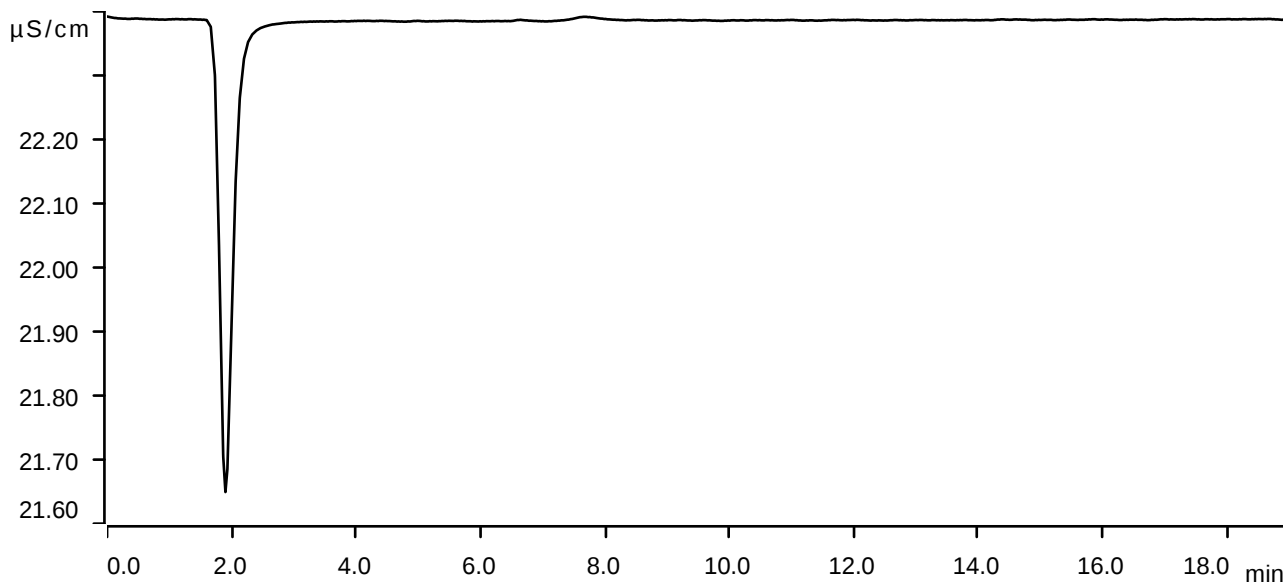Anions


Sample data

Ident LB134228BSW
 Sample type Check standard 1
 Determination start 2025-01-09 15:12:13 UTC-5
 Method IC1-121824
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.60 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

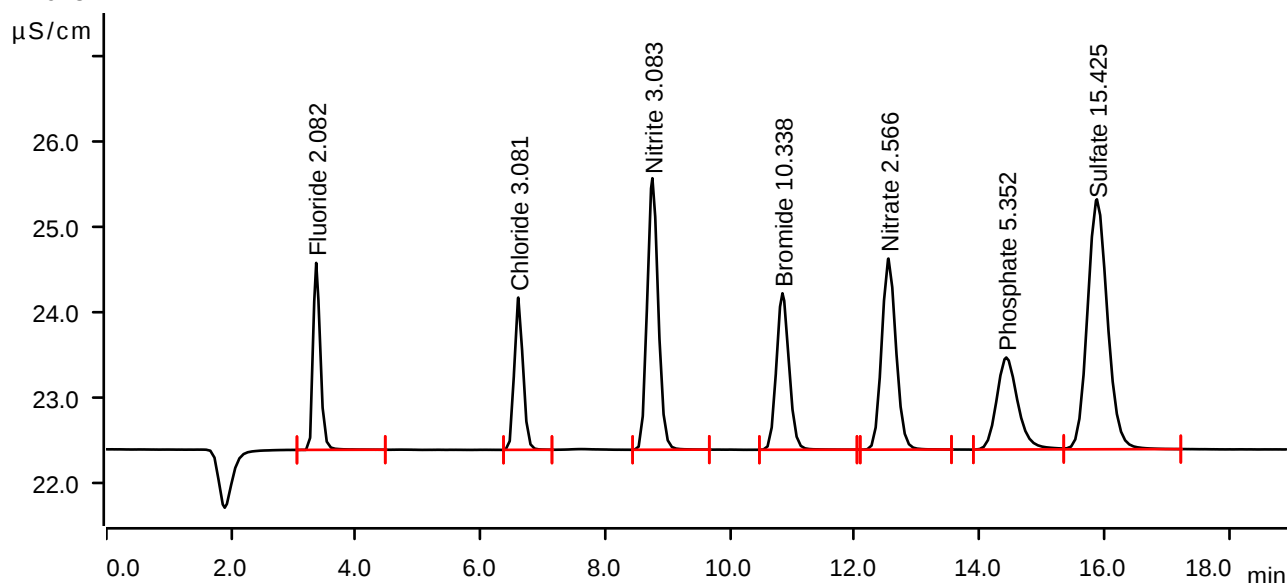

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.365	0.2877	2.190	2.082	Fluoride
2	6.605	0.2886	1.784	3.081	Chloride
3	8.755	0.6525	3.181	3.083	Nitrite
4	10.840	0.4303	1.833	10.338	Bromide
5	12.540	0.5982	2.238	2.566	Nitrate
6	14.428	0.4234	1.078	5.352	Phosphate
7	15.882	1.0924	2.928	15.425	Sulfate


Sample data

Ident Q1049-01
Sample type Sample
Determination start 2025-01-09 15:51:27 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

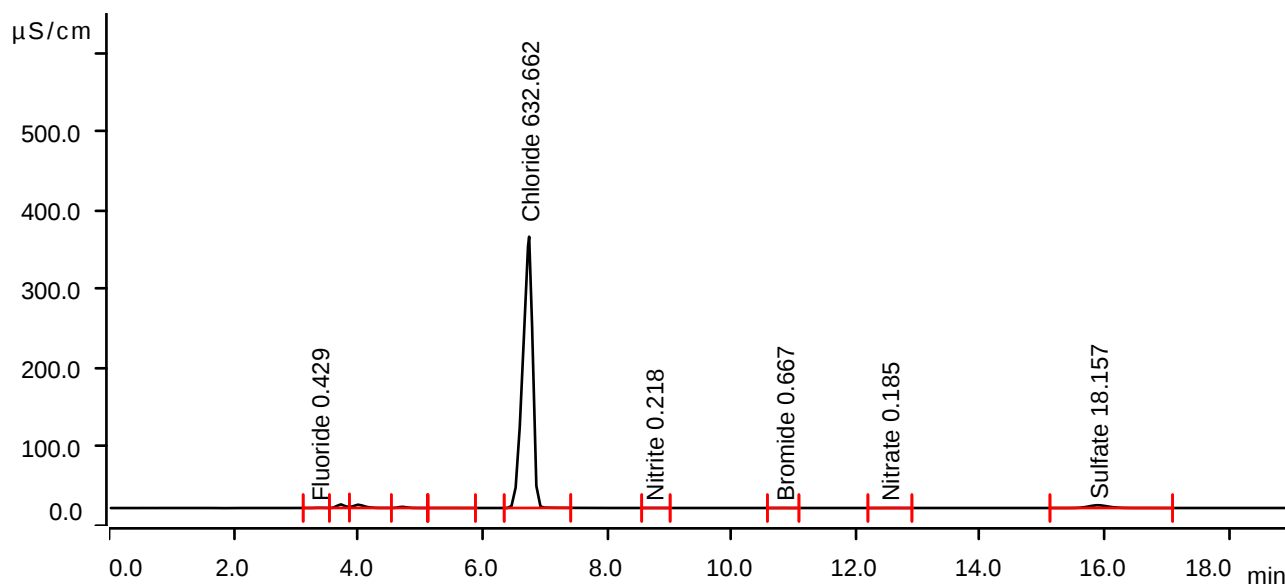

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.377	0.0436	0.256	0.429	Fluoride
2	3.722	0.6846	4.466	invalid	
3	4.003	0.8904	4.172	invalid	
4	4.712	0.2373	1.469	invalid	
5	5.320	0.0060	0.018	invalid	
6	6.752	62.6715	344.239	632.662	Chloride
7	8.748	0.0049	0.026	0.218	Nitrite
8	10.847	0.0026	0.011	0.667	Bromide
9	12.535	0.0051	0.020	0.185	Nitrate
10	15.888	1.3015	3.513	18.157	Sulfate


Sample data

Ident Q1049-01MS
Sample type Sample
Determination start 2025-01-09 16:13:05 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

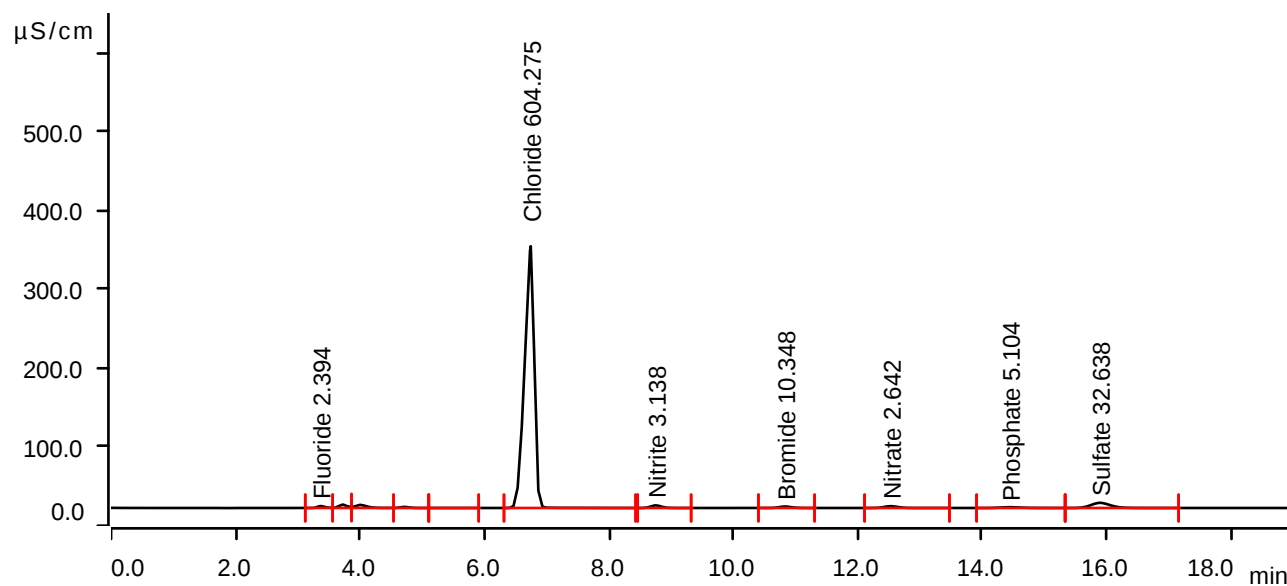

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.368	0.3337	2.453	2.394	Fluoride
2	3.722	0.6529	4.225	invalid	
3	4.007	0.8489	3.936	invalid	
4	4.713	0.2248	1.388	invalid	
5	5.323	0.0062	0.018	invalid	
6	6.745	59.8587	332.209	604.275	Chloride
7	8.753	0.6649	3.323	3.138	Nitrite
8	10.830	0.4307	1.870	10.348	Bromide
9	12.528	0.6170	2.320	2.642	Nitrate
10	14.442	0.4016	1.020	5.104	Phosphate
11	15.892	2.4101	6.566	32.638	Sulfate


Sample data

Ident Q1049-01MSD
Sample type Sample
Determination start 2025-01-09 16:34:39 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

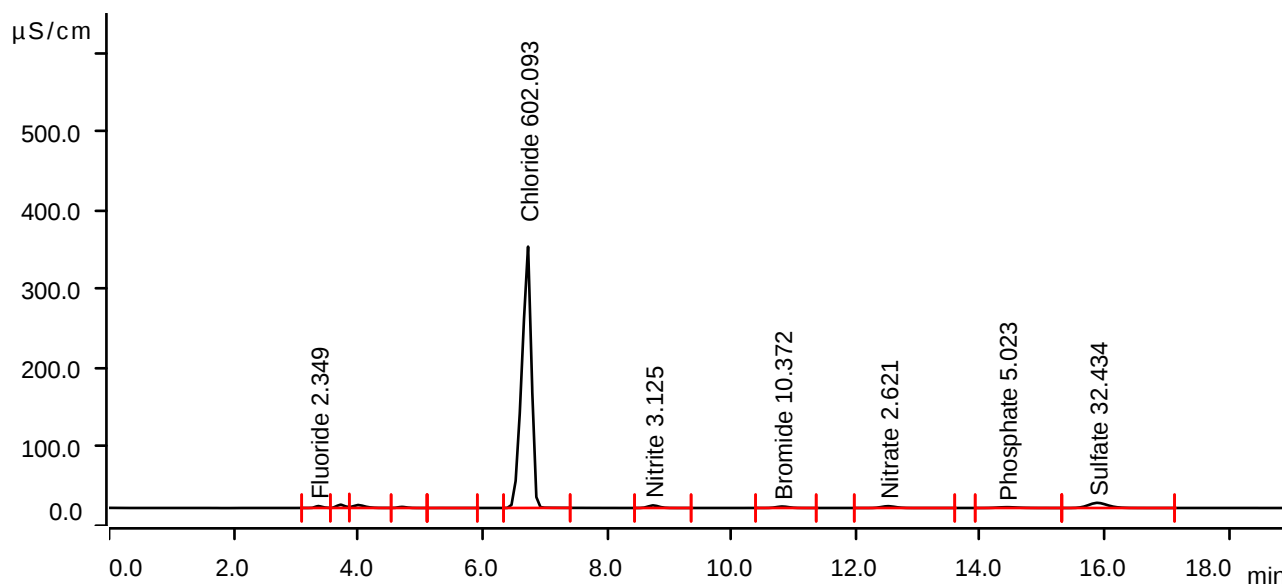

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.365	0.3271	2.409	2.349	Fluoride
2	3.718	0.6489	4.160	invalid	
3	4.005	0.8479	3.788	invalid	
4	4.707	0.2251	1.367	invalid	
5	5.330	0.0062	0.018	invalid	
6	6.733	59.6425	331.573	602.093	Chloride
7	8.745	0.6619	3.281	3.125	Nitrite
8	10.818	0.4318	1.862	10.372	Bromide
9	12.518	0.6118	2.299	2.621	Nitrate
10	14.427	0.3945	1.007	5.023	Phosphate
11	15.882	2.3945	6.536	32.434	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-01-09 16:56:13 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

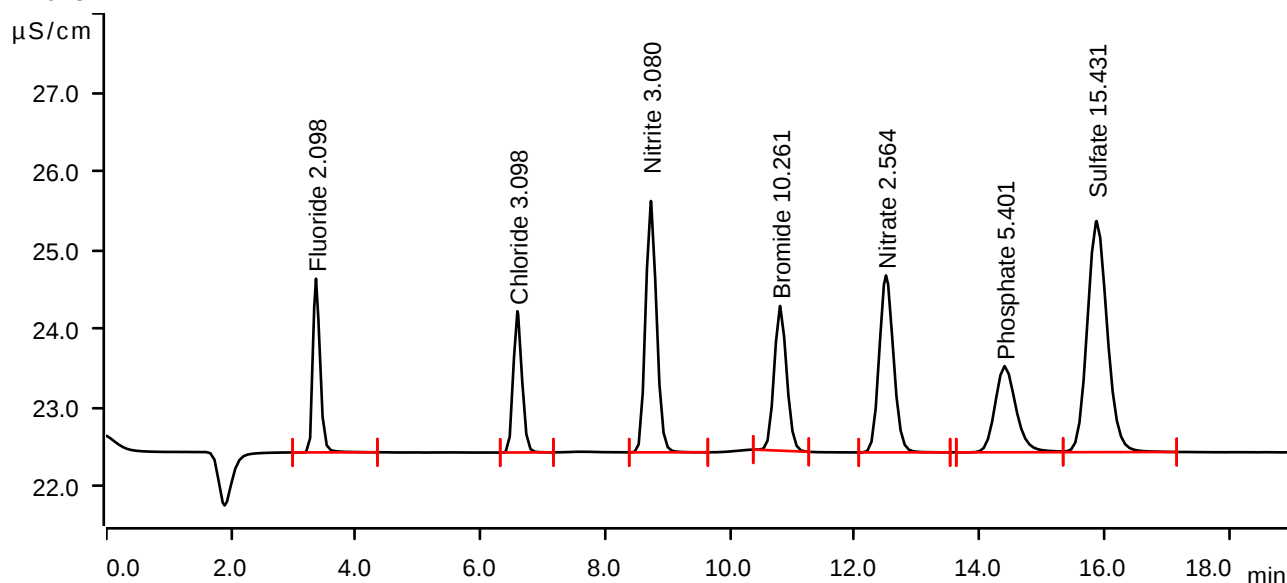

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.362	0.2901	2.204	2.098	Fluoride
2	6.590	0.2902	1.793	3.098	Chloride
3	8.730	0.6519	3.189	3.080	Nitrite
4	10.803	0.4269	1.837	10.261	Bromide
5	12.500	0.5977	2.246	2.564	Nitrate
6	14.402	0.4276	1.094	5.401	Phosphate
7	15.877	1.0929	2.934	15.431	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-01-09 17:17:43 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

