


LB134346

7471B

INSTRUMENT IN CVL

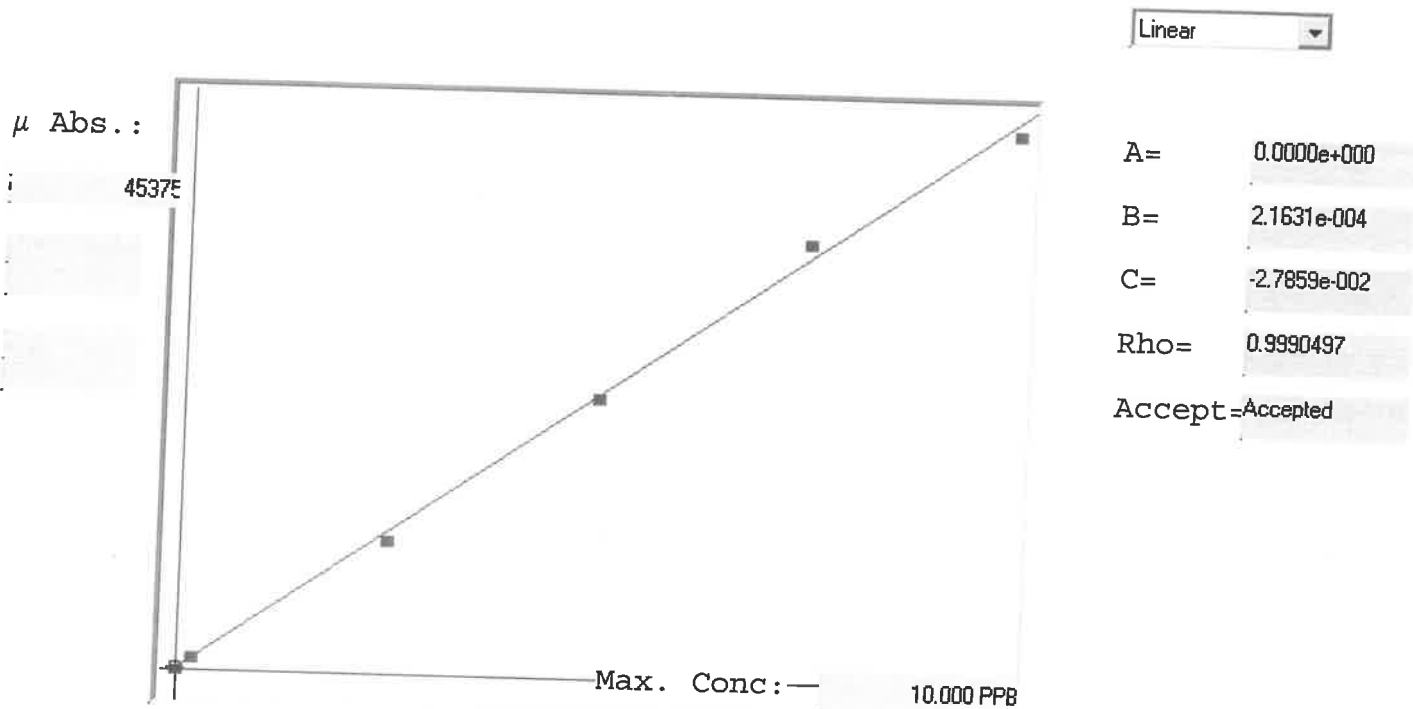

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.020	0.020	219	0.000	219					
0.2	0.200	0.213	0.013	1114	0.0 %	1114					
2.5	2.500	2.380	-0.120	11133	0.0 %	11133					
5.0	5.000	4.992	-0.008	23206	0.0 %	23206					
7.5	7.500	7.808	0.308	36226	0.0 %	36226					
10.0	10.000	9.787	-0.213	45375	0.0 %	45375					

9/05

6

-5

0

4

-2

LB134346 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 20 Jan 2025 13:32:15

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	219	-	0.0000	7471B	PPB	20 Jan 2025 13:34:47	S	Std
0.2 - 1	50.2	1114	-	0.2000	7471B	PPB	20 Jan 2025 13:37:06	S	Std
2.5 - 1	52.5	11133	-	2.5000	7471B	PPB	20 Jan 2025 13:39:23	S	Std
5.0 - 1	55	23206	-	5.0000	7471B	PPB	20 Jan 2025 13:41:41	S	Std
7.5 - 1	57.5	36226	-	7.5000	7471B	PPB	20 Jan 2025 13:43:59	S	Std
10.0 - 1	510	45375	-	10.0000	7471B	PPB	20 Jan 2025 13:46:18	S	Std
ICV63 - 1	ICV63	17787	3.8196	-7471B	PPB	20 Jan 2025 13:49:23	U	SMPL	
ICB63 - 1	ICB63	-171	-0.0648	-7471B	PPB	20 Jan 2025 13:51:38	U	SMPL	
CCV54 - 1	CCV54	22809	4.9059	-7471B	PPB	20 Jan 2025 13:53:57	U	SMPL	
CCB54 - 1	CCB54	-154	-0.0612	-7471B	PPB	20 Jan 2025 13:56:11	U	SMPL	
CRA - 1	CRA	1045	0.1982	-7471B	PPB	20 Jan 2025 13:58:31	U	SMPL	
HighStd - 1	HighStd	44704	9.6420	-7471B	PPB	20 Jan 2025 14:00:46	U	SMPL	
ChkStd - 1	ChkStd	33157	7.1443	-7471B	PPB	20 Jan 2025 14:03:01	U	SMPL	
PB166149BL - 1	PB166149BL	-83	-0.0458	-7471B	PPB	20 Jan 2025 14:05:28	U	SMPL	
PB166149BS - 1	PB166149BS	16990	3.6472	-7471B	PPB	20 Jan 2025 14:07:50	U	SMPL	
Q1103-01 - 1	VNJ-241	2406	0.4926	-7471B	PPB	20 Jan 2025 14:10:07	U	SMPL	
Q1110-01 - 1	BIN-1	2943	0.6087	-7471B	PPB	20 Jan 2025 14:12:27	U	SMPL	
Q1115-01 - 1	366	2481	0.5088	-7471B	PPB	20 Jan 2025 14:14:46	U	SMPL	
Q1115-04 - 1	VNJ-214	5584	1.1800	-7471B	PPB	20 Jan 2025 14:17:05	U	SMPL	
Q1115-07 - 1	72-11995	3801	0.7943	-7471B	PPB	20 Jan 2025 14:19:22	U	SMPL	
CCV55 - 1	CCV55	22493	4.8376	-7471B	PPB	20 Jan 2025 14:29:40	U	SMPL	
CCB55 - 1	CCB55	-201	-0.0713	-7471B	PPB	20 Jan 2025 14:31:55	U	SMPL	
Q1115-10 - 1	VNJ-213	4610	0.9693	-7471B	PPB	20 Jan 2025 14:34:14	U	SMPL	
Q1118-01 - 1	OK-01-1-16-2025	730	0.1300	-7471B	PPB	20 Jan 2025 14:41:02	U	SMPL	
Q1118-01DUP - 1	OK-01-1-16-2025DUP	637	0.1099	-7471B	PPB	20 Jan 2025 14:43:17	U	SMPL	
Q1118-01MS - 1	OK-01-1-16-2025MS	17424	3.7411	-7471B	PPB	20 Jan 2025 14:45:32	U	SMPL	
Q1118-01MSD - 1	OK-01-1-16-2025MSD	18075	3.8819	-7471B	PPB	20 Jan 2025 14:47:48	U	SMPL	
Q1123-01 - 1	BU-03-1172025	2214	0.4510	-7471B	PPB	20 Jan 2025 14:50:08	U	SMPL	
Q1132-01 - 1	HD-1-011725	2817	0.5815	-7471B	PPB	20 Jan 2025 14:52:29	U	SMPL	
Q1132-04 - 1	HD-2-011725	2080	0.4221	-7471B	PPB	20 Jan 2025 14:54:46	U	SMPL	
Q1133-01 - 1	TR-04-1172025	1349	0.2639	-7471B	PPB	20 Jan 2025 14:57:04	U	SMPL	
Q1134-01 - 1	EO-1-011725	2711	0.5586	-7471B	PPB	20 Jan 2025 14:59:20	U	SMPL	
CCV56 - 1	CCV56	22905	4.9267	-7471B	PPB	20 Jan 2025 15:01:36	U	SMPL	
CCB56 - 1	CCB56	-104	-0.0504	-7471B	PPB	20 Jan 2025 15:03:52	U	SMPL	
Q1118-01LX5 - 1		81	-0.0103	-7471B	PPB	20 Jan 2025 15:10:12	U	SMPL	
Q1118-01A - 1		18197	3.9083	-7471B	PPB	20 Jan 2025 15:12:27	U	SMPL	
CCV57 - 1	CCV57	21589	4.6420	-7471B	PPB	20 Jan 2025 15:14:42	U	SMPL	
CCB57 - 1	CCB57	-155	-0.0614	-7471B	PPB	20 Jan 2025 15:17:02	U	SMPL	