

Ident	Instrument IC-1				Analyst: NF		Method: 300.0 / 9056A		Initial Analyst		
	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name		date time	
STD1	0	0	0	0	0	0	0	0	IC1-012025	1/20/2025 11:14	10 NF/IZ
STD2	0.396	0.602	0.613	2.019	0.511	0.994	3.09	3.09	IC1-012025	1/20/2025 11:36	10 NF/IZ
STD3	0.835	1.258	1.254	4.184	1.047	2.089	6.324	6.324	IC1-012025	1/20/2025 11:57	10 NF/IZ
STD4	0.967	1.463	1.466	4.879	1.221	2.469	7.299	7.299	IC1-012025	1/20/2025 12:18	10 NF/IZ
STD5	1.996	2.973	2.959	9.912	2.468	4.936	14.741	14.741	IC1-012025	1/20/2025 12:40	10 NF/IZ
STD6	4.016	5.977	5.973	19.887	4.964	9.97	29.788	29.788	IC1-012025	1/20/2025 13:01	10 NF/IZ
STD7	4.99	7.527	7.535	25.119	6.289	12.542	37.258	37.258	IC1-012025	1/20/2025 13:23	10 NF/IZ
ICV	2.059	3.086	3.062	10.267	2.569	5.158	15.361	15.361	IC1-012025	1/20/2025 13:44	10 NF/IZ
ICB	0	0	0	0	0	0	0	0	IC1-012025	1/20/2025 14:06	10 NF/IZ
CCV	2.048	3.091	3.08	10.314	2.571	5.193	15.367	15.367	IC1-012025	1/24/2025 9:57	10 NF/IZ
CCB	0	0	0	0	0	0	0	0	IC1-012025	1/24/2025 10:18	10 NF/IZ
LB134413BLW	0	0	0	0	0	0	0	0	IC1-012025	1/24/2025 10:40	10 NF/IZ
LB134413BSW	2.04	3.089	3.079	10.297	2.564	5.167	15.281	15.281	IC1-012025	1/24/2025 11:01	10 NF/IZ
Q1168-08	0.415	0.626	0.642	2.139	0.536	1.037	3.237	3.237	IC1-012025	1/24/2025 11:23	10 NF/IZ
Q1168-07	0.221	0.344	0.364	1.171	0.302	0.55	1.823	1.823	IC1-012025	1/24/2025 11:44	10 NF/IZ
Q1168-07RE 0.25ML	0.141	0.209	0.231	0.727	0.191	0.329	1.173	1.173	IC1-012025	1/24/2025 12:06	10 NF/IZ
CCV	2.063	3.089	3.073	10.298	2.568	5.163	15.318	15.318	IC1-012025	1/24/2025 12:28	10 NF/IZ
CCB	0	0	0	0	0	0	0	0	IC1-012025	1/24/2025 12:49	10 NF/IZ

Clear table


Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A

ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0	0	0	0	0	0	0	0 IC1-012025	1/20/2025 11:14	10	NF/IZ
STD2	0.396	0.602	0.613	2.019	0.511	0.994	3.09	IC1-012025	1/20/2025 11:36	10	NF/IZ
STD3	0.835	1.258	1.254	4.184	1.047	2.089	6.324	IC1-012025	1/20/2025 11:57	10	NF/IZ
STD4	0.967	1.463	1.466	4.879	1.221	2.469	7.299	IC1-012025	1/20/2025 12:18	10	NF/IZ
STD5	1.996	2.973	2.959	9.912	2.468	4.936	14.741	IC1-012025	1/20/2025 12:40	10	NF/IZ
STD6	4.016	5.977	5.973	19.887	4.964	9.97	29.788	IC1-012025	1/20/2025 13:01	10	NF/IZ
STD7	4.99	7.527	7.535	25.119	6.289	12.542	37.258	IC1-012025	1/20/2025 13:23	10	NF/IZ

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1	-1.0000	0.3333	2.1667	0.9500	2.2000	-0.6000	3.0000
STD2	4.3750	4.8333	4.5000	4.6000	4.7000	4.4500	5.4000
STD3	-3.3000	-2.4667	-2.2667	-2.4200	-2.3200	-1.2400	-2.6800
STD4	-0.2000	-0.9000	-1.3667	-0.8800	-1.2800	-1.2800	-1.7267
STD5	0.4000	-0.3833	-0.4500	-0.5650	-0.7200	-0.3000	-0.7067
STD6	-0.2000	0.3600	0.4667	0.4760	0.6240	0.3360	0.6973

Fluoride (Anions)

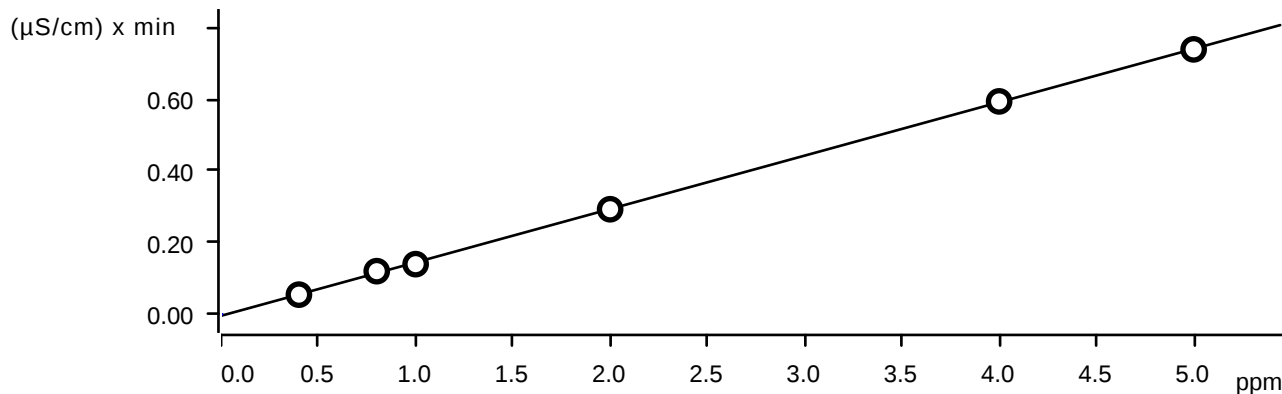


Function: $A = -4.02271E-3 + 0.0148839 \times Q$

Relative standard deviation 1.203859 %

Correlation coefficient 0.999923

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.400	10.0	1.0	1.0	0.055	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	0.800	10.0	1.0	1.0	0.120	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.000	10.0	1.0	1.0	0.140	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	2.000	10.0	1.0	1.0	0.293	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	4.000	10.0	1.0	1.0	0.594	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	5.000	10.0	1.0	1.0	0.739	STD7	2025-01-20 13:23:08 UTC-5	used

Chloride (Anions)

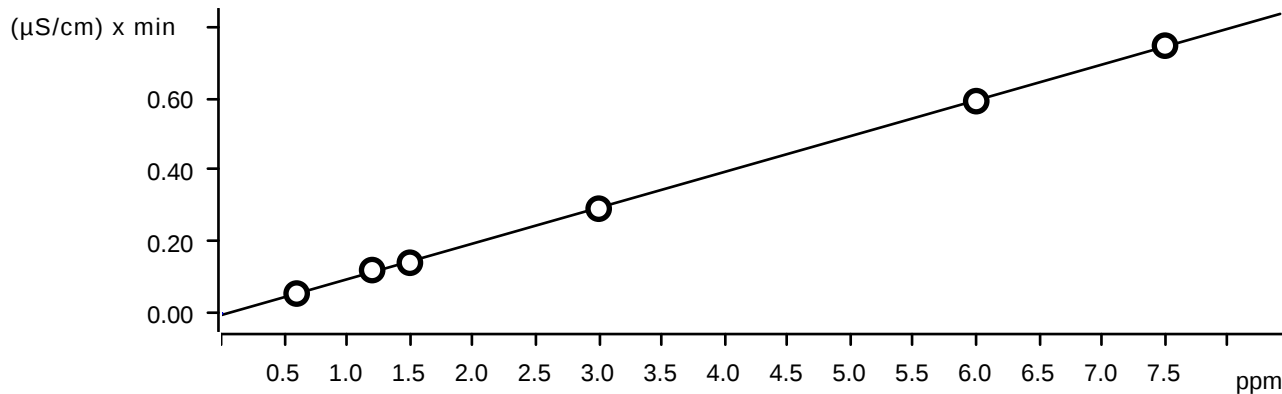

Function: $A = -4.62538E-3 + 9.98029E-3 \times Q$


Relative standard deviation 1.261416 %

Correlation coefficient 0.999916

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.055	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.121	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.141	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.292	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	0.592	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	0.747	STD7	2025-01-20 13:23:08 UTC-5	used

Nitrite (Anions)

($\mu\text{S/cm}$) $\times$ min

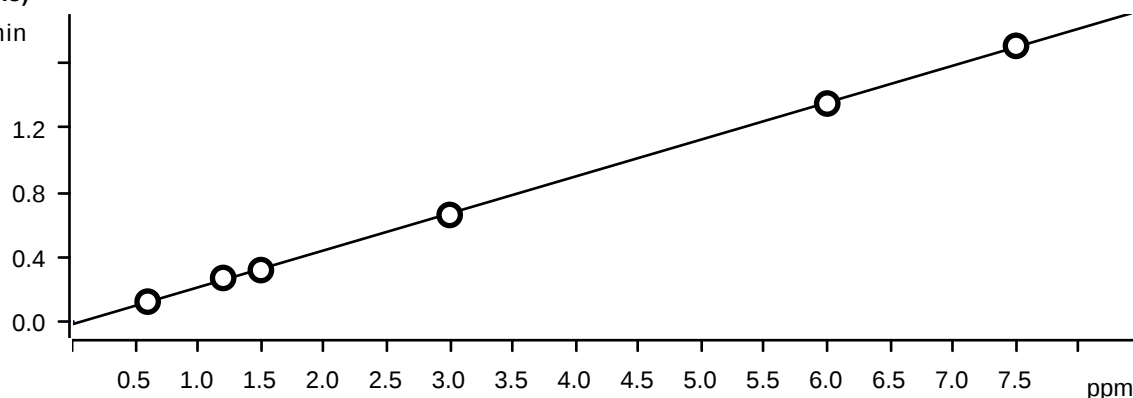

Function: $A = -0.0179856 + 0.0228967 \times Q$


Relative standard deviation 1.369596 %

Correlation coefficient 0.999903

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.122	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.269	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.660	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	1.350	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	1.707	STD7	2025-01-20 13:23:08 UTC-5	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

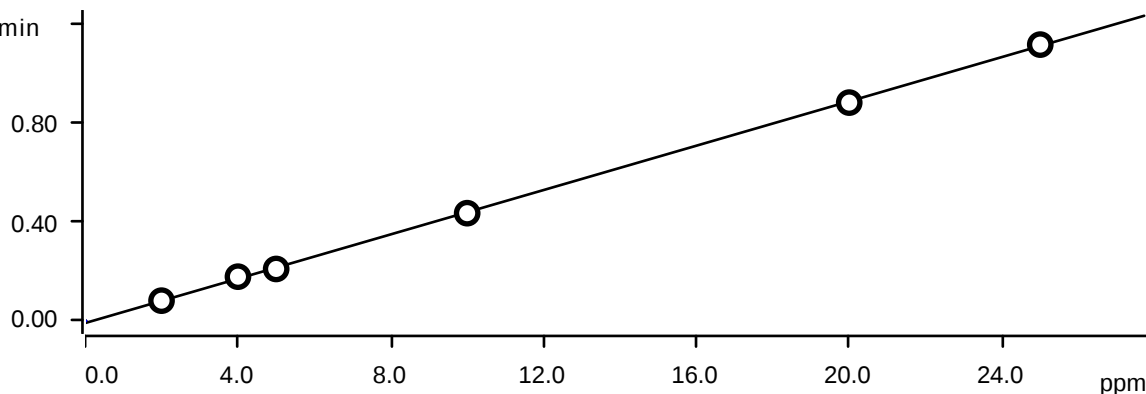

Function: $A = -8.89651E-3 + 4.46429E-3 \times Q$


Relative standard deviation: 1.338167 %

Correlation coefficient: 0.999906

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	2.000	10.0	1.0	1.0	0.081	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	4.000	10.0	1.0	1.0	0.178	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	5.000	10.0	1.0	1.0	0.209	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	10.000	10.0	1.0	1.0	0.434	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	20.000	10.0	1.0	1.0	0.879	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	25.000	10.0	1.0	1.0	1.112	STD7	2025-01-20 13:23:08 UTC-5	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

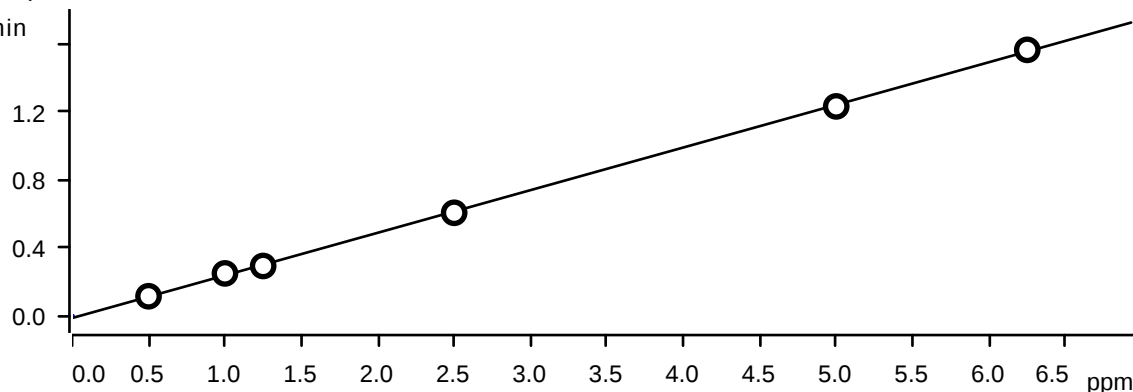


Function: $A = -0.0155875 + 0.0250988 \times Q$

Relative standard deviation: 1.561944 %

Correlation coefficient 0.999873


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.500	10.0	1.0	1.0	0.113	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	1.000	10.0	1.0	1.0	0.247	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.250	10.0	1.0	1.0	0.291	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	2.500	10.0	1.0	1.0	0.604	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	5.000	10.0	1.0	1.0	1.230	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	6.250	10.0	1.0	1.0	1.563	STD7	2025-01-20 13:23:08 UTC-5	used

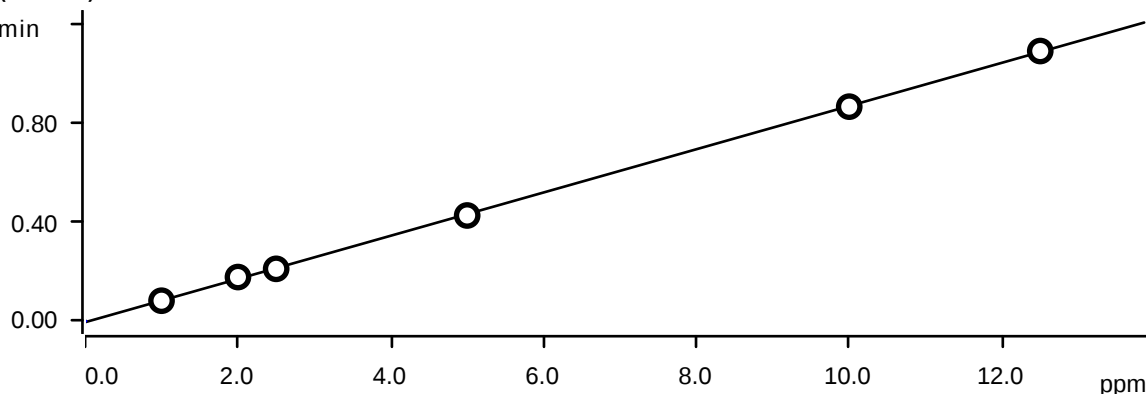Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -4.38887E-3 + 8.70711E-3 \times Q$

Relative standard deviation 1.148005 %

Correlation coefficient 0.999929

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	1.000	10.0	1.0	1.0	0.082	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	2.000	10.0	1.0	1.0	0.177	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	2.500	10.0	1.0	1.0	0.211	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	5.000	10.0	1.0	1.0	0.425	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	10.000	10.0	1.0	1.0	0.864	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-01-20 13:23:08 UTC-5	used

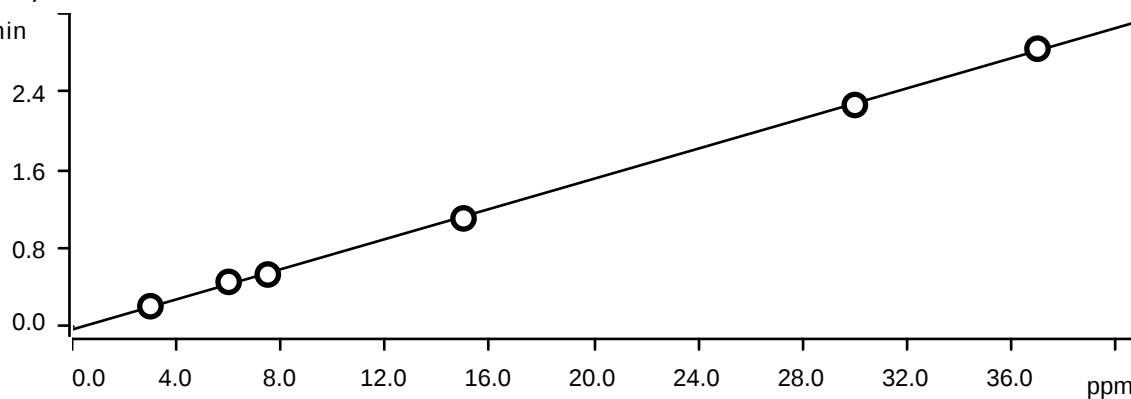Sulfate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0310554 + 7.70543E-3 \times Q$

Relative standard deviation 1.797524 %

Correlation coefficient 0.999831


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	3.000	10.0	1.0	1.0	0.207	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	6.000	10.0	1.0	1.0	0.456	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	7.500	10.0	1.0	1.0	0.531	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	15.000	10.0	1.0	1.0	1.105	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	30.000	10.0	1.0	1.0	2.264	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	37.000	10.0	1.0	1.0	2.840	STD7	2025-01-20 13:23:08 UTC-5	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-01-20 11:14:39 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

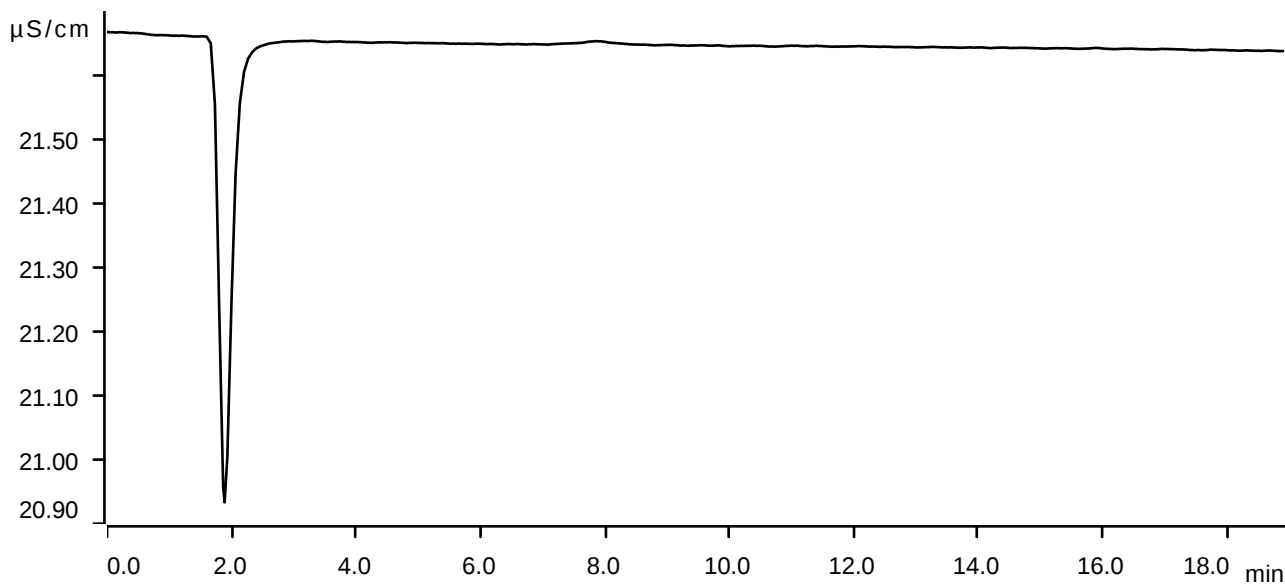Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-01-20 11:36:02 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

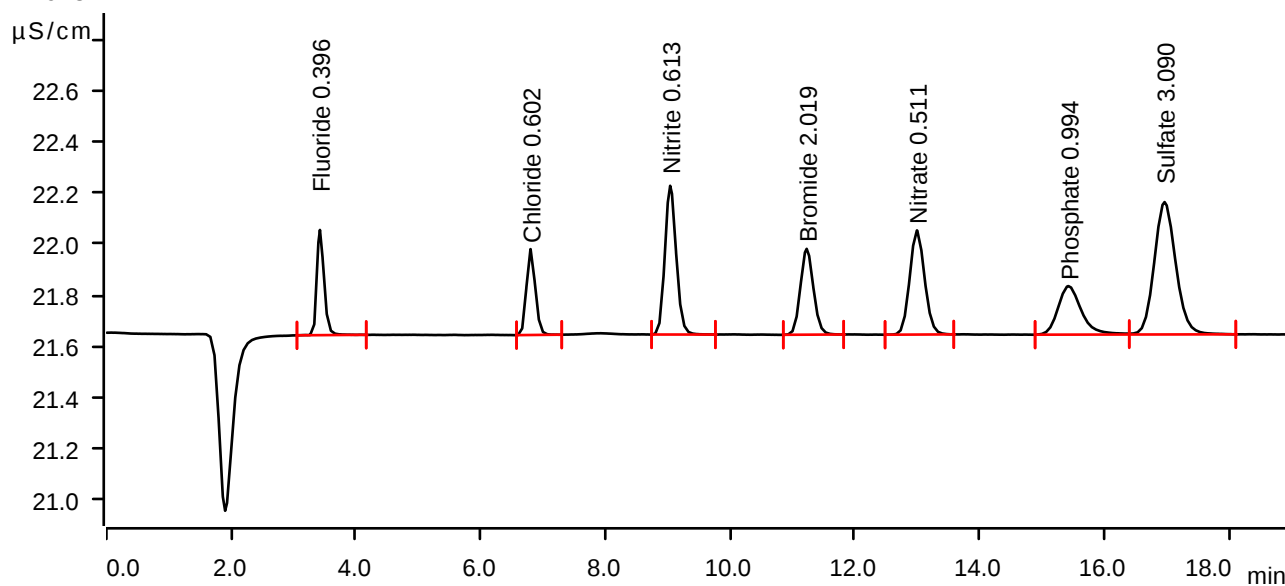

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.425	0.0549	0.411	0.396	Fluoride
2	6.802	0.0555	0.335	0.602	Chloride
3	9.040	0.1223	0.581	0.613	Nitrite
4	11.228	0.0813	0.335	2.019	Bromide
5	12.995	0.1126	0.407	0.511	Nitrate
6	15.423	0.0822	0.190	0.994	Phosphate
7	16.967	0.2070	0.517	3.090	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-01-20 11:57:26 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

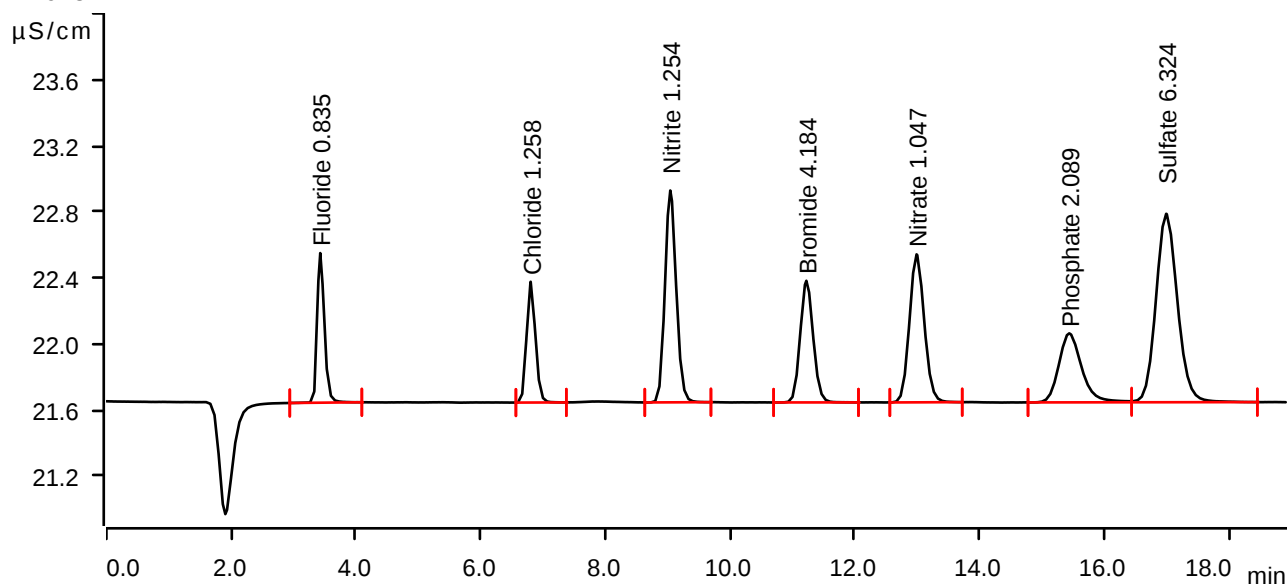

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.1203	0.906	0.835	Fluoride
2	6.803	0.1209	0.731	1.258	Chloride
3	9.042	0.2691	1.282	1.254	Nitrite
4	11.223	0.1779	0.736	4.184	Bromide
5	12.990	0.2472	0.896	1.047	Nitrate
6	15.438	0.1775	0.418	2.089	Phosphate
7	16.992	0.4562	1.141	6.324	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-01-20 12:18:50 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

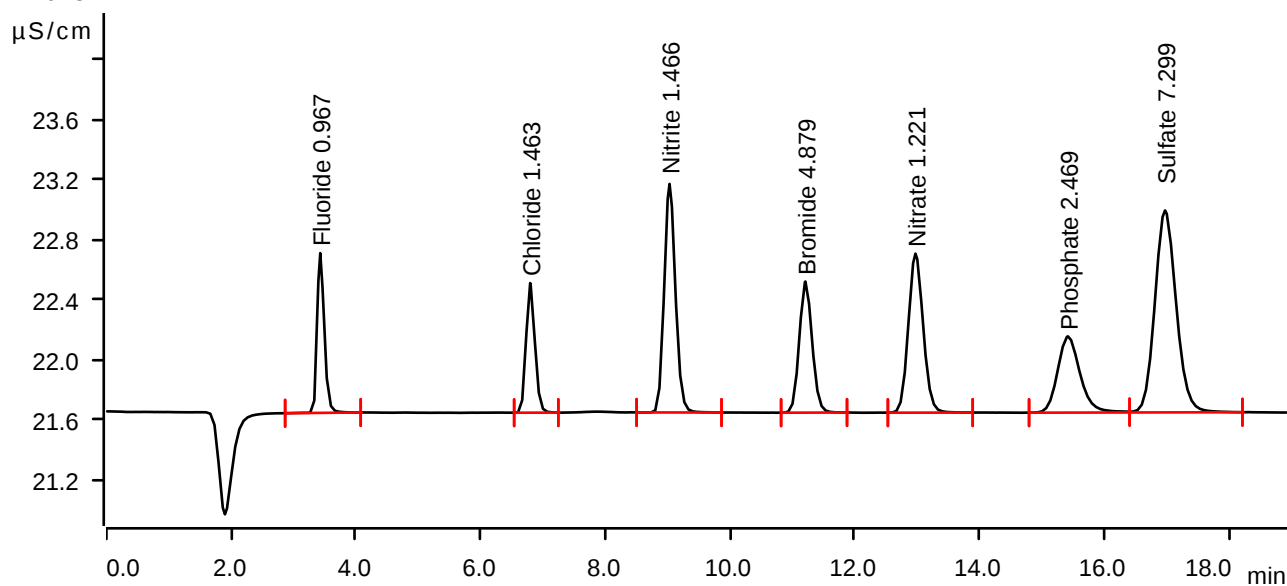

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.1399	1.061	0.967	Fluoride
2	6.795	0.1414	0.860	1.463	Chloride
3	9.030	0.3178	1.517	1.466	Nitrite
4	11.208	0.2089	0.870	4.879	Bromide
5	12.972	0.2908	1.056	1.221	Nitrate
6	15.417	0.2105	0.506	2.469	Phosphate
7	16.973	0.5314	1.341	7.299	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-01-20 12:40:15 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

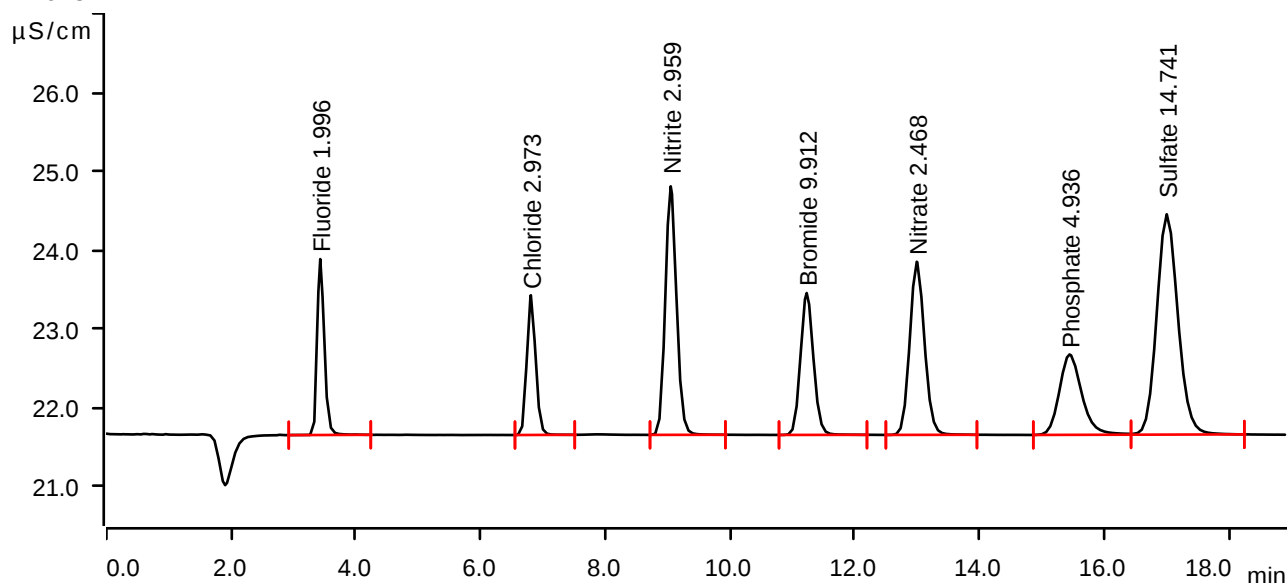

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.2930	2.233	1.996	Fluoride
2	6.807	0.2921	1.773	2.973	Chloride
3	9.048	0.6595	3.154	2.959	Nitrite
4	11.228	0.4336	1.801	9.912	Bromide
5	12.993	0.6039	2.197	2.468	Nitrate
6	15.443	0.4254	1.020	4.936	Phosphate
7	17.002	1.1048	2.795	14.741	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-01-20 13:01:41 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

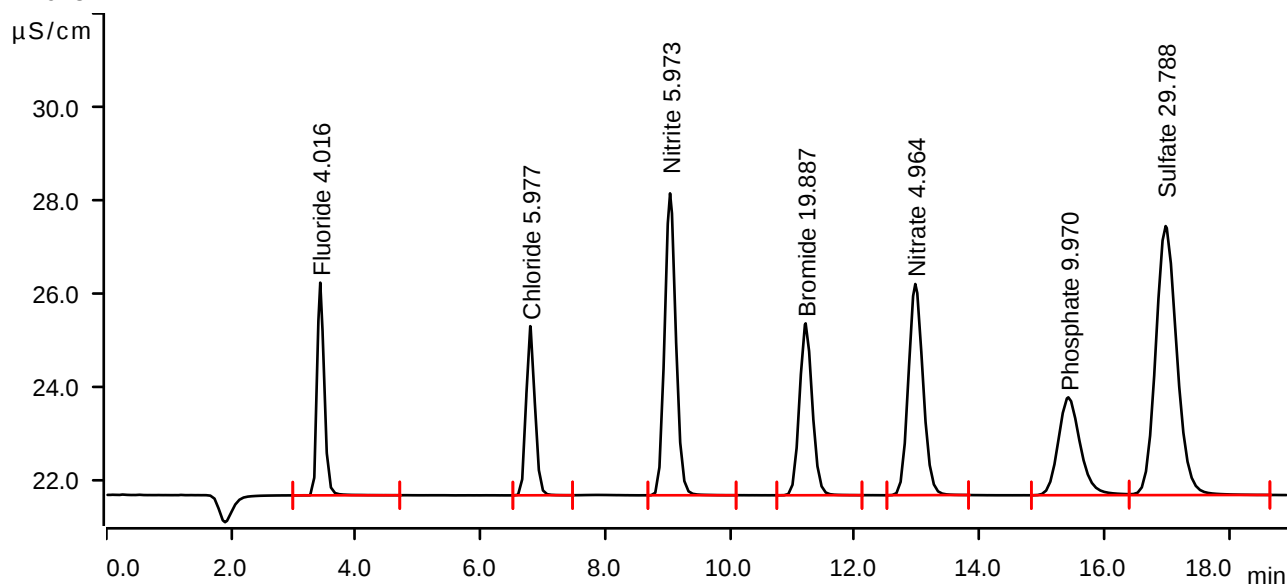

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.5937	4.568	4.016	Fluoride
2	6.797	0.5919	3.633	5.977	Chloride
3	9.038	1.3497	6.484	5.973	Nitrite
4	11.212	0.8789	3.691	19.887	Bromide
5	12.970	1.2302	4.535	4.964	Nitrate
6	15.423	0.8637	2.101	9.970	Phosphate
7	16.983	2.2643	5.777	29.788	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-01-20 13:23:08 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

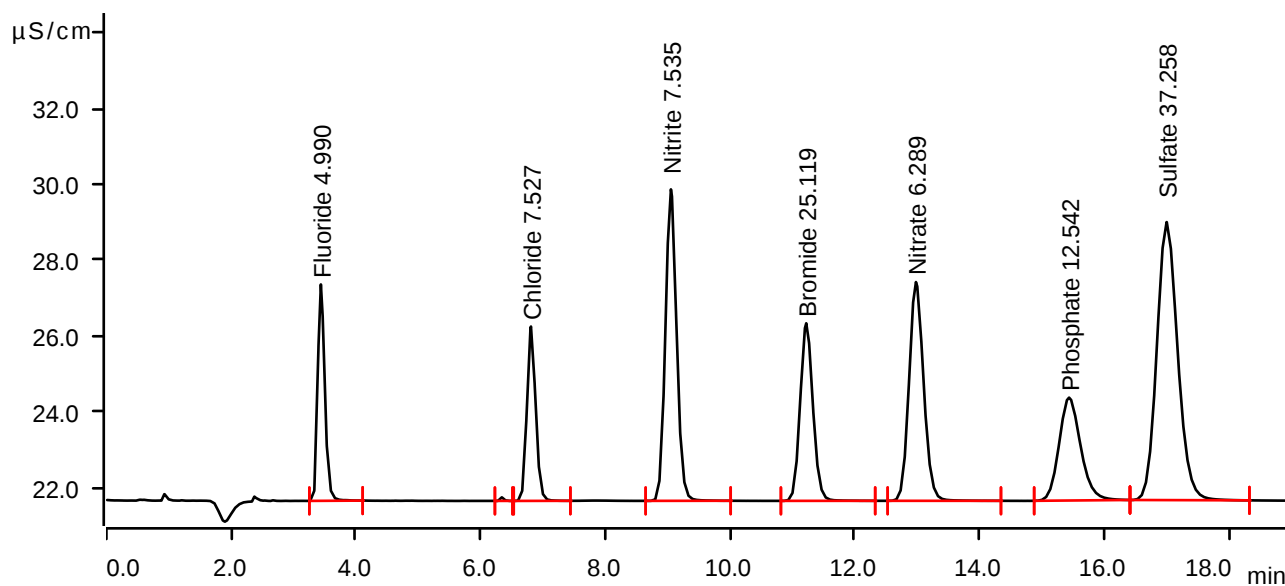

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.440	0.7387	5.703	4.990	Fluoride
2	6.342	0.0051	0.093	invalid	
3	6.808	0.7466	4.595	7.527	Chloride
4	9.052	1.7073	8.209	7.535	Nitrite
5	11.222	1.1125	4.681	25.119	Bromide
6	12.980	1.5629	5.766	6.289	Nitrate
7	15.435	1.0877	2.713	12.542	Phosphate
8	16.998	2.8398	7.327	37.258	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-01-20 13:44:36 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

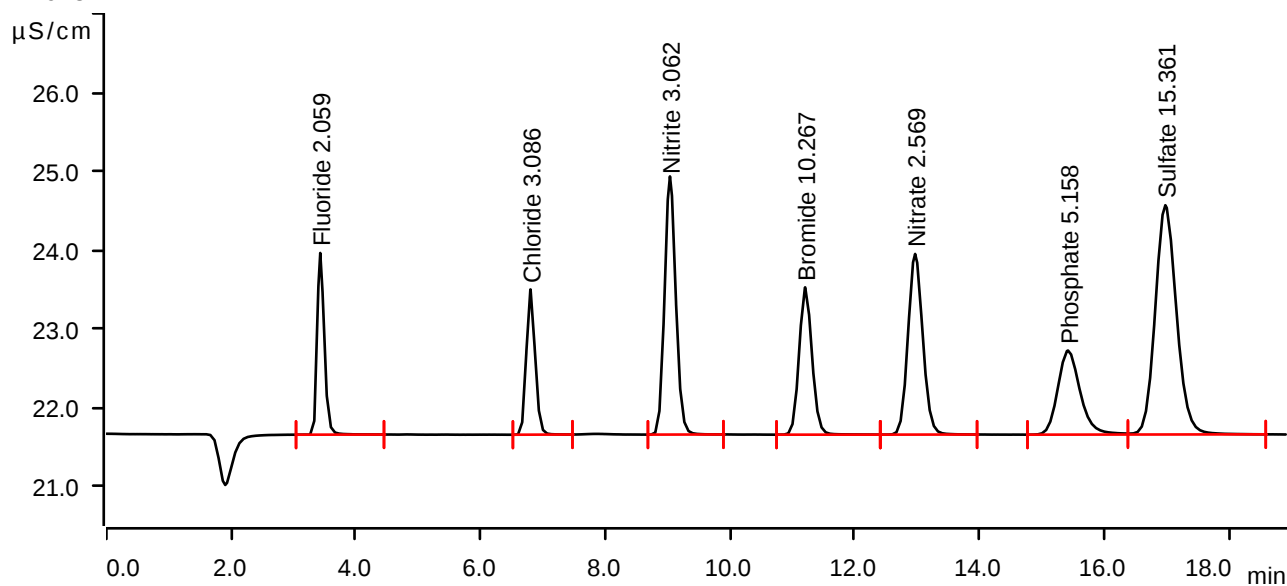

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.3025	2.306	2.059	Fluoride
2	6.798	0.3033	1.843	3.086	Chloride
3	9.037	0.6832	3.276	3.062	Nitrite
4	11.205	0.4495	1.869	10.267	Bromide
5	12.967	0.6293	2.293	2.569	Nitrate
6	15.418	0.4447	1.067	5.158	Phosphate
7	16.978	1.1525	2.909	15.361	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2025-01-20 14:06:05 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

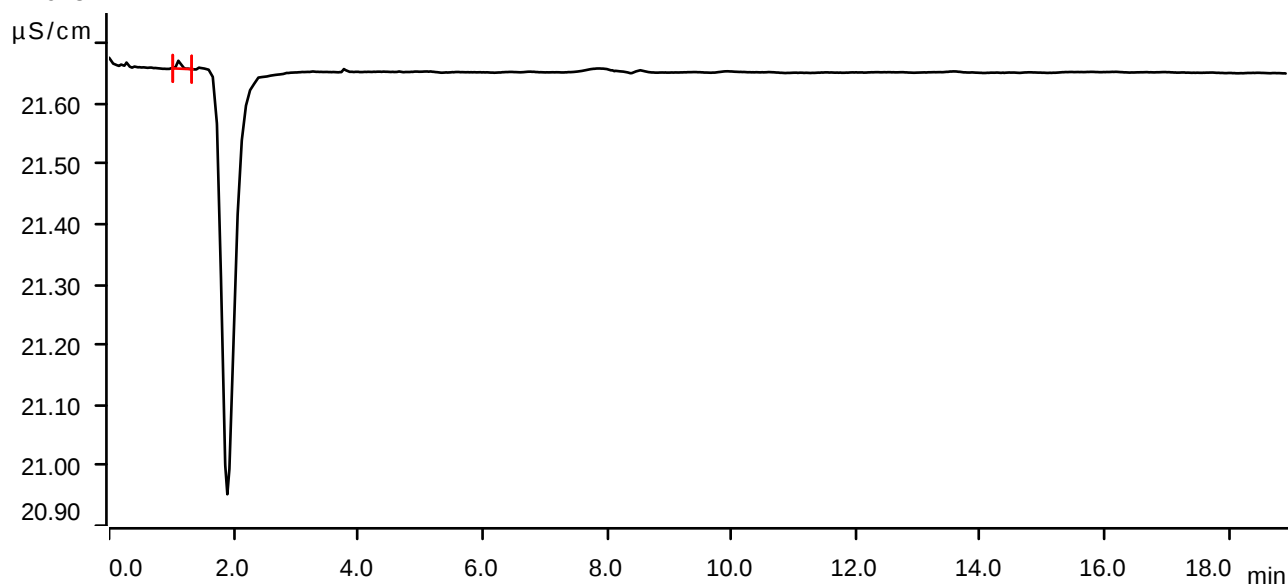

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	1.115	0.0010	0.013	invalid	


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-01-24 09:57:16 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.33 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

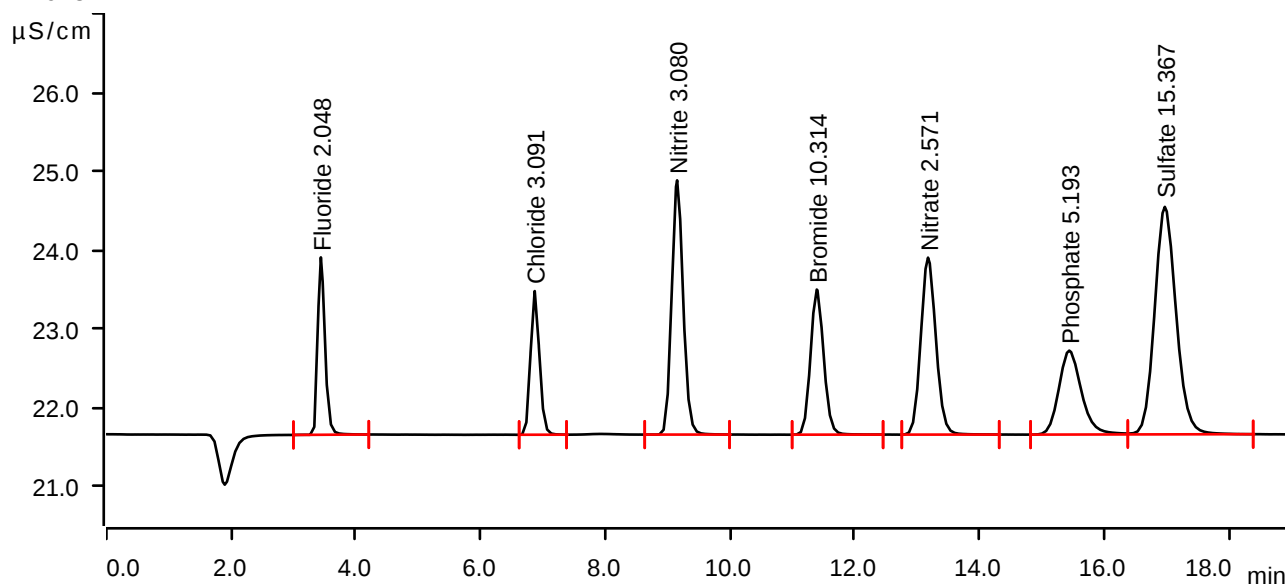


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.440	0.3008	2.251	2.048	Fluoride
2	6.867	0.3039	1.823	3.091	Chloride
3	9.152	0.6873	3.227	3.080	Nitrite
4	11.392	0.4515	1.841	10.314	Bromide
5	13.173	0.6296	2.246	2.571	Nitrate
6	15.438	0.4478	1.065	5.193	Phosphate
7	16.970	1.1530	2.887	15.367	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-01-24 10:18:46 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

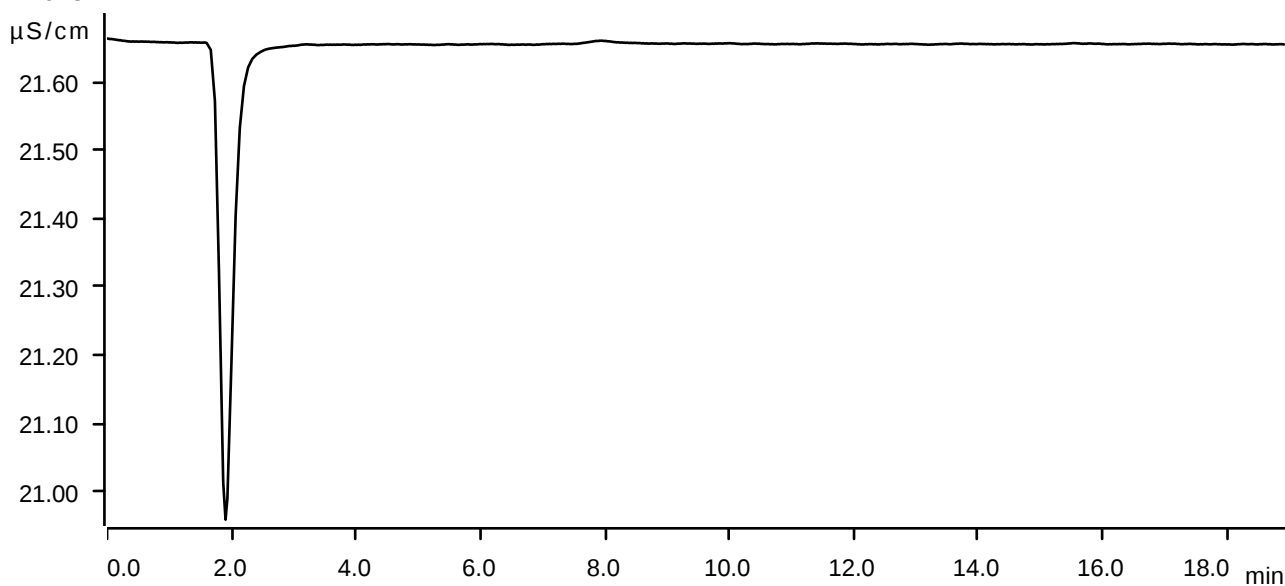
Anions

Sample data

Ident LB134413BLW
Sample type Sample
Determination start 2025-01-24 10:40:16 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

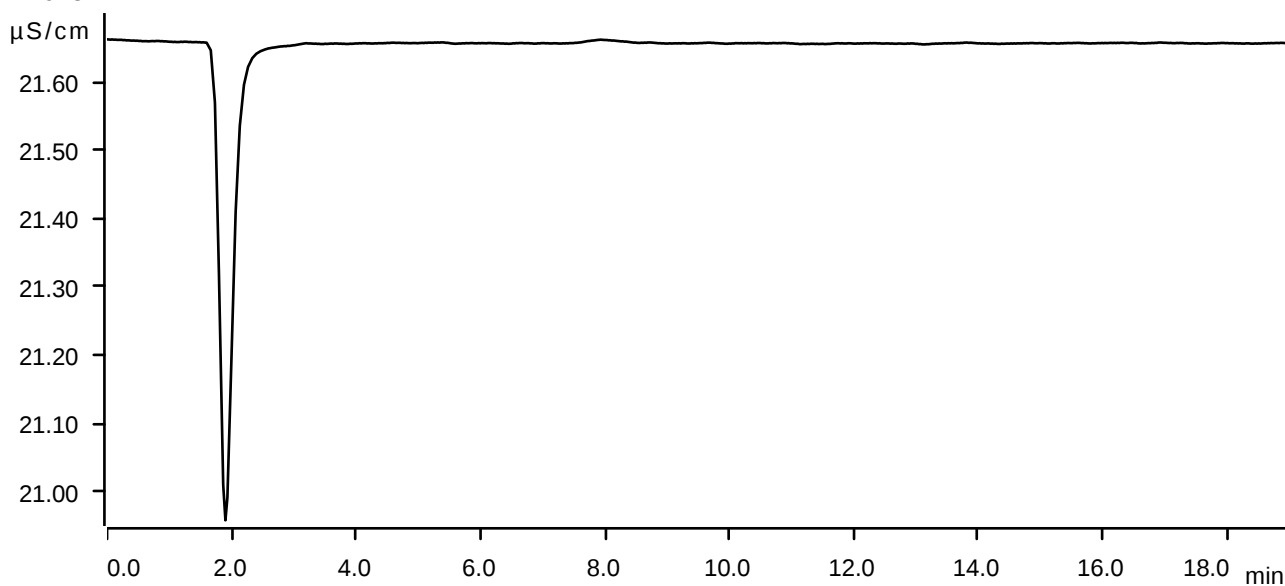Anions


Sample data

Ident LB134413BSW
Sample type Check standard 1
Determination start 2025-01-24 11:01:47 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

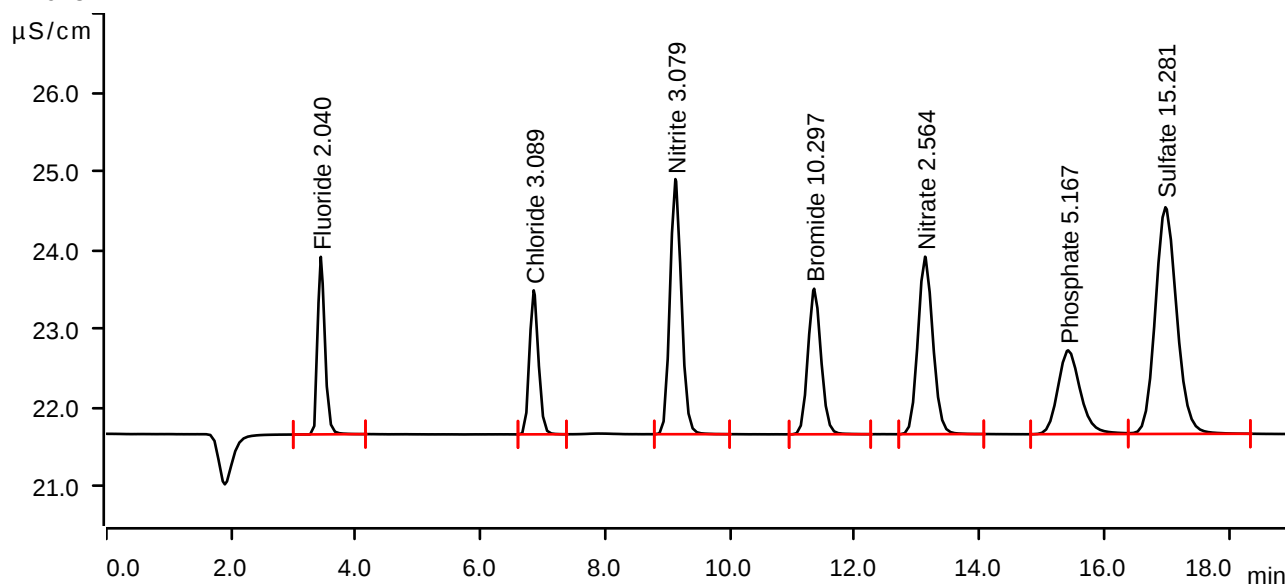

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.438	0.2995	2.253	2.040	Fluoride
2	6.852	0.3037	1.828	3.089	Chloride
3	9.123	0.6870	3.237	3.079	Nitrite
4	11.348	0.4508	1.847	10.297	Bromide
5	13.127	0.6279	2.253	2.564	Nitrate
6	15.420	0.4455	1.063	5.167	Phosphate
7	16.980	1.1464	2.877	15.281	Sulfate


Sample data

Ident Q1168-08
Sample type Sample
Determination start 2025-01-24 11:23:19 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

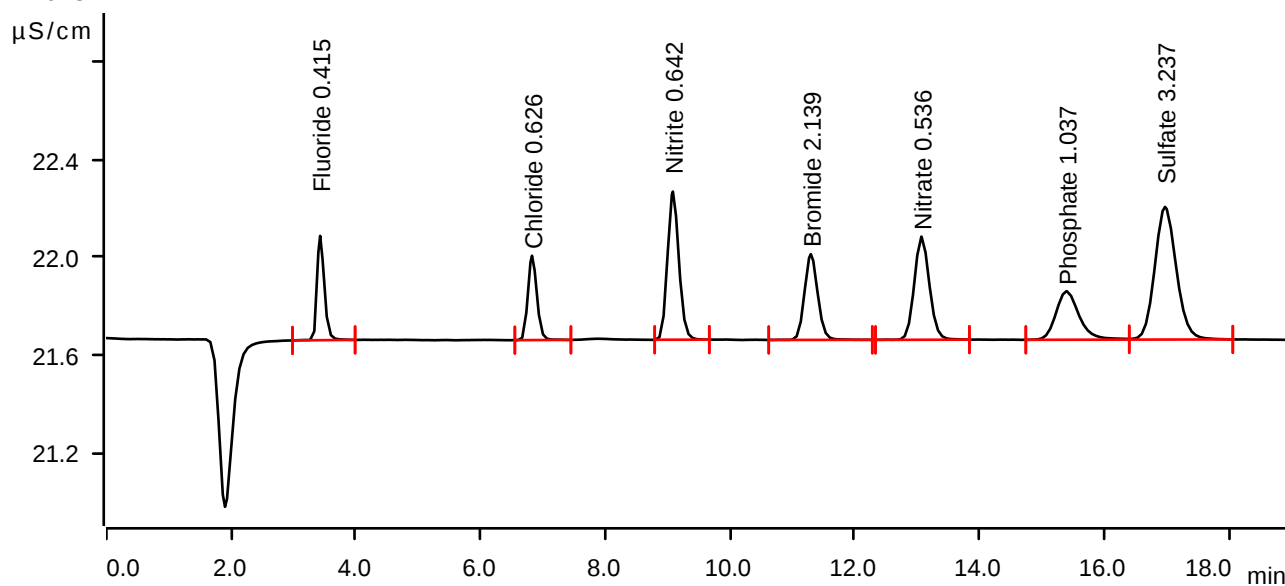

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.428	0.0578	0.428	0.415	Fluoride
2	6.825	0.0579	0.346	0.626	Chloride
3	9.083	0.1290	0.607	0.642	Nitrite
4	11.295	0.0866	0.352	2.139	Bromide
5	13.070	0.1188	0.423	0.536	Nitrate
6	15.392	0.0859	0.199	1.037	Phosphate
7	16.973	0.2184	0.544	3.237	Sulfate


Sample data

Ident Q1168-07
Sample type Sample
Determination start 2025-01-24 11:44:52 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

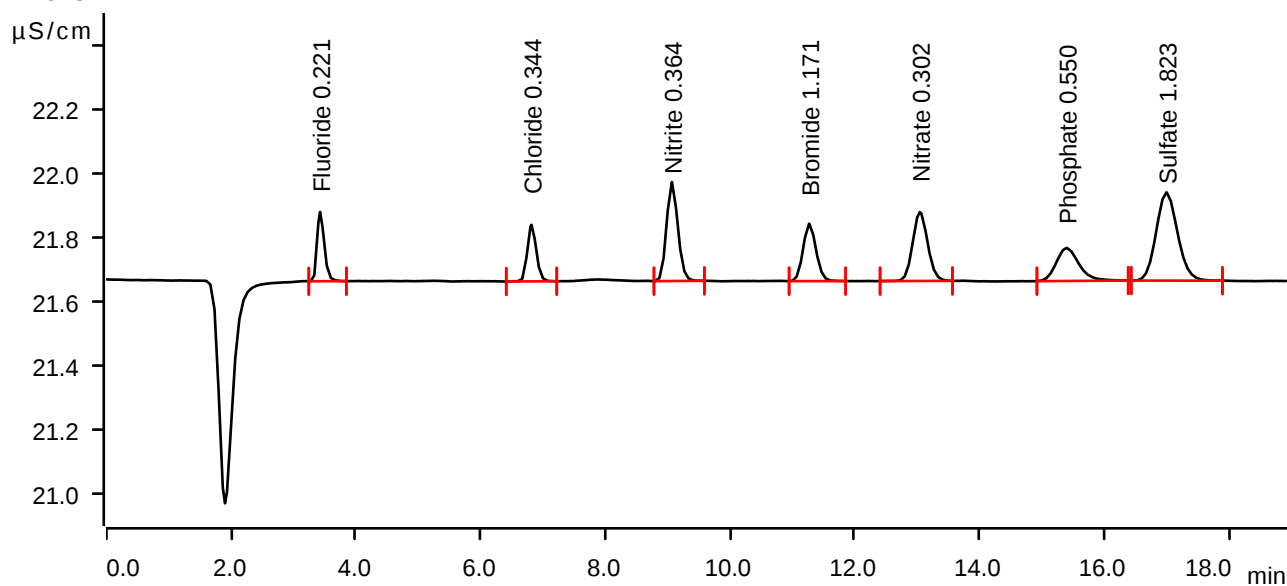

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.427	0.0289	0.217	0.221	Fluoride
2	6.817	0.0297	0.177	0.344	Chloride
3	9.067	0.0653	0.309	0.364	Nitrite
4	11.270	0.0434	0.179	1.171	Bromide
5	13.043	0.0603	0.215	0.302	Nitrate
6	15.395	0.0435	0.103	0.550	Phosphate
7	16.997	0.1094	0.276	1.823	Sulfate


Sample data

Ident Q1168-07RE 0.25ML
Sample type Sample
Determination start 2025-01-24 12:06:25 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

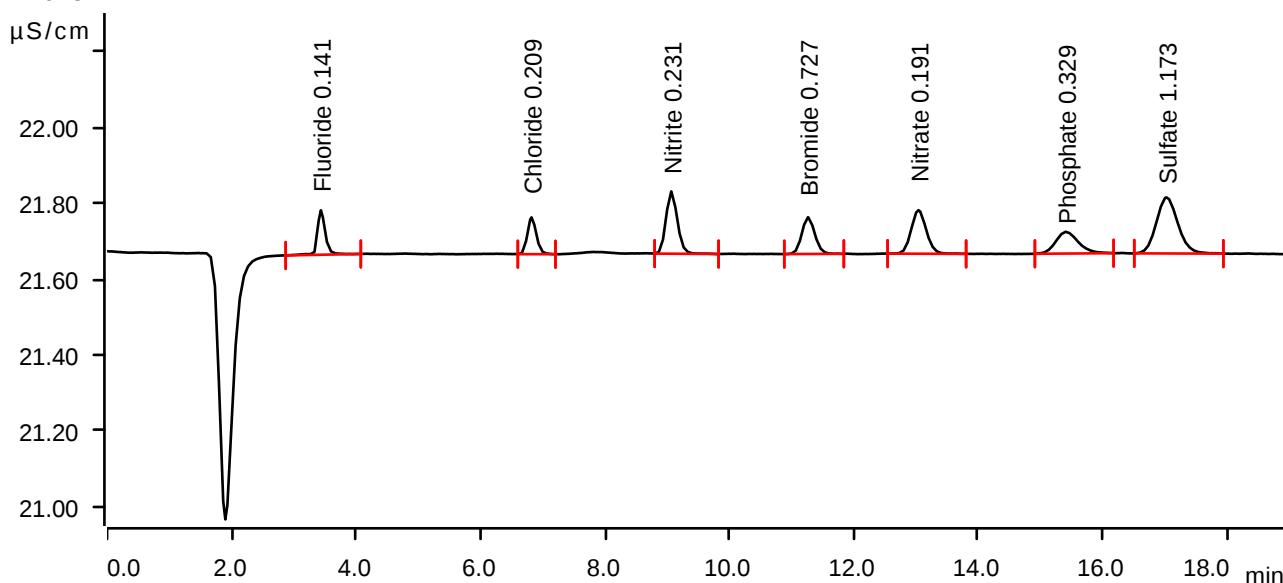

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.437	0.0170	0.117	0.141	Fluoride
2	6.822	0.0162	0.097	0.209	Chloride
3	9.068	0.0349	0.164	0.231	Nitrite
4	11.263	0.0235	0.097	0.727	Bromide
5	13.038	0.0324	0.115	0.191	Nitrate
6	15.407	0.0242	0.057	0.329	Phosphate
7	17.025	0.0593	0.148	1.173	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-01-24 12:28:00 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.33 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

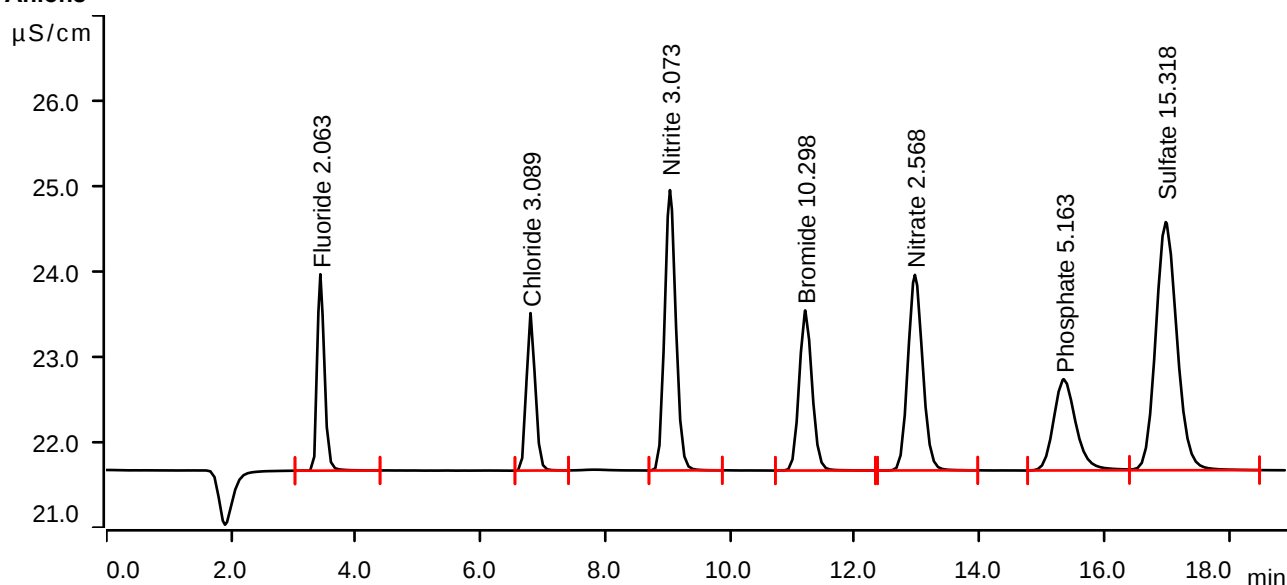

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.432	0.3031	2.301	2.063	Fluoride
2	6.802	0.3037	1.844	3.089	Chloride
3	9.037	0.6856	3.284	3.073	Nitrite
4	11.207	0.4508	1.876	10.298	Bromide
5	12.963	0.6289	2.291	2.568	Nitrate
6	15.350	0.4452	1.069	5.163	Phosphate
7	16.985	1.1492	2.907	15.318	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-01-24 12:49:30 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions