

LB134454


7470A

INSTRUMENT ID: CV1

Linear

μ Abs.:

39892

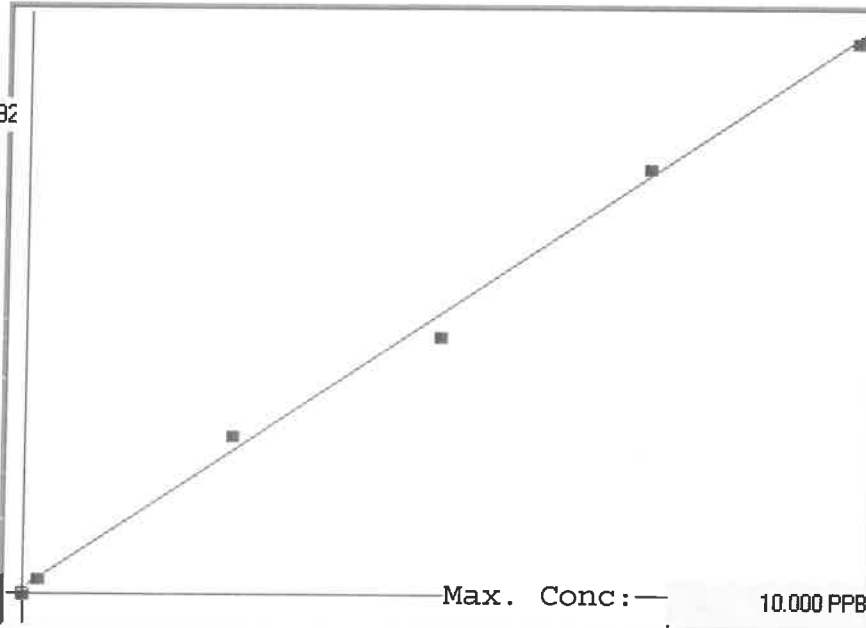

A= 0.0000e+000

B= 2.5139e-004

C= -8.3090e-002

Rho= 0.9983091

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/013
0.0	0.000	-0.065	-0.065	71	0.000	71	0				1
0.2	0.200	0.196	-0.004	1112	0.0 %	1112					2
2.5	2.500	2.816	0.316	11533	0.0 %	11533					13
5.0	5.000	4.630	-0.370	18746	0.0 %	18746					17
7.5	7.500	7.678	0.178	30871	0.0 %	30871					2
10.0	10.000	9.945	-0.055	39892	0.0 %	39892					1

LB134454 INMSTUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 28 Jan 2025 11:57:36

Sample ID	Extended ID	µ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	71	-	0.0000	7470A	PPB	28 Jan 2025 12:02:39	S	Std
0.2 - 1	50-2	1112	-	0.2000	7470A	PPB	28 Jan 2025 12:04:56	S	Std
2.5 - 1	52-4	11533	-	2.5000	7470A	PPB	28 Jan 2025 12:07:13	S	Std
5.0 - 1	35	18746	-	5.0000	7470A	PPB	28 Jan 2025 12:09:30	S	Std
7.5 - 1	33.5	30871	-	7.5000	7470A	PPB	28 Jan 2025 12:11:47	S	Std
10.0 - 1	318	39892	-	10.0000	7470A	PPB	28 Jan 2025 12:34:33	S	Std
ICV72 - 1	ICV72	15968	3.9311	-	7470A	PPB	28 Jan 2025 12:39:58	U	SMPL
ICB72 - 1	ICB72	300	-0.0077	-	7470A	PPB	28 Jan 2025 12:42:13	U	SMPL
CCV79 - 1	CCV79	20208	4.9970	-	7470A	PPB	28 Jan 2025 12:44:30	U	SMPL
CCB79 - 1	CCB79	237	-0.0235	-	7470A	PPB	28 Jan 2025 12:46:45	U	SMPL
CRA - 1	CRA	1105	0.1947	-	7470A	PPB	28 Jan 2025 12:49:02	U	SMPL
HighStd - 1	HighStd	39870	9.9399	-	7470A	PPB	28 Jan 2025 12:51:17	U	SMPL
ChkStd - 1	ChkStd	28134	6.9896	-	7470A	PPB	28 Jan 2025 12:53:33	U	SMPL
PB166290BL - 1	PBW	283	-0.0119	-	7470A	PPB	28 Jan 2025 12:55:50	U	SMPL
PB166290BS - 1	LCSW	18251	4.5051	-	7470A	PPB	28 Jan 2025 12:58:08	U	SMPL
Q1076-05 - 1	ARS20-0006	-3	-0.0838	-	7470A	PPB	28 Jan 2025 13:00:24	U	SMPL
Q1169-02 - 1	ARS20-0006	110	-0.0554	-	7470A	PPB	28 Jan 2025 13:02:42	U	SMPL
Q1169-04 - 1	REGULATOR-BUILDING-GRAVEL	82	-0.0625	-	7470A	PPB	28 Jan 2025 13:05:00	U	SMPL
Q1169-06 - 1	SPILL-SITE	154	-0.0444	-	7470A	PPB	28 Jan 2025 13:07:17	U	SMPL
Q1169-06DUP - 1	SPILL-SITEDUP	103	-0.0572	-	7470A	PPB	28 Jan 2025 13:09:32	U	SMPL
CCV80 - 1	CCV80	20524	5.0765	-	7470A	PPB	28 Jan 2025 13:11:48	U	SMPL
CCB80 - 1	CCB80	361	0.0077	-	7470A	PPB	28 Jan 2025 13:14:03	U	SMPL
Q1169-06MS - 1	SPILL-SITEMS	19217	4.7479	-	7470A	PPB	28 Jan 2025 13:16:20	U	SMPL
Q1169-06MSD - 1	SPILL-SITEMSD	19075	4.7122	-	7470A	PPB	28 Jan 2025 13:18:35	U	SMPL
PB166291BL - 1	PBW	44	-0.0720	-	7470A	PPB	28 Jan 2025 13:23:25	U	SMPL
PB166291BS - 1	LCSW	18283	4.5131	-	7470A	PPB	28 Jan 2025 13:27:59	U	SMPL
Q1193-01 - 1	TAPIAL3-MW04S-012425-00-T3	-90	-0.1057	-	7470A	PPB	28 Jan 2025 13:30:16	U	SMPL
Q1193-01DUP - 1	TAPIAL3-MW04S-012425-00-T3DUP	245	-0.0215	-	7470A	PPB	28 Jan 2025 13:32:33	U	SMPL
Q1193-01MS - 1	TAPIAL3-MW04S-012425-00-T3MS	18308	4.5194	-	7470A	PPB	28 Jan 2025 13:34:49	U	SMPL
Q1193-01MSD - 1	TAPIAL3-MW04S-012425-00-T3MSD	18362	4.5330	-	7470A	PPB	28 Jan 2025 13:37:07	U	SMPL
Q1193-02 - 1	TAPIAL2-MW01-012425-00-T2	-117	-0.1125	-	7470A	PPB	28 Jan 2025 13:39:25	U	SMPL
Q1194-08 - 1	EB	147	-0.0461	-	7470A	PPB	28 Jan 2025 13:41:42	U	SMPL
CCV81 - 1	CCV81	20751	5.1335	-	7470A	PPB	28 Jan 2025 13:46:41	U	SMPL
CCB81 - 1	CCB81	261	-0.0175	-	7470A	PPB	28 Jan 2025 13:48:57	U	SMPL
PB166211TB - 1	PB166211TB	107	-0.0562	-	7470A	PPB	28 Jan 2025 13:51:14	U	SMPL
Q1169-06LX5 - 1		18	-0.0786	-	7470A	PPB	28 Jan 2025 13:53:29	U	SMPL
Q1169-06A - 1		18894	4.6667	-	7470A	PPB	28 Jan 2025 13:55:45	U	SMPL
Q1193-01LX5 - 1		-80	-0.1032	-	7470A	PPB	28 Jan 2025 13:58:01	U	SMPL
Q1193-01A - 1		17404	4.2921	-	7470A	PPB	28 Jan 2025 14:00:18	U	SMPL
CCV82 - 1	CCV82	19615	4.8480	-	7470A	PPB	28 Jan 2025 14:07:14	U	SMPL
CCB82 - 1	CCB82	293	-0.0094	-	7470A	PPB	28 Jan 2025 14:09:32	U	SMPL