

Instrument II		IC-1		Analyst :		NF		Method: :00.0 / 9056A			
Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	al wt/Fina	Analyst
STD1	0	0	0	0	0	0	0	IC1-012025	1/20/2025 11:14	10	NF/IZ
STD2	0.396	0.602	0.613	2.019	0.511	0.994	3.09	IC1-012025	1/20/2025 11:36	10	NF/IZ
STD3	0.835	1.258	1.254	4.184	1.047	2.089	6.324	IC1-012025	1/20/2025 11:57	10	NF/IZ
STD4	0.967	1.463	1.466	4.879	1.221	2.469	7.299	IC1-012025	1/20/2025 12:18	10	NF/IZ
STD5	1.996	2.973	2.959	9.912	2.468	4.936	14.741	IC1-012025	1/20/2025 12:40	10	NF/IZ
STD6	4.016	5.977	5.973	19.887	4.964	9.97	29.788	IC1-012025	1/20/2025 13:01	10	NF/IZ
STD7	4.99	7.527	7.535	25.119	6.289	12.542	37.258	IC1-012025	1/20/2025 13:23	10	NF/IZ
ICV	2.059	3.086	3.062	10.267	2.569	5.158	15.361	IC1-012025	1/20/2025 13:44	10	NF/IZ
ICB	0	0	0	0	0	0	0	IC1-012025	1/20/2025 14:06	10	NF/IZ
CCV	2.038	3.099	3.025	10.182	2.546	4.967	15.168	IC1-012025	2/7/2025 11:07	10	NF/IZ
CCB	0	0	0	0	0	0	0	IC1-012025	2/7/2025 11:28	10	NF/IZ
LB134634BLW	0	0	0	0	0.138	0	0.585	IC1-012025	2/7/2025 11:50	10	NF/IZ
LB134634BSW	2.007	3.015	3.008	10.033	2.509	5.109	14.977	IC1-012025	2/7/2025 12:11	10	NF/IZ
Q1322-01	0.066	156.333	0.099	0	0.465	0.869	16.135	IC1-012025	2/7/2025 12:33	10	NF/IZ
Q1322-01MS	1.859	152.315	2.83	9.327	2.765	5.411	29.643	IC1-012025	2/7/2025 12:55	10	NF/IZ
Q1322-01MSD	1.883	152.593	2.829	9.321	2.759	5.53	29.677	IC1-012025	2/7/2025 13:16	10	NF/IZ
CCV	2.039	3.108	3.038	10.217	2.552	5.118	15.174	IC1-012025	2/7/2025 13:38	10	NF/IZ
CCB	0.042	0	0	0	0	0	0	IC1-012025	2/7/2025 15:41	10	NF/IZ

Clear table


Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A

ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0	0	0	0	0	0	0	0 IC1-012025	1/20/2025 11:14	10	NF/IZ
STD2	0.396	0.602	0.613	2.019	0.511	0.994	3.09	IC1-012025	1/20/2025 11:36	10	NF/IZ
STD3	0.835	1.258	1.254	4.184	1.047	2.089	6.324	IC1-012025	1/20/2025 11:57	10	NF/IZ
STD4	0.967	1.463	1.466	4.879	1.221	2.469	7.299	IC1-012025	1/20/2025 12:18	10	NF/IZ
STD5	1.996	2.973	2.959	9.912	2.468	4.936	14.741	IC1-012025	1/20/2025 12:40	10	NF/IZ
STD6	4.016	5.977	5.973	19.887	4.964	9.97	29.788	IC1-012025	1/20/2025 13:01	10	NF/IZ
STD7	4.99	7.527	7.535	25.119	6.289	12.542	37.258	IC1-012025	1/20/2025 13:23	10	NF/IZ

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1	-1.0000	0.3333	2.1667	0.9500	2.2000	-0.6000	3.0000
STD2	4.3750	4.8333	4.5000	4.6000	4.7000	4.4500	5.4000
STD3	-3.3000	-2.4667	-2.2667	-2.4200	-2.3200	-1.2400	-2.6800
STD4	-0.2000	-0.9000	-1.3667	-0.8800	-1.2800	-1.2800	-1.7267
STD5	0.4000	-0.3833	-0.4500	-0.5650	-0.7200	-0.3000	-0.7067
STD6	-0.2000	0.3600	0.4667	0.4760	0.6240	0.3360	0.6973

Fluoride (Anions)

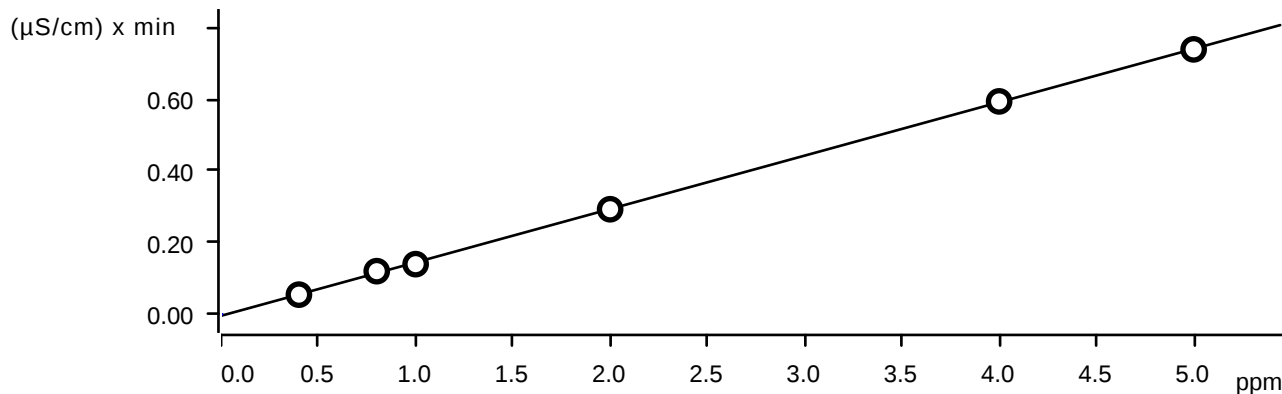


Function: $A = -4.02271E-3 + 0.0148839 \times Q$

Relative standard deviation 1.203859 %

Correlation coefficient 0.999923

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.400	10.0	1.0	1.0	0.055	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	0.800	10.0	1.0	1.0	0.120	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.000	10.0	1.0	1.0	0.140	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	2.000	10.0	1.0	1.0	0.293	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	4.000	10.0	1.0	1.0	0.594	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	5.000	10.0	1.0	1.0	0.739	STD7	2025-01-20 13:23:08 UTC-5	used

Chloride (Anions)

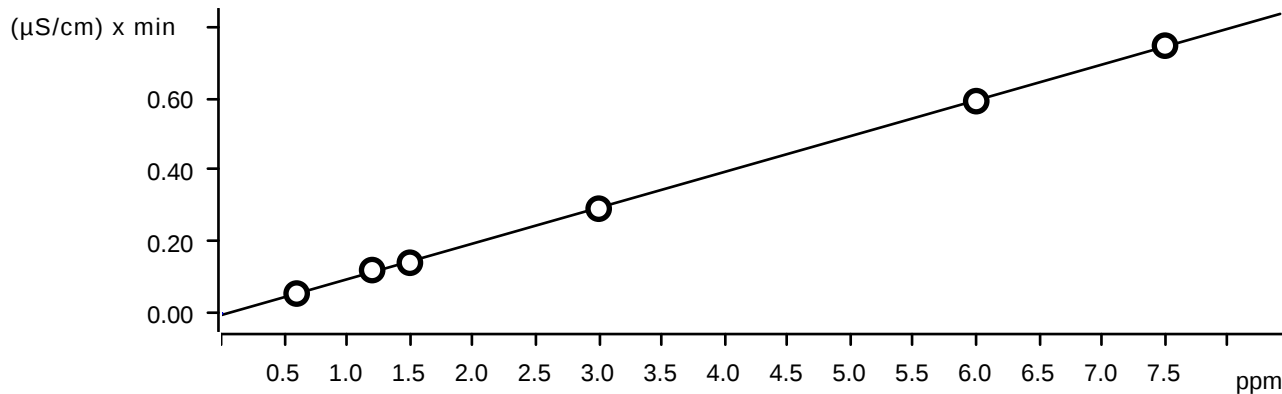

Function: $A = -4.62538E-3 + 9.98029E-3 \times Q$


Relative standard deviation 1.261416 %

Correlation coefficient 0.999916

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.055	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.121	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.141	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.292	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	0.592	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	0.747	STD7	2025-01-20 13:23:08 UTC-5	used

Nitrite (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

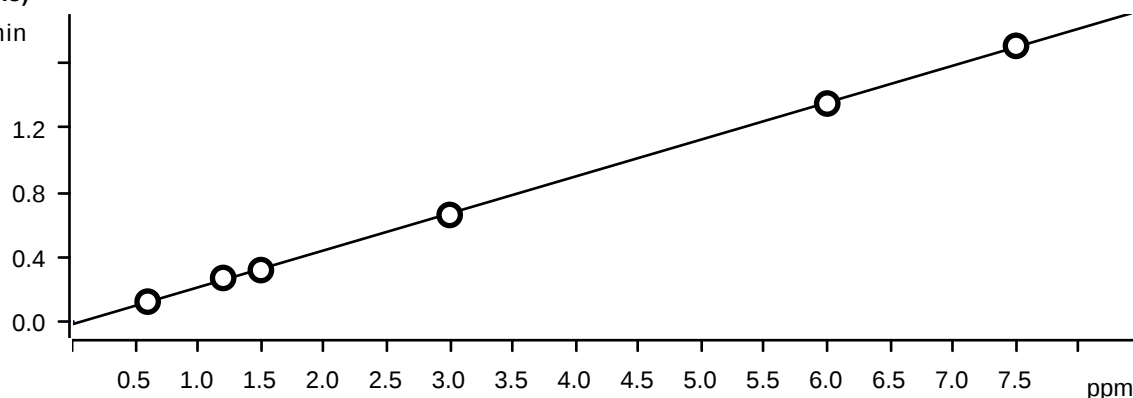

Function: $A = -0.0179856 + 0.0228967 \times Q$


Relative standard deviation 1.369596 %

Correlation coefficient 0.999903

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.122	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.269	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.660	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	1.350	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	1.707	STD7	2025-01-20 13:23:08 UTC-5	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

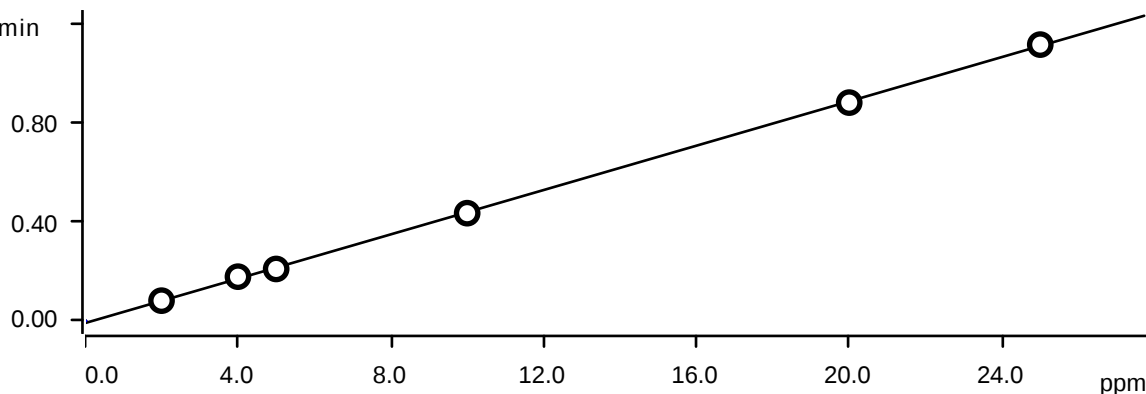

Function: $A = -8.89651E-3 + 4.46429E-3 \times Q$


Relative standard deviation: 1.338167 %

Correlation coefficient: 0.999906

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	2.000	10.0	1.0	1.0	0.081	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	4.000	10.0	1.0	1.0	0.178	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	5.000	10.0	1.0	1.0	0.209	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	10.000	10.0	1.0	1.0	0.434	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	20.000	10.0	1.0	1.0	0.879	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	25.000	10.0	1.0	1.0	1.112	STD7	2025-01-20 13:23:08 UTC-5	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

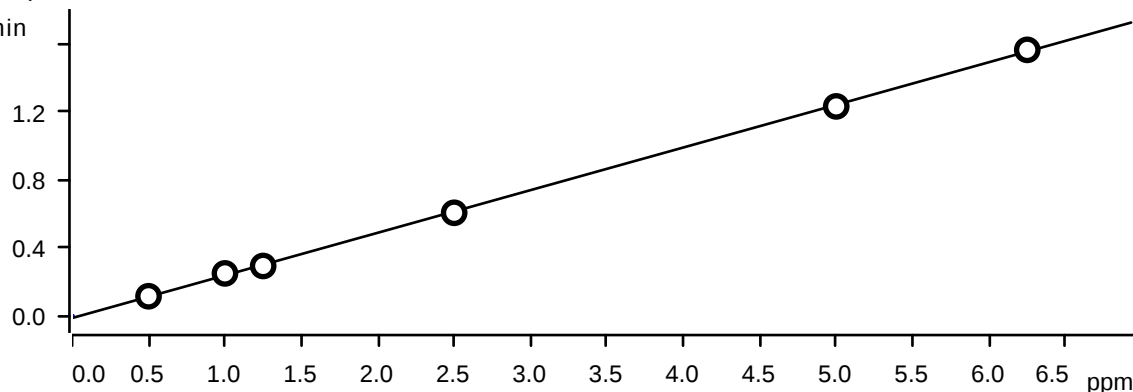


Function: $A = -0.0155875 + 0.0250988 \times Q$

Relative standard deviation: 1.561944 %

Correlation coefficient 0.999873

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.500	10.0	1.0	1.0	0.113	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	1.000	10.0	1.0	1.0	0.247	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.250	10.0	1.0	1.0	0.291	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	2.500	10.0	1.0	1.0	0.604	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	5.000	10.0	1.0	1.0	1.230	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	6.250	10.0	1.0	1.0	1.563	STD7	2025-01-20 13:23:08 UTC-5	used

Phosphate (Anions)

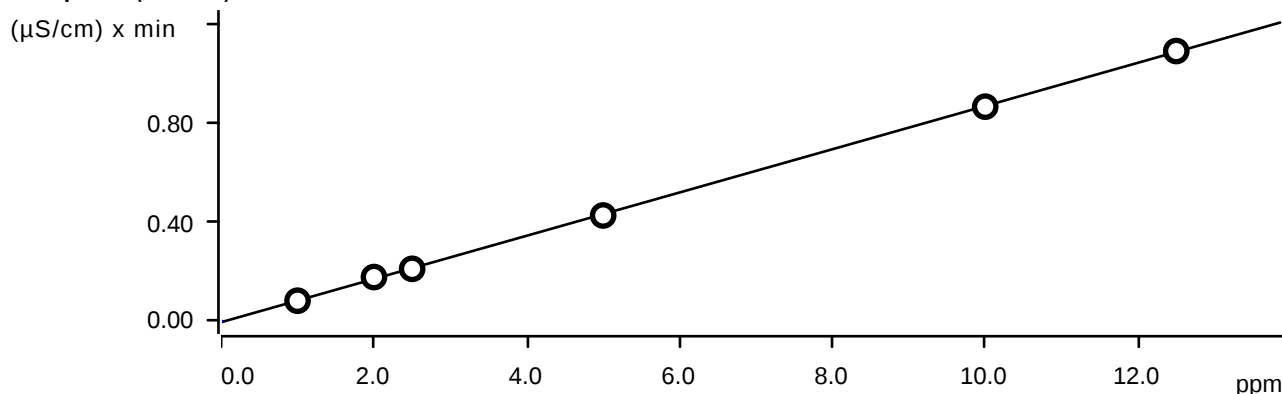


Function: $A = -4.38887E-3 + 8.70711E-3 \times Q$

Relative standard deviation 1.148005 %

Correlation coefficient 0.999929

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	1.000	10.0	1.0	1.0	0.082	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	2.000	10.0	1.0	1.0	0.177	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	2.500	10.0	1.0	1.0	0.211	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	5.000	10.0	1.0	1.0	0.425	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	10.000	10.0	1.0	1.0	0.864	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-01-20 13:23:08 UTC-5	used

Sulfate (Anions)

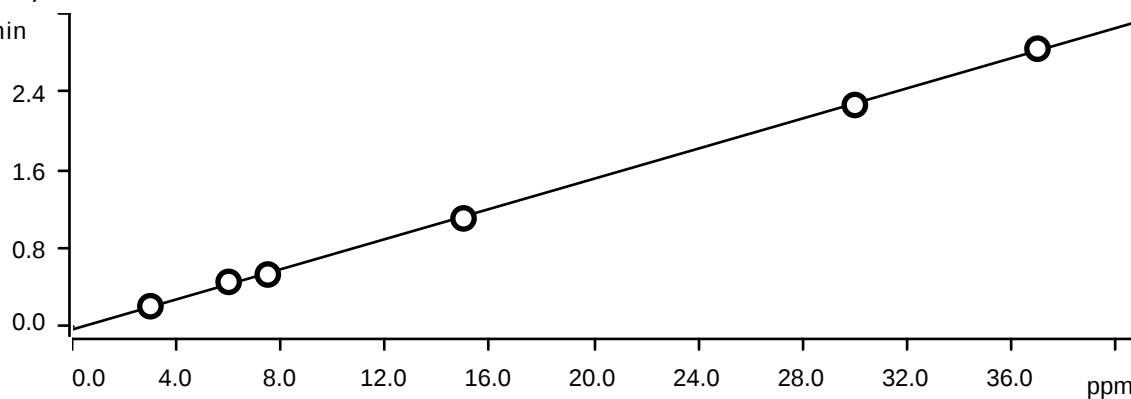 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0310554 + 7.70543E-3 \times Q$

Relative standard deviation 1.797524 %

Correlation coefficient 0.999831


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	3.000	10.0	1.0	1.0	0.207	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	6.000	10.0	1.0	1.0	0.456	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	7.500	10.0	1.0	1.0	0.531	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	15.000	10.0	1.0	1.0	1.105	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	30.000	10.0	1.0	1.0	2.264	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	37.000	10.0	1.0	1.0	2.840	STD7	2025-01-20 13:23:08 UTC-5	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-01-20 11:14:39 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

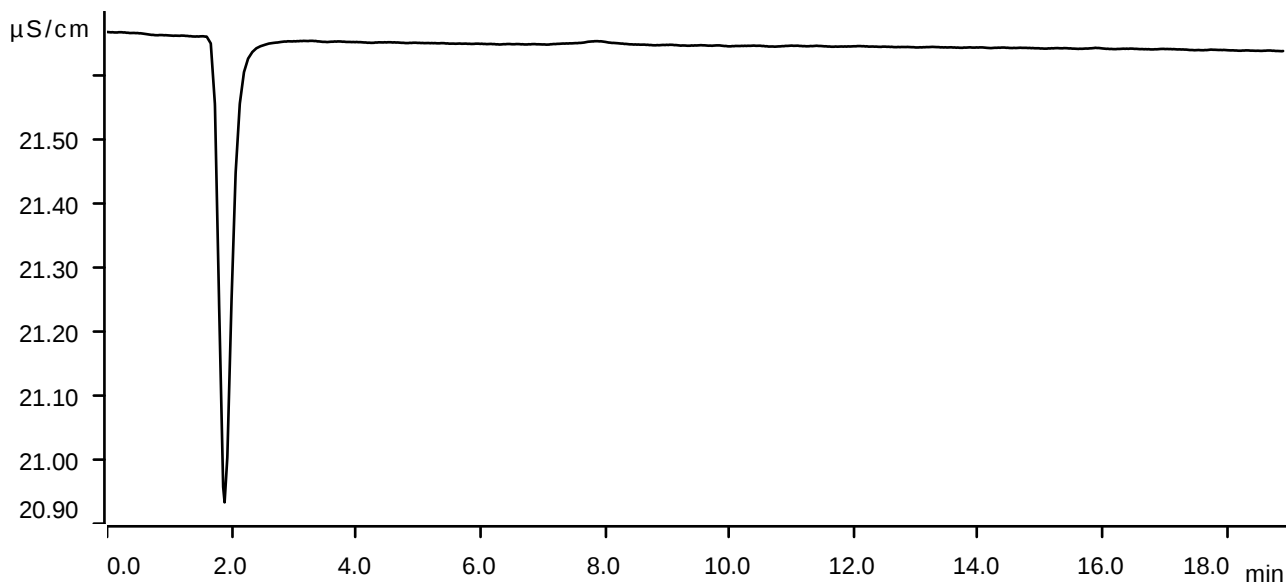Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-01-20 11:36:02 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

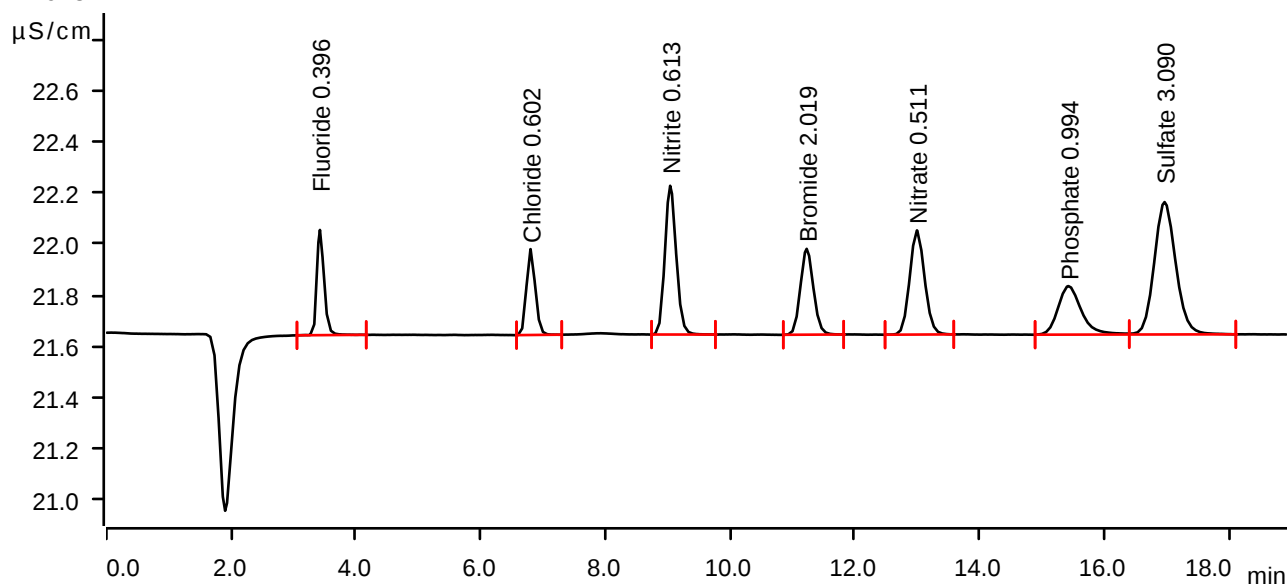

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.425	0.0549	0.411	0.396	Fluoride
2	6.802	0.0555	0.335	0.602	Chloride
3	9.040	0.1223	0.581	0.613	Nitrite
4	11.228	0.0813	0.335	2.019	Bromide
5	12.995	0.1126	0.407	0.511	Nitrate
6	15.423	0.0822	0.190	0.994	Phosphate
7	16.967	0.2070	0.517	3.090	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-01-20 11:57:26 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

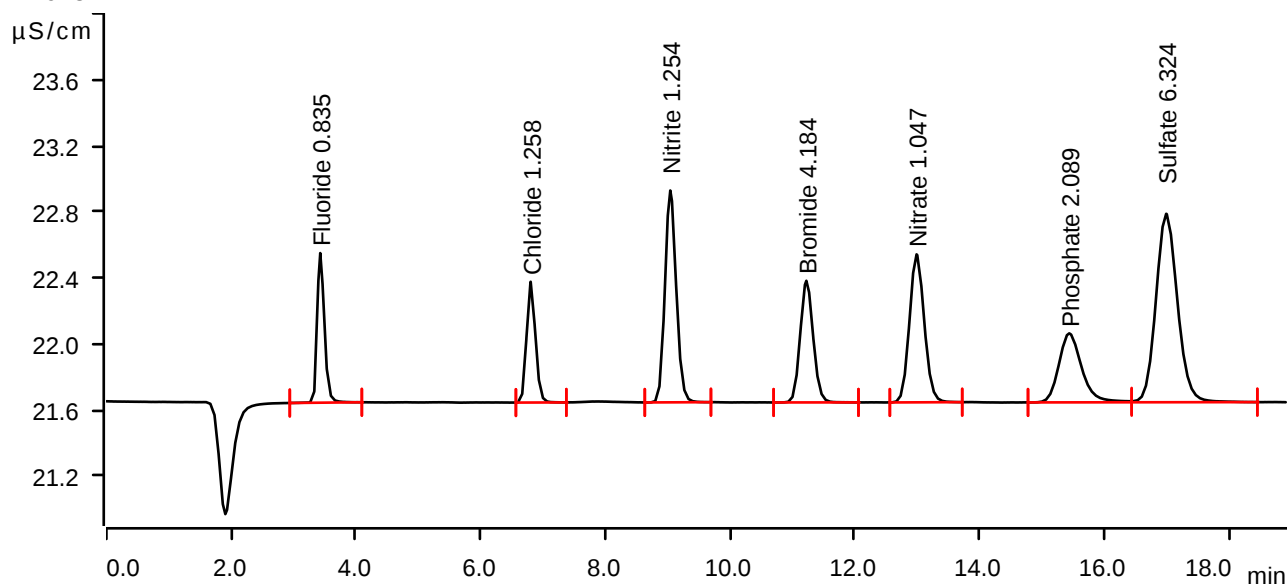

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.1203	0.906	0.835	Fluoride
2	6.803	0.1209	0.731	1.258	Chloride
3	9.042	0.2691	1.282	1.254	Nitrite
4	11.223	0.1779	0.736	4.184	Bromide
5	12.990	0.2472	0.896	1.047	Nitrate
6	15.438	0.1775	0.418	2.089	Phosphate
7	16.992	0.4562	1.141	6.324	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-01-20 12:18:50 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

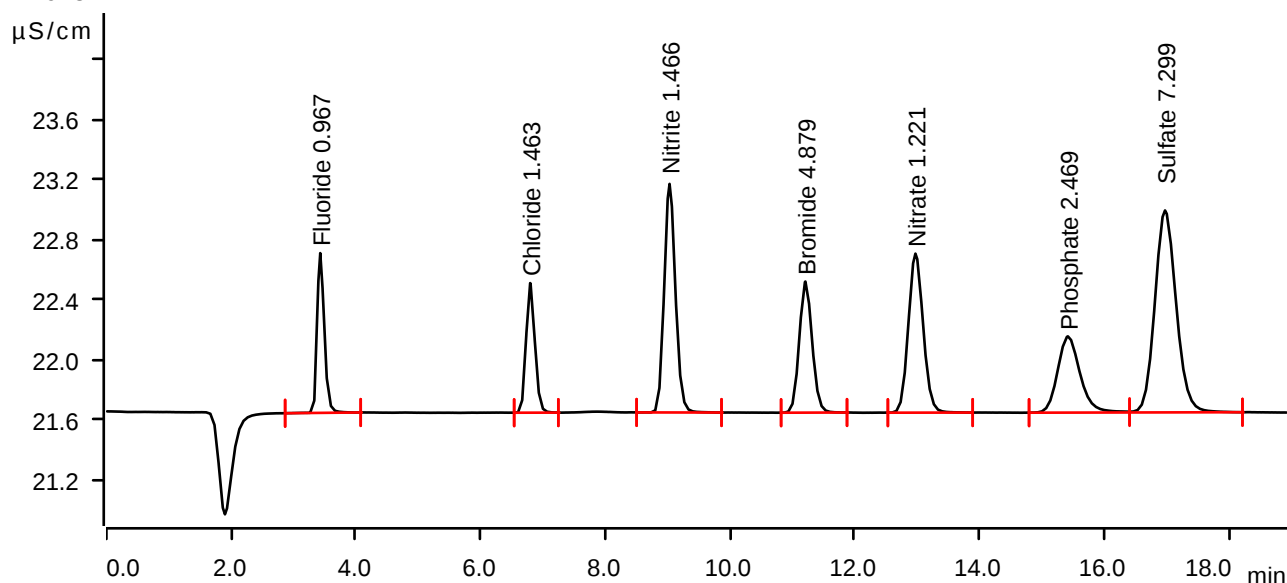

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.1399	1.061	0.967	Fluoride
2	6.795	0.1414	0.860	1.463	Chloride
3	9.030	0.3178	1.517	1.466	Nitrite
4	11.208	0.2089	0.870	4.879	Bromide
5	12.972	0.2908	1.056	1.221	Nitrate
6	15.417	0.2105	0.506	2.469	Phosphate
7	16.973	0.5314	1.341	7.299	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-01-20 12:40:15 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

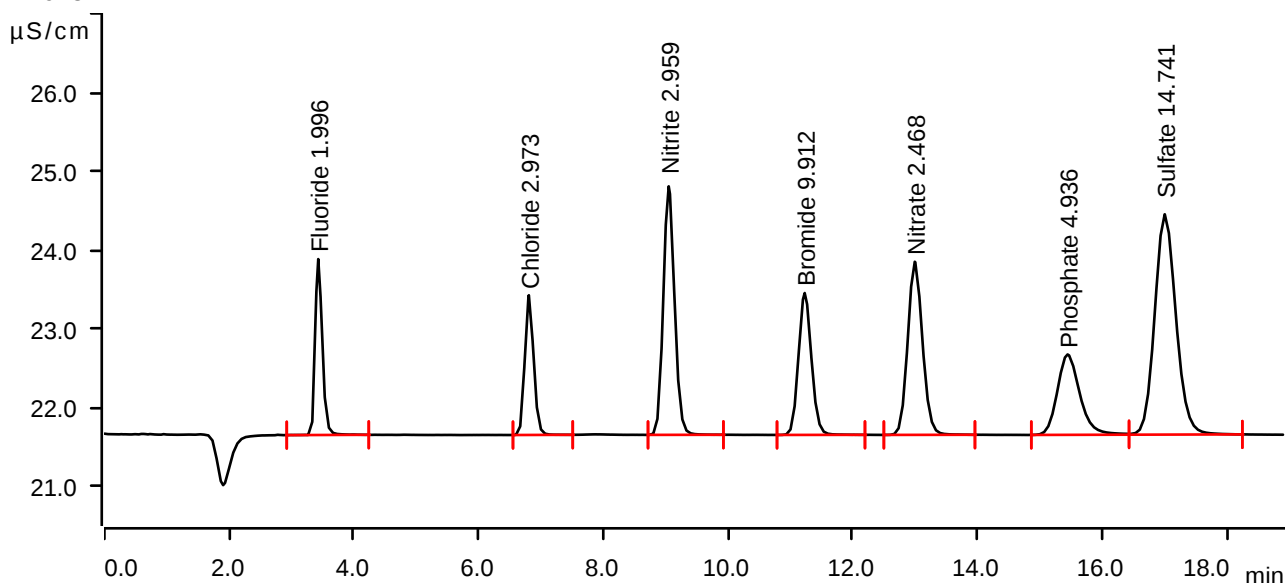

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.2930	2.233	1.996	Fluoride
2	6.807	0.2921	1.773	2.973	Chloride
3	9.048	0.6595	3.154	2.959	Nitrite
4	11.228	0.4336	1.801	9.912	Bromide
5	12.993	0.6039	2.197	2.468	Nitrate
6	15.443	0.4254	1.020	4.936	Phosphate
7	17.002	1.1048	2.795	14.741	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-01-20 13:01:41 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

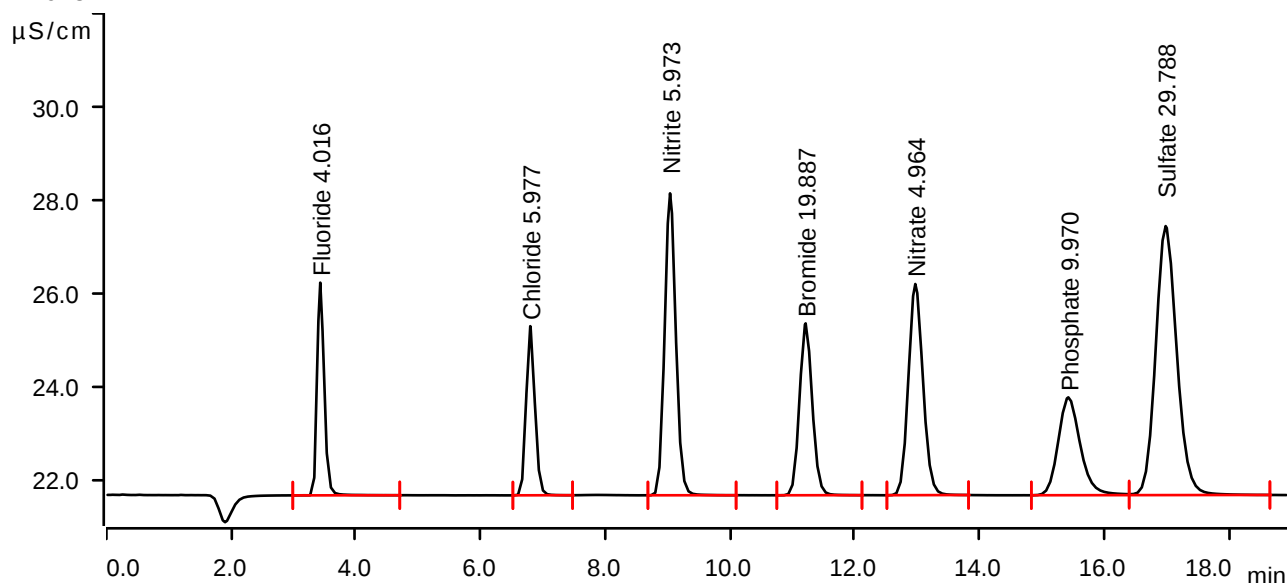

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.5937	4.568	4.016	Fluoride
2	6.797	0.5919	3.633	5.977	Chloride
3	9.038	1.3497	6.484	5.973	Nitrite
4	11.212	0.8789	3.691	19.887	Bromide
5	12.970	1.2302	4.535	4.964	Nitrate
6	15.423	0.8637	2.101	9.970	Phosphate
7	16.983	2.2643	5.777	29.788	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-01-20 13:23:08 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

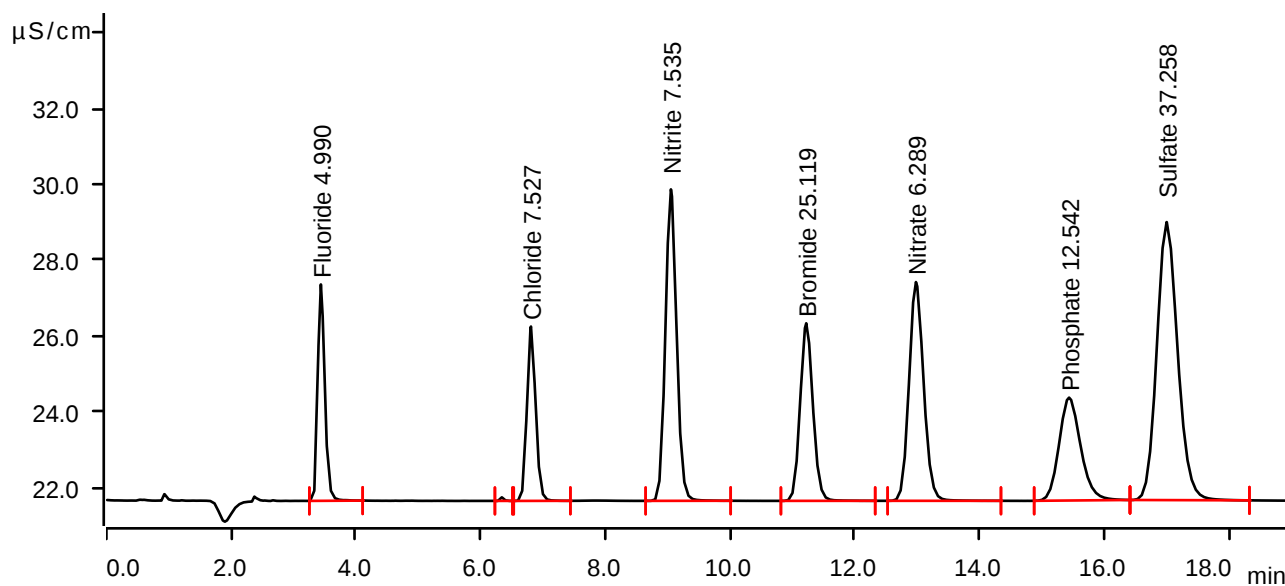

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.440	0.7387	5.703	4.990	Fluoride
2	6.342	0.0051	0.093	invalid	
3	6.808	0.7466	4.595	7.527	Chloride
4	9.052	1.7073	8.209	7.535	Nitrite
5	11.222	1.1125	4.681	25.119	Bromide
6	12.980	1.5629	5.766	6.289	Nitrate
7	15.435	1.0877	2.713	12.542	Phosphate
8	16.998	2.8398	7.327	37.258	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-01-20 13:44:36 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

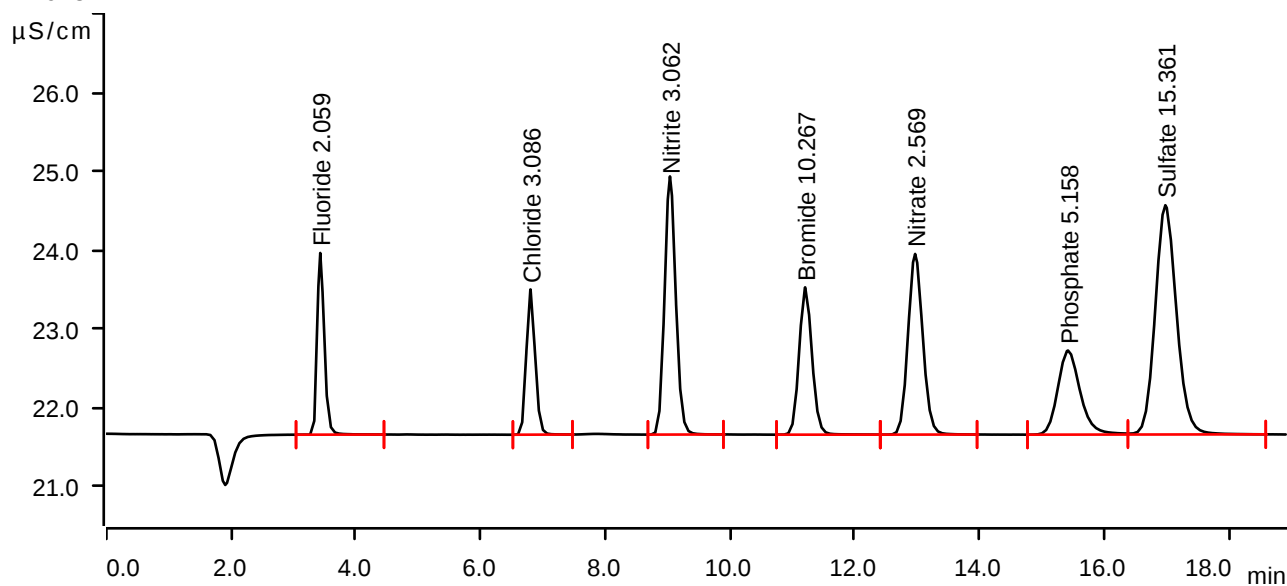

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.3025	2.306	2.059	Fluoride
2	6.798	0.3033	1.843	3.086	Chloride
3	9.037	0.6832	3.276	3.062	Nitrite
4	11.205	0.4495	1.869	10.267	Bromide
5	12.967	0.6293	2.293	2.569	Nitrate
6	15.418	0.4447	1.067	5.158	Phosphate
7	16.978	1.1525	2.909	15.361	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2025-01-20 14:06:05 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

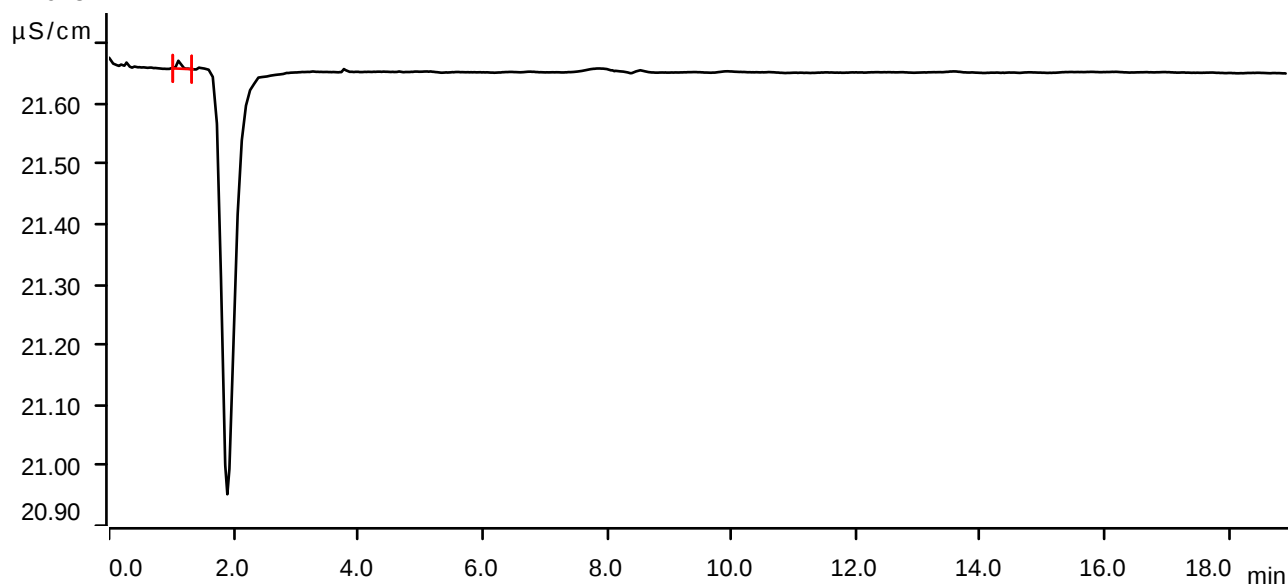

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	1.115	0.0010	0.013	invalid	


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-02-07 11:07:22 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

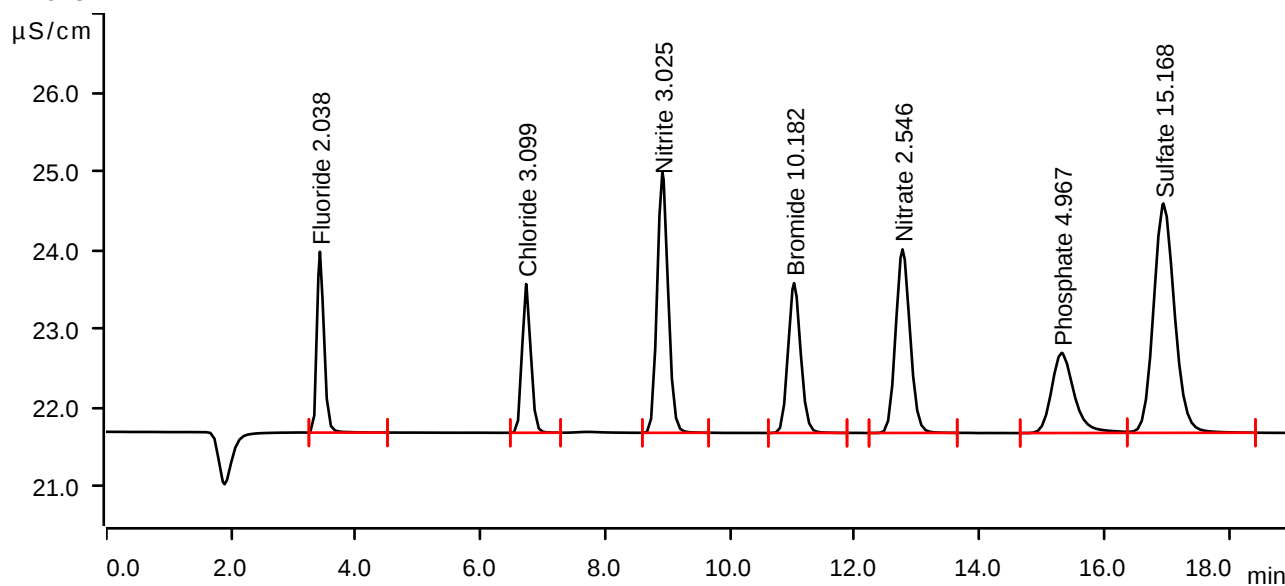


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.425	0.2993	2.296	2.038	Fluoride
2	6.730	0.3047	1.887	3.099	Chloride
3	8.915	0.6746	3.311	3.025	Nitrite
4	11.027	0.4457	1.902	10.182	Bromide
5	12.765	0.6234	2.330	2.546	Nitrate
6	15.317	0.4281	1.017	4.967	Phosphate
7	16.948	1.1377	2.911	15.168	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-02-07 11:28:52 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

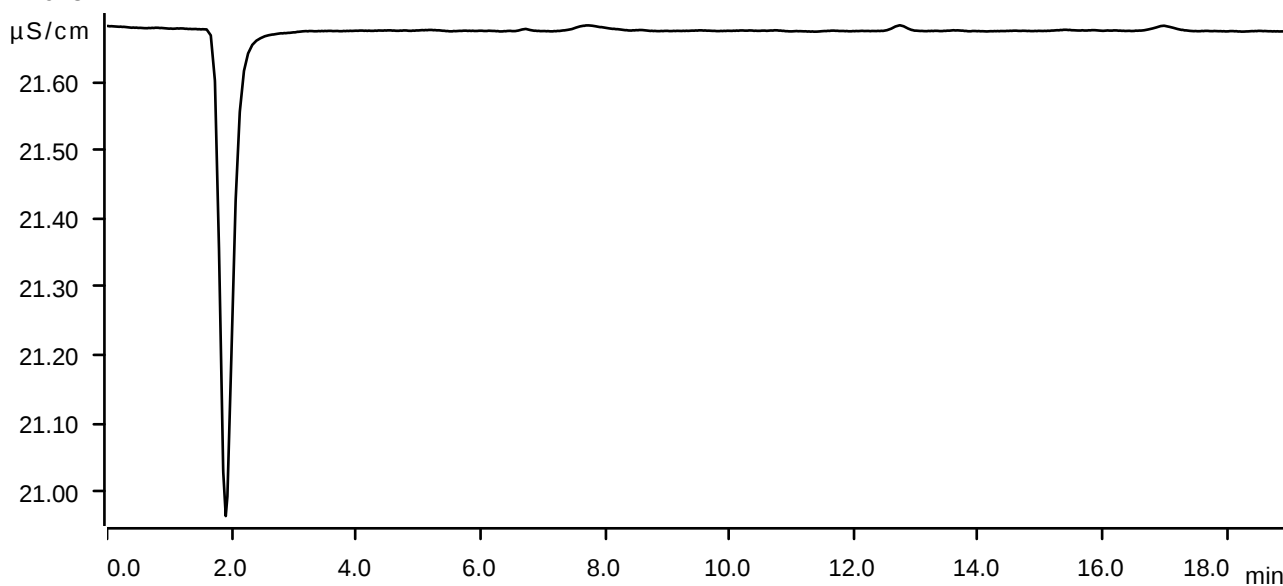Anions


Sample data

Ident LB134634BLW
 Sample type Sample
 Determination start 2025-02-07 11:50:23 UTC-5
 Method IC1-012025
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.26 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

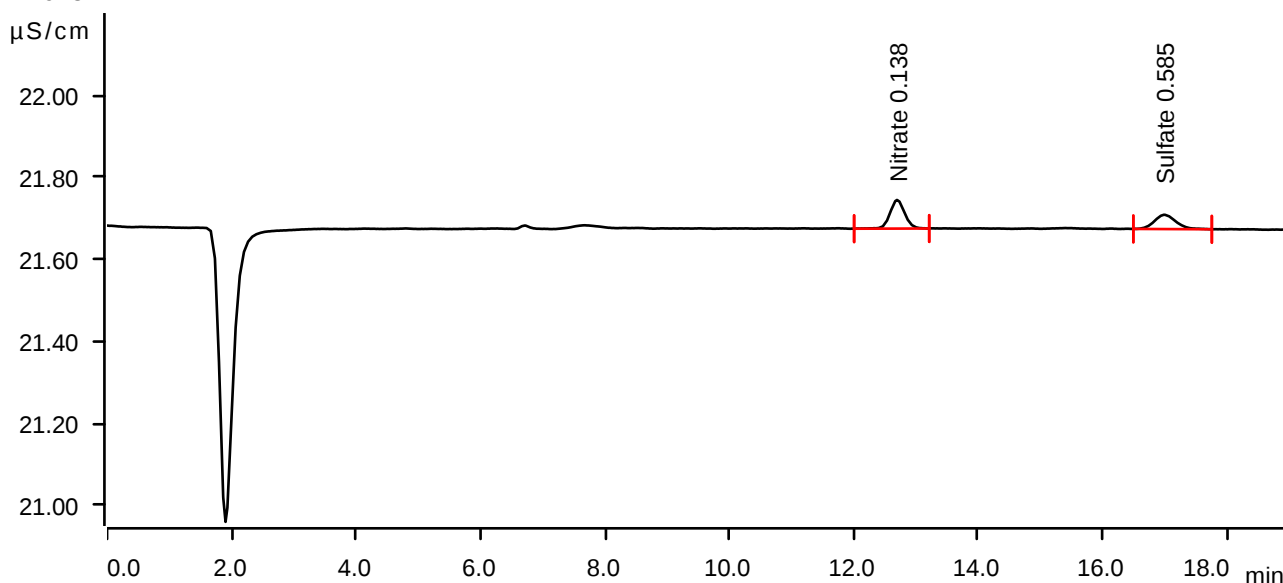

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	12.695	0.0191	0.070	0.138	Nitrate
2	16.982	0.0140	0.035	0.585	Sulfate


Sample data

Ident LB134634BSW
Sample type Check standard 1
Determination start 2025-02-07 12:11:54 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

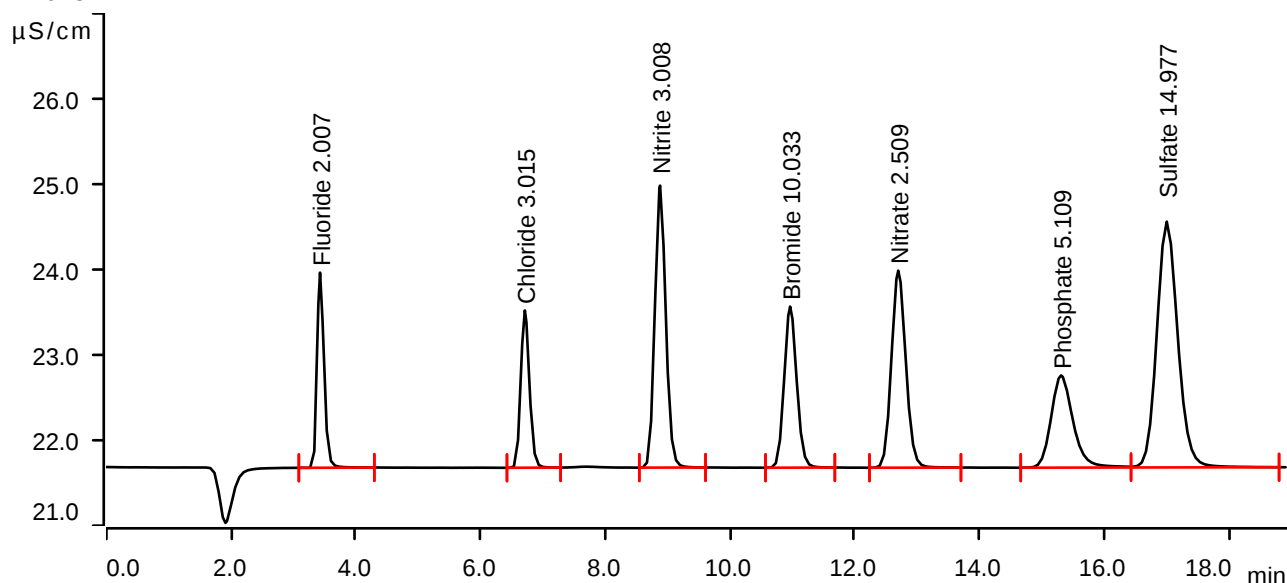

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.427	0.2947	2.286	2.007	Fluoride
2	6.710	0.2963	1.842	3.015	Chloride
3	8.878	0.6708	3.303	3.008	Nitrite
4	10.963	0.4390	1.887	10.033	Bromide
5	12.697	0.6142	2.308	2.509	Nitrate
6	15.307	0.4405	1.080	5.109	Phosphate
7	17.002	1.1230	2.879	14.977	Sulfate


Sample data

Ident Q1322-01
Sample type Sample
Determination start 2025-02-07 12:33:27 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.20 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

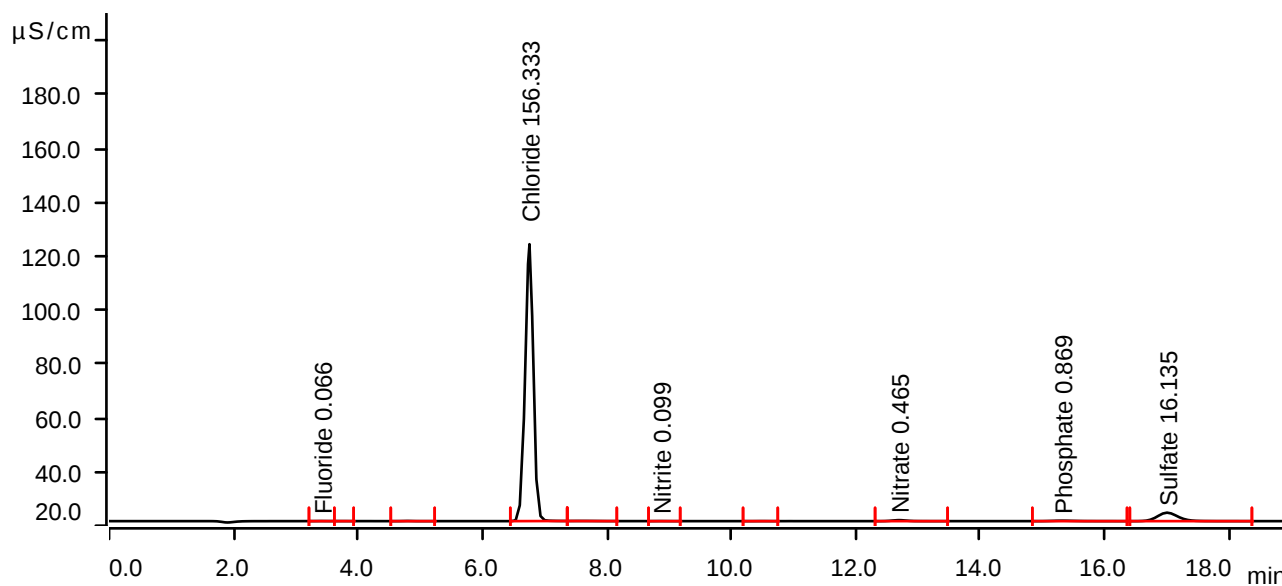

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.422	0.0058	0.034	0.066	Fluoride
2	3.748	0.0031	0.017	invalid	
3	4.795	0.0118	0.068	invalid	
4	6.757	15.5978	102.723	156.333	Chloride
5	7.595	0.0114	0.032	invalid	
6	8.865	0.0047	0.024	0.099	Nitrite
7	10.478	0.0038	0.017	invalid	
8	12.693	0.1012	0.373	0.465	Nitrate
9	15.317	0.0713	0.167	0.869	Phosphate
10	17.002	1.2122	3.141	16.135	Sulfate


Sample data

Ident Q1322-01MS
Sample type Sample
Determination start 2025-02-07 12:55:01 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.20 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

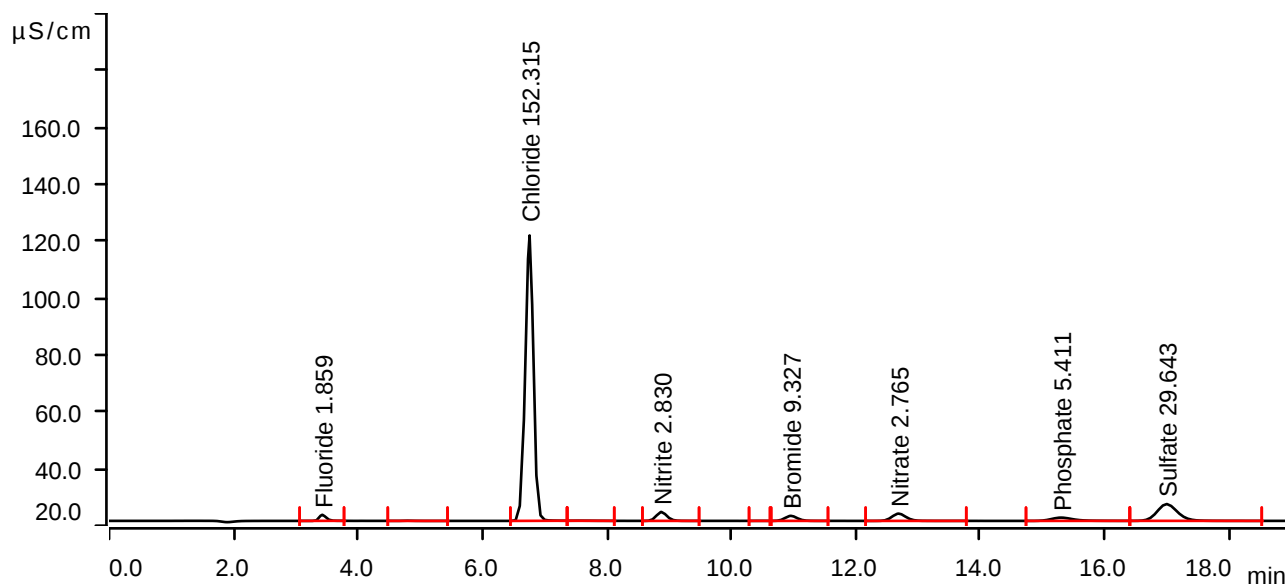

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.428	0.2727	2.141	1.859	Fluoride
2	4.797	0.0118	0.068	invalid	
3	6.758	15.1968	100.293	152.315	Chloride
4	7.590	0.0113	0.032	invalid	
5	8.877	0.6300	3.130	2.830	Nitrite
6	10.478	0.0022	0.012	invalid	
7	10.957	0.4075	1.768	9.327	Bromide
8	12.688	0.6784	2.555	2.765	Nitrate
9	15.300	0.4668	1.148	5.411	Phosphate
10	16.995	2.2530	5.891	29.643	Sulfate


Sample data

Ident Q1322-01MSD
Sample type Sample
Determination start 2025-02-07 13:16:35 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.15 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

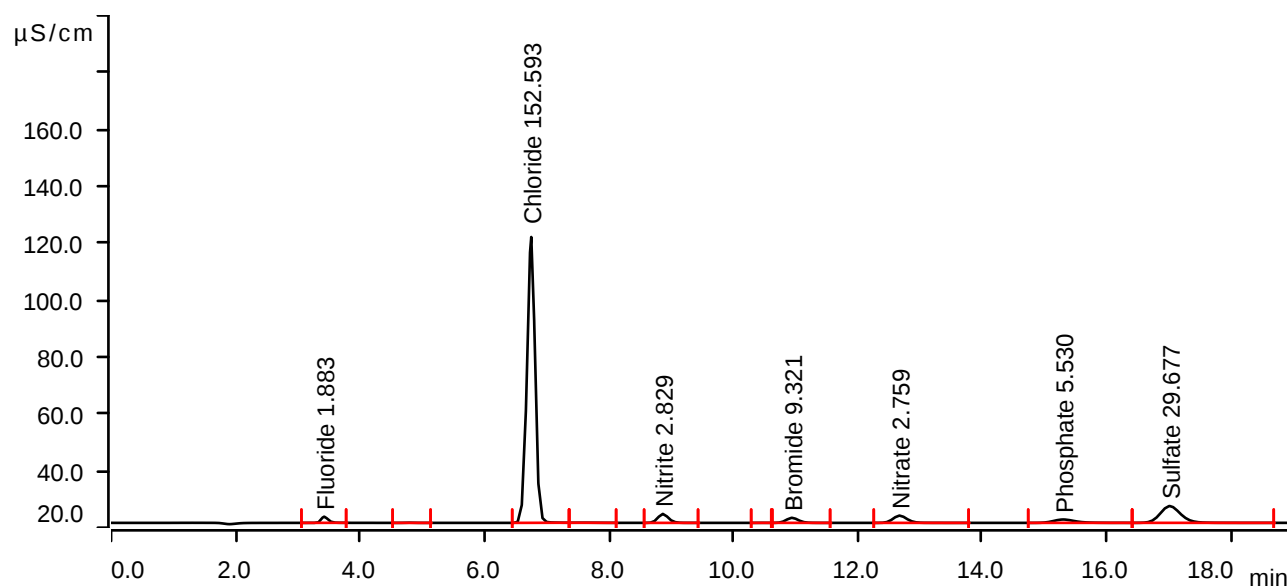

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.427	0.2763	2.166	1.883	Fluoride
2	4.795	0.0114	0.067	invalid	
3	6.753	15.2246	100.443	152.593	Chloride
4	7.588	0.0113	0.032	invalid	
5	8.868	0.6298	3.133	2.829	Nitrite
6	10.472	0.0020	0.012	invalid	
7	10.943	0.4072	1.769	9.321	Bromide
8	12.672	0.6769	2.552	2.759	Nitrate
9	15.300	0.4771	1.184	5.530	Phosphate
10	17.013	2.2557	5.898	29.677	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-02-07 13:38:09 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.09 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

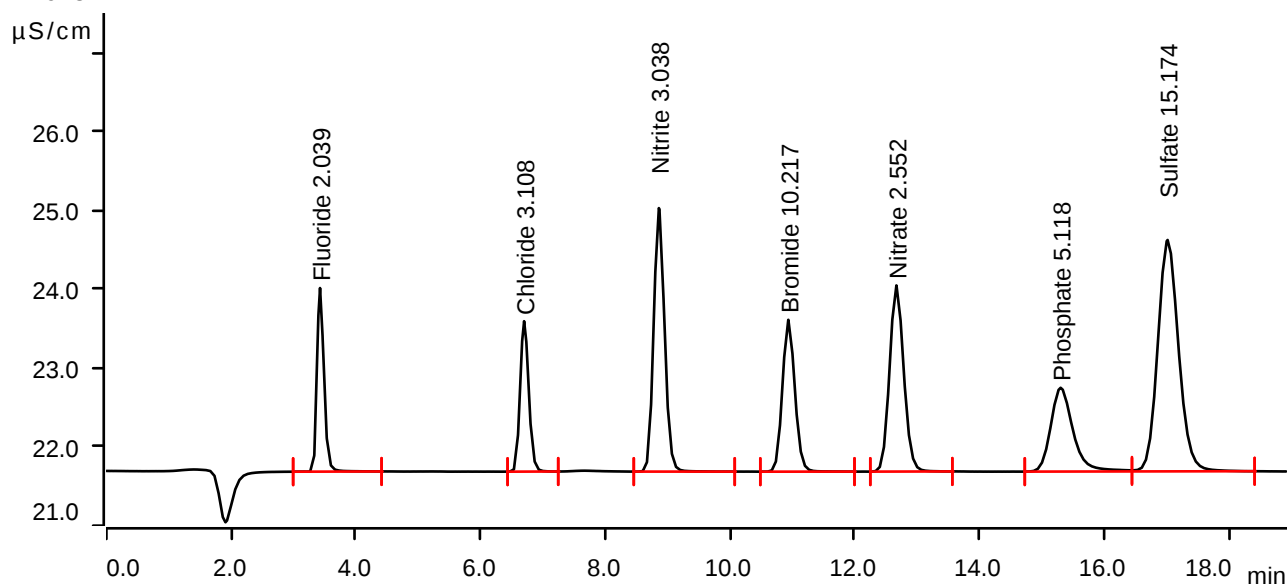

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.427	0.2995	2.330	2.039	Fluoride
2	6.698	0.3056	1.909	3.108	Chloride
3	8.858	0.6777	3.344	3.038	Nitrite
4	10.935	0.4472	1.927	10.217	Bromide
5	12.667	0.6248	2.362	2.552	Nitrate
6	15.300	0.4413	1.063	5.118	Phosphate
7	17.015	1.1382	2.937	15.174	Sulfate


Sample data

Ident CCB
 Sample type Sample
 Determination start 2025-02-07 15:41:13 UTC-5
 Method IC1-012025
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.94 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

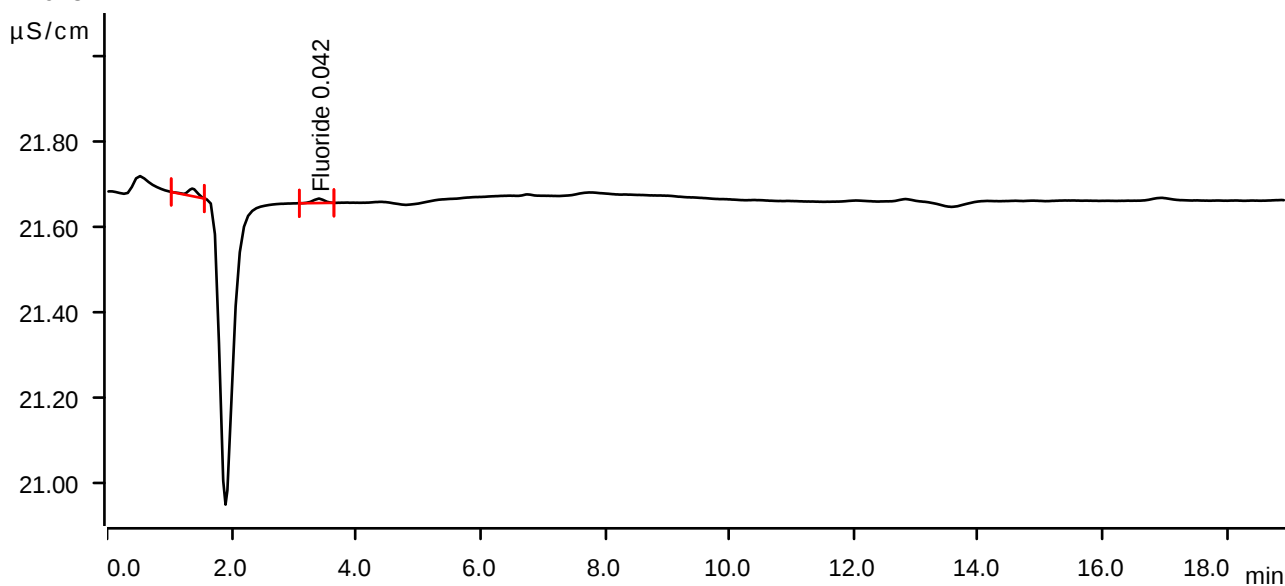

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.370	0.0031	0.018	invalid	
2	3.410	0.0022	0.010	0.042	Fluoride