


Instrument II			IC-1		Analyst :		NF		Method: .00.0 / 9056A			
Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	wt/Fir	Analyst	
STD1	0	0	0	0	0	0	0	IC1-012025	1/20/2025 11:14	10	NF/IZ	
STD2	0.396	0.602	0.613	2.019	0.511	0.994	3.09	IC1-012025	1/20/2025 11:36	10	NF/IZ	
STD3	0.835	1.258	1.254	4.184	1.047	2.089	6.324	IC1-012025	1/20/2025 11:57	10	NF/IZ	
STD4	0.967	1.463	1.466	4.879	1.221	2.469	7.299	IC1-012025	1/20/2025 12:18	10	NF/IZ	
STD5	1.996	2.973	2.959	9.912	2.468	4.936	14.741	IC1-012025	1/20/2025 12:40	10	NF/IZ	
STD6	4.016	5.977	5.973	19.887	4.964	9.97	29.788	IC1-012025	1/20/2025 13:01	10	NF/IZ	
STD7	4.99	7.527	7.535	25.119	6.289	12.542	37.258	IC1-012025	1/20/2025 13:23	10	NF/IZ	
ICV	2.059	3.086	3.062	10.267	2.569	5.158	15.361	IC1-012025	1/20/2025 13:44	10	NF/IZ	
ICB	0	0	0	0	0	0	0	IC1-012025	1/20/2025 14:06	10	NF/IZ	
CCV	2.022	3.038	3.027	10.116	2.536	4.999	15.036	IC1-012025	2/11/2025 11:07	10	NF/IZ	
CCB	0	0	0	0	0	0	0	IC1-012025	2/11/2025 11:29	10	NF/IZ	
LB134705BLW	0	0	0	0	0	0	0	IC1-012025	2/11/2025 11:50	10	NF/IZ	
LB134705BSW	2.031	3.065	3.051	10.198	2.553	5.035	15.104	IC1-012025	2/11/2025 12:12	10	NF/IZ	
Q1355-01	0.29	335.648	0	0.56	0	0	103.314	IC1-012025	2/11/2025 14:49	10	NF/IZ	
Q1355-01MS	1.071	322.702	2.87	9.952	2.405	0.567	115.268	IC1-012025	2/11/2025 15:10	10	NF/IZ	
Q1355-01MSD	2.203	322.879	2.839	9.846	2.365	2.653	115.013	IC1-012025	2/11/2025 15:32	10	NF/IZ	
Q1355-01DLX5	0.08	53.651	0	0.279	0	0	18.384	IC1-012025	2/11/2025 15:54	10	NF/IZ	
CCV	2.035	3.063	3.054	10.198	2.554	5.174	15.127	IC1-012025	2/11/2025 16:15	10	NF/IZ	
CCB	0	0.065	0	0	0	0	0	IC1-012025	2/11/2025 16:37	10	NF/IZ	

Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A

ident	concentratio tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0	0	0	0	0	0	0	0 IC1-012025	1/20/2025 11:14	10	NF/IZ
STD2	0.396	0.602	0.613	2.019	0.511	0.994	3.09	IC1-012025	1/20/2025 11:36	10	NF/IZ
STD3	0.835	1.258	1.254	4.184	1.047	2.089	6.324	IC1-012025	1/20/2025 11:57	10	NF/IZ
STD4	0.967	1.463	1.466	4.879	1.221	2.469	7.299	IC1-012025	1/20/2025 12:18	10	NF/IZ
STD5	1.996	2.973	2.959	9.912	2.468	4.936	14.741	IC1-012025	1/20/2025 12:40	10	NF/IZ
STD6	4.016	5.977	5.973	19.887	4.964	9.97	29.788	IC1-012025	1/20/2025 13:01	10	NF/IZ
STD7	4.99	7.527	7.535	25.119	6.289	12.542	37.258	IC1-012025	1/20/2025 13:23	10	NF/IZ
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4				
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000				
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000				
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000				
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000				
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000				
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000				
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000				
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4				
STD1											
STD2	-1.0000	0.3333	2.1667	0.9500	2.2000	-0.6000	3.0000				
STD3	4.3750	4.8333	4.5000	4.6000	4.7000	4.4500	5.4000				
STD4	-3.3000	-2.4667	-2.2667	-2.4200	-2.3200	-1.2400	-2.6800				
STD5	-0.2000	-0.9000	-1.3667	-0.8800	-1.2800	-1.2800	-1.7267				
STD6	0.4000	-0.3833	-0.4500	-0.5650	-0.7200	-0.3000	-0.7067				
STD7	-0.2000	0.3600	0.4667	0.4760	0.6240	0.3360	0.6973				

Fluoride (Anions)

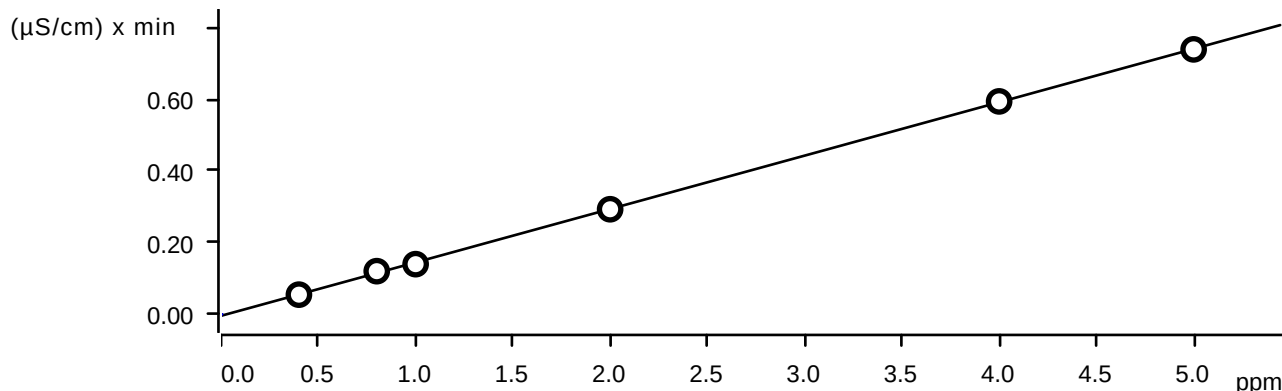


Function: $A = -4.02271E-3 + 0.0148839 \times Q$

Relative standard deviation 1.203859 %

Correlation coefficient 0.999923

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.400	10.0	1.0	1.0	0.055	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	0.800	10.0	1.0	1.0	0.120	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.000	10.0	1.0	1.0	0.140	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	2.000	10.0	1.0	1.0	0.293	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	4.000	10.0	1.0	1.0	0.594	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	5.000	10.0	1.0	1.0	0.739	STD7	2025-01-20 13:23:08 UTC-5	used

Chloride (Anions)

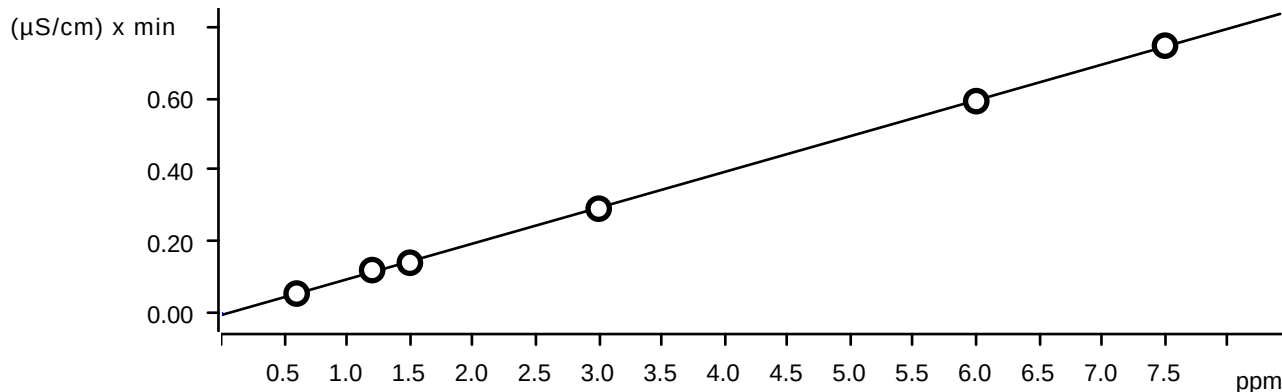

Function: $A = -4.62538E-3 + 9.98029E-3 \times Q$


Relative standard deviation 1.261416 %

Correlation coefficient 0.999916

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.055	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.121	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.141	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.292	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	0.592	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	0.747	STD7	2025-01-20 13:23:08 UTC-5	used

Nitrite (Anions)

($\mu\text{S/cm}$) $\times$ min

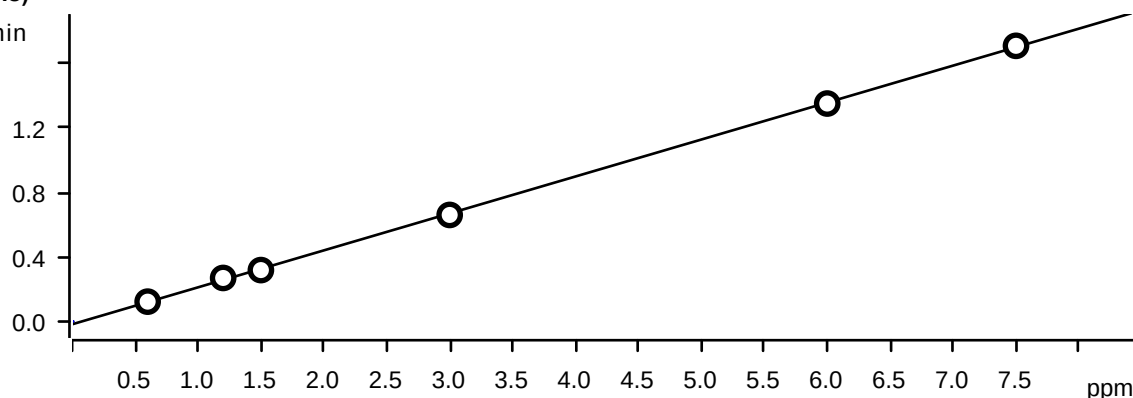


Function: $A = -0.0179856 + 0.0228967 \times Q$

Relative standard deviation 1.369596 %

Correlation coefficient 0.999903

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.122	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.269	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.660	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	1.350	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	1.707	STD7	2025-01-20 13:23:08 UTC-5	used

Bromide (Anions)

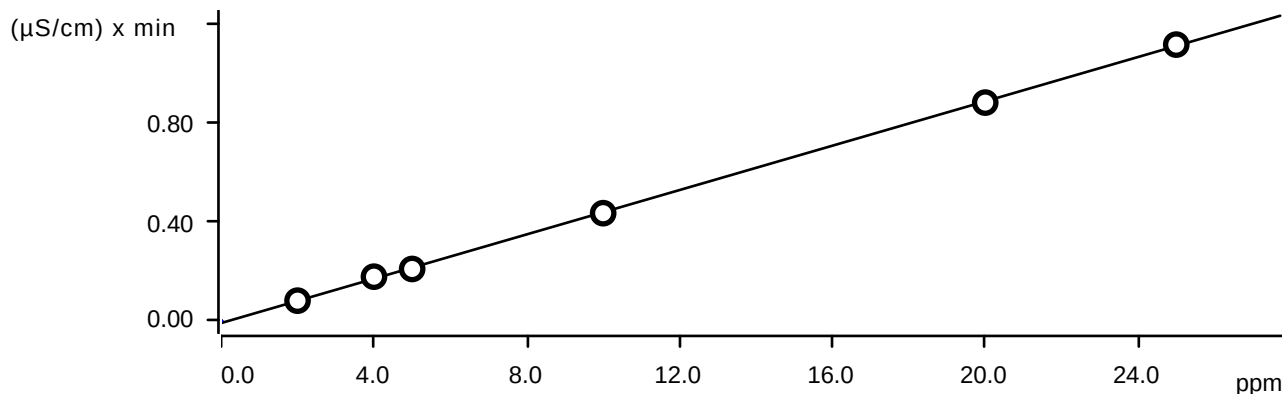


Function: $A = -8.89651E-3 + 4.46429E-3 \times Q$

Relative standard deviation 1.338167 %

Correlation coefficient 0.999906

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	2.000	10.0	1.0	1.0	0.081	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	4.000	10.0	1.0	1.0	0.178	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	5.000	10.0	1.0	1.0	0.209	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	10.000	10.0	1.0	1.0	0.434	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	20.000	10.0	1.0	1.0	0.879	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	25.000	10.0	1.0	1.0	1.112	STD7	2025-01-20 13:23:08 UTC-5	used

Nitrate (Anions)

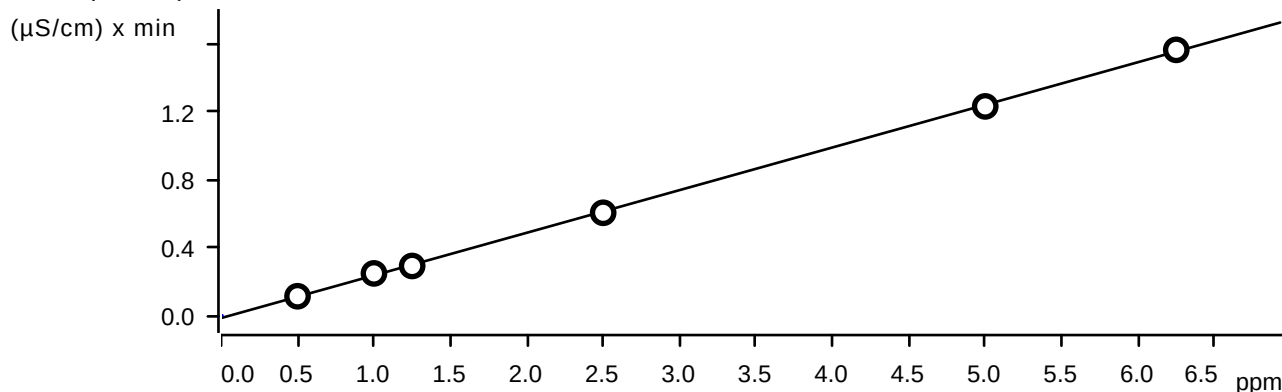


Function: $A = -0.0155875 + 0.0250988 \times Q$

Relative standard deviation 1.561944 %

Correlation coefficient 0.999873


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.500	10.0	1.0	1.0	0.113	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	1.000	10.0	1.0	1.0	0.247	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.250	10.0	1.0	1.0	0.291	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	2.500	10.0	1.0	1.0	0.604	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	5.000	10.0	1.0	1.0	1.230	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	6.250	10.0	1.0	1.0	1.563	STD7	2025-01-20 13:23:08 UTC-5	used

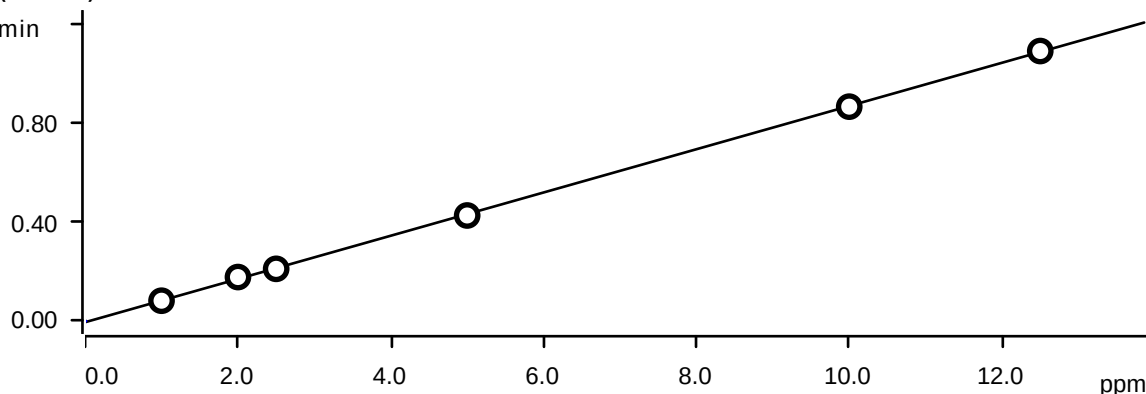Phosphate (Anions) $(\mu\text{S/cm}) \times \text{min}$ Function: $A = -4.38887E-3 + 8.70711E-3 \times Q$

Relative standard deviation 1.148005 %

Correlation coefficient 0.999929

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	1.000	10.0	1.0	1.0	0.082	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	2.000	10.0	1.0	1.0	0.177	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	2.500	10.0	1.0	1.0	0.211	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	5.000	10.0	1.0	1.0	0.425	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	10.000	10.0	1.0	1.0	0.864	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-01-20 13:23:08 UTC-5	used

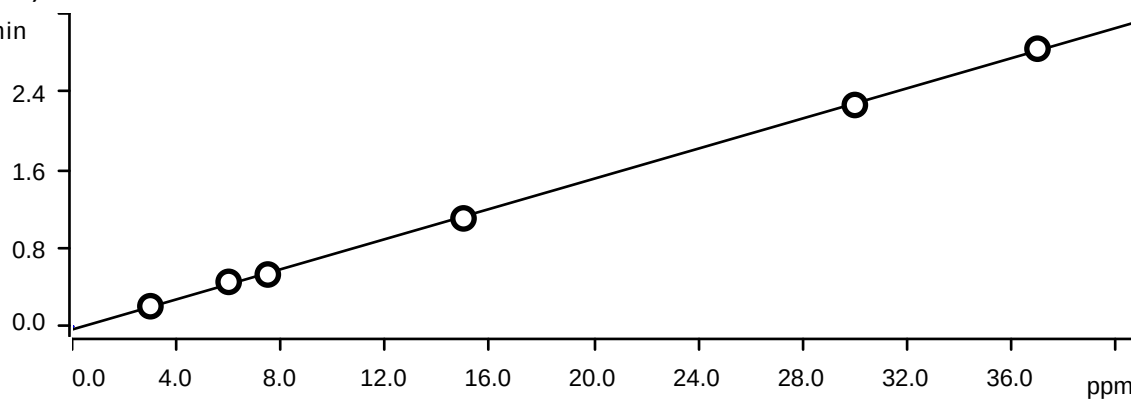Sulfate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0310554 + 7.70543E-3 \times Q$

Relative standard deviation 1.797524 %

Correlation coefficient 0.999831


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	3.000	10.0	1.0	1.0	0.207	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	6.000	10.0	1.0	1.0	0.456	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	7.500	10.0	1.0	1.0	0.531	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	15.000	10.0	1.0	1.0	1.105	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	30.000	10.0	1.0	1.0	2.264	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	37.000	10.0	1.0	1.0	2.840	STD7	2025-01-20 13:23:08 UTC-5	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-01-20 11:14:39 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

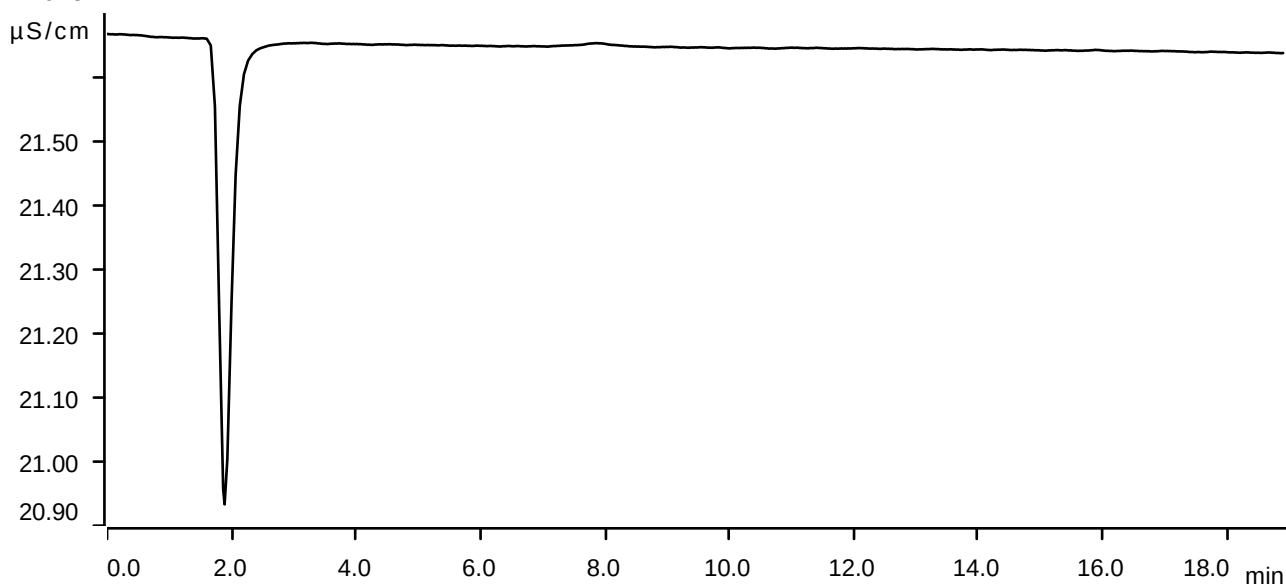Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-01-20 11:36:02 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

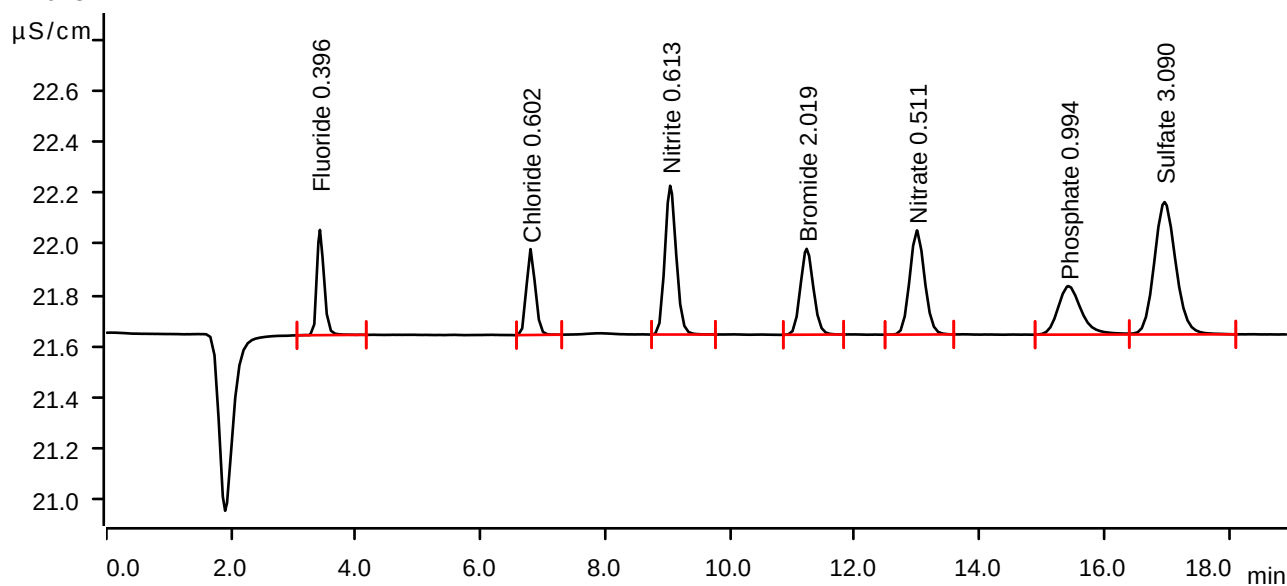

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.425	0.0549	0.411	0.396	Fluoride
2	6.802	0.0555	0.335	0.602	Chloride
3	9.040	0.1223	0.581	0.613	Nitrite
4	11.228	0.0813	0.335	2.019	Bromide
5	12.995	0.1126	0.407	0.511	Nitrate
6	15.423	0.0822	0.190	0.994	Phosphate
7	16.967	0.2070	0.517	3.090	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-01-20 11:57:26 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

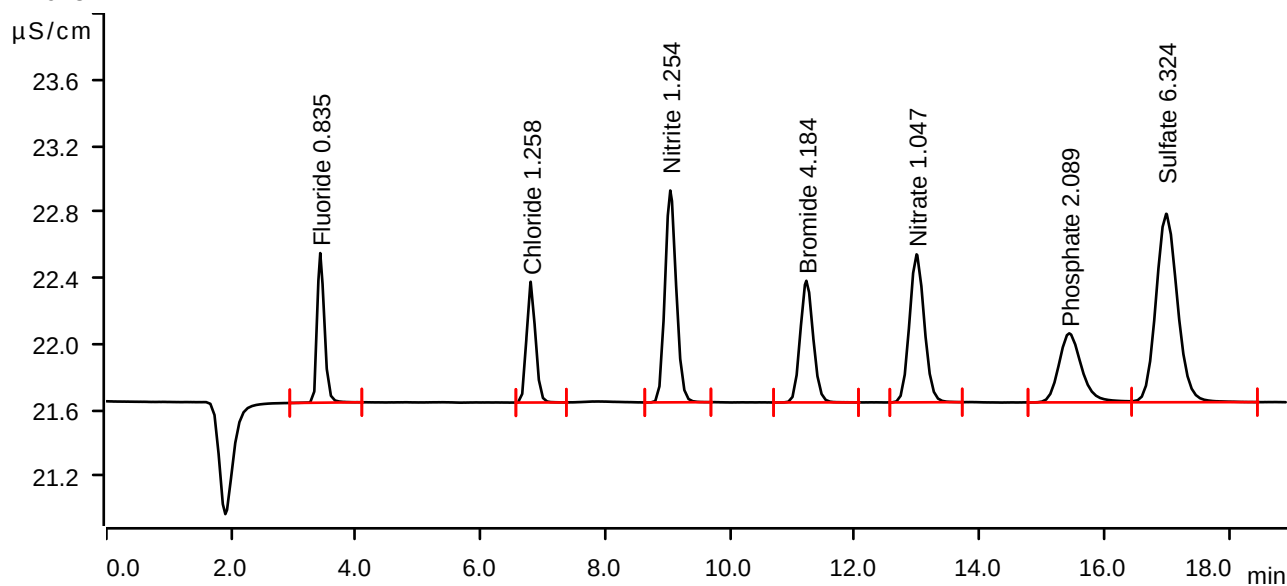

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.1203	0.906	0.835	Fluoride
2	6.803	0.1209	0.731	1.258	Chloride
3	9.042	0.2691	1.282	1.254	Nitrite
4	11.223	0.1779	0.736	4.184	Bromide
5	12.990	0.2472	0.896	1.047	Nitrate
6	15.438	0.1775	0.418	2.089	Phosphate
7	16.992	0.4562	1.141	6.324	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-01-20 12:18:50 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

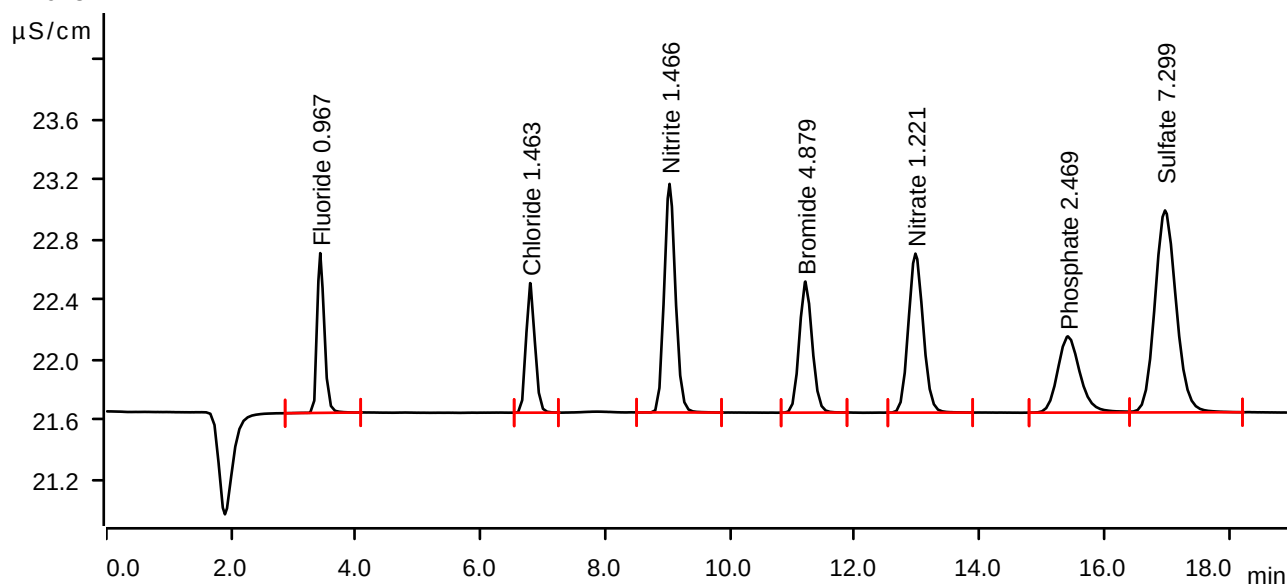

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.1399	1.061	0.967	Fluoride
2	6.795	0.1414	0.860	1.463	Chloride
3	9.030	0.3178	1.517	1.466	Nitrite
4	11.208	0.2089	0.870	4.879	Bromide
5	12.972	0.2908	1.056	1.221	Nitrate
6	15.417	0.2105	0.506	2.469	Phosphate
7	16.973	0.5314	1.341	7.299	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-01-20 12:40:15 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

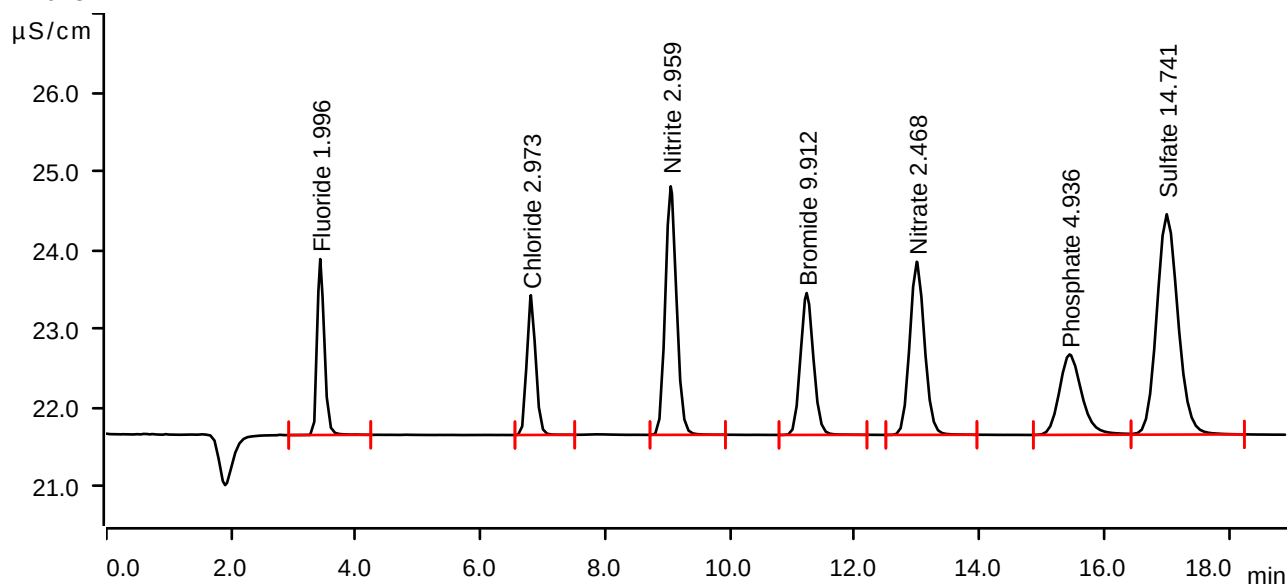

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.2930	2.233	1.996	Fluoride
2	6.807	0.2921	1.773	2.973	Chloride
3	9.048	0.6595	3.154	2.959	Nitrite
4	11.228	0.4336	1.801	9.912	Bromide
5	12.993	0.6039	2.197	2.468	Nitrate
6	15.443	0.4254	1.020	4.936	Phosphate
7	17.002	1.1048	2.795	14.741	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-01-20 13:01:41 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

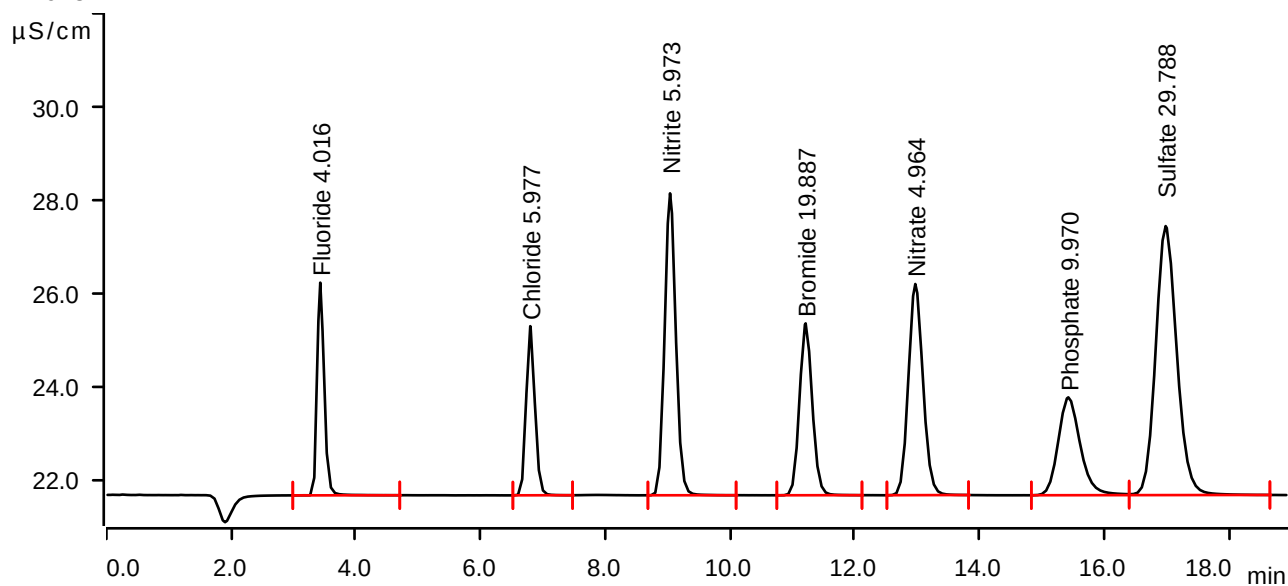

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.5937	4.568	4.016	Fluoride
2	6.797	0.5919	3.633	5.977	Chloride
3	9.038	1.3497	6.484	5.973	Nitrite
4	11.212	0.8789	3.691	19.887	Bromide
5	12.970	1.2302	4.535	4.964	Nitrate
6	15.423	0.8637	2.101	9.970	Phosphate
7	16.983	2.2643	5.777	29.788	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-01-20 13:23:08 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

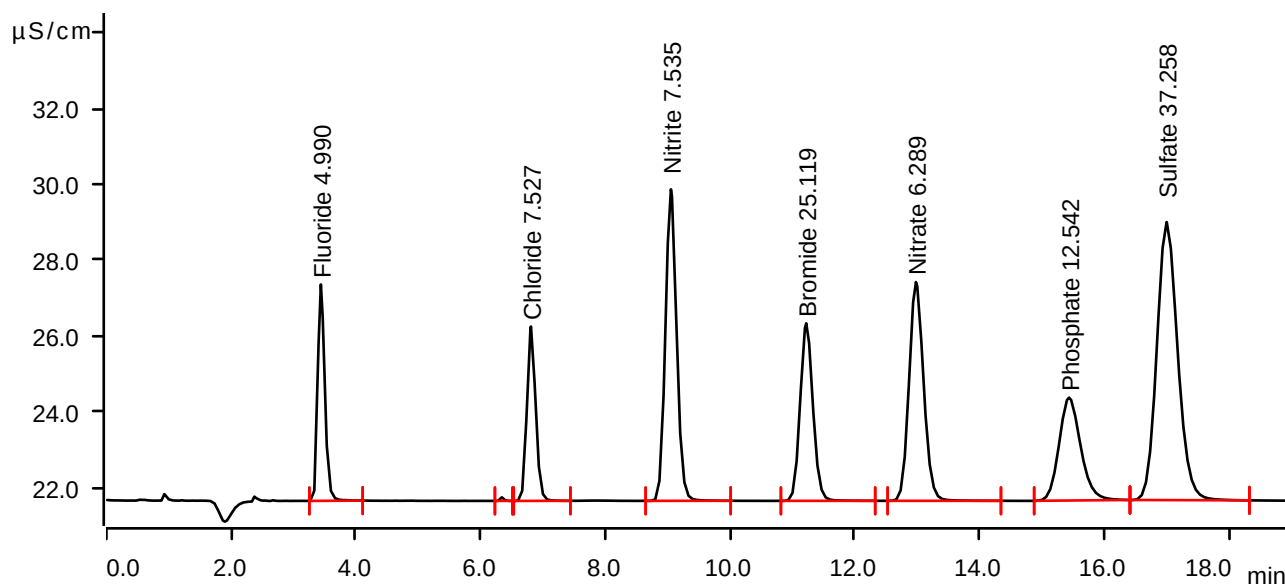

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.440	0.7387	5.703	4.990	Fluoride
2	6.342	0.0051	0.093	invalid	
3	6.808	0.7466	4.595	7.527	Chloride
4	9.052	1.7073	8.209	7.535	Nitrite
5	11.222	1.1125	4.681	25.119	Bromide
6	12.980	1.5629	5.766	6.289	Nitrate
7	15.435	1.0877	2.713	12.542	Phosphate
8	16.998	2.8398	7.327	37.258	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-01-20 13:44:36 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

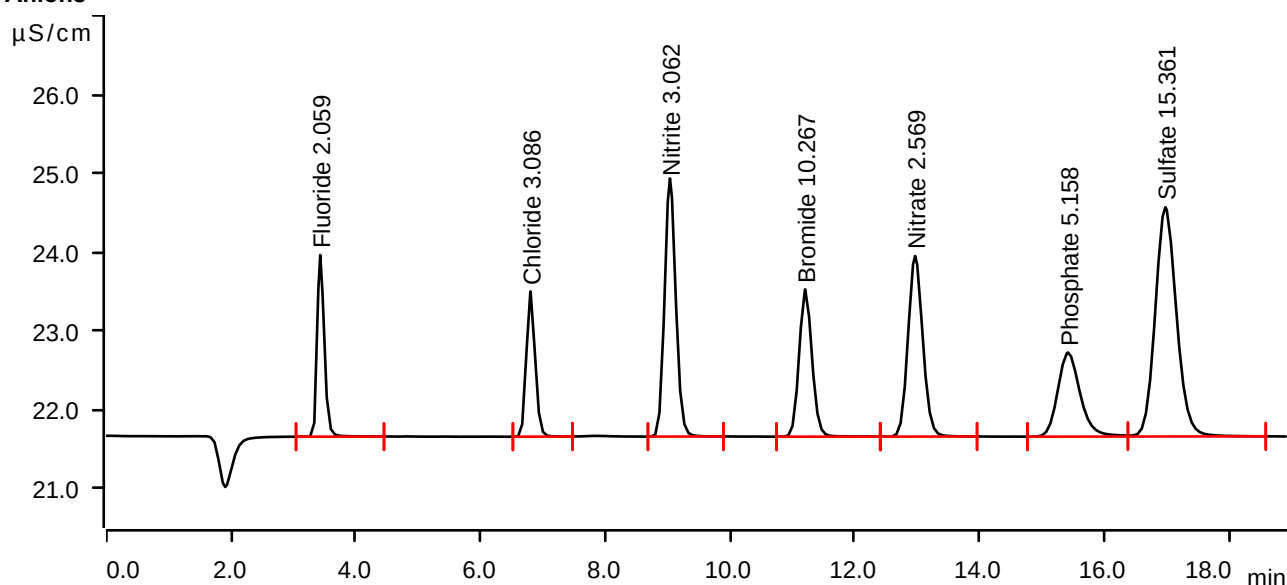

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	3.430	0.3025	2.306	2.059	Fluoride
2	6.798	0.3033	1.843	3.086	Chloride
3	9.037	0.6832	3.276	3.062	Nitrite
4	11.205	0.4495	1.869	10.267	Bromide
5	12.967	0.6293	2.293	2.569	Nitrate
6	15.418	0.4447	1.067	5.158	Phosphate
7	16.978	1.1525	2.909	15.361	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2025-01-20 14:06:05 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

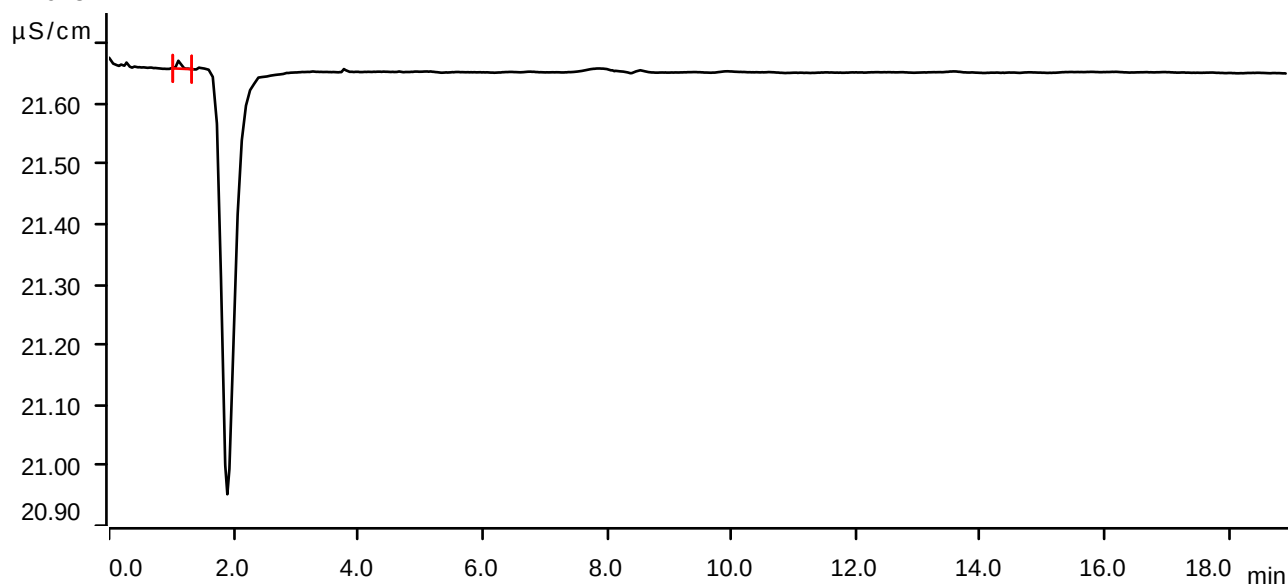

Peak number	Retention time min	Area (μS/cm) x min	Height μS/cm	Concentration ppm	Component name
1	1.115	0.0010	0.013	invalid	


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-02-11 11:07:44 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

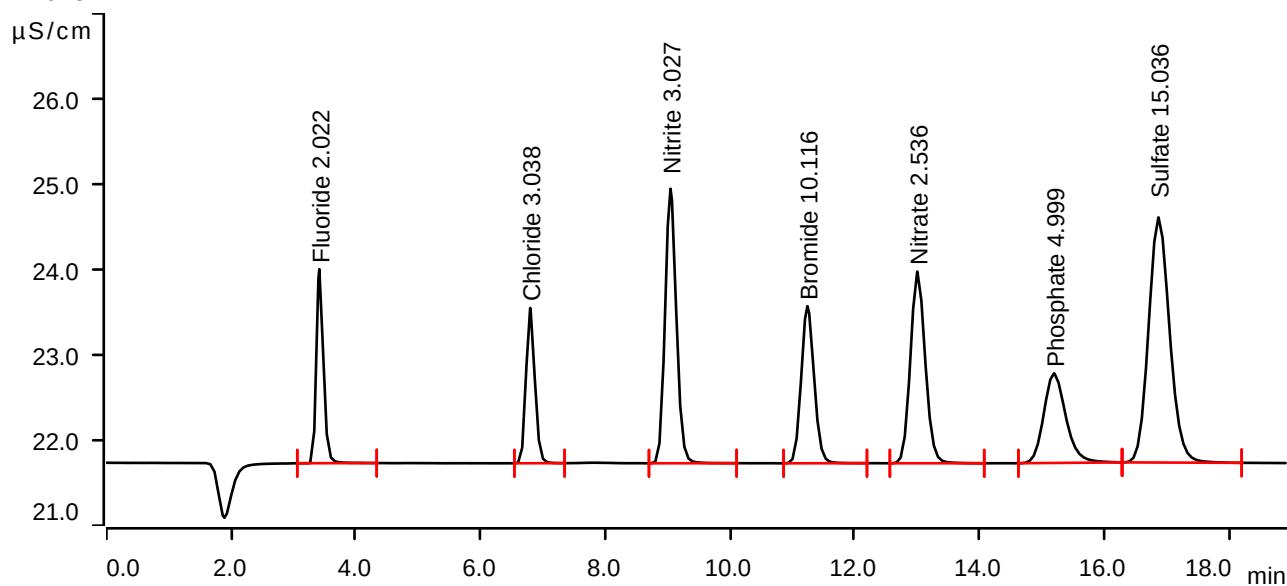


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.415	0.2970	2.273	2.022	Fluoride
2	6.795	0.2986	1.819	3.038	Chloride
3	9.045	0.6750	3.216	3.027	Nitrite
4	11.240	0.4427	1.841	10.116	Bromide
5	13.003	0.6209	2.246	2.536	Nitrate
6	15.193	0.4309	1.049	4.999	Phosphate
7	16.870	1.1275	2.871	15.036	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-02-11 11:29:14 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

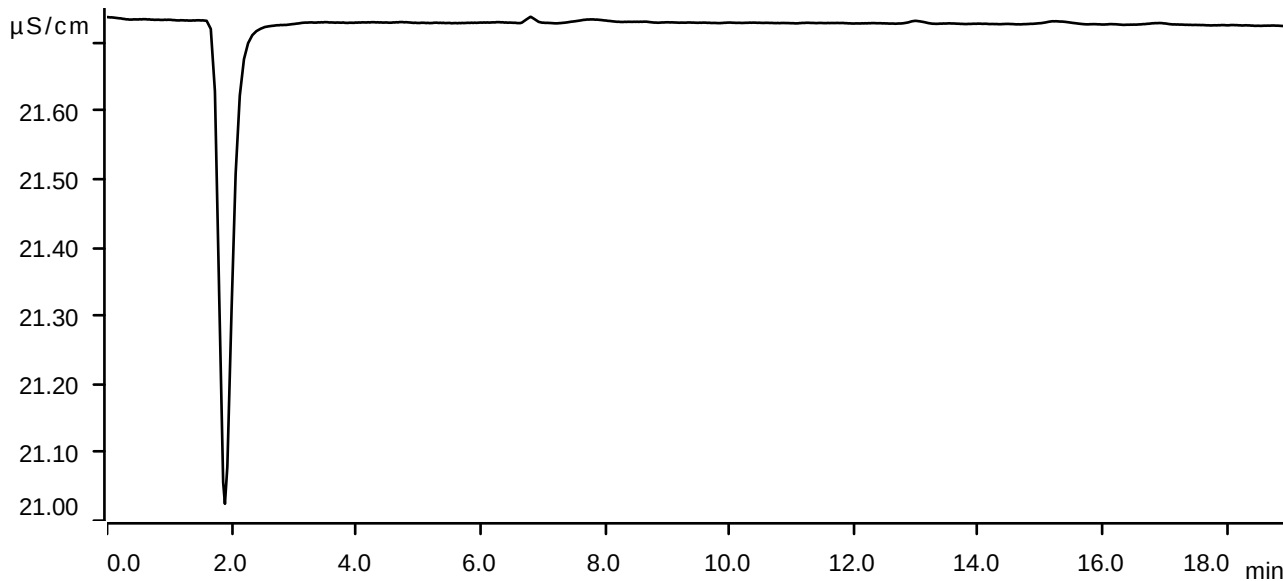
Anions

Sample data

Ident LB134705BLW
Sample type Sample
Determination start 2025-02-11 11:50:45 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

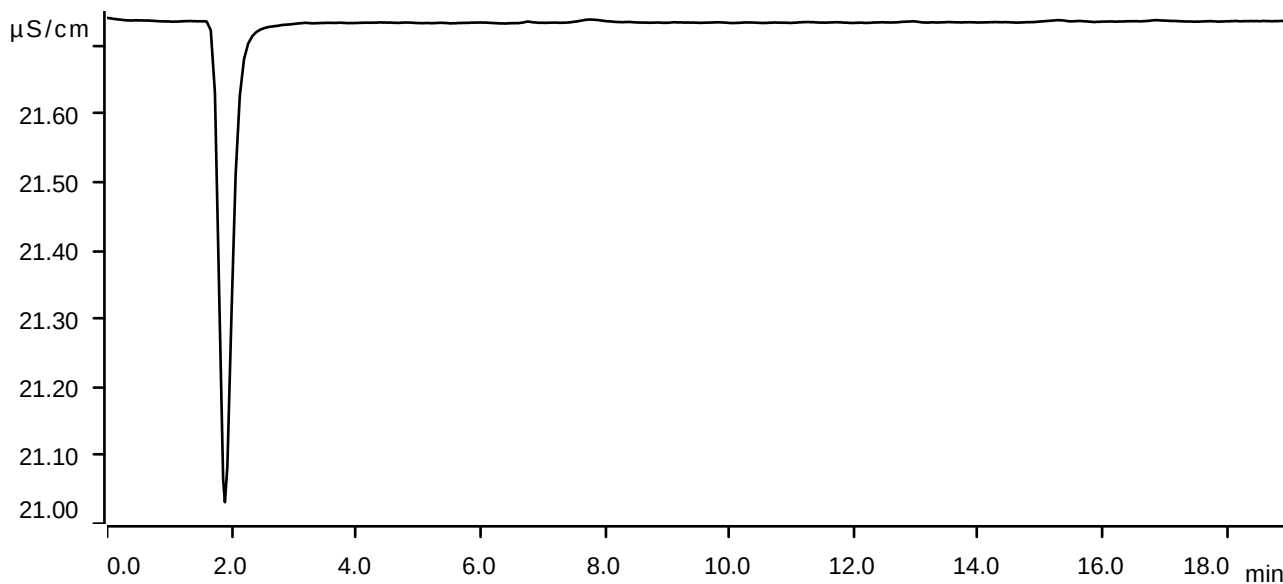Anions


Sample data

Ident LB134705BSW
Sample type Check standard 1
Determination start 2025-02-11 12:12:16 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

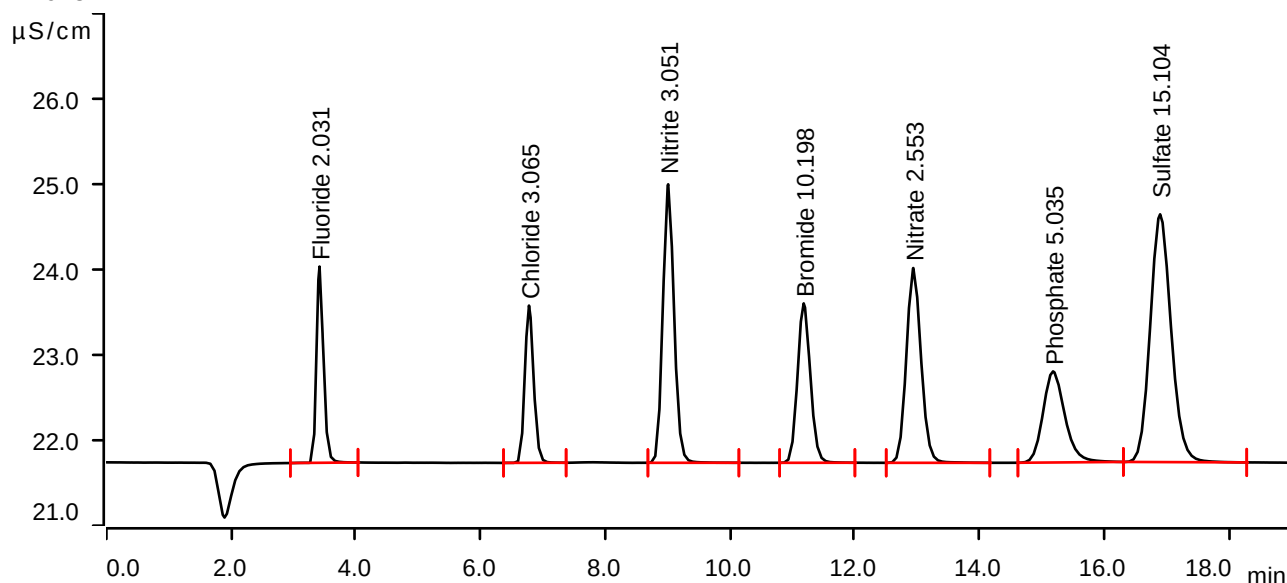

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.418	0.2982	2.299	2.031	Fluoride
2	6.777	0.3013	1.842	3.065	Chloride
3	9.008	0.6807	3.262	3.051	Nitrite
4	11.180	0.4464	1.867	10.198	Bromide
5	12.938	0.6253	2.282	2.553	Nitrate
6	15.178	0.4341	1.067	5.035	Phosphate
7	16.895	1.1328	2.902	15.104	Sulfate


Sample data

Ident Q1355-01
Sample type Sample
Determination start 2025-02-11 14:49:16 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.78 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

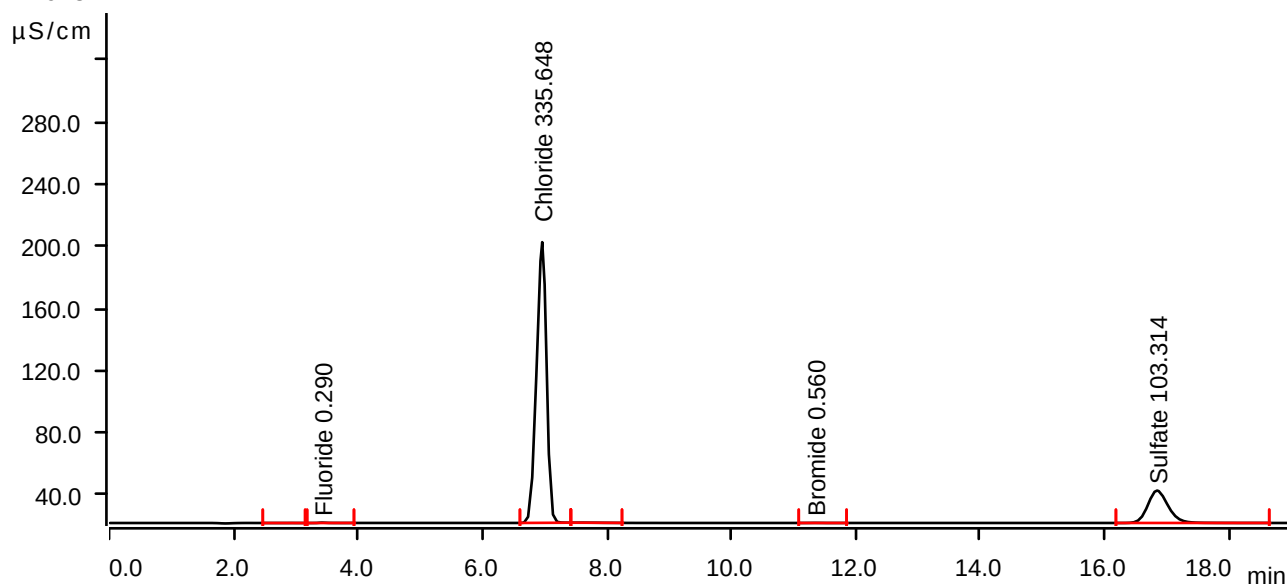

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	2.940	0.0054	0.017	invalid	
2	3.423	0.0391	0.254	0.290	Fluoride
3	6.962	33.4940	180.841	335.648	Chloride
4	7.620	0.0289	0.072	invalid	
5	11.347	0.0161	0.068	0.560	Bromide
6	16.842	7.9298	20.892	103.314	Sulfate


Sample data

Ident Q1355-01MS
Sample type Sample
Determination start 2025-02-11 15:10:54 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.33 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

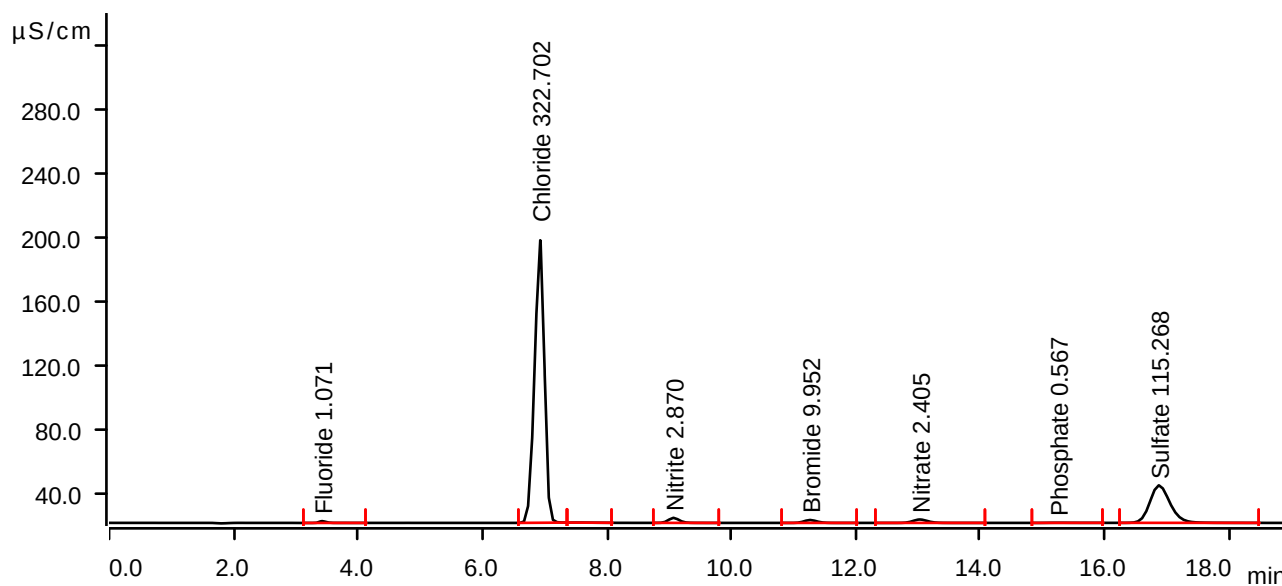

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.425	0.1554	1.137	1.071	Fluoride
2	6.930	32.2020	176.495	322.702	Chloride
3	7.512	0.0206	0.056	invalid	
4	9.072	0.6391	3.138	2.870	Nitrite
5	11.265	0.4354	1.813	9.952	Bromide
6	13.030	0.5879	2.131	2.405	Nitrate
7	15.252	0.0450	0.096	0.567	Phosphate
8	16.872	8.8508	23.415	115.268	Sulfate


Sample data

Ident Q1355-01MSD
Sample type Sample
Determination start 2025-02-11 15:32:28 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

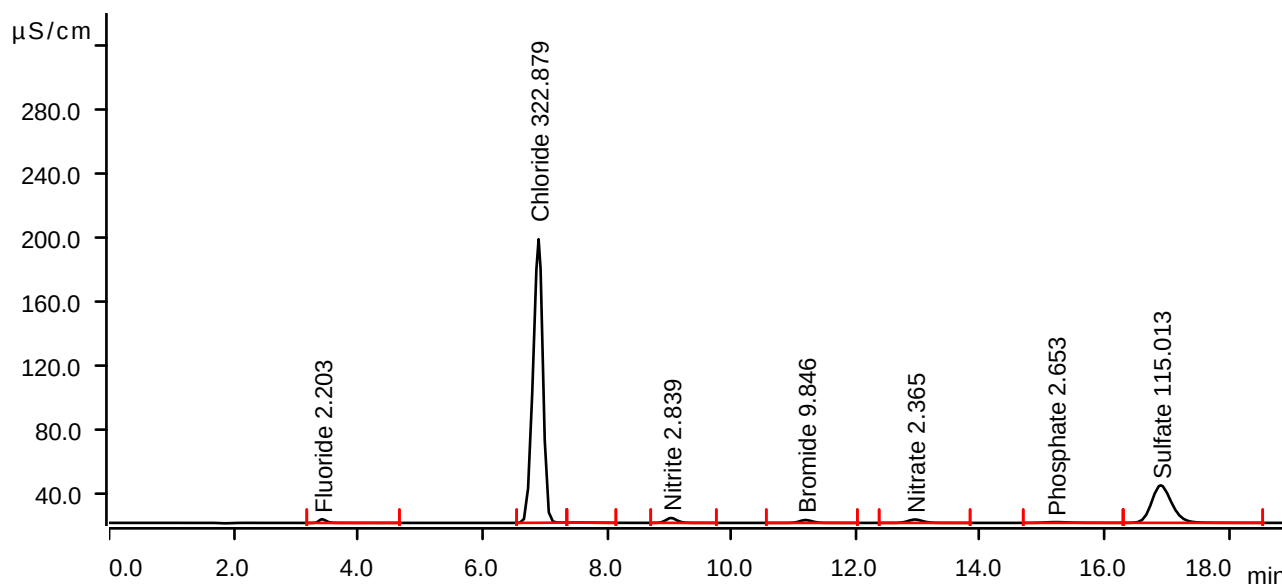

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.425	0.3239	2.356	2.203	Fluoride
2	6.903	32.2196	177.140	322.879	Chloride
3	7.558	0.0273	0.071	invalid	
4	9.032	0.6319	3.075	2.839	Nitrite
5	11.195	0.4307	1.810	9.846	Bromide
6	12.950	0.5779	2.124	2.365	Nitrate
7	15.210	0.2266	0.500	2.653	Phosphate
8	16.900	8.8312	23.472	115.013	Sulfate


Sample data

Ident Q1355-01DLX5
Sample type Sample
Determination start 2025-02-11 15:54:03 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

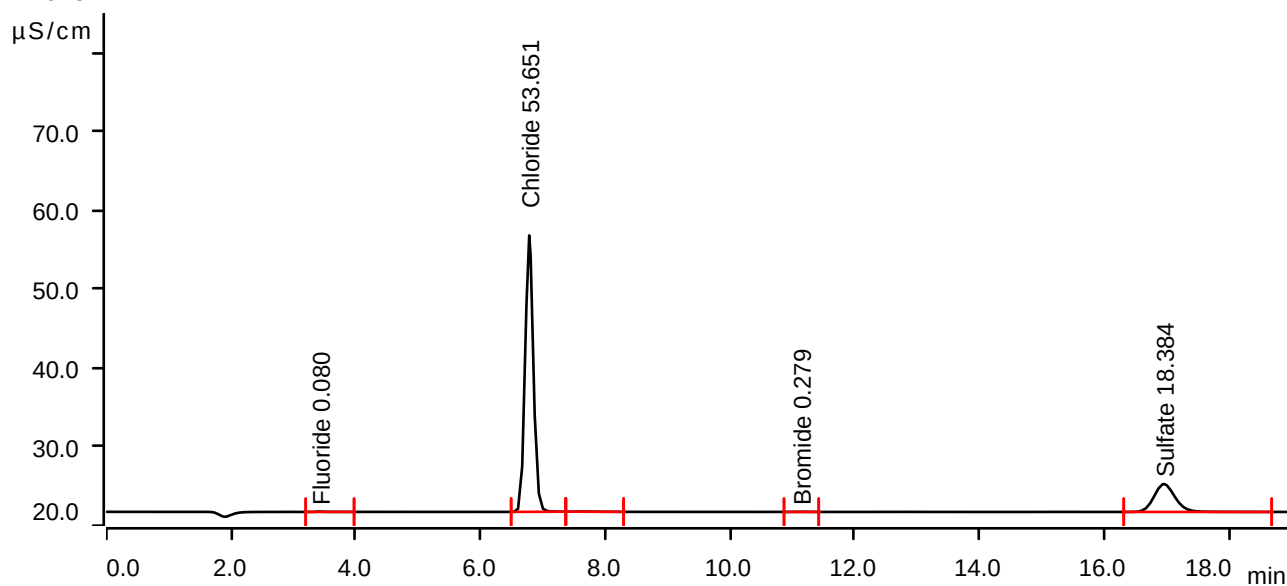

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.422	0.0078	0.051	0.080	Fluoride
2	6.780	5.3499	35.076	53.651	Chloride
3	7.653	0.0107	0.027	invalid	
4	11.132	0.0036	0.015	0.279	Bromide
5	16.955	1.3855	3.546	18.384	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-02-11 16:15:38 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

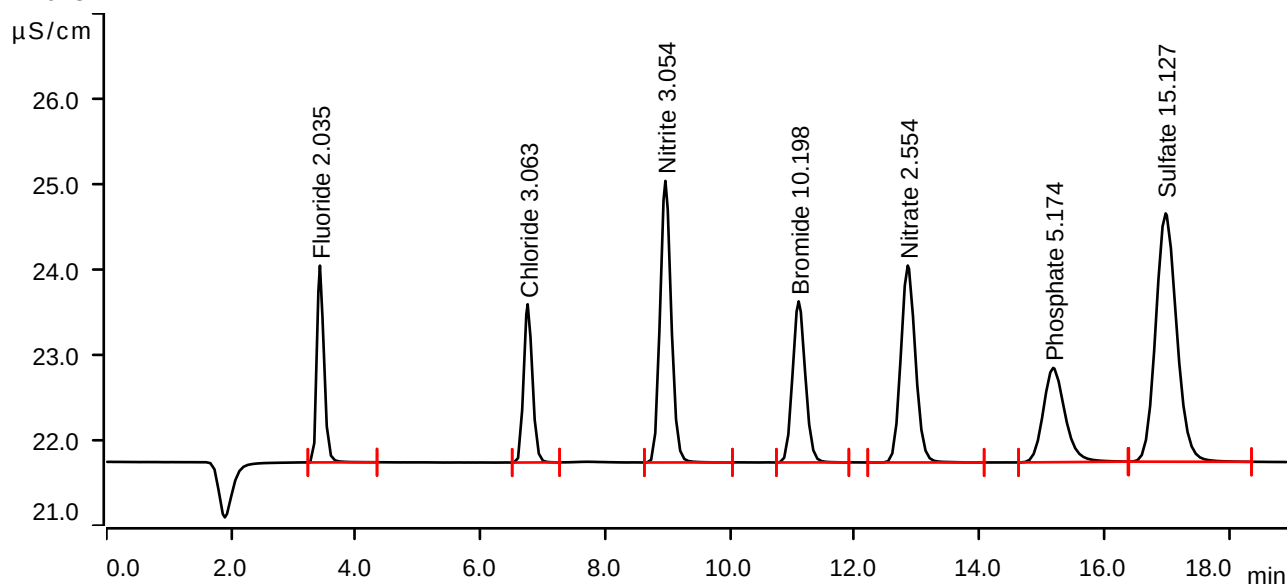

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.425	0.2988	2.305	2.035	Fluoride
2	6.755	0.3011	1.853	3.063	Chloride
3	8.963	0.6813	3.298	3.054	Nitrite
4	11.100	0.4464	1.887	10.198	Bromide
5	12.848	0.6254	2.307	2.554	Nitrate
6	15.180	0.4461	1.104	5.174	Phosphate
7	16.983	1.1346	2.908	15.127	Sulfate


Sample data

Ident CCB
 Sample type Sample
 Determination start 2025-02-11 16:37:09 UTC-5
 Method IC1-012025
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.54 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

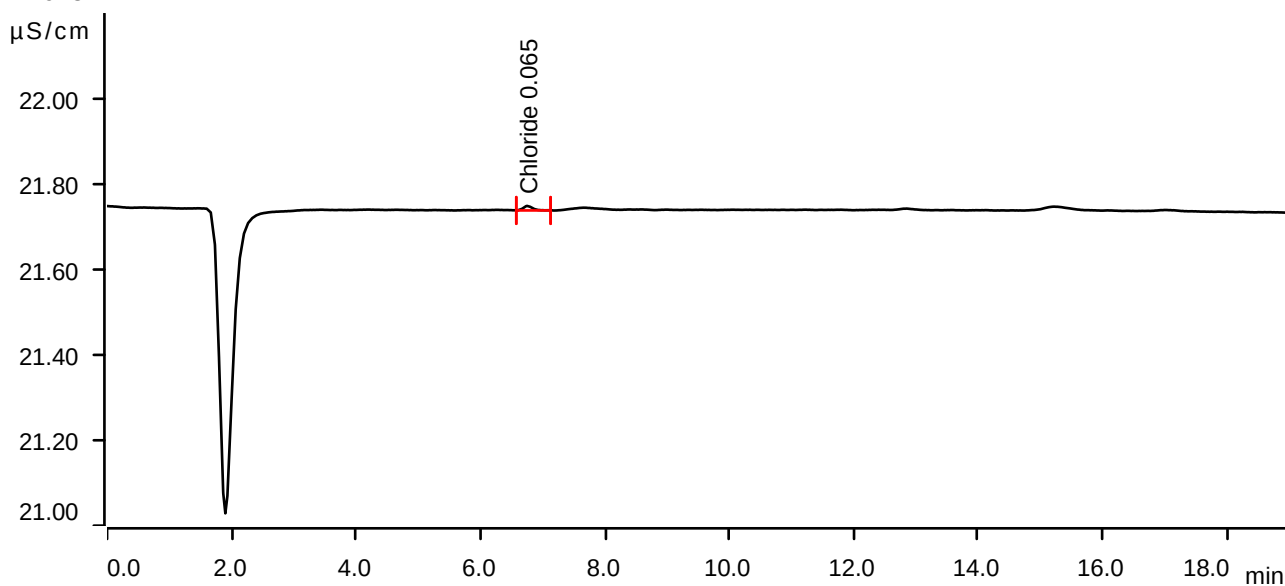

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.752	0.0019	0.011	0.065	Chloride