

LB134793


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

43491

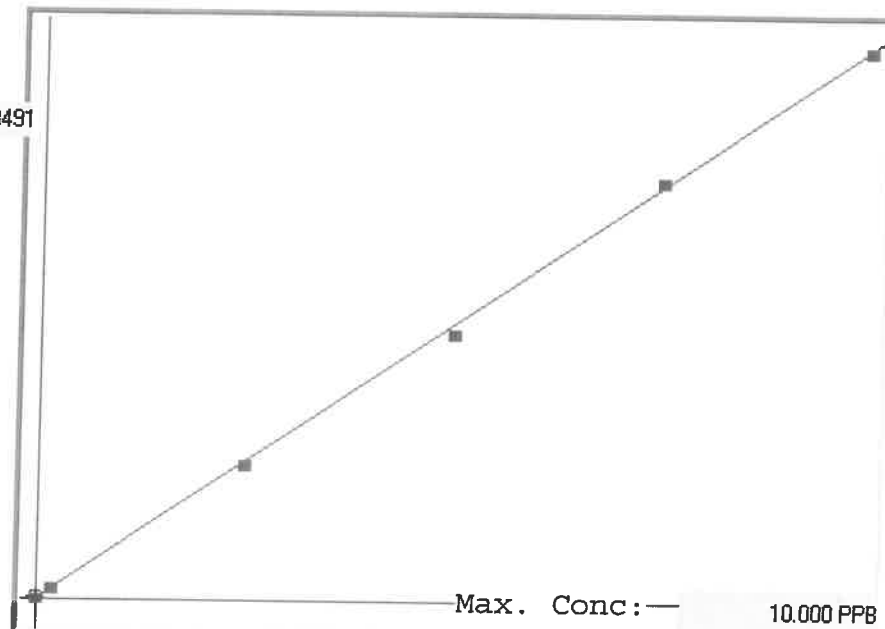

A= 0.0000e+000

B= 2.2964e-004

C= -6.3062e-003

Rho= 0.9997581

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%H
0.0	0.000	0.060	0.060	288	0.000	288					1
0.2	0.200	0.202	0.002	907	0.0 %	907					1
2.5	2.500	2.477	-0.023	10812	0.0 %	10812					1
5.0	5.000	4.858	-0.142	21184	0.0 %	21184					3
7.5	7.500	7.622	0.122	33220	0.0 %	33220					2
10.0	10.000	9.981	-0.019	43491	0.0 %	43491					6

LB134793 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 25 Feb 2025 11:33:22

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	288	-	0.0000	7470A	PPB	25 Feb 2025 11:33:39	S	Std
0.2 - 1	502	907	-	0.2000	7470A	PPB	25 Feb 2025 11:35:57	S	Std
2.5 - 1	52.55	10812	-	2.5000	7470A	PPB	25 Feb 2025 11:38:14	S	Std
5.0 - 1	55	21184	-	5.0000	7470A	PPB	25 Feb 2025 11:40:32	S	Std
7.5 - 1	57.5	33220	-	7.5000	7470A	PPB	25 Feb 2025 11:42:49	S	Std
10.0 - 1	51V	43491	-	10.0000	7470A	PPB	25 Feb 2025 11:45:07	S	Std
ICV16 - 1	ICV16	18952	4.3458	-	7470A	PPB	25 Feb 2025 11:48:00	U	SMPL
ICB16 - 1	ICB16	-28	-0.0127	-	7470A	PPB	25 Feb 2025 11:50:15	U	SMPL
CCV15 - 1	CCV15	21258	4.8754	-	7470A	PPB	25 Feb 2025 11:52:32	U	SMPL
CCB15 - 1	CCB15	-16	-0.0100	-	7470A	PPB	25 Feb 2025 11:54:48	U	SMPL
CRA - 1	CRA	787	0.1744	-	7470A	PPB	25 Feb 2025 11:57:05	U	SMPL
HighStd - 1	HighStd	43659	10.0195	-	7470A	PPB	25 Feb 2025 11:59:20	U	SMPL
ChkStd - 1	ChkStd	30509	6.9998	-	7470A	PPB	25 Feb 2025 12:01:36	U	SMPL
PB166850BL - 1	PBW	81	0.0123	-	7470A	PPB	25 Feb 2025 12:06:47	U	SMPL
PB166850BS - 1	LCSW	20003	4.5872	-	7470A	PPB	25 Feb 2025 12:09:02	U	SMPL
Q1395-02 - 1	BEL-25-0005	-336	-0.0835	-	7470A	PPB	25 Feb 2025 12:11:18	U	SMPL
Q1397-02 - 1	STOCK-PILE	-52	-0.0182	-	7470A	PPB	25 Feb 2025 12:13:37	U	SMPL
Q1397-04 - 1	TP7	-55	-0.0189	-	7470A	PPB	25 Feb 2025 12:15:54	U	SMPL
Q1397-06 - 1	TP8	-46	-0.0169	-	7470A	PPB	25 Feb 2025 12:18:11	U	SMPL
Q1397-06DUP - 1	TP8DUP	-31	-0.0134	-	7470A	PPB	25 Feb 2025 12:20:26	U	SMPL
CCV16 - 1	CCV16	21191	4.8600	-	7470A	PPB	25 Feb 2025 12:22:42	U	SMPL
CCB16 - 1	CCB16	0	-0.0063	-	7470A	PPB	25 Feb 2025 12:24:57	U	SMPL
Q1397-06MS - 1	TP8MS	18318	4.2002	-	7470A	PPB	25 Feb 2025 12:27:14	U	SMPL
Q1397-06MSD - 1	TP8MSD	14909	3.4174	-	7470A	PPB	25 Feb 2025 12:29:29	U	SMPL
PB166824TB - 1	PB166824TB	-277	-0.0699	-	7470A	PPB	25 Feb 2025 12:31:47	U	SMPL
Q1397-06LX5 - 1		8	-0.0045	-	7470A	PPB	25 Feb 2025 12:34:04	U	SMPL
Q1397-06A - 1		19325	4.4315	-	7470A	PPB	25 Feb 2025 12:36:20	U	SMPL
CCV17 - 1	CCV17	23251	5.3330	-	7470A	PPB	25 Feb 2025 13:00:16	U	SMPL
CCB17 - 1	CCB17	-51	-0.0180	-	7470A	PPB	25 Feb 2025 13:02:32	U	SMPL