


Instrument II		IC-1	Analyst:		NF	Method: :00.0 / 9056A		Method name		date time	al wt/Fina	Analyst
Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4					
STD1	0	0	0	0	0	0	0	IC1-022125		2/21/2025 11:05	10	NF/IZ
STD2	0.448	0.678	0.657	2.152	0.544	1.059	3.319	IC1-022125		2/21/2025 11:26	10	NF/IZ
STD3	0.821	1.223	1.216	4.052	1.014	2.009	6.104	IC1-022125		2/21/2025 11:48	10	NF/IZ
STD4	1.013	1.524	1.523	5.08	1.272	2.514	7.612	IC1-022125		2/21/2025 12:09	10	NF/IZ
STD5	1.919	2.879	2.894	9.683	2.411	4.896	14.423	IC1-022125		2/21/2025 12:31	10	NF/IZ
STD6	3.884	5.815	5.898	19.712	4.921	9.947	29.333	IC1-022125		2/21/2025 12:52	10	NF/IZ
STD7	5.115	7.682	7.613	25.321	6.339	12.575	37.71	IC1-022125		2/21/2025 13:13	10	NF/IZ
ICV	2.008	2.989	3.015	10.228	2.532	5.141	15.146	IC1-022125		2/21/2025 13:35	10	NF/IZ
ICB	0	0	0	0	0	0	0	IC1-022125		2/21/2025 13:56	10	NF/IZ
CCV	1.986	2.965	2.984	10.033	2.491	5.046	14.906	IC1-022125		2/27/2025 9:40	10	NF/IZ
CCB	0	0	0	0	0	0	0	IC1-022125		2/27/2025 10:01	10	NF/IZ
LB134838BLW	0	0	0	0	0	0	0	IC1-022125		2/27/2025 10:23	10	NF/IZ
LB134838BSW	1.985	2.961	2.986	10.018	2.499	5.06	14.74	IC1-022125		2/27/2025 10:44	10	NF/IZ
Q1435-01	0.269	525.523	0	0.421	0.843	0	42.45	IC1-022125		2/27/2025 11:06	10	NF/IZ
Q1439-01	0.494	234.169	0	0.562	0.212	0	43.42	IC1-022125		2/27/2025 12:10	10	NF/IZ
Q1439-01MS	2.458	226.024	3.068	10.644	2.717	5.252	57.928	IC1-022125		2/27/2025 12:32	10	NF/IZ
Q1439-01MSD	2.464	226.052	3.065	10.635	2.721	5.261	57.919	IC1-022125		2/27/2025 12:54	10	NF/IZ
CCV	1.956	2.966	3.001	10.048	2.499	4.729	14.895	IC1-022125		2/27/2025 13:15	10	NF/IZ
CCB	0	0	0	0	0	0	0	IC1-022125		2/27/2025 13:37	10	NF/IZ

Clear table


Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A									
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time
STD1	0	0	0	0	0	0	0	IC1-022125	2/21/2025 11:05
STD2	0.448	0.678	0.657	2.152	0.544	1.059	3.319	IC1-022125	2/21/2025 11:26
STD3	0.821	1.223	1.216	4.052	1.014	2.009	6.104	IC1-022125	2/21/2025 11:48
STD4	1.013	1.524	1.523	5.08	1.272	2.514	7.612	IC1-022125	2/21/2025 12:09
STD5	1.919	2.879	2.894	9.683	2.411	4.896	14.423	IC1-022125	2/21/2025 12:31
STD6	3.884	5.815	5.898	19.712	4.921	9.947	29.333	IC1-022125	2/21/2025 12:52
STD7	5.115	7.682	7.613	25.321	6.339	12.575	37.71	IC1-022125	2/21/2025 13:13
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000		
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4	Initial wt/ Final	Analyst
STD1								10	NF/IZ
STD2	12.0000	13.0000	9.5000	7.6000	8.8000	5.9000	10.6333	10	NF/IZ
STD3	2.6250	1.9167	1.3333	1.3000	1.4000	0.4500	1.7333	10	NF/IZ
STD4	1.3000	1.6000	1.5333	1.6000	1.7600	0.5600	1.4933	10	NF/IZ
STD5	-4.0500	-4.0333	-3.5333	-3.1700	-3.5600	-2.0800	-3.8467	10	NF/IZ
STD6	-2.9000	-3.0833	-1.7000	-1.4400	-1.5800	-0.5300	-2.2233	10	NF/IZ
STD7	2.3000	2.4267	1.5067	1.2840	1.4240	0.6000	1.9189	10	NF/IZ

Anions

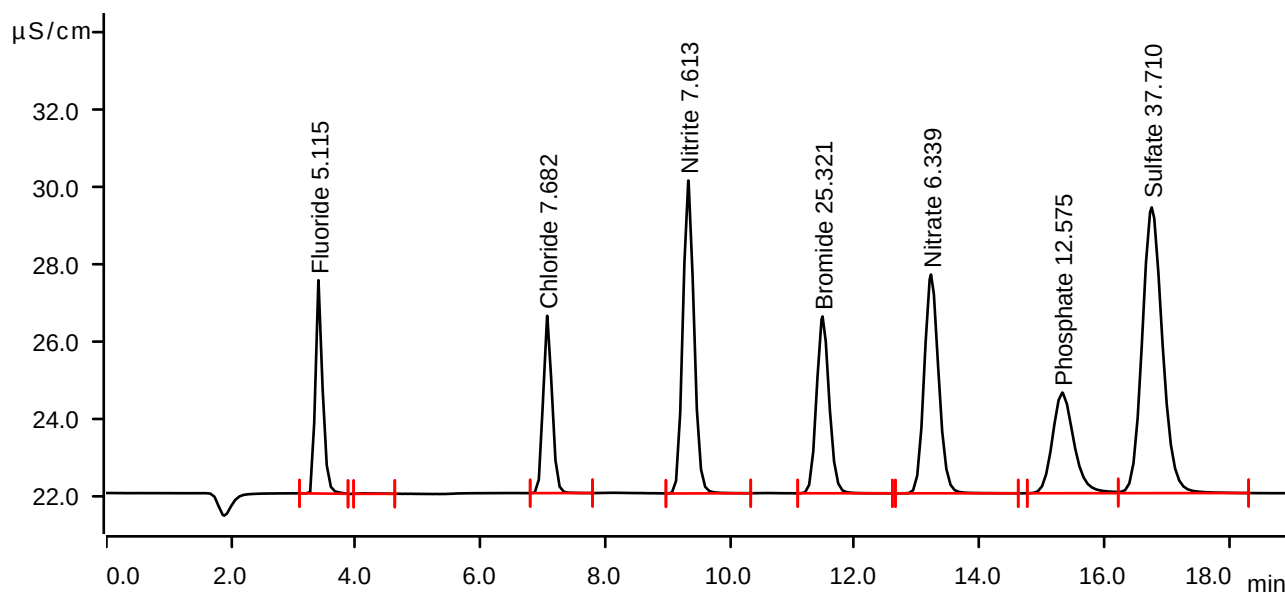

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.400	0.7457	5.535	5.115	Fluoride
2	4.197	0.0046	0.012	invalid	
3	7.070	0.7592	4.602	7.682	Chloride
4	9.330	1.6810	8.120	7.613	Nitrite
5	11.483	1.0784	4.588	25.321	Bromide
6	13.222	1.5233	5.678	6.339	Nitrate
7	15.325	1.0441	2.611	12.575	Phosphate
8	16.760	2.7982	7.416	37.710	Sulfate

Fluoride (Anions)

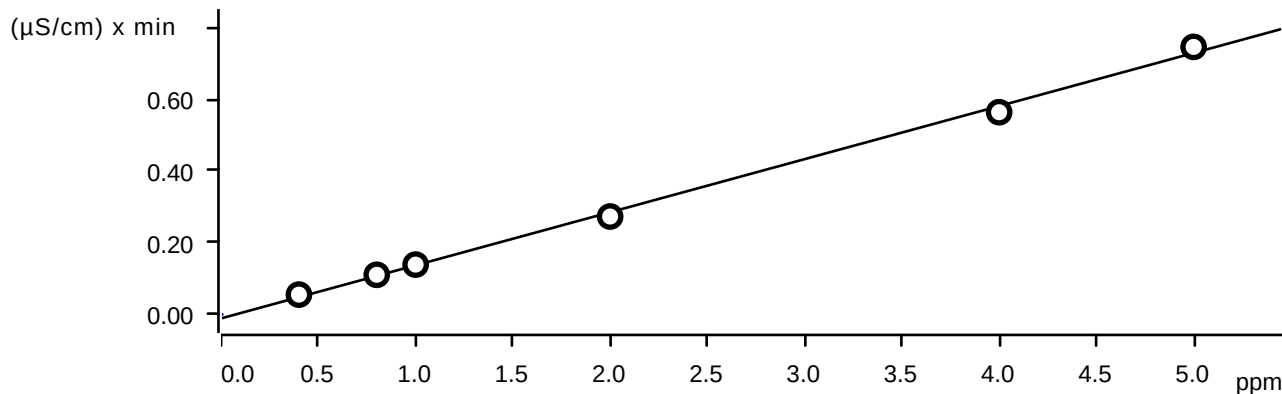


Function: $A = -0.0112463 + 0.0147980 \times Q$

Relative standard deviation 4.464159 %

Correlation coefficient 0.998989

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-02-21 11:05:25 UTC-5	used
Standard 2	1	0.400	10.0	1.0	1.0	0.055	STD2	2025-02-21 11:26:47 UTC-5	used
Standard 3	1	0.800	10.0	1.0	1.0	0.110	STD3	2025-02-21 11:48:11 UTC-5	used
Standard 4	1	1.000	10.0	1.0	1.0	0.139	STD4	2025-02-21 12:09:35 UTC-5	used
Standard 5	1	2.000	10.0	1.0	1.0	0.273	STD5	2025-02-21 12:31:01 UTC-5	used
Standard 6	1	4.000	10.0	1.0	1.0	0.564	STD6	2025-02-21 12:52:27 UTC-5	used
Standard 7	1	5.000	10.0	1.0	1.0	0.746	STD7	2025-02-21 13:13:53 UTC-5	used

Chloride (Anions)

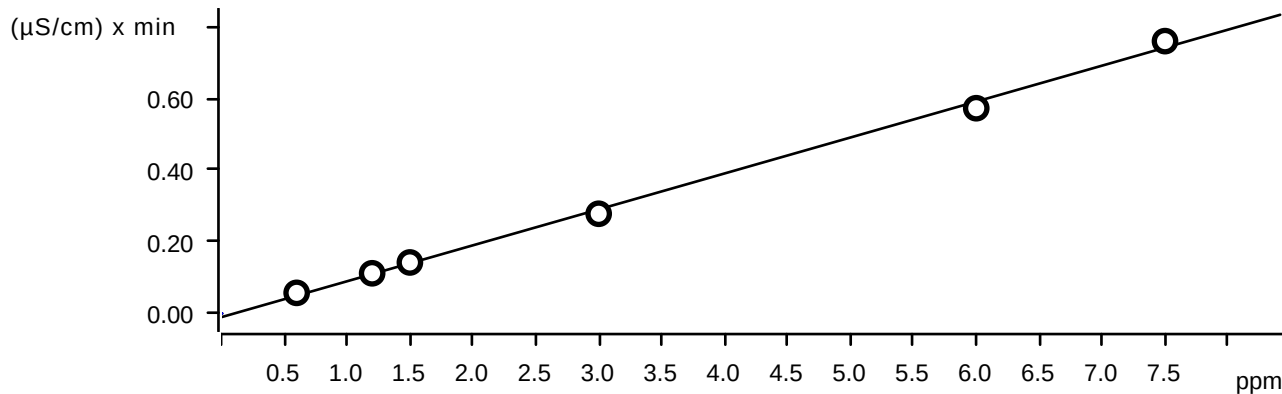

Function: $A = -0.0105167 + 0.0100207 \times Q$


Relative standard deviation 4.669067 %

Correlation coefficient 0.998888

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-02-21 11:05:25 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.057	STD2	2025-02-21 11:26:47 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.112	STD3	2025-02-21 11:48:11 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.142	STD4	2025-02-21 12:09:35 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.278	STD5	2025-02-21 12:31:01 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	0.572	STD6	2025-02-21 12:52:27 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	0.759	STD7	2025-02-21 13:13:53 UTC-5	used

Nitrite (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

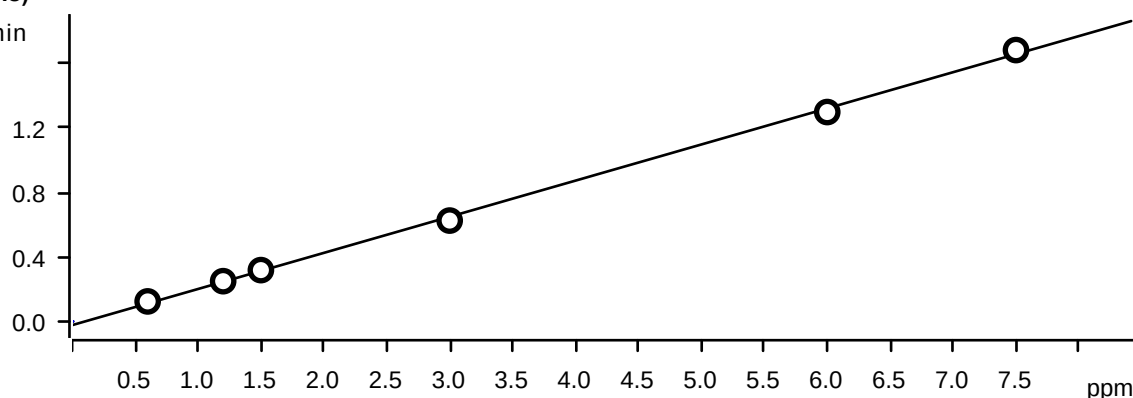


Function: $A = -0.0232250 + 0.0223870 \times Q$

Relative standard deviation 3.068725 %

Correlation coefficient 0.999519

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-02-21 11:05:25 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.124	STD2	2025-02-21 11:26:47 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.249	STD3	2025-02-21 11:48:11 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-02-21 12:09:35 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.625	STD5	2025-02-21 12:31:01 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	1.297	STD6	2025-02-21 12:52:27 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	1.681	STD7	2025-02-21 13:13:53 UTC-5	used

Bromide (Anions)

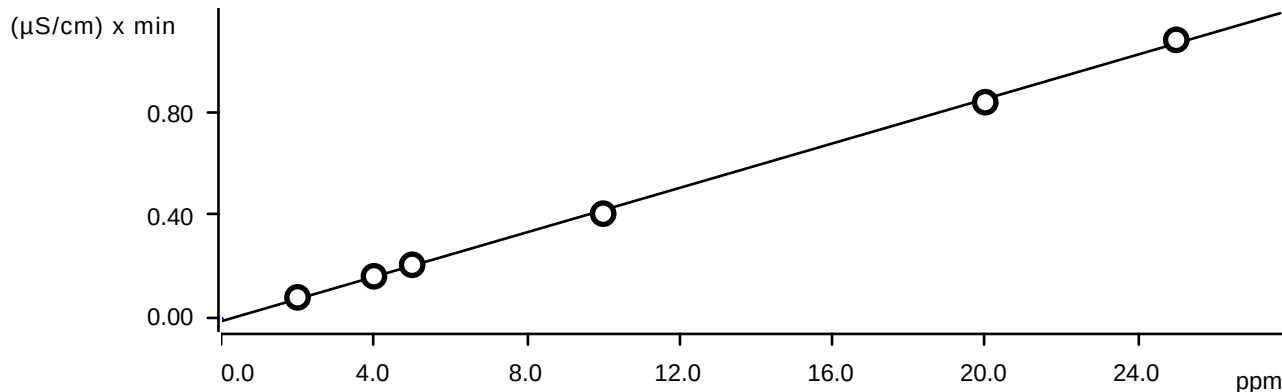


Function: $A = -0.0113202 + 4.30364E-3 \times Q$

Relative standard deviation 2.628989 %

Correlation coefficient 0.999641

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-02-21 11:05:25 UTC-5	used
Standard 2	1	2.000	10.0	1.0	1.0	0.081	STD2	2025-02-21 11:26:47 UTC-5	used
Standard 3	1	4.000	10.0	1.0	1.0	0.163	STD3	2025-02-21 11:48:11 UTC-5	used
Standard 4	1	5.000	10.0	1.0	1.0	0.207	STD4	2025-02-21 12:09:35 UTC-5	used
Standard 5	1	10.000	10.0	1.0	1.0	0.405	STD5	2025-02-21 12:31:01 UTC-5	used
Standard 6	1	20.000	10.0	1.0	1.0	0.837	STD6	2025-02-21 12:52:27 UTC-5	used
Standard 7	1	25.000	10.0	1.0	1.0	1.078	STD7	2025-02-21 13:13:53 UTC-5	used

Nitrate (Anions)

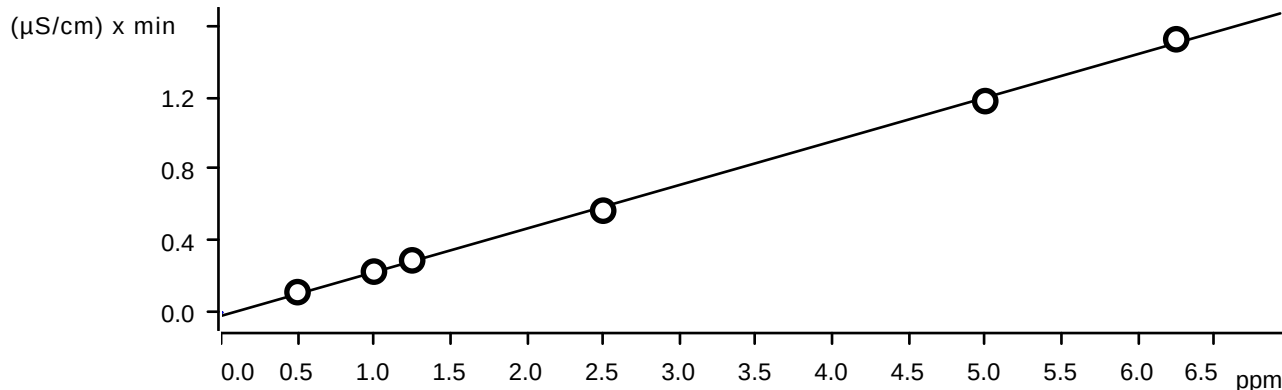

Function: $A = -0.0190446 + 0.0243327 \times Q$


Relative standard deviation 2.936394 %

Correlation coefficient 0.999557

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-02-21 11:05:25 UTC-5	used
Standard 2	1	0.500	10.0	1.0	1.0	0.113	STD2	2025-02-21 11:26:47 UTC-5	used
Standard 3	1	1.000	10.0	1.0	1.0	0.228	STD3	2025-02-21 11:48:11 UTC-5	used
Standard 4	1	1.250	10.0	1.0	1.0	0.290	STD4	2025-02-21 12:09:35 UTC-5	used
Standard 5	1	2.500	10.0	1.0	1.0	0.568	STD5	2025-02-21 12:31:01 UTC-5	used
Standard 6	1	5.000	10.0	1.0	1.0	1.178	STD6	2025-02-21 12:52:27 UTC-5	used
Standard 7	1	6.250	10.0	1.0	1.0	1.523	STD7	2025-02-21 13:13:53 UTC-5	used

Phosphate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

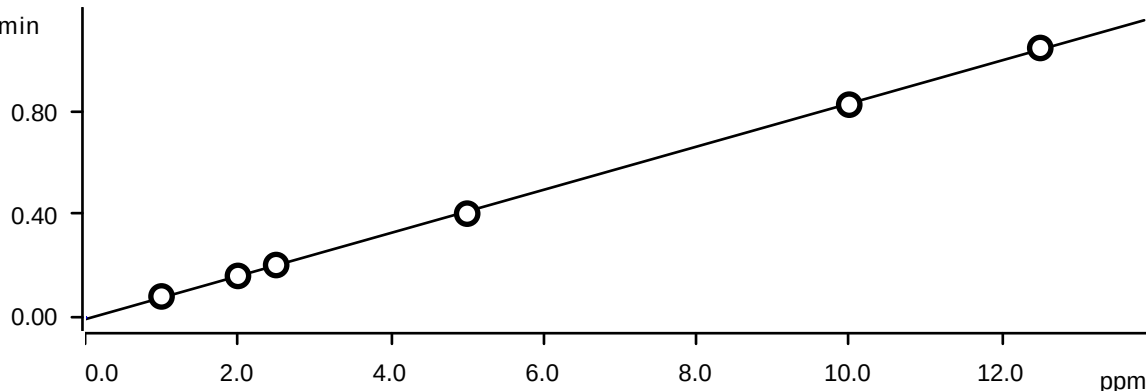


Function: $A = -6.44326E-3 + 8.35469E-3 \times Q$

Relative standard deviation 1.393773 %

Correlation coefficient 0.999897

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-02-21 11:05:25 UTC-5	used
Standard 2	1	1.000	10.0	1.0	1.0	0.082	STD2	2025-02-21 11:26:47 UTC-5	used
Standard 3	1	2.000	10.0	1.0	1.0	0.161	STD3	2025-02-21 11:48:11 UTC-5	used
Standard 4	1	2.500	10.0	1.0	1.0	0.204	STD4	2025-02-21 12:09:35 UTC-5	used
Standard 5	1	5.000	10.0	1.0	1.0	0.403	STD5	2025-02-21 12:31:01 UTC-5	used
Standard 6	1	10.000	10.0	1.0	1.0	0.825	STD6	2025-02-21 12:52:27 UTC-5	used
Standard 7	1	12.500	10.0	1.0	1.0	1.044	STD7	2025-02-21 13:13:53 UTC-5	used

Sulfate (Anions)

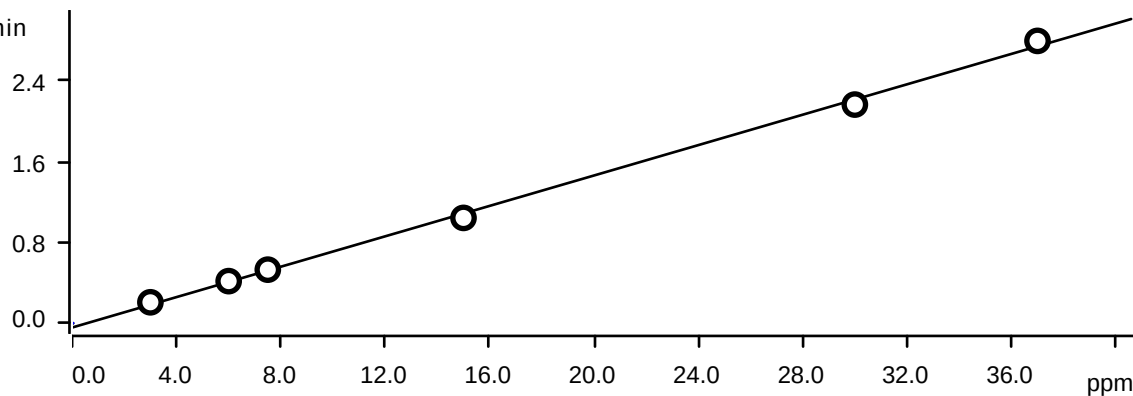 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0430107 + 7.53437E-3 \times Q$

Relative standard deviation 3.742757 %

Correlation coefficient 0.999282

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-02-21 11:05:25 UTC-5	used
Standard 2	1	3.000	10.0	1.0	1.0	0.207	STD2	2025-02-21 11:26:47 UTC-5	used
Standard 3	1	6.000	10.0	1.0	1.0	0.417	STD3	2025-02-21 11:48:11 UTC-5	used
Standard 4	1	7.500	10.0	1.0	1.0	0.531	STD4	2025-02-21 12:09:35 UTC-5	used
Standard 5	1	15.000	10.0	1.0	1.0	1.044	STD5	2025-02-21 12:31:01 UTC-5	used
Standard 6	1	30.000	10.0	1.0	1.0	2.167	STD6	2025-02-21 12:52:27 UTC-5	used
Standard 7	1	37.000	10.0	1.0	1.0	2.798	STD7	2025-02-21 13:13:53 UTC-5	used


Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-02-21 11:05:25 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

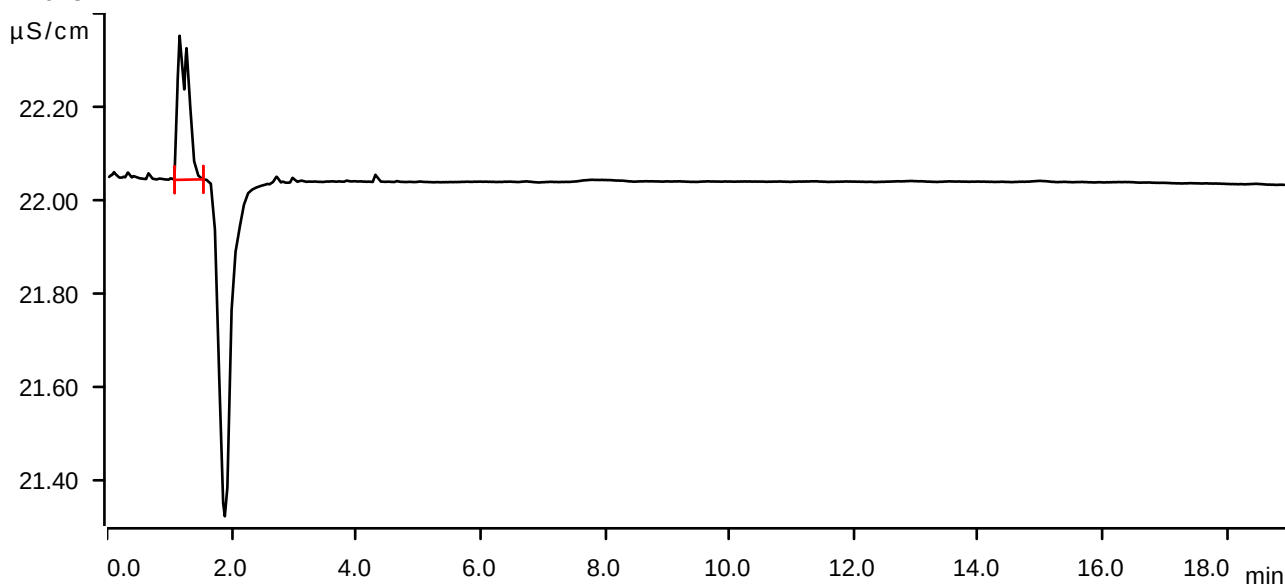

Peak number	Retention time	Area	Height	Concentration	Component name
	min	($\mu\text{S/cm}$) x min	$\mu\text{S/cm}$	ppm	
1	1.167	0.0607	0.309	invalid	


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-02-21 11:26:47 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

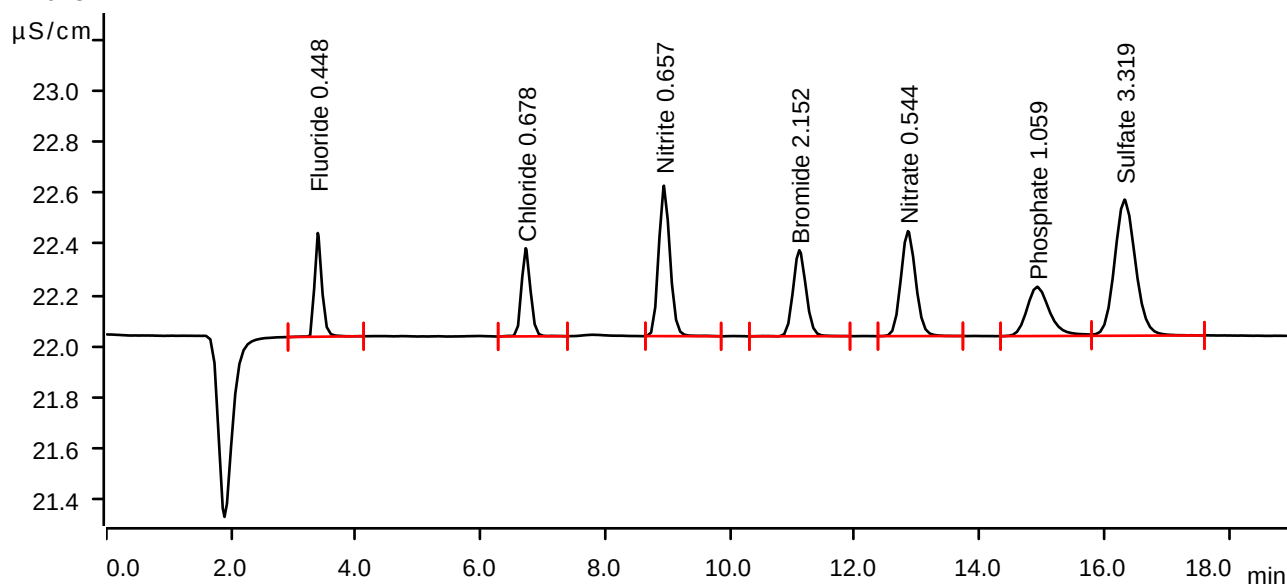

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.0550	0.405	0.448	Fluoride
2	6.723	0.0574	0.344	0.678	Chloride
3	8.940	0.1238	0.587	0.657	Nitrite
4	11.110	0.0813	0.336	2.152	Bromide
5	12.852	0.1132	0.410	0.544	Nitrate
6	14.923	0.0820	0.192	1.059	Phosphate
7	16.323	0.2071	0.531	3.319	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-02-21 11:48:11 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

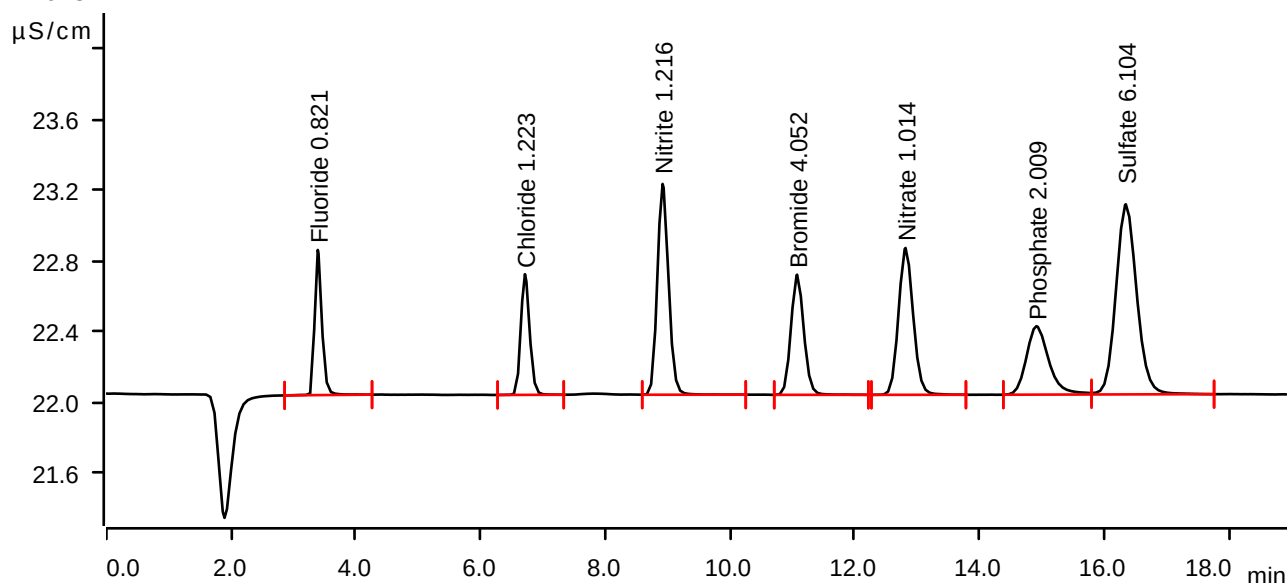

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.1102	0.822	0.821	Fluoride
2	6.712	0.1120	0.683	1.223	Chloride
3	8.918	0.2491	1.193	1.216	Nitrite
4	11.075	0.1631	0.680	4.052	Bromide
5	12.813	0.2277	0.831	1.014	Nitrate
6	14.912	0.1614	0.387	2.009	Phosphate
7	16.345	0.4169	1.076	6.104	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-02-21 12:09:35 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

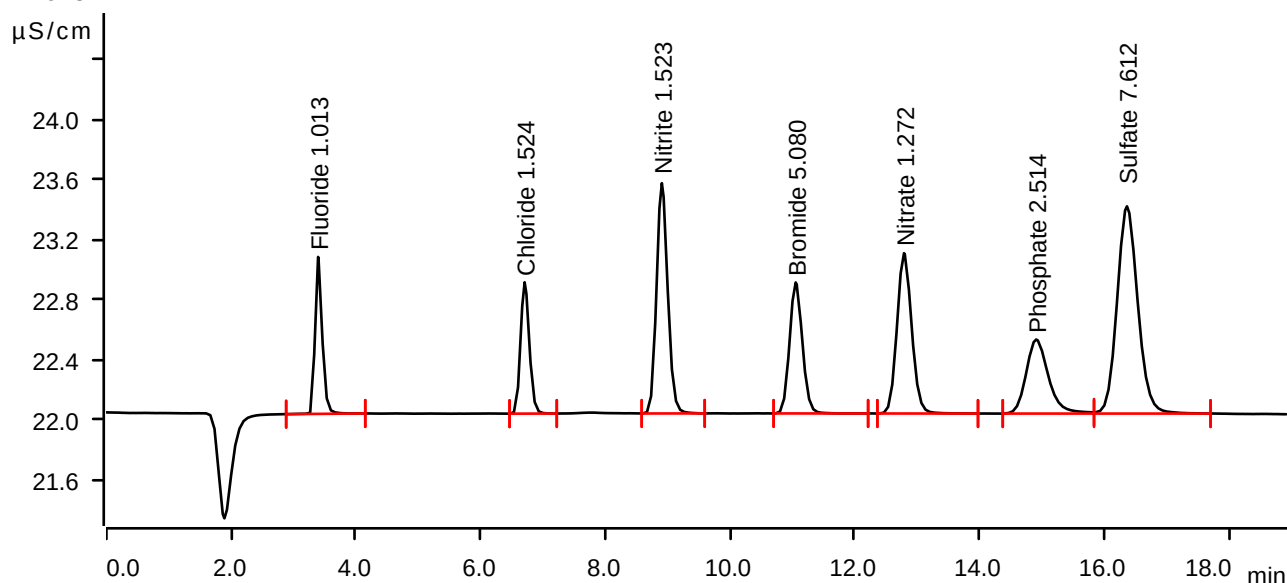

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.1386	1.042	1.013	Fluoride
2	6.707	0.1422	0.872	1.524	Chloride
3	8.907	0.3178	1.529	1.523	Nitrite
4	11.052	0.2073	0.870	5.080	Bromide
5	12.788	0.2904	1.064	1.272	Nitrate
6	14.908	0.2036	0.492	2.514	Phosphate
7	16.363	0.5305	1.376	7.612	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-02-21 12:31:01 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

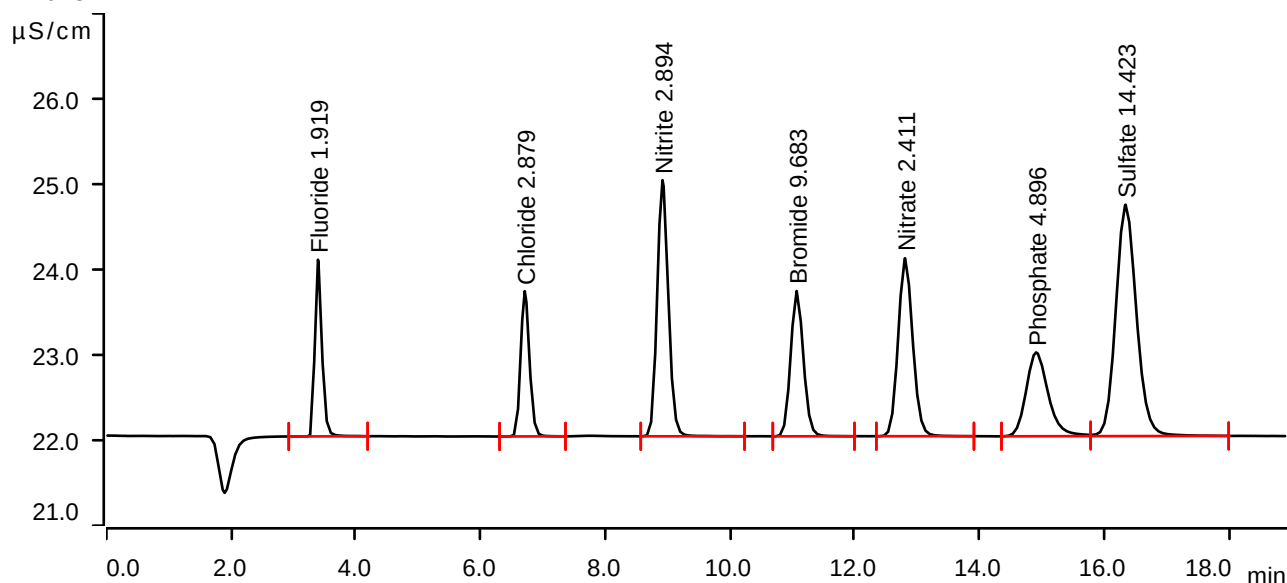

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.393	0.2728	2.069	1.919	Fluoride
2	6.708	0.2780	1.702	2.879	Chloride
3	8.917	0.6246	3.000	2.894	Nitrite
4	11.068	0.4054	1.702	9.683	Bromide
5	12.807	0.5675	2.085	2.411	Nitrate
6	14.907	0.4026	0.982	4.896	Phosphate
7	16.342	1.0436	2.711	14.423	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-02-21 12:52:27 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

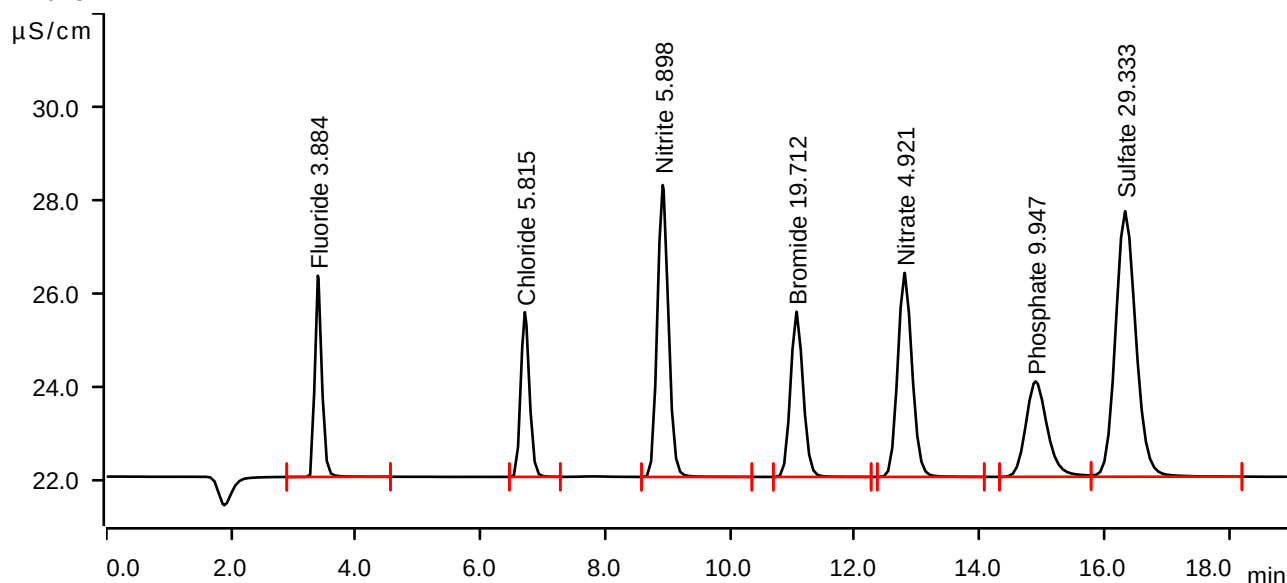

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.392	0.5636	4.320	3.884	Fluoride
2	6.710	0.5722	3.536	5.815	Chloride
3	8.920	1.2971	6.268	5.898	Nitrite
4	11.065	0.8370	3.548	19.712	Bromide
5	12.797	1.1784	4.381	4.921	Nitrate
6	14.898	0.8246	2.050	9.947	Phosphate
7	16.333	2.1670	5.703	29.333	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-02-21 13:13:53 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

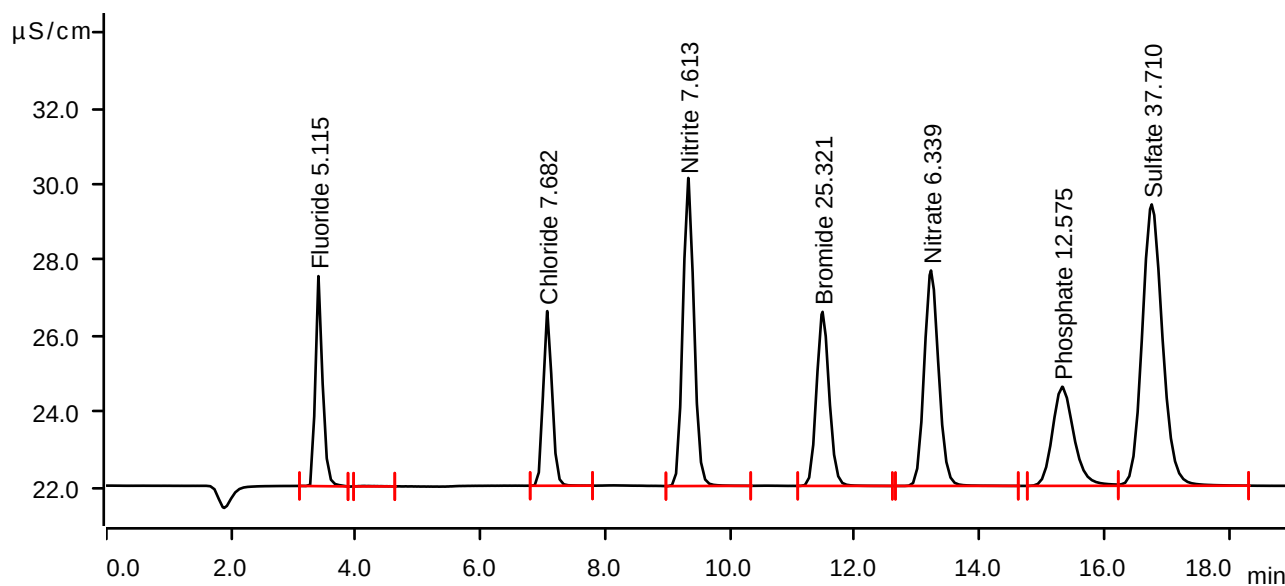

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.400	0.7457	5.535	5.115	Fluoride
2	4.197	0.0046	0.012	invalid	
3	7.070	0.7592	4.602	7.682	Chloride
4	9.330	1.6810	8.120	7.613	Nitrite
5	11.483	1.0784	4.588	25.321	Bromide
6	13.222	1.5233	5.678	6.339	Nitrate
7	15.325	1.0441	2.611	12.575	Phosphate
8	16.760	2.7982	7.416	37.710	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-02-21 13:35:21 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

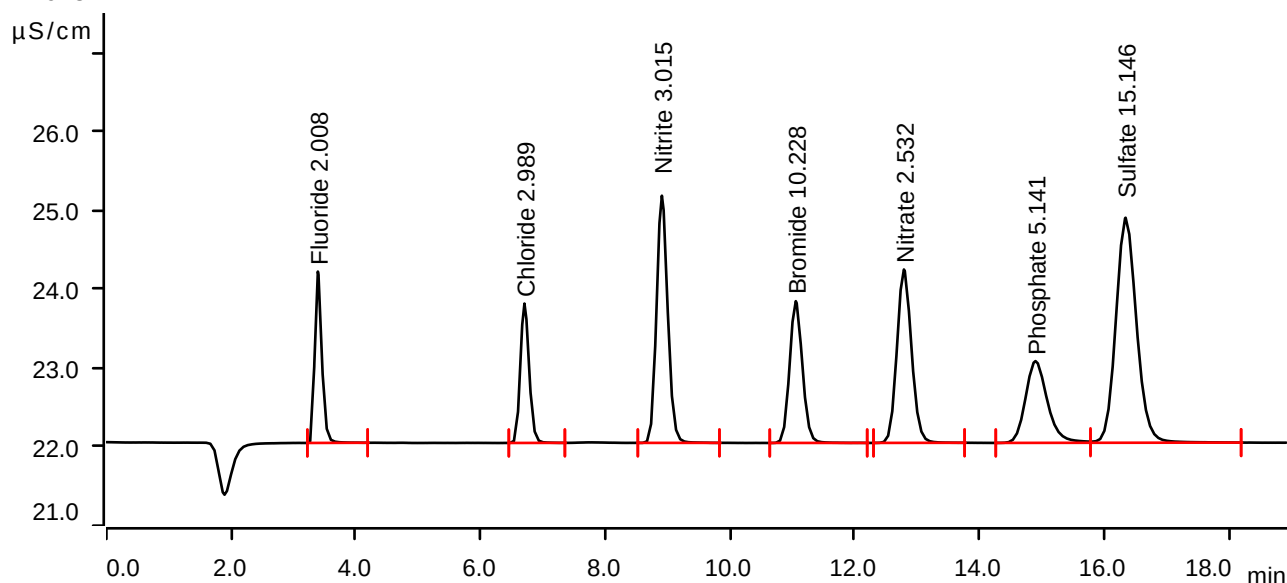


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.392	0.2859	2.174	2.008	Fluoride
2	6.703	0.2890	1.769	2.989	Chloride
3	8.907	0.6518	3.137	3.015	Nitrite
4	11.053	0.4289	1.799	10.228	Bromide
5	12.787	0.5971	2.200	2.532	Nitrate
6	14.897	0.4230	1.038	5.141	Phosphate
7	16.342	1.0982	2.855	15.146	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2025-02-21 13:56:49 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

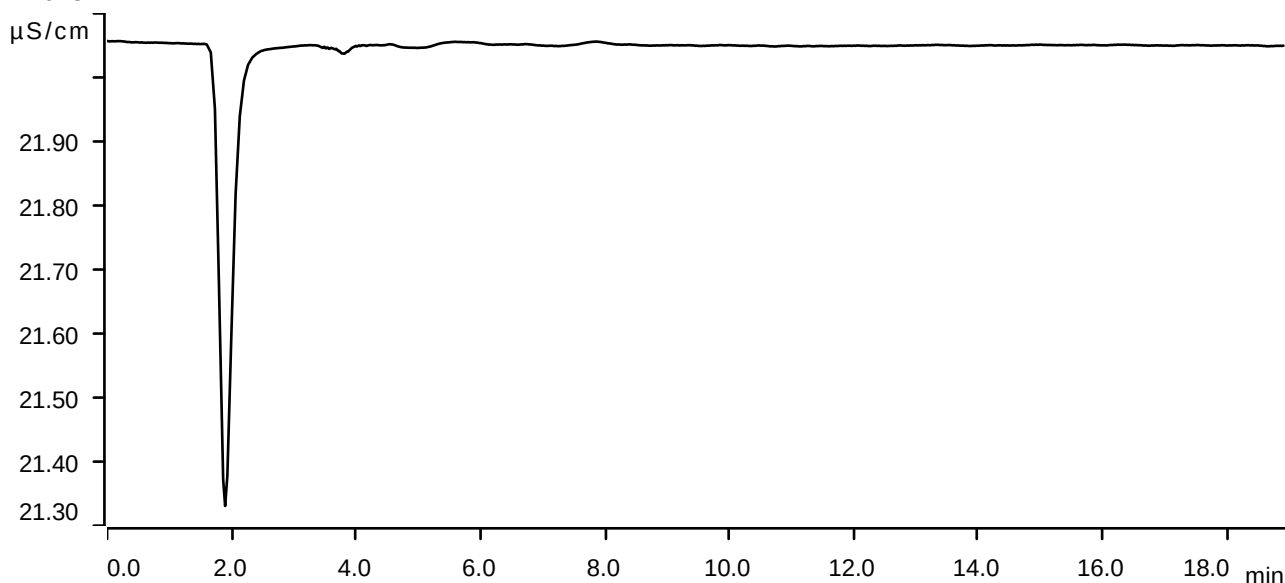Anions


Sample data

Ident CCV
 Sample type Check standard 1
 Determination start 2025-02-27 09:40:08 UTC-5
 Method IC1-022125
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.32 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

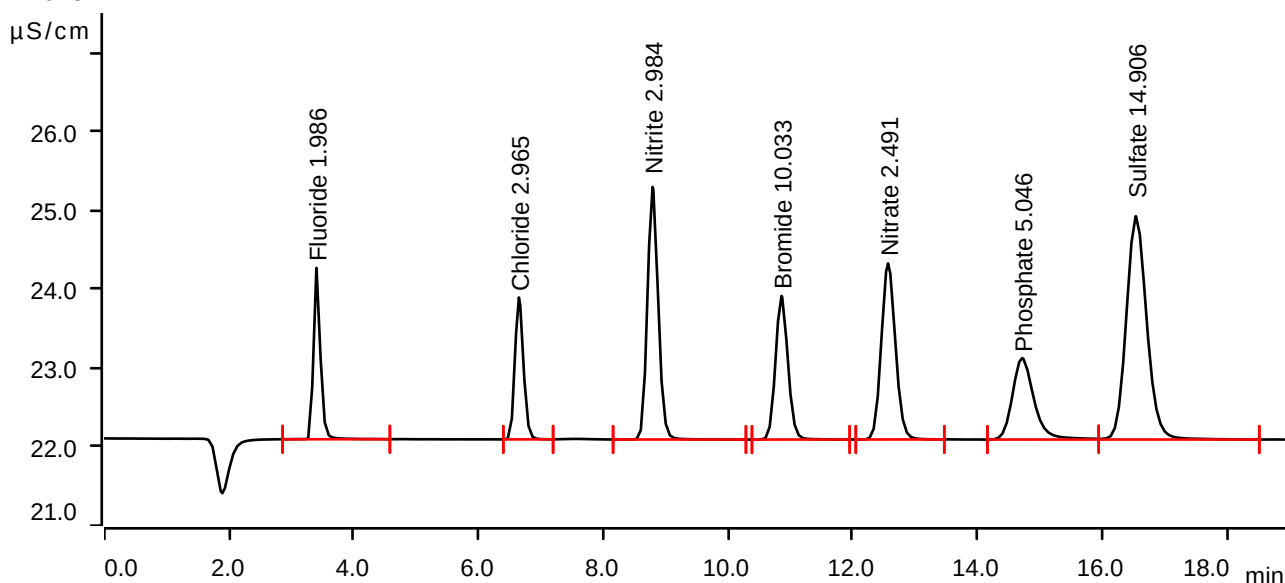


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.400	0.2827	2.174	1.986	Fluoride
2	6.647	0.2866	1.801	2.965	Chloride
3	8.790	0.6448	3.205	2.984	Nitrite
4	10.857	0.4205	1.822	10.033	Bromide
5	12.565	0.5871	2.235	2.491	Nitrate
6	14.715	0.4151	1.035	5.046	Phosphate
7	16.540	1.0801	2.834	14.906	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-02-27 10:01:38 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

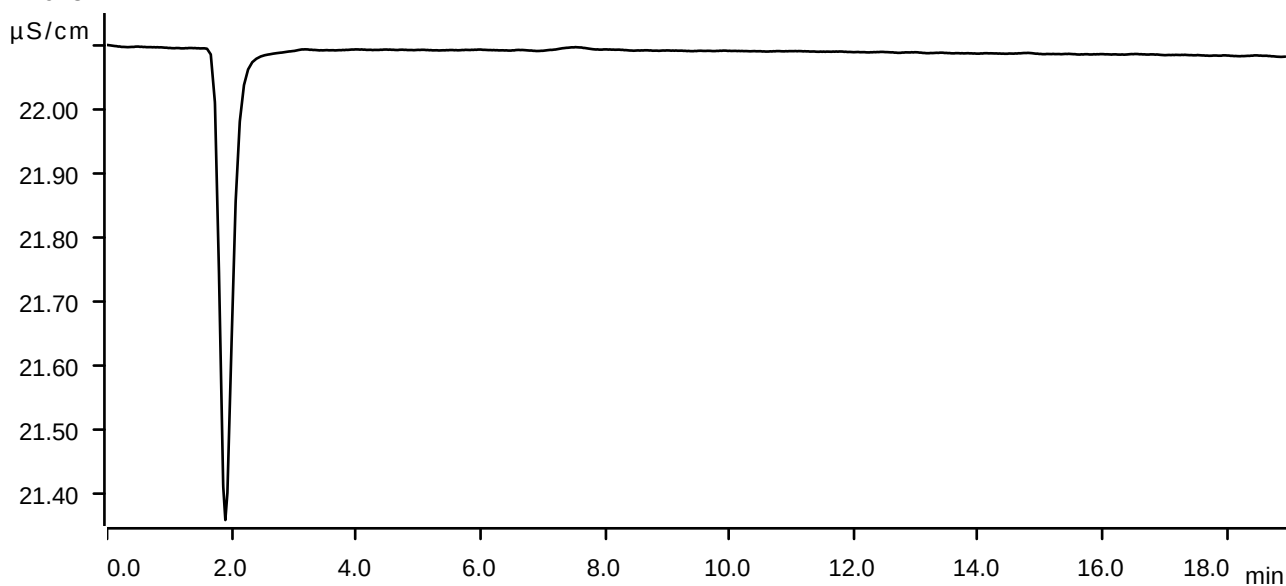
Anions

Sample data

Ident LB134838BLW
Sample type Sample
Determination start 2025-02-27 10:23:08 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

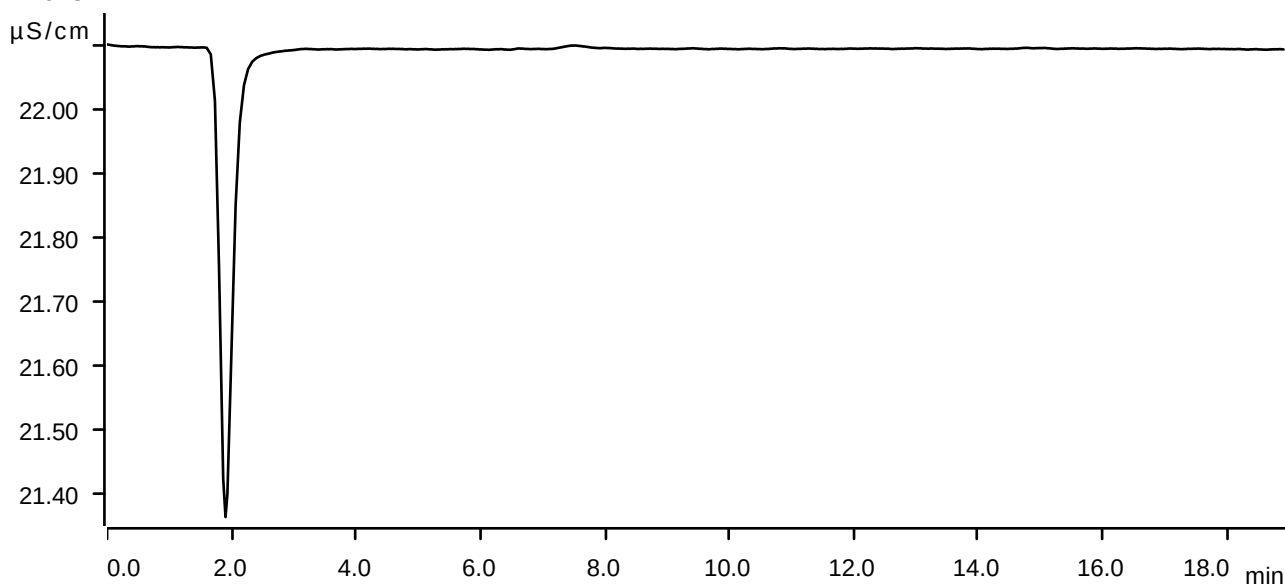Anions


Sample data

Ident LB134838BSW
 Sample type Check standard 1
 Determination start 2025-02-27 10:44:39 UTC-5
 Method IC1-022125
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.37 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

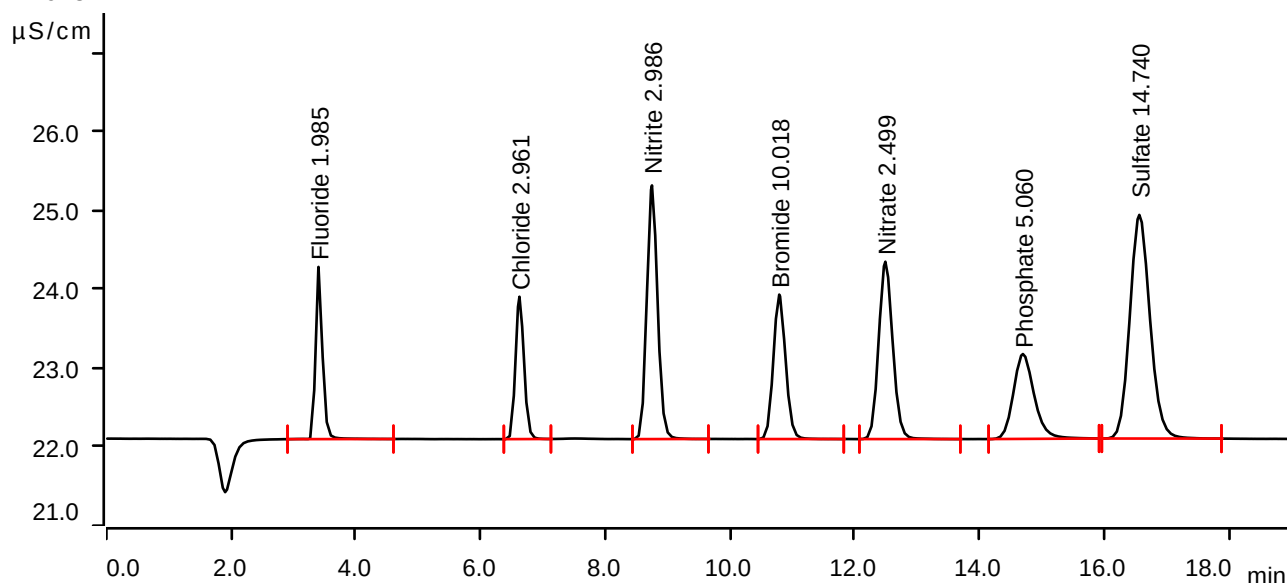

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.402	0.2825	2.185	1.985	Fluoride
2	6.623	0.2862	1.807	2.961	Chloride
3	8.748	0.6452	3.219	2.986	Nitrite
4	10.788	0.4198	1.833	10.018	Bromide
5	12.490	0.5891	2.251	2.499	Nitrate
6	14.695	0.4163	1.077	5.060	Phosphate
7	16.562	1.0676	2.838	14.740	Sulfate


Sample data

Ident Q1435-01
Sample type Sample
Determination start 2025-02-27 11:06:11 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

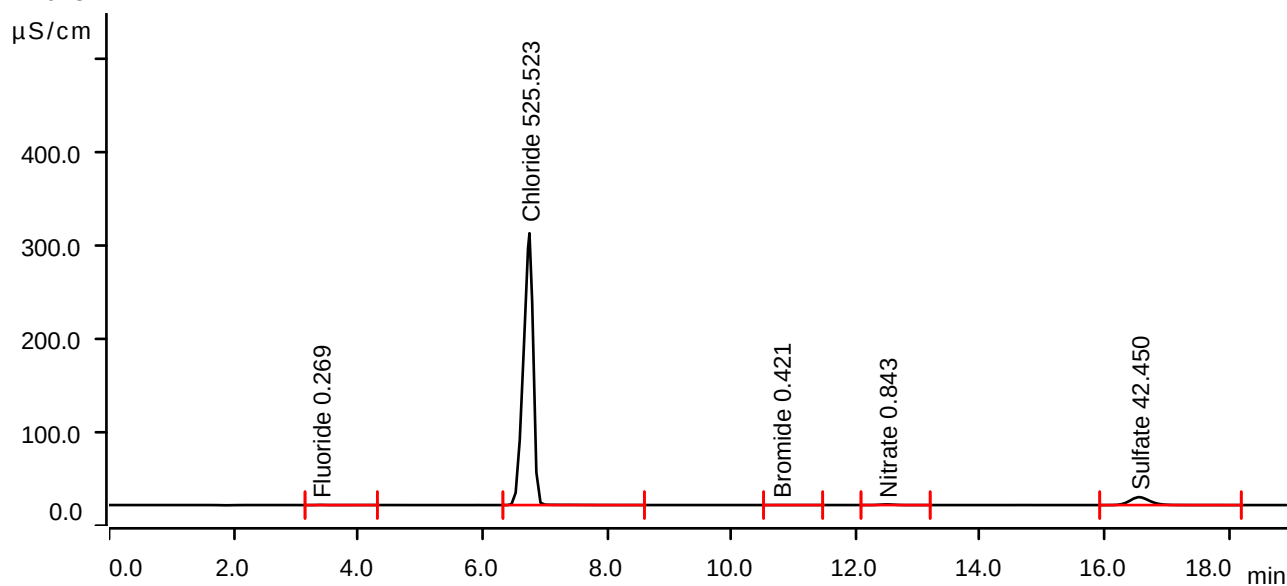

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.397	0.0286	0.199	0.269	Fluoride
2	6.757	52.6505	291.872	525.523	Chloride
3	10.793	0.0068	0.029	0.421	Bromide
4	12.498	0.1861	0.709	0.843	Nitrate
5	16.552	3.1554	8.528	42.450	Sulfate


Sample data

Ident Q1439-01
Sample type Sample
Determination start 2025-02-27 12:10:52 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

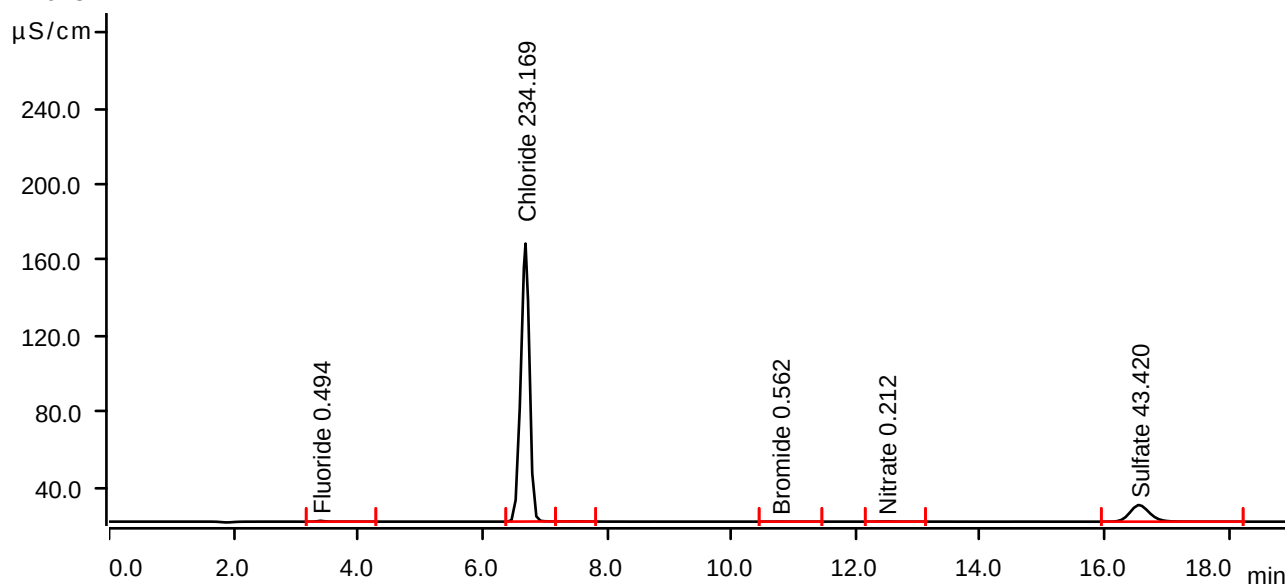

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.397	0.0618	0.452	0.494	Fluoride
2	6.693	23.4548	146.513	234.169	Chloride
3	7.340	0.0133	0.038	invalid	
4	10.780	0.0129	0.054	0.562	Bromide
5	12.487	0.0327	0.124	0.212	Nitrate
6	16.552	3.2284	8.738	43.420	Sulfate


Sample data

Ident Q1439-01MS
Sample type Sample
Determination start 2025-02-27 12:32:27 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.15 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

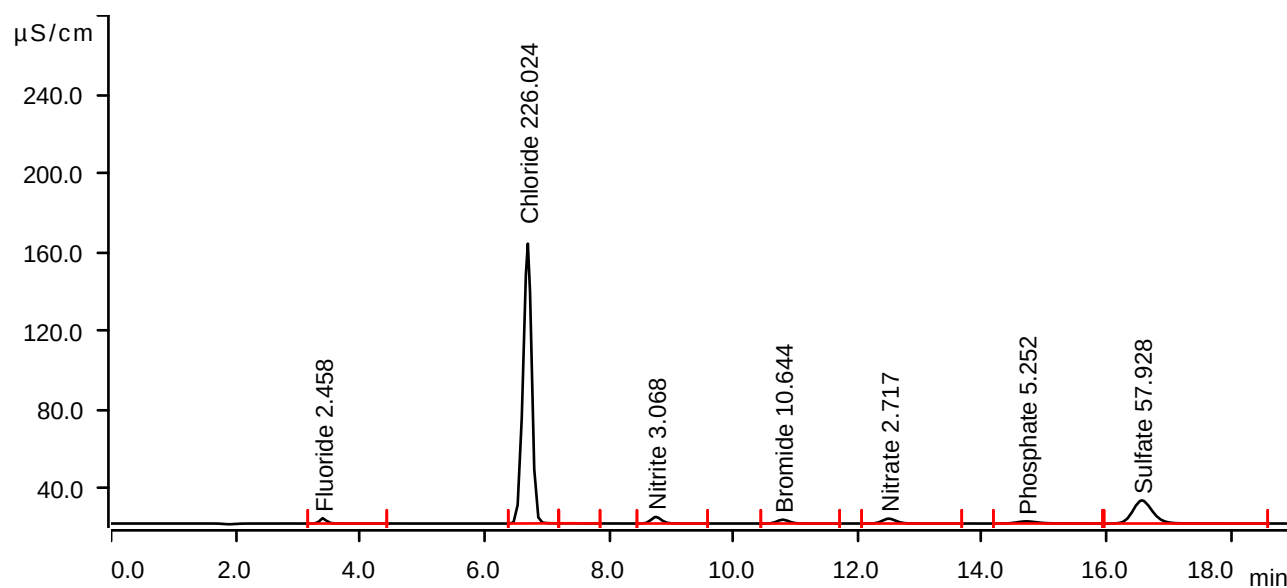

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.402	0.3524	2.709	2.458	Fluoride
2	6.698	22.6387	142.029	226.024	Chloride
3	7.372	0.0135	0.041	invalid	
4	8.757	0.6635	3.344	3.068	Nitrite
5	10.795	0.4467	1.957	10.644	Bromide
6	12.498	0.6421	2.464	2.717	Nitrate
7	14.708	0.4324	1.097	5.252	Phosphate
8	16.565	4.3215	11.744	57.928	Sulfate


Sample data

Ident Q1439-01MSD
Sample type Sample
Determination start 2025-02-27 12:54:02 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.09 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

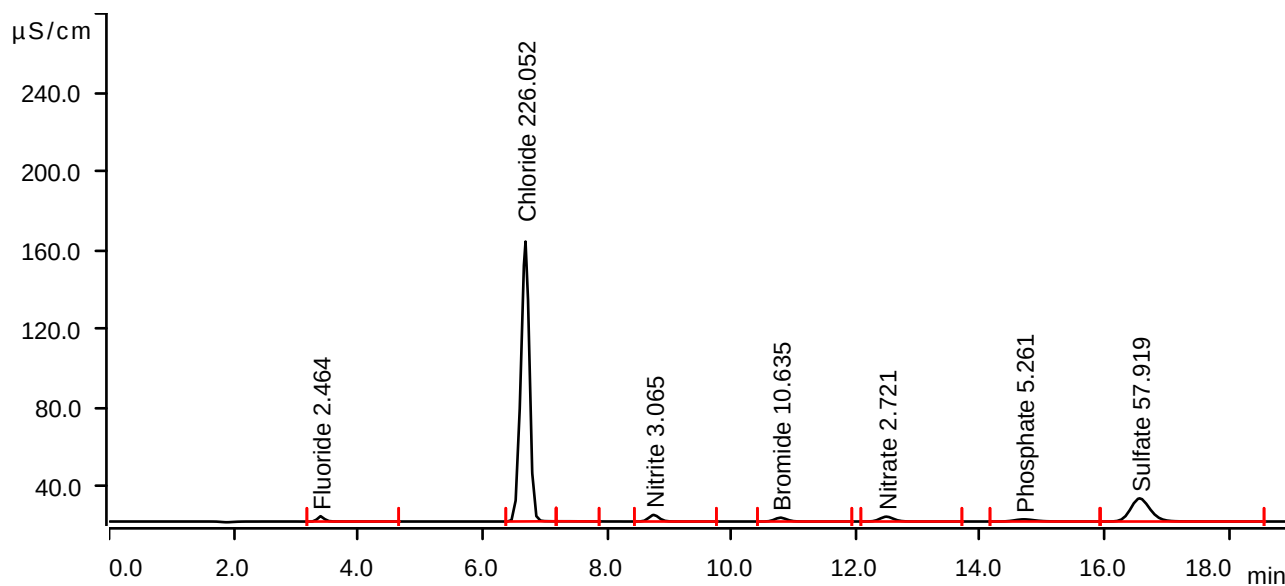

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.398	0.3534	2.701	2.464	Fluoride
2	6.693	22.6415	142.051	226.052	Chloride
3	7.357	0.0138	0.040	invalid	
4	8.753	0.6629	3.338	3.065	Nitrite
5	10.790	0.4464	1.955	10.635	Bromide
6	12.492	0.6431	2.464	2.721	Nitrate
7	14.702	0.4331	1.102	5.261	Phosphate
8	16.562	4.3208	11.746	57.919	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-02-27 13:15:36 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

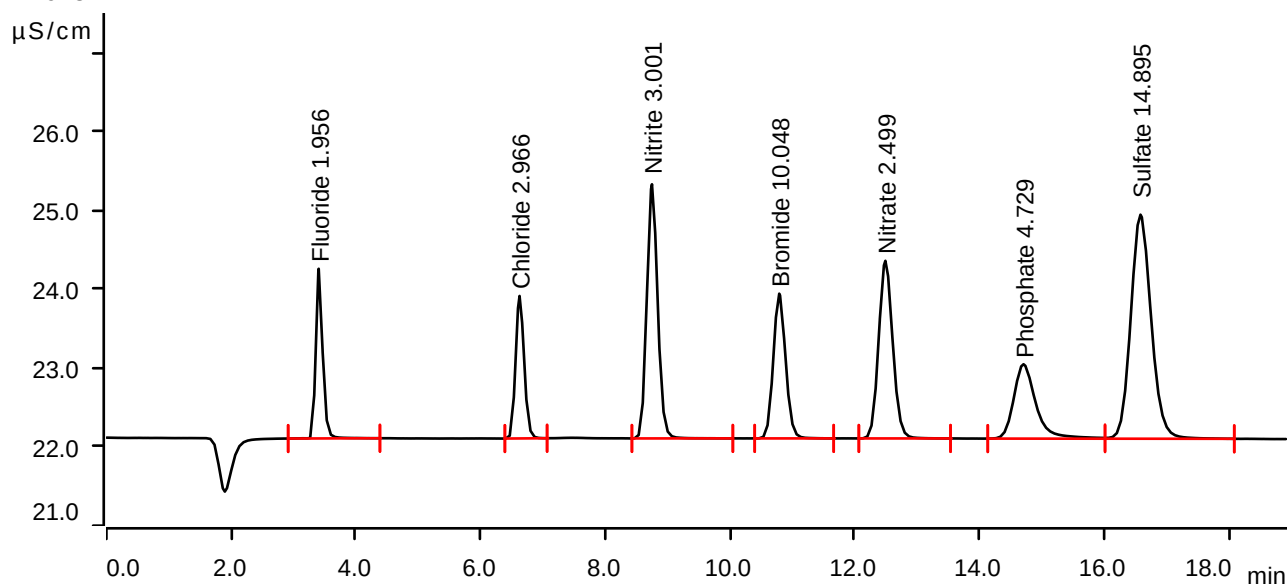

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.405	0.2783	2.153	1.956	Fluoride
2	6.625	0.2867	1.808	2.966	Chloride
3	8.748	0.6486	3.225	3.001	Nitrite
4	10.788	0.4211	1.837	10.048	Bromide
5	12.490	0.5891	2.254	2.499	Nitrate
6	14.705	0.3886	0.944	4.729	Phosphate
7	16.580	1.0792	2.844	14.895	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-02-27 13:37:06 UTC-5
Method IC1-022125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.15 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

