

16134857

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

2/28/2025 12:58

Reviewed by : RM

Instrument ID : Konelab

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.972	0.0	0.100	
ICB1	0.003	0.0	0.004	
CCV1	0.969	0.0	0.099	
CCB1	0.009	0.0	0.005	
PB166867BL	0.011	0.0	0.005	
PB166867BS	0.987	0.0	0.101	
Q1417-01	0.005	0.0	0.004	
Q1417-01DUP	0.008	0.0	0.005	
Q1417-01MS	1.060	0.0	0.108	
Q1417-01MSD	1.048	0.0	0.107	
CCV2	0.962	0.0	0.099	
CCB2	0.006	0.0	0.005	

N	12
Mean	0.503
SD	0.5192
CV%	103.14

Aquakem v. 7.2AQ1

Results from time period:

Fri Feb 28 11:05:18 2025

Fri Feb 28 12:55:47 2025

Sample Id	Sam/Ctr/c/	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.0012	mg/l	2/28/2025 11:48:20	
0.05PPM	A	Phenolics-	P	0.0377	mg/l	2/28/2025 11:48:21	
0.1PPM	A	Phenolics-	P	0.1043	mg/l	2/28/2025 11:48:22	
0.25PPM	A	Phenolics-	P	0.2615	mg/l	2/28/2025 11:48:23	
0.50PPM	A	Phenolics-	P	0.5023	mg/l	2/28/2025 11:48:24	
1.0PPM	A	Phenolics-	P	0.9945	mg/l	2/28/2025 11:48:25	
2.0PPM	A	Phenolics-	P	2.0008	mg/l	2/28/2025 11:48:26	
ICV1	S	Phenolics-	P	0.9716	mg/l	2/28/2025 12:48:54	
ICB1	S	Phenolics-	P	0.0034	mg/l	2/28/2025 12:48:57	
CCV1	S	Phenolics-	P	0.9688	mg/l	2/28/2025 12:48:59	
CCB1	S	Phenolics-	P	0.0092	mg/l	2/28/2025 12:49:00	
PB166867BL	S	Phenolics-	P	0.0111	mg/l	2/28/2025 12:49:03	
PB166867BS	S	Phenolics-	P	0.9871	mg/l	2/28/2025 12:49:04	
Q1417-01	S	Phenolics-	P	0.0045	mg/l	2/28/2025 12:55:40	
Q1417-01DUP	S	Phenolics-	P	0.0079	mg/l	2/28/2025 12:55:41	
Q1417-01MS	S	Phenolics-	P	1.0602	mg/l	2/28/2025 12:55:42	
Q1417-01MSD	S	Phenolics-	P	1.0483	mg/l	2/28/2025 12:55:43	
CCV2	S	Phenolics-	P	0.9624	mg/l	2/28/2025 12:55:44	
CCB2	S	Phenolics-	P	0.0063	mg/l	2/28/2025 12:55:46	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

2/28/2025 11:54 Reviewed by : RM Instrument ID : Konelab


Test Phenolics-

Accepted 2/28/2025 11:54

Factor 10.15
Bias 0.004

Coeff. of det. 0.999892

Errors

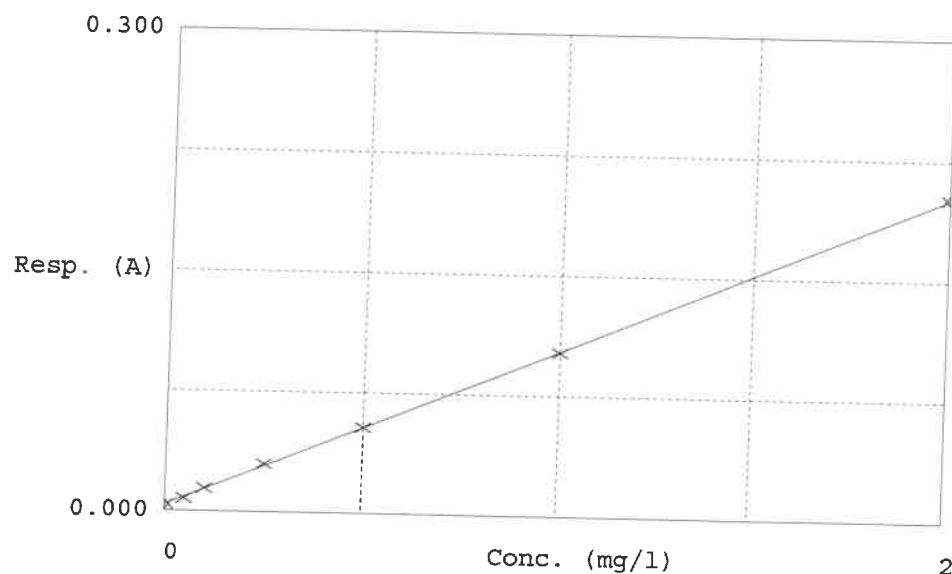

	Calibrator	Response	Calc. con.	Conc.	^{RM} Errors
1	0.00PPM	0.004	-0.0012	0.0000	-
2	Phenol-2	0.008	0.0377	0.0500	-24.6
3	Phenol-2	0.014	0.1043	0.1000	4.3
4	Phenol-2	0.030	0.2615	0.2500	4.6
5	Phenol-2	0.053	0.5023	0.5000	0.5
6	Phenol-2	0.102	0.9945	1.0000	-0.5
7	Phenol-2	0.201	2.0008	2.0000	0.0

02/28/2025
RM