


LB134869

7471B

INSTRUMENT ID: CV1

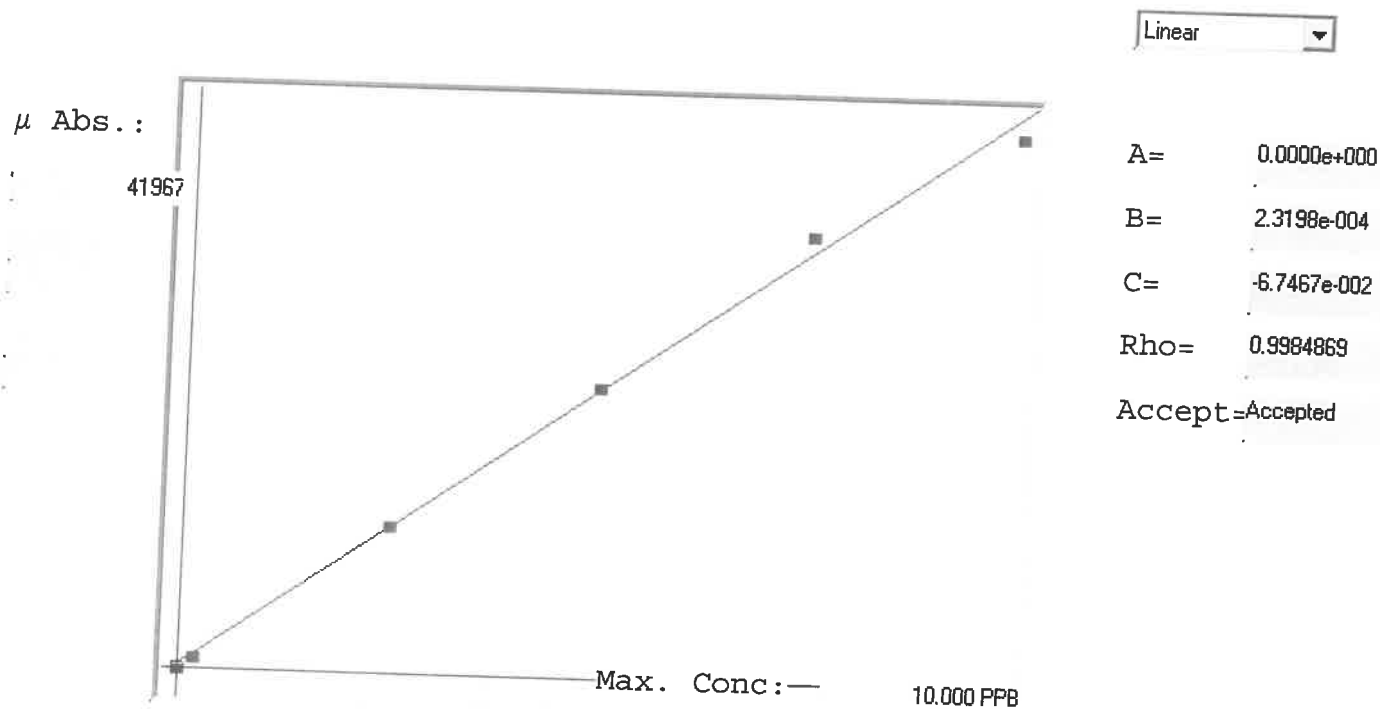

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	σ/d
0.0	0.000	-0.075	-0.075	-32	0.000	-32					
0.2	0.200	0.148	-0.052	928	0.0 %	928					
2.5	2.500	2.534	0.034	11213	0.0 %	11213					
5.0	5.000	5.077	0.077	22174	0.0 %	22174					
7.5	7.500	7.849	0.349	34124	0.0 %	34124					
10.0	10.000	9.668	-0.332	41967	0.0 %	41967					

Method: 7471B

Operator: Admin

LB134869 INSTRUMENTY ID : CV1

Date of Analysis: 03 Mar 2025 10:18:25

Operator: Admin		Date of Analysis: 03 Mar 2025 10:18:25							
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-32	-	0.0000	7471B	PPB	03 Mar 2025 10:49:12	S	Std
0.2 - 1	50.2	928	-	0.2000	7471B	PPB	03 Mar 2025 10:51:29	S	Std
2.5 - 1	52.5	11213	-	2.5000	7471B	PPB	03 Mar 2025 10:53:46	S	Std
5.0 - 1	55	22174	-	5.0000	7471B	PPB	03 Mar 2025 10:58:44	S	Std
7.5 - 1	57.5	34124	-	7.5000	7471B	PPB	03 Mar 2025 11:01:02	S	Std
10.0 - 1	510	41967	-	10.0000	7471B	PPB	03 Mar 2025 11:16:14	S	Std
ICV25 - 1	ICV25	19053	4.3525	-	7471B	PPB	03 Mar 2025 11:19:49	U	SMPL
ICB25 - 1	ICB25	44	-0.0573	-	7471B	PPB	03 Mar 2025 11:22:04	U	SMPL
CCV49 - 1	CCV49	22689	5.1960	-	7471B	PPB	03 Mar 2025 11:24:21	U	SMPL
CCB49 - 1	CCB49	67	-0.0519	-	7471B	PPB	03 Mar 2025 11:26:36	U	SMPL
CRA - 1	CRA	892	0.1395	-	7471B	PPB	03 Mar 2025 11:28:55	U	SMPL
HighStd - 1	HighStd	41992	9.6739	-	7471B	PPB	03 Mar 2025 11:33:55	U	SMPL
ChkStd - 1	ChkStd	31749	7.2977	-	7471B	PPB	03 Mar 2025 11:36:10	U	SMPL
PB166952BL - 1	PBS	246	-0.0104	-	7471B	PPB	03 Mar 2025 11:42:00	U	SMPL
PB166952BS - 1	LCSS	15546	3.5389	-	7471B	PPB	03 Mar 2025 11:44:16	U	SMPL
Q1457-01 - 1	HR-0-02272025	2006	0.3979	-	7471B	PPB	03 Mar 2025 11:46:32	U	SMPL
Q1457-01DUP - 1	HR-0-02272025DUP	2307	0.4677	-	7471B	PPB	03 Mar 2025 11:48:52	U	SMPL
Q1457-01MS - 1	HR-0-02272025MS	17493	3.9906	-	7471B	PPB	03 Mar 2025 11:51:12	U	SMPL
Q1457-01MSD - 1	HR-0-02272025MSD	18141	4.1409	-	7471B	PPB	03 Mar 2025 11:53:30	U	SMPL
Q1458-01 - 1	SP-SOIL	4724	1.0284	-	7471B	PPB	03 Mar 2025 11:55:49	U	SMPL
CCV50 - 1	CCV50	21648	4.9545	-	7471B	PPB	03 Mar 2025 11:58:07	U	SMPL
CCB50 - 1	CCB50	-1	-0.0677	-	7471B	PPB	03 Mar 2025 12:00:24	U	SMPL
Q1457-01LX5 - 1		413	0.0283	-	7471B	PPB	03 Mar 2025 12:02:42	U	SMPL
Q1457-01A - 1		18561	4.2384	-	7471B	PPB	03 Mar 2025 12:04:58	U	SMPL
CCV51 - 1	CCV51	22175	5.0767	-	7471B	PPB	03 Mar 2025 12:07:13	U	SMPL
CCB51 - 1	CCB51	85	-0.0477	-	7471B	PPB	03 Mar 2025 12:13:46	U	SMPL