

LB134924 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 Mar 2025 12:56:13

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	58	47	-	0.0000	7470A	PPB	06 Mar 2025 12:57:42	S	Std
0.2 - 1	50.2	928	-	0.2000	7470A	PPB	06 Mar 2025 12:59:59	S	Std
2.5 - 1	52.5	11137	-	2.5000	7470A	PPB	06 Mar 2025 13:02:16	S	Std
5.0 - 1	55	22234	-	5.0000	7470A	PPB	06 Mar 2025 13:04:33	S	Std
7.5 - 1	59.5	35861	-	7.5000	7470A	PPB	06 Mar 2025 13:09:38	S	Std
10.0 - 1	57.1	45131	-	10.0000	7470A	PPB	06 Mar 2025 13:14:35	S	Std
ICV34 - 1	ICV34	18801	4.1082	-	7470A	PPB	06 Mar 2025 13:25:15	U	SMPL
ICB34 - 1	ICB34	-278	-0.0401	-	7470A	PPB	06 Mar 2025 13:27:30	U	SMPL
CCV72 - 1	CCV72	21398	4.6729	-	7470A	PPB	06 Mar 2025 13:29:47	U	SMPL
CCB72 - 1	CCB72	-215	-0.0264	-	7470A	PPB	06 Mar 2025 13:32:03	U	SMPL
CRA - 1	CRA	696	0.1717	-	7470A	PPB	06 Mar 2025 13:34:21	U	SMPL
HighStd - 1	HighStd	44987	9.8018	-	7470A	PPB	06 Mar 2025 13:36:36	U	SMPL
ChkStd - 1	ChkStd	33225	7.2444	-	7470A	PPB	06 Mar 2025 13:38:51	U	SMPL
PB167014BL - 1	PBW	-457	-0.0790	-	7470A	PPB	06 Mar 2025 13:41:11	U	SMPL
PB167014BS - 1	LCSW	19162	4.1867	-	7470A	PPB	06 Mar 2025 13:46:18	U	SMPL
Q1478-13 - 1	IDW-SO-COMP-022825	-279	-0.0403	-	7470A	PPB	06 Mar 2025 13:48:34	U	SMPL
Q1480-08 - 1	TP-1	113	0.0450	-	7470A	PPB	06 Mar 2025 13:50:53	U	SMPL
Q1480-16 - 1	TP-2	16	0.0239	-	7470A	PPB	06 Mar 2025 13:53:10	U	SMPL
Q1480-24 - 1	TP-3	59	0.0332	-	7470A	PPB	06 Mar 2025 13:55:27	U	SMPL
Q1480-32 - 1	TP-4	58	0.0330	-	7470A	PPB	06 Mar 2025 13:57:43	U	SMPL
CCV73 - 1	CCV73	25124	5.4830	-	7470A	PPB	06 Mar 2025 13:59:58	U	SMPL
CCB73 - 1	CCB73	-275	-0.0394	-	7470A	PPB	06 Mar 2025 14:02:13	U	SMPL
Q1481-02 - 1	WC-K1311	-4	0.0195	-	7470A	PPB	06 Mar 2025 14:04:31	U	SMPL
Q1484-06 - 1	TR-OTR-COMP-01	18	0.0243	-	7470A	PPB	06 Mar 2025 14:06:47	U	SMPL
Q1489-04 - 1	TP-1	66	0.0347	-	7470A	PPB	06 Mar 2025 14:09:02	U	SMPL
Q1489-08 - 1	TP-2	185	0.0606	-	7470A	PPB	06 Mar 2025 14:11:18	U	SMPL
Q1489-12 - 1	TP-3	120	0.0465	-	7470A	PPB	06 Mar 2025 14:13:34	U	SMPL
Q1489-16 - 1	TP-4	24	0.0256	-	7470A	PPB	06 Mar 2025 14:15:51	U	SMPL
Q1489-16DUP - 1	TP-4DUP	48	0.0308	-	7470A	PPB	06 Mar 2025 14:18:08	U	SMPL
Q1489-16MS - 1	TP-4MS	18779	4.1035	-	7470A	PPB	06 Mar 2025 14:20:25	U	SMPL
Q1489-16MSD - 1	TP-4MSD	17411	3.8060	-	7470A	PPB	06 Mar 2025 14:22:42	U	SMPL
CCV74 - 1	CCV74	23083	5.0393	-	7470A	PPB	06 Mar 2025 14:27:58	U	SMPL
CCB74 - 1	CCB74	-273	-0.0390	-	7470A	PPB	06 Mar 2025 14:30:13	U	SMPL
Q1489-16LX5 - 1		45	0.0302	-	7470A	PPB	06 Mar 2025 14:32:31	U	SMPL
Q1489-16A - 1		18059	3.9469	-	7470A	PPB	06 Mar 2025 14:34:47	U	SMPL
PB166968TB - 1	PB166968TB	-155	-0.0133	-	7470A	PPB	06 Mar 2025 14:37:02	U	SMPL
CCV75 - 1	CCV75	22353	4.8805	-	7470A	PPB	06 Mar 2025 14:41:23	U	SMPL
CCB75 - 1	CCB75	-201	-0.0233	-	7470A	PPB	06 Mar 2025 14:43:38	U	SMPL

LB134924


7470A

INSTRUMENT ID: CVL

Linear

 μ Abs.:

45131

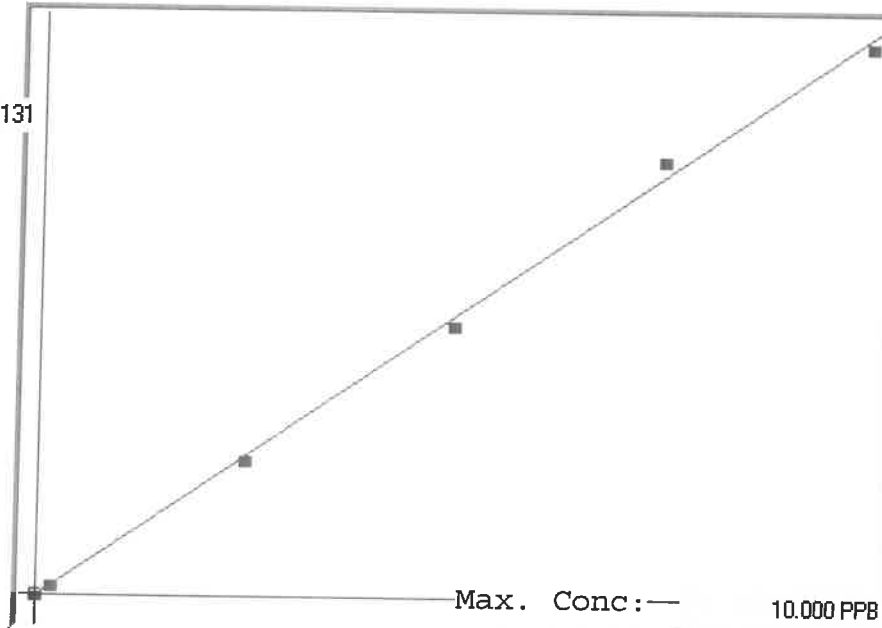

A= 0.0000e+000

B= 2.1743e-004

C= 2.0388e-002

Rho= 0.9990533

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o.k.)
0.0	0.000	0.031	0.031	47	0.000	47	0				1
0.2	0.200	0.222	0.022	928	0.0 %	928					1
2.5	2.500	2.442	-0.058	11137	0.0 %	11137					-2
5.0	5.000	4.855	-0.145	22234	0.0 %	22234					-3
7.5	7.500	7.818	0.318	35861	0.0 %	35861					-4
10.0	10.000	9.833	-0.167	45131	0.0 %	45131					-2