

LB135000 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 12 Mar 2025 14:16:05

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	80	80	-	0.0000	7471B	PPB	12 Mar 2025 14:21:13	S	Std
0.2 - 1	1186	1186	-	0.2000	7471B	PPB	12 Mar 2025 14:23:30	S	Std
2.5 - 1	14239	14239	-	2.5000	7471B	PPB	12 Mar 2025 14:25:48	S	Std
5.0 - 1	29555	29555	-	5.0000	7471B	PPB	12 Mar 2025 14:28:05	S	Std
7.5 - 1	44452	44452	-	7.5000	7471B	PPB	12 Mar 2025 14:30:23	S	Std
10.0 - 1	58157	58157	-	10.0000	7471B	PPB	12 Mar 2025 14:32:42	S	Std
ICV39 - 1	ICV39	22028	3.7589	-7471B	PPB	12 Mar 2025 14:35:30	U	SMPL	
ICB39 - 1	ICB39	43	0.0049	-7471B	PPB	12 Mar 2025 14:37:46	U	SMPL	
CCV01 - 1	CCV01	28500	4.8640	-7471B	PPB	12 Mar 2025 14:40:04	U	SMPL	
CCB01 - 1	CCB01	-23	-0.0063	-7471B	PPB	12 Mar 2025 14:42:19	U	SMPL	
CRA - 1	CRA	1100	0.1854	-7471B	PPB	12 Mar 2025 14:44:37	U	SMPL	
HighStd - 1	HighStd	57444	9.8062	-7471B	PPB	12 Mar 2025 14:46:53	U	SMPL	
ChkStd - 1	ChkStd	40609	6.9316	-7471B	PPB	12 Mar 2025 14:49:08	U	SMPL	
PB167105BL - 1	PBS	-188	-0.0345	-7471B	PPB	12 Mar 2025 14:51:33	U	SMPL	
PB167105BS - 1	LCSS	24058	4.1055	-7471B	PPB	12 Mar 2025 14:53:53	U	SMPL	
Q1534-01 - 1	OR-363-COMP-16	4339	0.7385	-7471B	PPB	12 Mar 2025 14:56:10	U	SMPL	
Q1534-07 - 1	OR-363-COMP-17	6210	1.0579	-7471B	PPB	12 Mar 2025 14:58:29	U	SMPL	
Q1534-13 - 1	OR-363-COMP-18	31374	5.3547	-7471B	PPB	12 Mar 2025 15:00:48	U	SMPL	
Q1534-19 - 1	OR-363-COMP-19	10886	1.8564	-7471B	PPB	12 Mar 2025 15:03:08	U	SMPL	
Q1535-01 - 1	SU-03-03102025	4112	0.6997	-7471B	PPB	12 Mar 2025 15:05:26	U	SMPL	
CCV02 - 1	CCV02	28863	4.9259	-7471B	PPB	12 Mar 2025 15:07:43	U	SMPL	
CCB02 - 1	CCB02	-151	-0.0282	-7471B	PPB	12 Mar 2025 15:10:00	U	SMPL	
Q1537-01 - 1	COMP-1	4016	0.6833	-7471B	PPB	12 Mar 2025 15:12:20	U	SMPL	
Q1537-02 - 1	COMP-2	143	0.0220	-7471B	PPB	12 Mar 2025 15:14:36	U	SMPL	
Q1537-03 - 1	COMP-3	149	0.0230	-7471B	PPB	12 Mar 2025 15:16:53	U	SMPL	
Q1545-01 - 1	BU-02-031125	332	0.0543	-7471B	PPB	12 Mar 2025 15:19:09	U	SMPL	
Q1545-01DUP - 1	BU-02-031125DUP	757	0.1268	-7471B	PPB	12 Mar 2025 15:21:25	U	SMPL	
Q1545-01MS - 1	BU-02-031125MS	22822	3.8944	-7471B	PPB	12 Mar 2025 15:23:42	U	SMPL	
Q1545-01MSD - 1	BU-02-031125MSD	22409	3.8239	-7471B	PPB	12 Mar 2025 15:25:58	U	SMPL	
Q1545-01LX5 - 1		360	0.0591	-7471B	PPB	12 Mar 2025 15:30:01	U	SMPL	
Q1545-01A - 1		22969	3.9195	-7471B	PPB	12 Mar 2025 15:32:18	U	SMPL	
CCV03 - 1	CCV03	28457	4.8566	-7471B	PPB	12 Mar 2025 15:34:34	U	SMPL	
CCB03 - 1	CCB03	-217	-0.0395	-7471B	PPB	12 Mar 2025 15:36:56	U	SMPL	

LB135000


7471B

INSTRUMENT ID: 7471

Linear

 μ Abs.:

58157

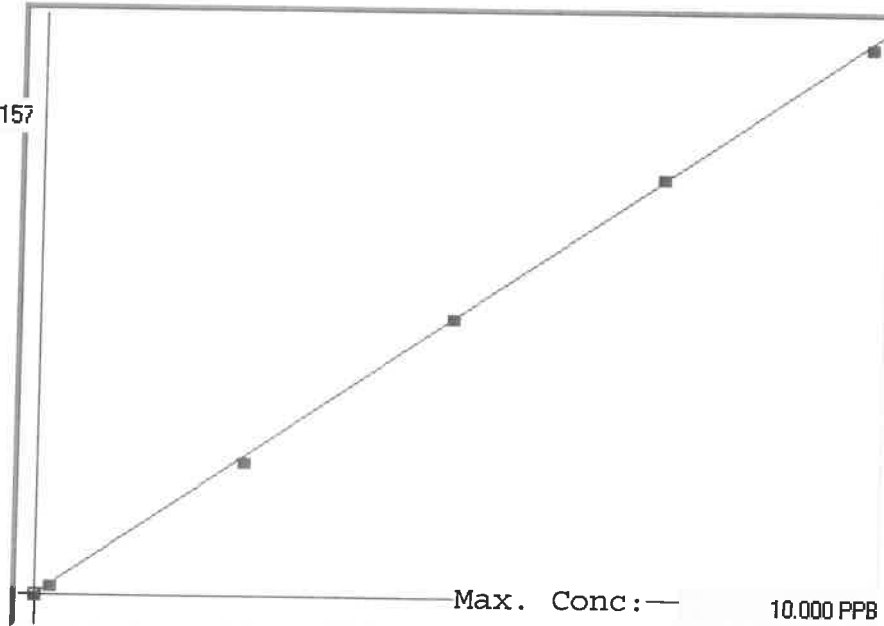

A= 0.0000e+000

B= 1.7075e-004

C= -2.4145e-003

Rho= 0.9998774

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% RD
0.0	0.000	0.011	0.011	80	0.000	80					
0.2	0.200	0.200	0.000	1186	0.0 %	1186					
2.5	2.500	2.429	-0.071	14239	0.0 %	14239					
5.0	5.000	5.044	0.044	29555	0.0 %	29555					
7.5	7.500	7.588	0.088	44452	0.0 %	44452					
10.0	10.000	9.928	-0.072	58157	0.0 %	58157					

0.10
1.3
1.1
1.1