


LB135120

SFAM01.1

INSTRUMENT ID: CV1

Linear

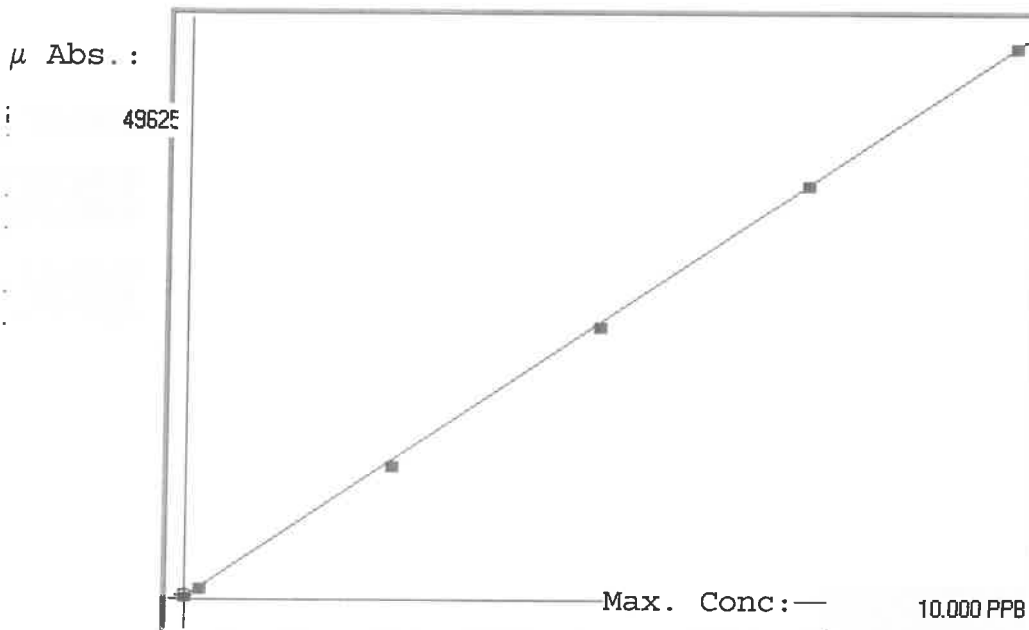

A= 0.0000e+000

B= 2.0245e-004 *slope*C= -3.1477e-002 *intercept*

Rho= 0.9999421

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.057	0.057	438	0.000	438					
0.05	0.050										
0.20	0.200	0.204	0.004	1165	0.0 %	1165					
2.50	2.500	2.432	-0.068	12170	0.0 %	12170					
5.00	5.000	4.970	-0.030	24704	0.0 %	24704					
7.50	7.500	7.521	0.021	37307	0.0 %	37307					
10.0	10.000	10.015	0.015	49625	0.0 %	49625					

Handwritten notes:
 0.00
 0.05
 0.20
 2.50
 5.00
 7.50
 10.00

LB135120
INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 SS0	438	-		0 SFAM01.1	PPB	3/21/2025 9:00	Std
	0.2 S01	1165	-		0.2 SFAM01.1	PPB	3/21/2025 9:03	Std
	2.5 S02	12170	-		2.5 SFAM01.1	PPB	3/21/2025 9:05	Std
	5 S03	24704	-		5 SFAM01.1	PPB	3/21/2025 9:07	Std
	7.5 S04	37307	-		7.5 SFAM01.1	PPB	3/21/2025 9:09	Std
	10 S05	49625	-		10 SFAM01.1	PPB	3/21/2025 9:12	Std
ICV051	ICV051	20013	4.0201 -		SFAM01.1	PPB	3/21/2025 9:15	SMPL
ICB051	ICB051	138	-0.0035 -		SFAM01.1	PPB	3/21/2025 9:17	SMPL
CCV035	CCV035	24940	5.0176 -		SFAM01.1	PPB	3/21/2025 9:19	SMPL
CCB035	CCB035	123	-0.0066 -		SFAM01.1	PPB	3/21/2025 9:22	SMPL
PB167256BL	PBW256	94	-0.0124 -		SFAM01.1	PPB	3/21/2025 9:27	SMPL
Q1546-01	MDL-WATER	445	0.0586 -		SFAM01.1	PPB	3/21/2025 9:44	SMPL
CCV036	CCV036	24314	4.8909 -		SFAM01.1	PPB	3/21/2025 9:47	SMPL
CCB036	CCB036	228	0.0147 -		SFAM01.1	PPB	3/21/2025 9:49	SMPL